

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092421\
 Data File : BM032138.D
 Acq On : 24 Sep 2021 19:35
 Operator : CG/JU
 Sample : SST02034
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SST020041

Quant Time: Sep 25 00:20:09 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 25 00:18:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.666	152	409358	20.000	ng/u1	0.00
20) Naphthalene-d8	10.466	136	1710546	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.319	164	1071545	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.042	188	2125394	20.000	ng/u1	0.00
79) Chrysene-d12	21.201	240	1814828	20.000	ng/u1	0.00
88) Perylene-d12	23.371	264	1581983	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.990	96	79989	8.050	ng/uL	0.00
4) Pyridine-d5	3.413	84	567880	18.028	ng/u1	0.00
7) Phenol-d5	6.848	99	664859	17.772	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.990	67	407887	18.114	ng/u1	0.00
11) 2-Chlorophenol-d4	7.207	132	518124	19.390	ng/u1	0.00
15) 4-Methylphenol-d8	8.395	113	516351	17.075	ng/u1	0.00
21) Nitrobenzene-d5	8.825	128	212081	21.767	ng/u1	0.00
24) 2-Nitrophenol-d4	9.548	143	222357	24.066	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.089	165	519192	20.794	ng/u1	0.00
31) 4-Chloroaniline-d4	10.595	131	707276	19.147	ng/u1	0.00
46) Dimethylphthalate-d6	13.719	166	1486314	19.857	ng/u1	0.00
49) Acenaphthylene-d8	14.007	160	1899635	20.142	ng/u1	0.00
54) 4-Nitrophenol-d4	14.513	143	229116	18.980	ng/u1	0.00
60) Fluorene-d10	15.301	176	1269815	20.431	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.419	200	181549	23.367	ng/u1	0.00
73) Anthracene-d10	17.136	188	1905871	20.861	ng/u1	0.00
81) Pyrene-d10	19.424	212	2015063	22.869	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.236	264	1583118	20.379	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.025	88	87786	7.807	ng/uL	100
5) Pyridine	3.437	79	562490	18.183	ng/u1	100
6) Benzaldehyde	6.790	77	433078	19.642	ng/u1	100
8) Phenol	6.878	94	678327	17.806	ng/u1	100
10) Bis(2-Chloroethyl)ether	7.084	93	546826	18.414	ng/u1	100
12) 2-Chlorophenol	7.237	128	545544	19.631	ng/u1	100
13) 2-Methylphenol	8.125	108	510674	17.497	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.201	45	760327	19.724	ng/u1	100
16) Acetophenone	8.484	105	840801	17.960	ng/u1	100
17) N-Nitroso-di-n-propyla...	8.478	70	412534	15.821	ng/u1	100
18) 4-Methylphenol	8.454	108	554806	17.709	ng/u1	100
19) Hexachloroethane	8.760	117	219379	19.093	ng/u1	100
22) Nitrobenzene	8.866	77	555773	20.136	ng/u1	100
23) Isophorone	9.384	82	1167389	17.174	ng/u1	100
25) 2-Nitrophenol	9.578	139	259852	24.335	ng/u1	100
26) 2,4-Dimethylphenol	9.654	107	620980	19.090	ng/u1	100
27) Bis(2-Chloroethoxy)met...	9.872	93	737791	18.997	ng/u1	100
29) 2,4-Dichlorophenol	10.119	162	509212	20.830	ng/u1	100
30) Naphthalene	10.513	128	1766764	20.971	ng/u1	100
32) 4-Chloroaniline	10.619	127	738230	19.528	ng/u1	100
33) Hexachlorobutadiene	10.825	225	344992	21.573	ng/u1	100
34) Caprolactam	11.342	113	150475	14.408	ng/u1	100
35) 4-Chloro-3-methylphenol	11.754	107	553320	18.151	ng/u1	100
36) 2-Methylnaphthalene	12.125	142	1194219	20.146	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092421\
 Data File : BM032138.D
 Acq On : 24 Sep 2021 19:35
 Operator : CG/JU
 Sample : SST02034
 Misc :
 ALS Vial : 4 Sample Multiplier: 1


Instrument :
 BNA_M
 ClientSampleId :
 SST020041


Quant Time: Sep 25 00:20:09 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 25 00:18:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.348	142	1211703	20.082	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.507	216	644748	22.498	ng/ul	100
40) Hexachlorocyclopentadiene	12.501	237	332528	19.525	ng/ul	100
41) 2,4,6-Trichlorophenol	12.748	196	401180	21.610	ng/ul	100
42) 2,4,5-Trichlorophenol	12.819	196	426847	21.861	ng/ul	100
43) 1,1'-Biphenyl	13.142	154	1610479	21.535	ng/ul	100
44) 2-Chloronaphthalene	13.183	162	1208928	21.307	ng/ul	100
45) 2-Nitroaniline	13.383	65	273767	21.445	ng/ul	100
47) Dimethylphthalate	13.766	163	1487167	19.938	ng/ul	100
48) 2,6-Dinitrotoluene	13.877	165	246236	23.310	ng/ul	100
50) Acenaphthylene	14.036	152	2012828	20.872	ng/ul	100
51) 3-Nitroaniline	14.207	138	260762	21.178	ng/ul	100
52) Acenaphthene	14.377	153	1284487	20.445	ng/ul	100
53) 2,4-Dinitrophenol	14.407	184	105377	19.244	ng/ul	100
55) 4-Nitrophenol	14.524	109	195261	16.892	ng/ul	100
56) Dibenzofuran	14.713	168	1850794	20.923	ng/ul	100
57) 2,4-Dinitrotoluene	14.666	165	351526	22.850	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	14.942	232	352818	21.434	ng/ul	100
59) Diethylphthalate	15.130	149	1460578	18.797	ng/ul	100
61) Fluorene	15.360	166	1467018	20.569	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.348	204	735451	21.051	ng/ul	100
63) 4-Nitroaniline	15.366	138	238029	18.660	ng/ul	100
66) 4,6-Dinitro-2-methylph...	15.430	198	184366	22.964	ng/ul	100
67) N-Nitrosodiphenylamine	15.560	169	1257772	21.385	ng/ul	100
68) 4-Bromophenyl-phenylether	16.236	248	426344	21.257	ng/ul	100
69) Hexachlorobenzene	16.371	284	514140	22.866	ng/ul	100
70) Atrazine	16.501	200	440779	19.403	ng/ul	100
71) Pentachlorophenol	16.707	266	284645	22.071	ng/ul	100
72) Phenanthrene	17.083	178	2269488	21.168	ng/ul	100
74) Anthracene	17.171	178	2311214	21.120	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.119	216	673249	24.143	ng/ul	100
76) Pentachlorobenzene	14.648	250	661248	24.026	ng/ul	100
77) Carbazole	17.436	167	2022728	20.394	ng/ul	100
78) Di-n-butylphthalate	17.995	149	2307770	18.592	ng/ul	100
80) Fluoranthene	19.089	202	2516606	22.580	ng/ul	100
82) Pyrene	19.454	202	2586478	22.966	ng/ul	100
83) Butylbenzylphthalate	20.336	149	743805	16.839	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.118	252	627226	16.380	ng/ul	100
85) Benzo(a)anthracene	21.189	228	2191245	19.967	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.112	149	1130992	16.867	ng/ul	100
87) Chrysene	21.236	228	2181369	20.553	ng/ul	100
89) Di-n-octyl phthalate	21.959	149	1632405	18.325	ng/ul	100
90) Benzo(b)fluoranthene	22.724	252	1998176	21.459	ng/ul	100
91) Benzo(k)fluoranthene	22.765	252	1919118	22.457	ng/ul	100
93) Benzo(a)pyrene	23.277	252	1883181	20.903	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	25.524	276	1882363	18.113	ng/ul	100
95) Dibenzo(a,h)anthracene	25.530	278	1559347	17.694	ng/ul	100
96) Benzo(g,h,i)perylene	26.183	276	1640526	18.387	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Sep 25 00:20:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 25 00:18:47 2021
Response via : Initial Calibration







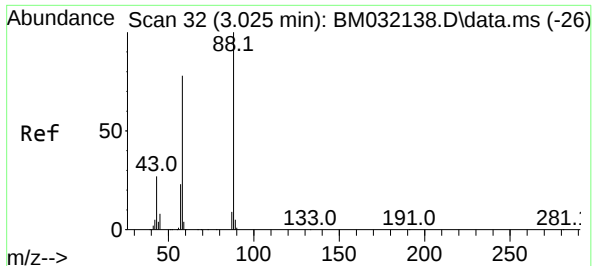

#2
1,4-Dioxane
Concen: 7.807 ng/uL
RT: 3.025 min Scan# 32
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion	Ratio	Lower	Upper
88	100		
43	27.9	22.3	33.5
58	78.0	62.4	93.6



#5
Pyridine
Concen: 18.183 ng/uL
RT: 3.437 min Scan# 102
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion	Ratio	Lower	Upper
79	100		
52	72.9	58.3	87.5
51	36.4	29.1	43.7









#6
Benzaldehyde
Concen: 19.642 ng/ul
RT: 6.790 min Scan# 672
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion: 77 Resp: 433078
Ion Ratio Lower Upper
77 100
105 96.2 77.0 115.4
106 92.7 74.2 111.2



#8
Phenol
Concen: 17.806 ng/ul
RT: 6.878 min Scan# 687
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion: 94 Resp: 678327
Ion Ratio Lower Upper
94 100
65 28.0 22.4 33.6
66 37.4 29.9 44.9









#10
 Bis(2-Chloroethyl)ether
 Concen: 18.414 ng/ul
 RT: 7.084 min Scan# 722
 Delta R.T. 0.000 min
 Lab File: BM032138.D
 Acq: 24 Sep 2021 19:35

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020041

Tgt Ion: 93 Resp: 546826




Ion	Ratio	Lower	Upper
93	100		
63	79.3	63.4	95.2
95	31.9	25.5	38.3




#12
 2-Chlorophenol
 Concen: 19.631 ng/ul
 RT: 7.237 min Scan# 748
 Delta R.T. 0.000 min
 Lab File: BM032138.D
 Acq: 24 Sep 2021 19:35

Tgt Ion:128 Resp: 545544

Ion	Ratio	Lower	Upper
128	100		
64	47.9	38.3	57.5
130	32.3	25.8	38.8









#13
2-Methylphenol
Concen: 17.497 ng/ul
RT: 8.125 min Scan# 899
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:108 Resp: 510674
Ion Ratio Lower Upper
108 100
107 89.5 71.6 107.4



#14
2,2'-oxybis(1-Chloropropane)
Concen: 19.724 ng/ul
RT: 8.201 min Scan# 912
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion: 45 Resp: 760327
Ion Ratio Lower Upper
45 100
77 14.0 11.2 16.8
79 11.4 9.1 13.7









#16
Acetophenone
Concen: 17.960 ng/ul
RT: 8.484 min Scan# 960
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:105 Resp: 840801
Ion Ratio Lower Upper
105 100
77 78.7 63.0 94.4
51 27.7 22.2 33.2



#17
N-Nitroso-di-n-propylamine
Concen: 15.821 ng/ul
RT: 8.478 min Scan# 959
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion: 70 Resp: 412534
Ion Ratio Lower Upper
70 100
42 57.8 46.2 69.4
101 9.4 7.5 11.3
130 20.2 16.2 24.2









#18
4-Methylphenol
Concen: 17.709 ng/ul
RT: 8.454 min Scan# 955
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:108 Resp: 554806
Ion Ratio Lower Upper
108 100
107 111.4 89.1 133.7



#19
Hexachloroethane
Concen: 19.093 ng/ul
RT: 8.760 min Scan# 1007
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:117 Resp: 219379
Ion Ratio Lower Upper
117 100
201 99.4 79.5 119.3
199 61.4 49.1 73.7









#22
Nitrobenzene
Concen: 20.136 ng/ul
RT: 8.866 min Scan# 1025
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion: 77 Resp: 555773
Ion Ratio Lower Upper
77 100
123 45.1 36.1 54.1
65 13.8 11.0 16.6



#23
Isophorone
Concen: 17.174 ng/ul
RT: 9.384 min Scan# 1113
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion: 82 Resp: 1167389
Ion Ratio Lower Upper
82 100
95 7.2 5.8 8.6
138 17.6 14.1 21.1









#25
2-Nitrophenol
Concen: 24.335 ng/ul
RT: 9.578 min Scan# 1146
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:139 Resp: 259852
Ion Ratio Lower Upper
139 100
65 52.5 42.0 63.0
109 32.3 25.8 38.8



#26
2,4-Dimethylphenol
Concen: 19.090 ng/ul
RT: 9.654 min Scan# 1159
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:107 Resp: 620980
Ion Ratio Lower Upper
107 100
121 50.5 40.4 60.6
122 84.5 67.6 101.4









#27
 Bis(2-Chloroethoxy)methane
 Concen: 18.997 ng/ul
 RT: 9.872 min Scan# 1196
 Delta R.T. 0.000 min
 Lab File: BM032138.D
 Acq: 24 Sep 2021 19:35




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020041


Tgt Ion: 93	Resp: 737791
Ion Ratio	Lower Upper
93 100	
95 32.8	26.2 39.4
123 11.3	9.0 13.6



#29
 2,4-Dichlorophenol
 Concen: 20.830 ng/ul
 RT: 10.119 min Scan# 1238
 Delta R.T. 0.000 min
 Lab File: BM032138.D
 Acq: 24 Sep 2021 19:35

Tgt Ion:162	Resp: 509212
Ion Ratio	Lower Upper
162 100	
164 64.5	51.6 77.4
98 35.7	28.6 42.8









#30
Naphthalene
Concen: 20.971 ng/ul
RT: 10.513 min Scan# 1305
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:128 Resp: 1766764
Ion Ratio Lower Upper
128 100
129 10.9 8.7 13.1
127 12.8 10.2 15.4



#32
4-Chloroaniline
Concen: 19.528 ng/ul
RT: 10.619 min Scan# 1323
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:127 Resp: 738230
Ion Ratio Lower Upper
127 100
129 32.2 25.8 38.6









#33
Hexachlorobutadiene
Concen: 21.573 ng/ul
RT: 10.825 min Scan# 1358
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:225 Resp: 344992
Ion Ratio Lower Upper
225 100
223 63.3 50.6 76.0
227 65.3 52.2 78.4



#34
Caprolactam
Concen: 14.408 ng/ul
RT: 11.342 min Scan# 1446
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:113 Resp: 150475
Ion Ratio Lower Upper
113 100
55 172.6 138.1 207.1
56 132.5 106.0 159.0









#35
4-Chloro-3-methylphenol
Concen: 18.151 ng/ul
RT: 11.754 min Scan# 1516
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:107 Resp: 553320
Ion Ratio Lower Upper
107 100
144 25.4 20.3 30.5
142 78.5 62.8 94.2



#36
2-Methylnaphthalene
Concen: 20.146 ng/ul
RT: 12.125 min Scan# 1579
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:142 Resp: 1194219
Ion Ratio Lower Upper
142 100
141 87.7 70.2 105.2





#37

1-Methylnaphthalene

Concen: 20.082 ng/ul

RT: 12.348 min Scan# 1617

Delta R.T. 0.000 min

Lab File: BM032138.D

Acq: 24 Sep 2021 19:35

Instrument :

BNA_M

ClientSampleId :

SSTD020041





Tgt Ion:142 Resp: 1211703

Ion Ratio Lower Upper

142 100

141 92.9 74.3 111.5

116 3.8 3.0 4.6



#39

1,2,4,5-Tetrachlorobenzene

Concen: 22.498 ng/ul

RT: 12.507 min Scan# 1644

Delta R.T. 0.000 min

Lab File: BM032138.D

Acq: 24 Sep 2021 19:35

Tgt Ion:216 Resp: 644748




Ion Ratio Lower Upper


216 100

214 80.3 64.2 96.4

179 21.4 17.1 25.7

108 20.0 16.0 24.0









#40
Hexachlorocyclopentadiene
Concen: 19.525 ng/ul
RT: 12.501 min Scan# 1643
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:237 Resp: 332528
Ion Ratio Lower Upper
237 100
235 61.7 49.4 74.0
272 12.6 10.1 15.1



#41
2,4,6-Trichlorophenol
Concen: 21.610 ng/ul
RT: 12.748 min Scan# 1685
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:196 Resp: 401180
Ion Ratio Lower Upper
196 100
198 97.2 77.8 116.6
200 30.7 24.6 36.8









#42
2,4,5-Trichlorophenol
Concen: 21.861 ng/ul
RT: 12.819 min Scan# 1697
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:196 Resp: 426847
Ion Ratio Lower Upper
196 100
198 96.8 77.4 116.2
200 30.4 24.3 36.5



#43
1,1'-Biphenyl
Concen: 21.535 ng/ul
RT: 13.142 min Scan# 1752
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:154 Resp: 1610479
Ion Ratio Lower Upper
154 100
153 39.9 31.9 47.9
76 13.4 10.7 16.1









#44
2-Chloronaphthalene
Concen: 21.307 ng/ul
RT: 13.183 min Scan# 1759
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:162 Resp: 1208928
Ion Ratio Lower Upper
162 100
164 32.4 25.9 38.9
127 40.0 32.0 48.0



#45
2-Nitroaniline
Concen: 21.445 ng/ul
RT: 13.383 min Scan# 1793
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion: 65 Resp: 273767
Ion Ratio Lower Upper
65 100
92 68.1 54.5 81.7
138 105.1 84.1 126.1









#47
Dimethylphthalate
Concen: 19.938 ng/ul
RT: 13.766 min Scan# 1858
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:163 Resp: 1487167
Ion Ratio Lower Upper
163 100
194 4.1 3.3 4.9
164 10.1 8.1 12.1



#48
2,6-Dinitrotoluene
Concen: 23.310 ng/ul
RT: 13.877 min Scan# 1877
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:165 Resp: 246236
Ion Ratio Lower Upper
165 100
89 58.5 46.8 70.2
121 21.6 17.3 25.9









#50
Acenaphthylene
Concen: 20.872 ng/ul
RT: 14.036 min Scan# 1904
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:152 Resp: 2012828
Ion Ratio Lower Upper
152 100
151 19.6 15.7 23.5
153 13.2 10.6 15.8



#51
3-Nitroaniline
Concen: 21.178 ng/ul
RT: 14.207 min Scan# 1933
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:138 Resp: 260762
Ion Ratio Lower Upper
138 100
108 13.1 10.5 15.7
92 117.5 94.0 141.0









#52
Acenaphthene
Concen: 20.445 ng/ul
RT: 14.377 min Scan# 1962
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:153 Resp: 1284487
Ion Ratio Lower Upper
153 100
152 48.0 38.4 57.6
154 88.8 71.0 106.6



#53
2,4-Dinitrophenol
Concen: 19.244 ng/ul
RT: 14.407 min Scan# 1967
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:184 Resp: 105377
Ion Ratio Lower Upper
184 100
63 70.9 56.7 85.1
154 71.9 57.5 86.3









#55
4-Nitrophenol
Concen: 16.892 ng/ul
RT: 14.524 min Scan# 1987
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:109 Resp: 195261
Ion Ratio Lower Upper
109 100
139 129.6 103.7 155.5
65 136.8 109.4 164.2



#56
Dibenzofuran
Concen: 20.923 ng/ul
RT: 14.713 min Scan# 2019
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:168 Resp: 1850794
Ion Ratio Lower Upper
168 100
139 37.2 29.8 44.6









#57
2,4-Dinitrotoluene
Concen: 22.850 ng/ul
RT: 14.666 min Scan# 2011
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:165 Resp: 351526
Ion Ratio Lower Upper
165 100
63 42.7 34.2 51.2
182 2.9 2.3 3.5



#58
2,3,4,6-Tetrachlorophenol
Concen: 21.434 ng/ul
RT: 14.942 min Scan# 2058
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:232 Resp: 352818
Ion Ratio Lower Upper
232 100
131 45.2 36.2 54.2
130 2.4 1.9 2.9
166 31.0 24.8 37.2









#59
Diethylphthalate
Concen: 18.797 ng/ul
RT: 15.130 min Scan# 2090
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:149 Resp: 1460578
Ion Ratio Lower Upper
149 100
177 22.4 17.9 26.9
150 12.5 10.0 15.0



#61
Fluorene
Concen: 20.569 ng/ul
RT: 15.360 min Scan# 2129
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:166 Resp: 1467018
Ion Ratio Lower Upper
166 100
165 97.1 77.7 116.5
167 13.4 10.7 16.1









#62
4-Chlorophenyl-phenylether
Concen: 21.051 ng/ul
RT: 15.348 min Scan# 2127
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:204 Resp: 735451
Ion Ratio Lower Upper
204 100
206 32.2 25.8 38.6
141 59.9 47.9 71.9



#63
4-Nitroaniline
Concen: 18.660 ng/ul
RT: 15.366 min Scan# 2130
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:138 Resp: 238029
Ion Ratio Lower Upper
138 100
92 51.8 41.4 62.2
108 79.7 63.8 95.6









#66
4,6-Dinitro-2-methylphenol
Concen: 22.964 ng/ul
RT: 15.430 min Scan# 2141
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:198 Resp: 184366
Ion Ratio Lower Upper
198 100
182 4.8 3.8 5.8
77 24.8 19.8 29.8



#67
N-Nitrosodiphenylamine
Concen: 21.385 ng/ul
RT: 15.560 min Scan# 2163
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:169 Resp: 1257772
Ion Ratio Lower Upper
169 100
168 65.4 52.3 78.5
167 35.7 28.6 42.8









#68
4-Bromophenyl-phenylether
Concen: 21.257 ng/ul
RT: 16.236 min Scan# 2278
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:248 Resp: 426344
Ion Ratio Lower Upper
248 100
250 96.3 77.0 115.6
141 72.0 57.6 86.4



#69
Hexachlorobenzene
Concen: 22.866 ng/ul
RT: 16.371 min Scan# 2301
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:284 Resp: 514140
Ion Ratio Lower Upper
284 100
142 35.5 28.4 42.6
249 30.9 24.7 37.1









#70
Atrazine
Concen: 19.403 ng/ul
RT: 16.501 min Scan# 2323
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:200 Resp: 440779
Ion Ratio Lower Upper
200 100
173 26.7 21.4 32.0
215 49.3 39.4 59.2



#71
Pentachlorophenol
Concen: 22.071 ng/ul
RT: 16.707 min Scan# 2358
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:266 Resp: 284645
Ion Ratio Lower Upper
266 100
264 62.7 50.2 75.2
268 63.8 51.0 76.6









#72
Phenanthrene
Concen: 21.168 ng/ul
RT: 17.083 min Scan# 2422
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:178 Resp: 2269488
Ion Ratio Lower Upper
178 100
179 15.4 12.3 18.5
176 19.2 15.4 23.0



#74
Anthracene
Concen: 21.120 ng/ul
RT: 17.171 min Scan# 2437
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:178 Resp: 2311214
Ion Ratio Lower Upper
178 100
179 15.8 12.6 19.0
176 18.5 14.8 22.2









#75
1,2,3,4-Tetrachlorobenzene
Concen: 24.143 ng/uL
RT: 13.119 min Scan# 1748
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:216 Resp: 673249
Ion Ratio Lower Upper
216 100
214 78.4 62.7 94.1
218 48.4 38.7 58.1



#76
Pentachlorobenzene
Concen: 24.026 ng/uL
RT: 14.648 min Scan# 2008
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:250 Resp: 661248
Ion Ratio Lower Upper
250 100
248 62.5 50.0 75.0
252 64.5 51.6 77.4









#77
 Carbazole
 Concen: 20.394 ng/ul
 RT: 17.436 min Scan# 2482
 Delta R.T. 0.000 min
 Lab File: BM032138.D
 Acq: 24 Sep 2021 19:35




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020041


Tgt Ion:167 Resp: 2022728
 Ion Ratio Lower Upper
 167 100
 166 21.6 17.3 25.9
 139 12.9 10.3 15.5



#78
 Di-n-butylphthalate
 Concen: 18.592 ng/ul
 RT: 17.995 min Scan# 2577
 Delta R.T. 0.000 min
 Lab File: BM032138.D
 Acq: 24 Sep 2021 19:35

Tgt Ion:149 Resp: 2307770
 Ion Ratio Lower Upper
 149 100
 150 9.2 7.4 11.0
 104 5.2 4.2 6.2









#80
Fluoranthene
Concen: 22.580 ng/u1
RT: 19.089 min Scan# 2763
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:202 Resp: 2516606
Ion Ratio Lower Upper
202 100
101 11.5 9.2 13.8
100 8.6 6.9 10.3



#82
Pyrene
Concen: 22.966 ng/u1
RT: 19.454 min Scan# 2825
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:202 Resp: 2586478
Ion Ratio Lower Upper
202 100
101 12.6 10.1 15.1
100 10.5 8.4 12.6









#83
Butylbenzylphthalate
Concen: 16.839 ng/ul
RT: 20.336 min Scan# 2975
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:149 Resp: 743805
Ion Ratio Lower Upper
149 100
91 77.3 61.8 92.8
206 20.3 16.2 24.4



#84
3,3'-Dichlorobenzidine
Concen: 16.380 ng/ul
RT: 21.118 min Scan# 3108
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:252 Resp: 627226
Ion Ratio Lower Upper
252 100
254 65.2 52.2 78.2
126 11.0 8.8 13.2









#85
Benzo(a)anthracene
Concen: 19.967 ng/ul
RT: 21.189 min Scan# 3120
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:228 Resp: 2191245
Ion Ratio Lower Upper
228 100
229 19.9 15.9 23.9
226 27.1 21.7 32.5



#86
Bis(2-ethylhexyl)phthalate
Concen: 16.867 ng/ul
RT: 21.112 min Scan# 3107
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:149 Resp: 1130992
Ion Ratio Lower Upper
149 100
167 27.0 21.6 32.4
279 4.1 3.3 4.9









#87
Chrysene
Concen: 20.553 ng/ul
RT: 21.236 min Scan# 3128
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:228 Resp: 2181369
Ion Ratio Lower Upper
228 100
226 30.5 24.4 36.6
229 19.9 15.9 23.9



#89
Di-n-octyl phthalate
Concen: 18.325 ng/ul
RT: 21.959 min Scan# 3251
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:149 Resp: 1632405









#90
Benzo(b)fluoranthene
Concen: 21.459 ng/ul
RT: 22.724 min Scan# 3381
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:252 Resp: 1998176
Ion Ratio Lower Upper
252 100
253 22.8 18.2 27.4
125 10.6 8.5 12.7



#91
Benzo(k)fluoranthene
Concen: 22.457 ng/ul
RT: 22.765 min Scan# 3388
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:252 Resp: 1919118
Ion Ratio Lower Upper
252 100
253 22.4 17.9 26.9
125 10.5 8.4 12.6









#93
Benzo(a)pyrene
Concen: 20.903 ng/ul
RT: 23.277 min Scan# 3475
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35




Instrument :
BNA_M
ClientSampleId :
SSTD020041


Tgt Ion:252 Resp: 1883181
Ion Ratio Lower Upper
252 100
253 22.2 17.8 26.6
125 11.5 9.2 13.8



#94
Indeno(1,2,3-cd)pyrene
Concen: 18.113 ng/ul
RT: 25.524 min Scan# 3857
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:276 Resp: 1882363
Ion Ratio Lower Upper
276 100
138 26.9 21.5 32.3
277 26.3 21.0 31.6









#95
Dibenzo(a,h)anthracene
Concen: 17.694 ng/ul
RT: 25.530 min Scan# 3858
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Instrument :
BNA_M
ClientSampleId :
SSTD020041

Tgt Ion:278 Resp: 1559347
Ion Ratio Lower Upper
278 100
139 16.9 13.5 20.3
279 24.2 19.4 29.0



#96
Benzo(g,h,i)perylene
Concen: 18.387 ng/ul
RT: 26.183 min Scan# 3969
Delta R.T. 0.000 min
Lab File: BM032138.D
Acq: 24 Sep 2021 19:35

Tgt Ion:276 Resp: 1640526
Ion Ratio Lower Upper
276 100
138 22.4 17.9 26.9
277 23.3 18.6 28.0

