

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092421\
 Data File : BM032144.D
 Acq On : 24 Sep 2021 23:48
 Operator : CG/JU
 Sample : SP5707
 Misc : SFAM SURROGATE
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP010

Quant Time: Sep 25 01:29:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 25 01:15:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.666	152	371354	20.000	ng/ul	0.00
20) Naphthalene-d8	10.460	136	1547614	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.313	164	976568	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.042	188	1940772	20.000	ng/ul	0.00
79) Chrysene-d12	21.194	240	1601475	20.000	ng/ul	0.00
88) Perylene-d12	23.365	264	1449928	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.990	96	151779	17.258	ng/uL	0.00
4) Pyridine-d5	3.413	84	2108569	84.454	ng/ul	0.00
7) Phenol-d5	6.854	99	3001692	101.831	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.995	67	1794975	101.272	ng/ul	0.00
11) 2-Chlorophenol-d4	7.207	132	2412980	105.440	ng/ul	0.00
15) 4-Methylphenol-d8	8.395	113	2398642	104.065	ng/ul	0.00
21) Nitrobenzene-d5	8.825	128	1180111	127.668	ng/ul	0.00
24) 2-Nitrophenol-d4	9.548	143	1320160	135.067	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.089	165	2339450	104.703	ng/ul	0.00
31) 4-Chloroaniline-d4	10.595	131	3367590	111.513	ng/ul	0.00
46) Dimethylphthalate-d6	13.724	166	6581958	103.735	ng/ul	0.00
49) Acenaphthylene-d8	14.007	160	8169625	101.343	ng/ul	0.00
54) 4-Nitrophenol-d4	14.518	143	1178226	114.151	ng/ul	0.00
60) Fluorene-d10	15.307	176	5413485	99.989	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.418	200	1022793	111.513	ng/ul	0.00
73) Anthracene-d10	17.142	188	7858507	97.043	ng/ul	0.00
81) Pyrene-d10	19.424	212	7911873	93.897	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.235	264	7056986	103.710	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.043	88	155	0.016	ng/ul#	27
5) Pyridine	3.460	79	533	0.022	ng/ul#	1
6) Benzaldehyde	6.795	77	540	0.033	ng/ul#	2
8) Phenol	6.878	94	61	0.002	ng/ul#	1
10) Bis(2-Chloroethyl)ether	7.207	93	3652	0.153	ng/ul#	1
14) 2,2'-oxybis(1-Chloropr...	8.183	45	56	0.002	ng/ul#	1
17) N-Nitroso-di-n-propyla...	8.395	70	57264	3.214	ng/ul#	1
22) Nitrobenzene	8.895	77	48	0.002	ng/ul#	39
23) Isophorone	9.548	82	85234	1.717	ng/ul#	71
25) 2-Nitrophenol	9.560	139	72	0.006	ng/ul#	1
26) 2,4-Dimethylphenol	9.548	107	122	0.005	ng/ul#	15
29) 2,4-Dichlorophenol	10.095	162	217	0.010	ng/ul#	1
30) Naphthalene	10.595	128	3505	0.046	ng/ul#	1
32) 4-Chloroaniline	10.601	127	715	0.023	ng/ul#	1
34) Caprolactam	11.348	113	186	0.028	ng/ul#	16
44) 2-Chloronaphthalene	13.254	162	481	0.009	ng/ul#	38
47) Dimethylphthalate	13.724	163	4255	0.067	ng/ul#	1
48) 2,6-Dinitrotoluene	13.724	165	45529	4.332	ng/ul#	39
50) Acenaphthylene	14.018	152	179	0.002	ng/ul#	1
55) 4-Nitrophenol	14.524	109	929	0.110	ng/ul#	1
56) Dibenzofuran	14.707	168	176	0.002	ng/ul#	38
57) 2,4-Dinitrotoluene	14.683	165	211	0.014	ng/ul#	59
59) Diethylphthalate	15.124	149	435	0.007	ng/ul#	59
61) Fluorene	15.307	166	12672	0.207	ng/ul#	11

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092421\
 Data File : BM032144.D
 Acq On : 24 Sep 2021 23:48
 Operator : CG/JU
 Sample : SP5707
 Misc : SFAM SURROGATE
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP010

Quant Time: Sep 25 01:29:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 25 01:15:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


63) 4-Nitroaniline	15.312	138	3377	0.335	ng/ul#	1
66) 4,6-Dinitro-2-methylph...	15.418	198	3540	0.391	ng/ul#	1
67) N-Nitrosodiphenylamine	15.554	169	235	0.004	ng/ul#	73
72) Phenanthrene	17.077	178	984	0.010	ng/ul#	61
74) Anthracene	17.142	178	3101	0.032	ng/ul#	1
77) Carbazole	17.436	167	586	0.007	ng/ul#	63
78) Di-n-butylphthalate	17.995	149	2232	0.024	ng/ul#	78
80) Fluoranthene	19.089	202	1482	0.014	ng/ul#	76
82) Pyrene	19.430	202	11256	0.105	ng/ul#	1
83) Butylbenzylphthalate	20.324	149	352	0.011	ng/ul#	67
84) 3,3'-Dichlorobenzidine	21.106	252	163	0.006	ng/ul#	50
85) Benzo(a)anthracene	21.236	228	1442	0.016	ng/ul	97
86) Bis(2-ethylhexyl)phtha...	21.106	149	1660	0.036	ng/ul#	53
87) Chrysene	21.236	228	1442	0.016	ng/ul	98
89) Di-n-octyl phthalate	21.953	149	301	0.004	ng/ul	100
90) Benzo(b)fluoranthene	22.712	252	402	0.005	ng/ul#	1
91) Benzo(k)fluoranthene	22.759	252	969	0.012	ng/ul#	1
93) Benzo(a)pyrene	23.235	252	21039	0.260	ng/ul#	73
95) Dibenzo(a,h)anthracene	25.518	278	264	0.004	ng/ul#	1
96) Benzo(g,h,i)perylene	26.171	276	206	0.003	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092421\
 Data File : BM032144.D
 Acq On : 24 Sep 2021 23:48
 Operator : CG/JU
 Sample : SP5707
 Misc : SFAM SURROGATE
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP010

Quant Time: Sep 25 01:29:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 25 01:15:33 2021
 Response via : Initial Calibration




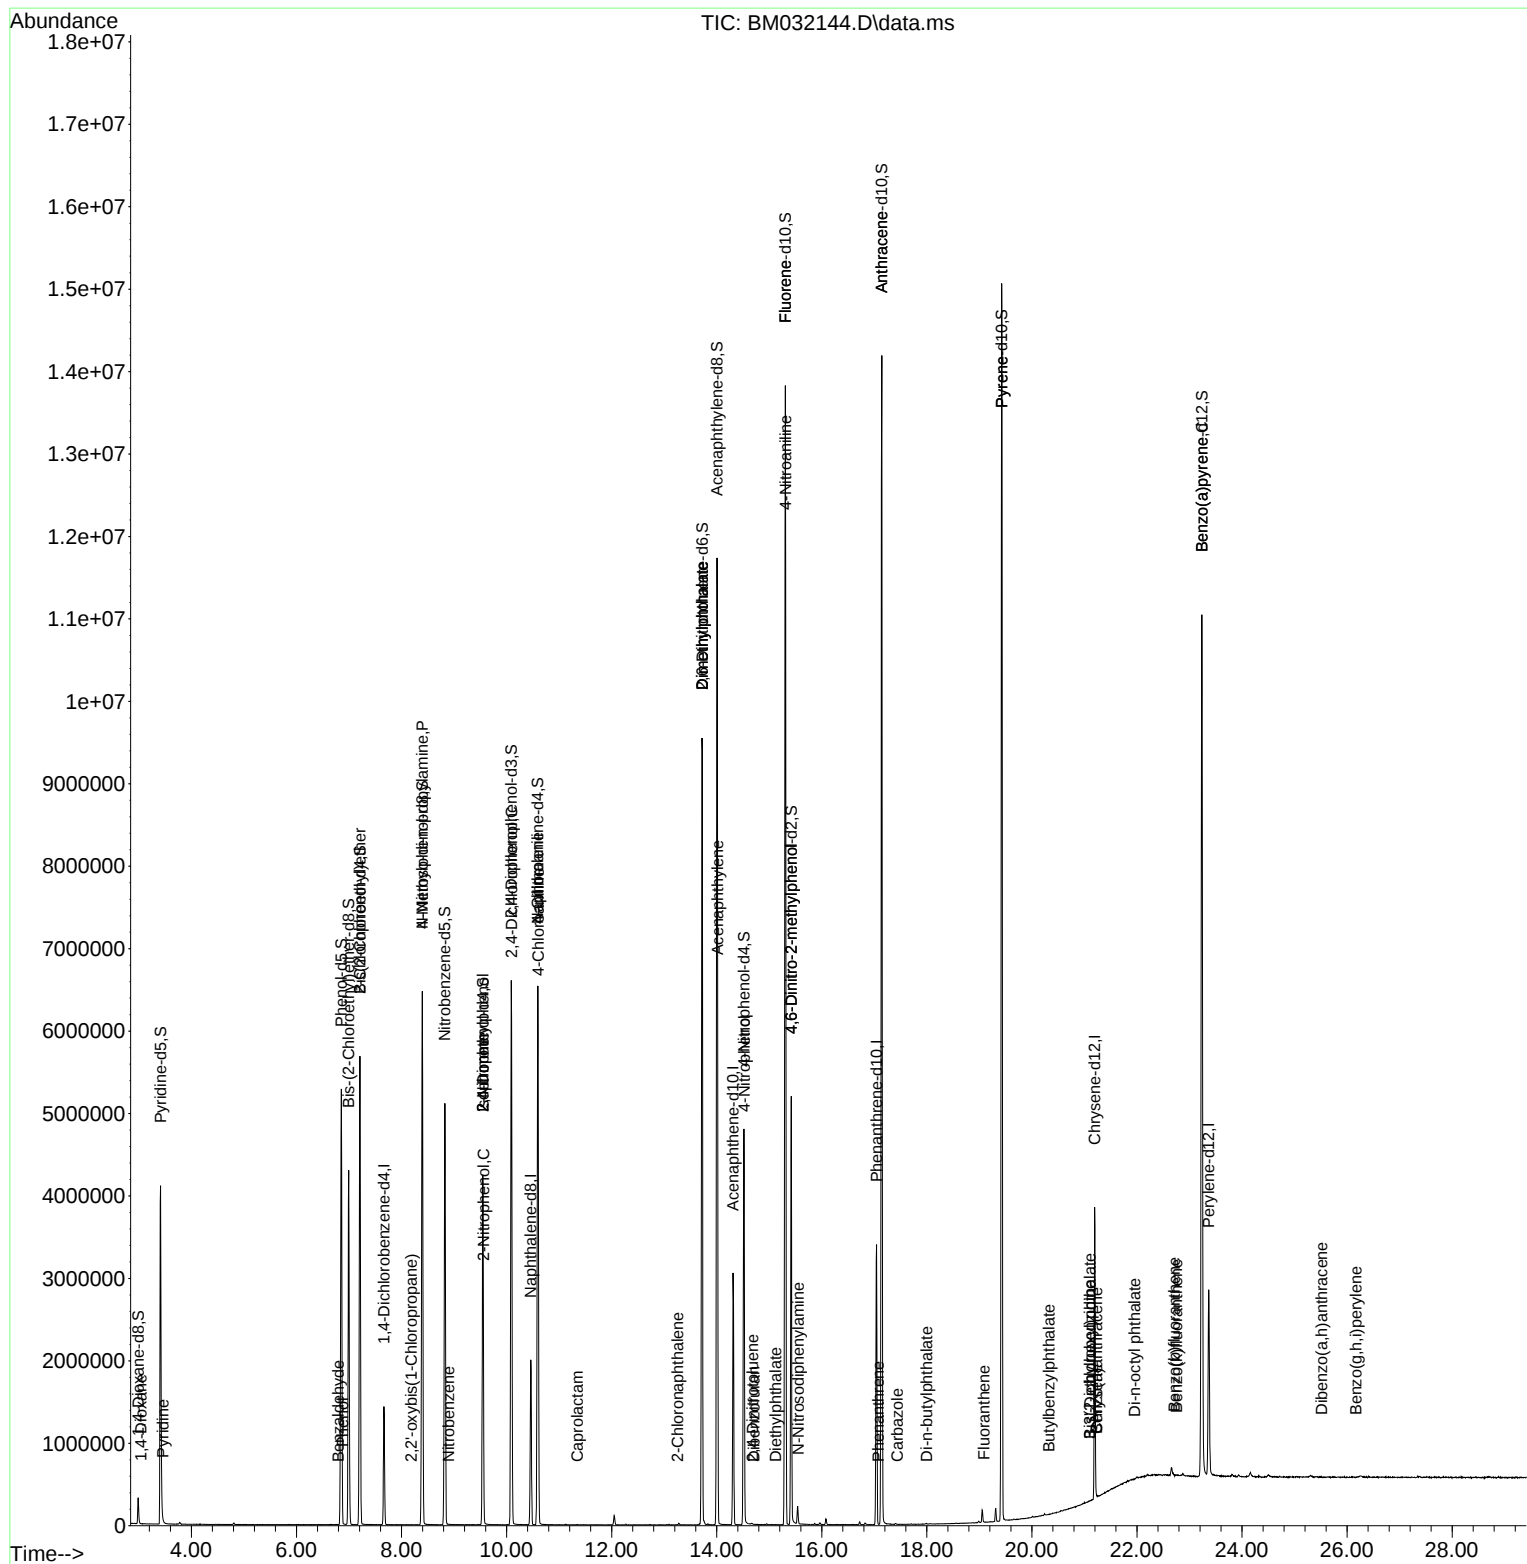


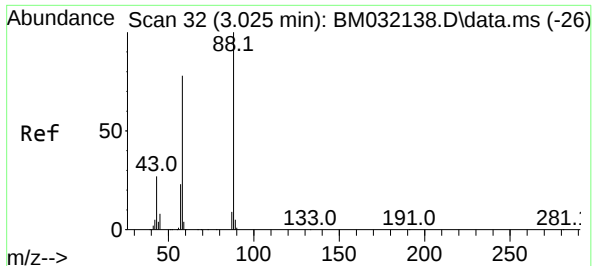

#2
1,4-Dioxane
Concen: 0.016 ng/uL
RT: 3.043 min Scan# 35
Delta R.T. 0.018 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampleId :
DFTPP010


Tgt Ion: 88 Resp: 155
Ion Ratio Lower Upper
88 100
43 42.5 22.3 33.5#
58 0.0 62.4 93.6#

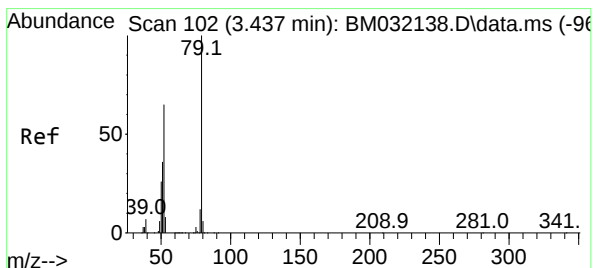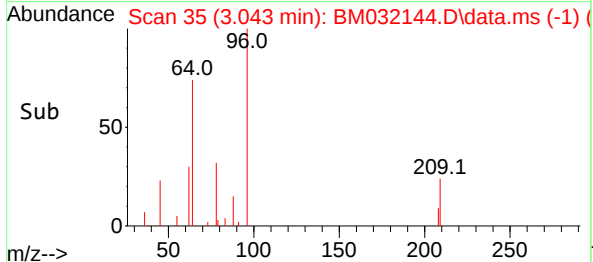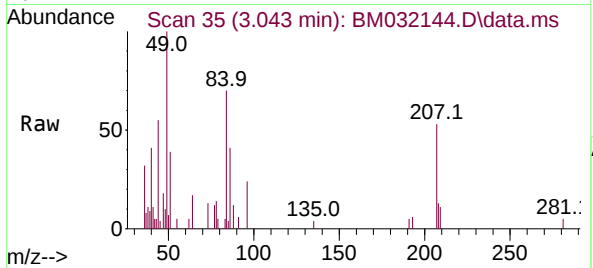

#5
Pyridine
Concen: 0.022 ng/uL
RT: 3.460 min Scan# 106
Delta R.T. 0.023 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion: 79 Resp: 533
Ion Ratio Lower Upper
79 100
52 1660.0 58.3 87.5#
51 397.7 29.1 43.7#


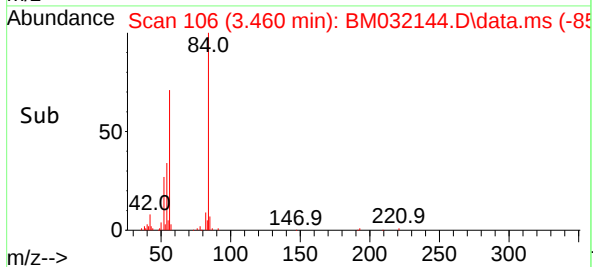

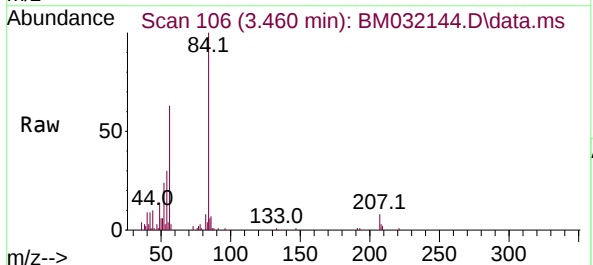




#6
Benzaldehyde
Concen: 0.033 ng/ul
RT: 6.795 min Scan# 673
Delta R.T. 0.006 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampled :
DFTPP010


Tgt Ion: 77 Resp: 540
Ion Ratio Lower Upper
77 100
105 0.0 77.0 115.4#
106 0.0 74.2 111.2#

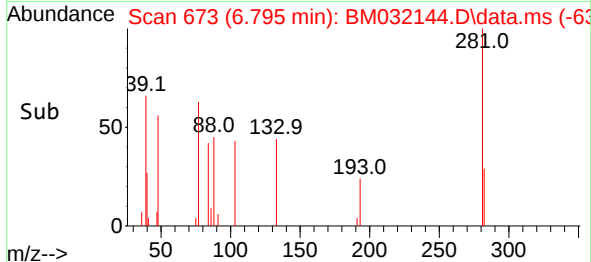

#8
Phenol
Concen: 0.002 ng/ul
RT: 6.878 min Scan# 687
Delta R.T. -0.000 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion: 94 Resp: 61
Ion Ratio Lower Upper
94 100
65 623.6 22.4 33.6#
66 1933.9 29.9 44.9#

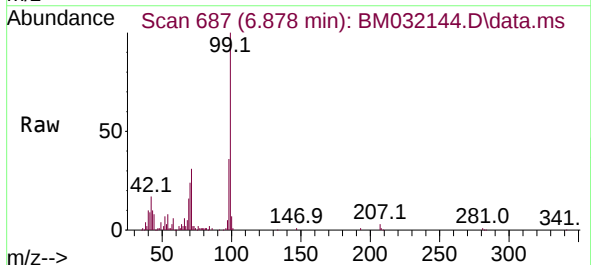







#10

Bis(2-Chloroethyl)ether
Concen: 0.153 ng/ul
RT: 7.207 min Scan# 743
Delta R.T. 0.123 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Instrument :
BNA_M
ClientSampleId :
DFTPP010




Tgt Ion: 93 Resp: 3652
Ion Ratio Lower Upper
93 100
63 754.5 63.4 95.2#
95 475.2 25.5 38.3#




#14

2,2'-oxybis(1-Chloropropane)
Concen: 0.002 ng/ul
RT: 8.183 min Scan# 909
Delta R.T. -0.018 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion: 45 Resp: 56
Ion Ratio Lower Upper
45 100
77 242.4 11.2 16.8#
79 0.0 9.1 13.7#









#17
N-Nitroso-di-n-propylamine
Concen: 3.214 ng/ul
RT: 8.395 min Scan# 945
Delta R.T. -0.083 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampleId :
DFTPP010


Tgt Ion:	70	Resp:	57264
Ion	Ratio	Lower	Upper
70	100		
42	368.5	46.2	69.4#
101	0.0	7.5	11.3#
130	0.0	16.2	24.2#

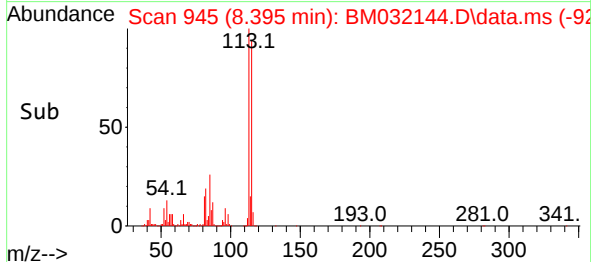

#22
Nitrobenzene
Concen: 0.002 ng/ul
RT: 8.895 min Scan# 1030
Delta R.T. 0.029 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion:	77	Resp:	48
Ion	Ratio	Lower	Upper
77	100		
123	0.0	36.1	54.1#
65	0.0	11.0	16.6#


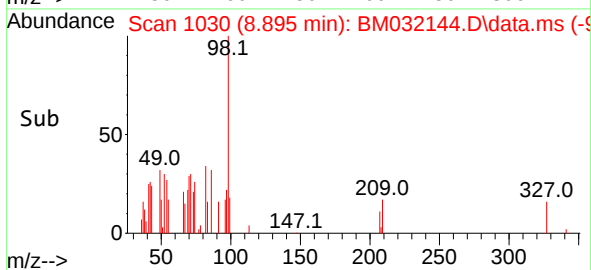






#23
Isophorone
Concen: 1.717 ng/ul
RT: 9.548 min Scan# 1141
Delta R.T. 0.164 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampled :
DFTPP010


Tgt Ion: 82 Resp: 85234
Ion Ratio Lower Upper
82 100
95 7.9 5.8 8.6
138 0.0 14.1 21.1#



#25
2-Nitrophenol
Concen: 0.006 ng/ul
RT: 9.560 min Scan# 1143
Delta R.T. -0.018 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion: 139 Resp: 72
Ion Ratio Lower Upper
139 100
65 9272.9 42.0 63.0#
109 800.5 25.8 38.8#


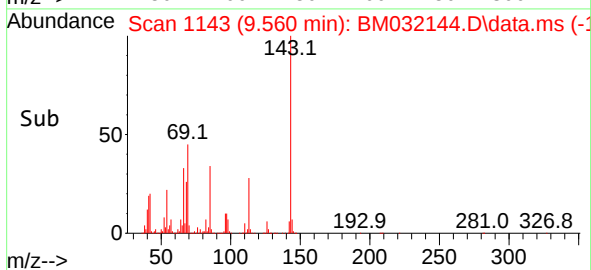






#26
2,4-Dimethylphenol
Concen: 0.005 ng/ul
RT: 9.548 min Scan# 1141
Delta R.T. -0.106 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampled :
DFTPP010


Tgt Ion:107 Resp: 122
Ion Ratio Lower Upper
107 100
121 0.0 40.4 60.6#
122 0.0 67.6 101.4#

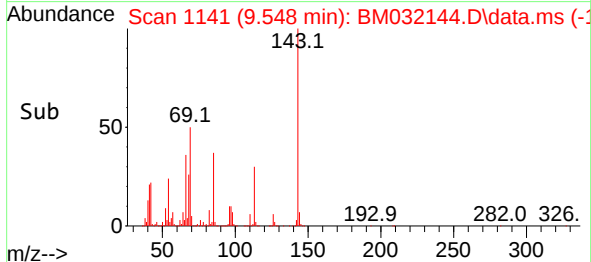

#29
2,4-Dichlorophenol
Concen: 0.010 ng/ul
RT: 10.095 min Scan# 1234
Delta R.T. -0.024 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion:162 Resp: 217
Ion Ratio Lower Upper
162 100
164 18876.4 51.6 77.4#
98 1354.7 28.6 42.8#




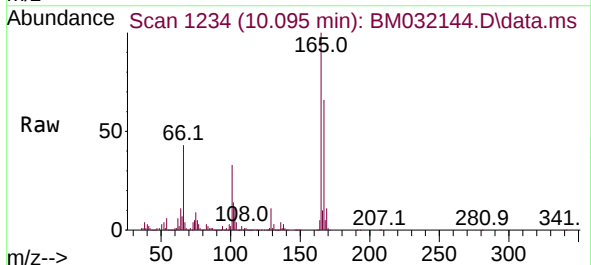




#30
Naphthalene
Concen: 0.046 ng/ul
RT: 10.595 min Scan# 1319
Delta R.T. 0.082 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampleId :
DFTPP010


Tgt Ion:128 Resp: 3505
Ion Ratio Lower Upper
128 100
129 283.2 8.7 13.1#
127 21.1 10.2 15.4#

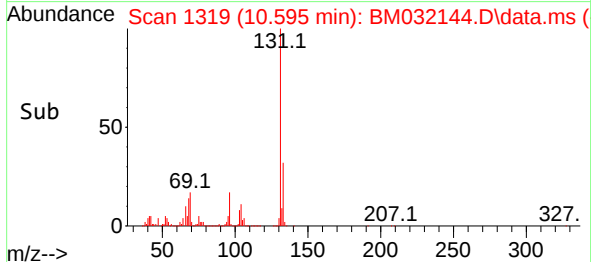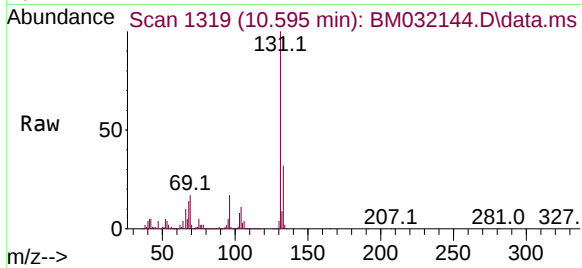

#32
4-Chloroaniline
Concen: 0.023 ng/ul
RT: 10.601 min Scan# 1320
Delta R.T. -0.018 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion:127 Resp: 715
Ion Ratio Lower Upper
127 100
129 855.6 25.8 38.6#




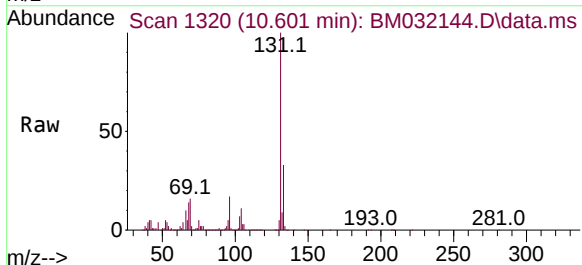




#34
Caprolactam
Concen: 0.028 ng/ul
RT: 11.348 min Scan# 1447
Delta R.T. 0.006 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampleId :
DFTPP010


Tgt Ion:113 Resp: 186
Ion Ratio Lower Upper
113 100
55 0.0 138.1 207.1#
56 167.5 106.0 159.0#

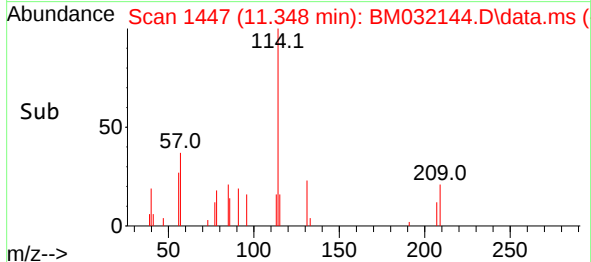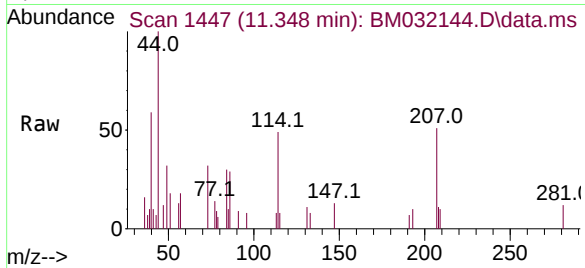

#44
2-Chloronaphthalene
Concen: 0.009 ng/ul
RT: 13.254 min Scan# 1771
Delta R.T. 0.070 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion:162 Resp: 481
Ion Ratio Lower Upper
162 100
164 0.0 25.9 38.9#
127 0.0 32.0 48.0#




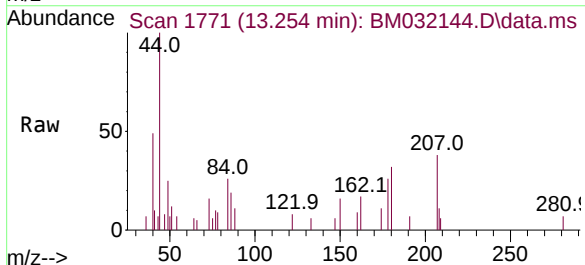


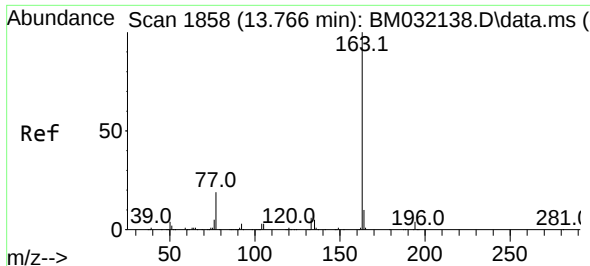

#47
Dimethylphthalate
Concen: 0.067 ng/ul
RT: 13.724 min Scan# 1851
Delta R.T. -0.041 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampleId :
DFTPP010


Tgt Ion:163 Resp: 4255
Ion Ratio Lower Upper
163 100
194 0.0 3.3 4.9#
164 309.0 8.1 12.1#

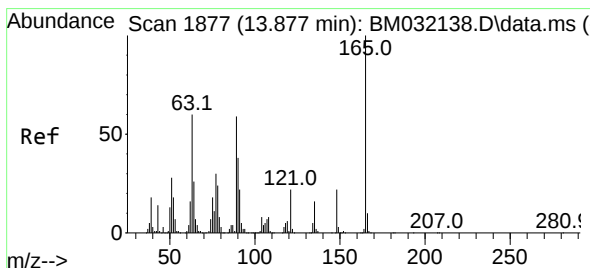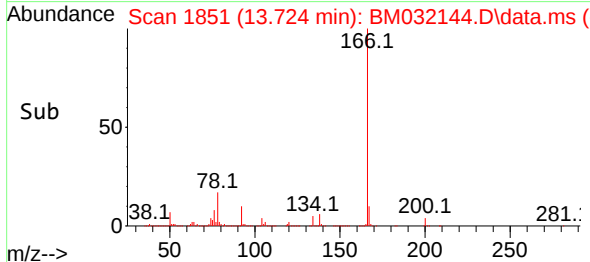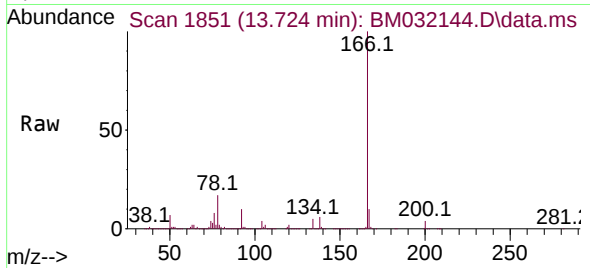

#48
2,6-Dinitrotoluene
Concen: 4.332 ng/ul
RT: 13.724 min Scan# 1851
Delta R.T. -0.153 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion:165 Resp: 45529
Ion Ratio Lower Upper
165 100
89 1.7 46.8 70.2#
121 31.6 17.3 25.9#


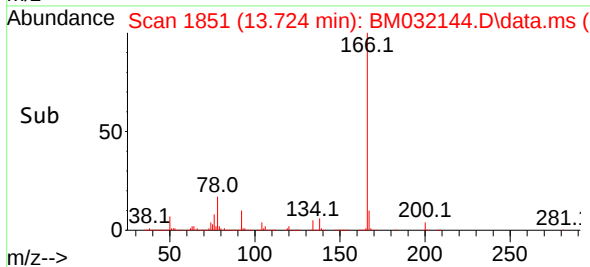

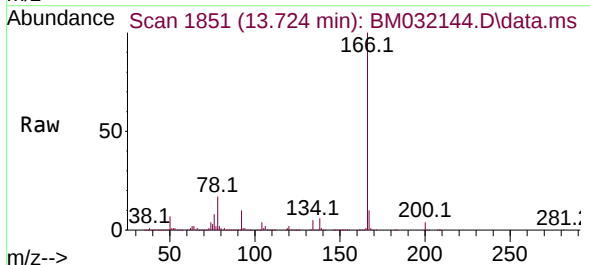




#50
Acenaphthylene
Concen: 0.002 ng/ul
RT: 14.018 min Scan# 1901
Delta R.T. -0.018 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampled :
DFTPP010


Tgt Ion:152 Resp: 179
Ion Ratio Lower Upper
152 100
151 0.0 15.7 23.5#
153 270.3 10.6 15.8#



#55
4-Nitrophenol
Concen: 0.110 ng/ul
RT: 14.524 min Scan# 1987
Delta R.T. -0.000 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion:109 Resp: 929
Ion Ratio Lower Upper
109 100
139 85.3 103.7 155.5#
65 6362.4 109.4 164.2#


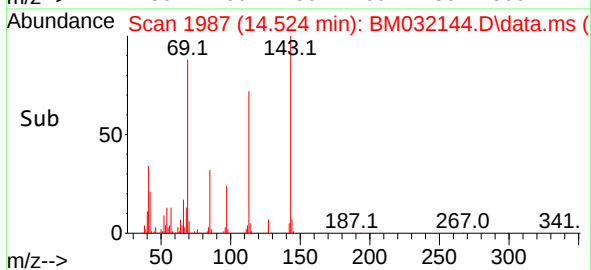






#56
Dibenzofuran
Concen: 0.002 ng/ul
RT: 14.707 min Scan# 2018
Delta R.T. -0.006 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampled :
DFTPP010


Tgt Ion:168 Resp: 176
Ion Ratio Lower Upper
168 100
139 0.0 29.8 44.6#



#57
2,4-Dinitrotoluene
Concen: 0.014 ng/ul
RT: 14.683 min Scan# 2014
Delta R.T. 0.017 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion:165 Resp: 211
Ion Ratio Lower Upper
165 100
63 70.0 34.2 51.2#
182 0.0 2.3 3.5#


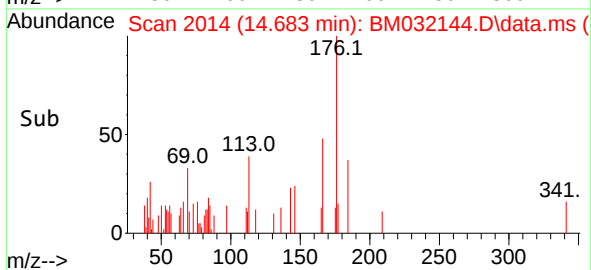






#59
Diethylphthalate
Concen: 0.007 ng/ul
RT: 15.124 min Scan# 2089
Delta R.T. -0.006 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampled :
DFTPP010


Tgt Ion:149	Resp:	435
Ion Ratio	Lower	Upper
149	100	
177	0.0	17.9 26.9#
150	0.0	10.0 15.0#

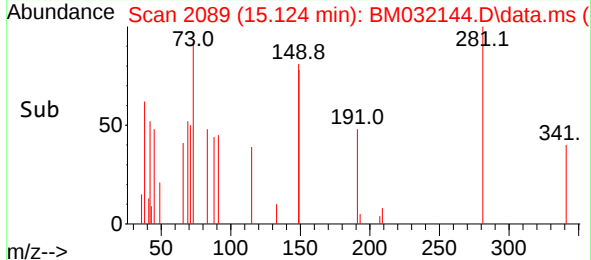

#61
Fluorene
Concen: 0.207 ng/ul
RT: 15.307 min Scan# 2120
Delta R.T. -0.053 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion:166	Resp:	12672
Ion Ratio	Lower	Upper
166	100	
165	6.0	77.7 116.5#
167	37.4	10.7 16.1#


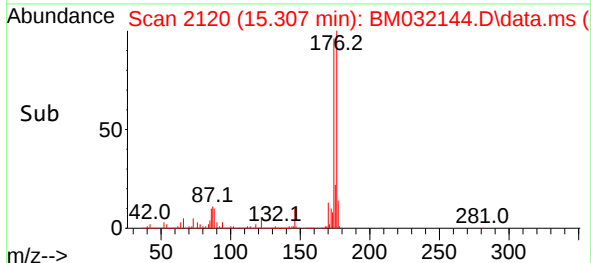
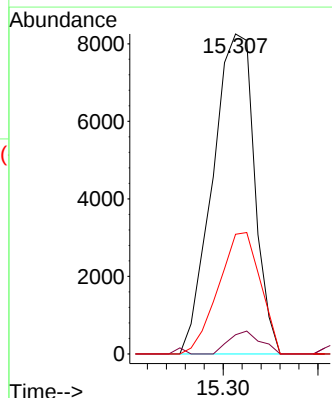





#63
4-Nitroaniline
Concen: 0.335 ng/ul
RT: 15.312 min Scan# 2121
Delta R.T. -0.053 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampleId :
DFTPP010


Tgt Ion:138 Resp: 3377
Ion Ratio Lower Upper
138 100
92 1188.6 41.4 62.2#
108 461.2 63.8 95.6#

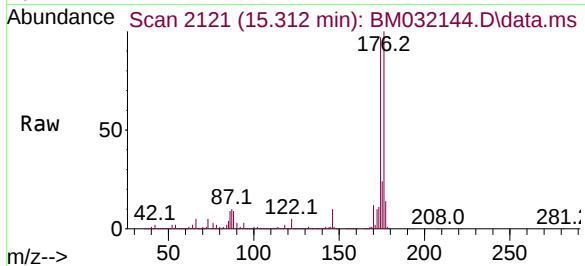

#66
4,6-Dinitro-2-methylphenol
Concen: 0.391 ng/ul
RT: 15.418 min Scan# 2139
Delta R.T. -0.012 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion:198 Resp: 3540
Ion Ratio Lower Upper
198 100
182 527.8 3.8 5.8#
77 1576.6 19.8 29.8#




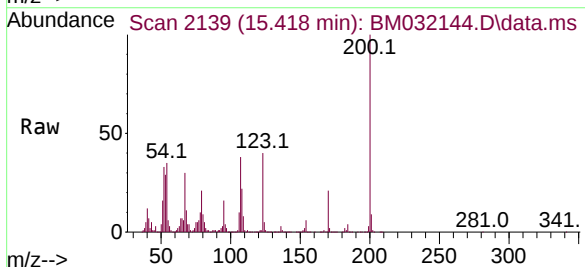




#67
N-Nitrosodiphenylamine
Concen: 0.004 ng/ul
RT: 15.554 min Scan# 2162
Delta R.T. -0.006 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampled :
DFTPP010


Tgt Ion:169 Resp: 235
Ion Ratio Lower Upper
169 100
168 58.1 52.3 78.5
167 0.0 28.6 42.8#

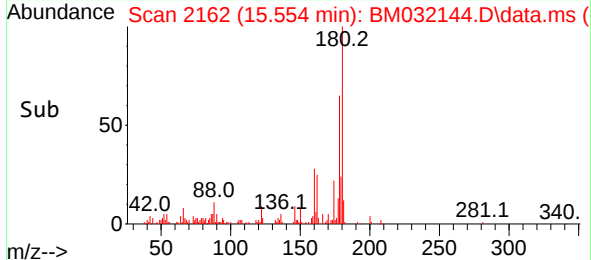

#72
Phenanthrene
Concen: 0.010 ng/ul
RT: 17.077 min Scan# 2421
Delta R.T. -0.006 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion:178 Resp: 984
Ion Ratio Lower Upper
178 100
179 29.6 12.3 18.5#
176 0.0 15.4 23.0#


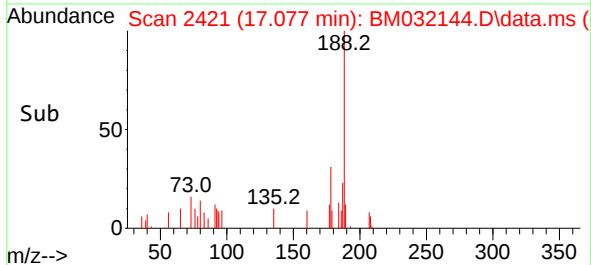






#74
 Anthracene
 Concen: 0.032 ng/ul
 RT: 17.142 min Scan# 2432
 Delta R.T. -0.030 min
 Lab File: BM032144.D
 Acq: 24 Sep 2021 23:48




Instrument :
 BNA_M
 ClientSampleId :
 DFTPP010


Tgt Ion:178 Resp: 3101
 Ion Ratio Lower Upper
 178 100
 179 259.6 12.6 19.0#
 176 0.0 14.8 22.2#

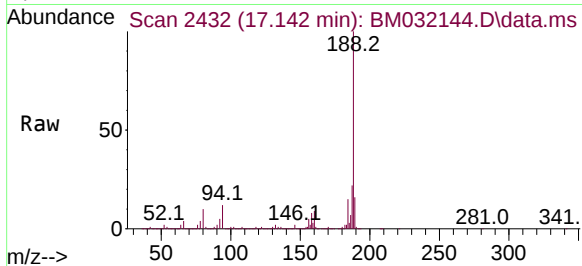

#77
 Carbazole
 Concen: 0.007 ng/ul
 RT: 17.436 min Scan# 2482
 Delta R.T. -0.000 min
 Lab File: BM032144.D
 Acq: 24 Sep 2021 23:48

Tgt Ion:167 Resp: 586
 Ion Ratio Lower Upper
 167 100
 166 40.6 17.3 25.9#
 139 0.0 10.3 15.5#



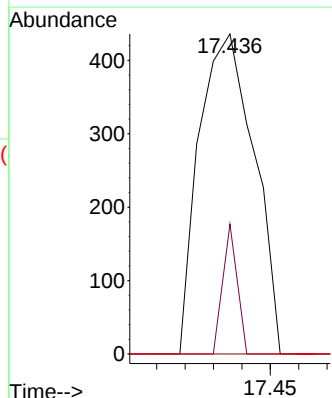
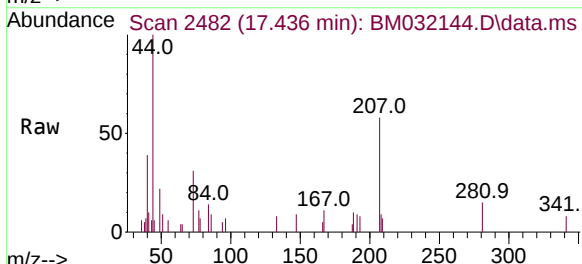




#78
Di-n-butylphthalate
Concen: 0.024 ng/ul
RT: 17.995 min Scan# 2577
Delta R.T. -0.000 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampled :
DFTPP010


Tgt Ion:149 Resp: 2232
Ion Ratio Lower Upper
149 100
150 0.0 7.4 11.0#
104 10.1 4.2 6.2#

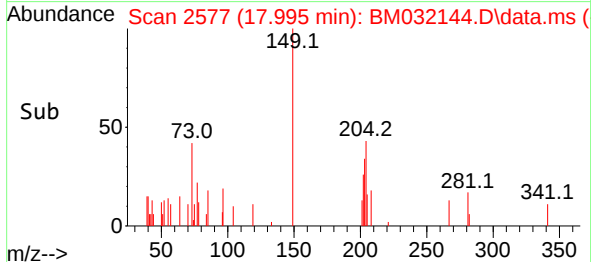

#80
Fluoranthene
Concen: 0.014 ng/ul
RT: 19.089 min Scan# 2763
Delta R.T. -0.000 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion:202 Resp: 1482
Ion Ratio Lower Upper
202 100
101 0.0 9.2 13.8#
100 14.7 6.9 10.3#




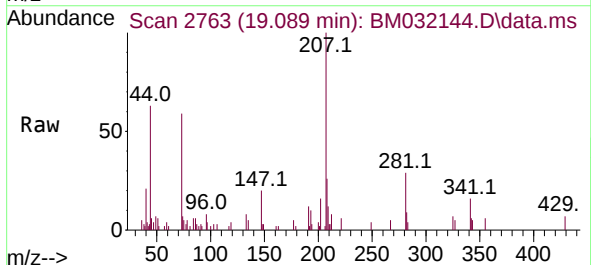




#82
Pyrene
Concen: 0.105 ng/ul
RT: 19.430 min Scan# 2821
Delta R.T. -0.024 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampleId :
DFTPP010


Tgt Ion:202 Resp: 11256
Ion Ratio Lower Upper
202 100
101 176.8 10.1 15.1#
100 1029.8 8.4 12.6#

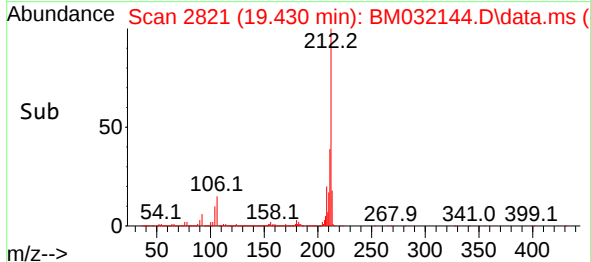

#83
Butylbenzylphthalate
Concen: 0.011 ng/ul
RT: 20.324 min Scan# 2973
Delta R.T. -0.012 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion:149 Resp: 352
Ion Ratio Lower Upper
149 100
91 44.0 61.8 92.8#
206 25.1 16.2 24.4#




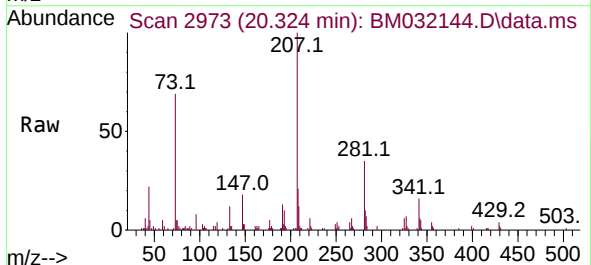




#84
3,3'-Dichlorobenzidine
Concen: 0.006 ng/ul
RT: 21.106 min Scan# 3106
Delta R.T. -0.012 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampled :
DFTPP010


Tgt Ion:252 Resp: 163
Ion Ratio Lower Upper
252 100
254 23.0 52.2 78.2#
126 0.0 8.8 13.2#

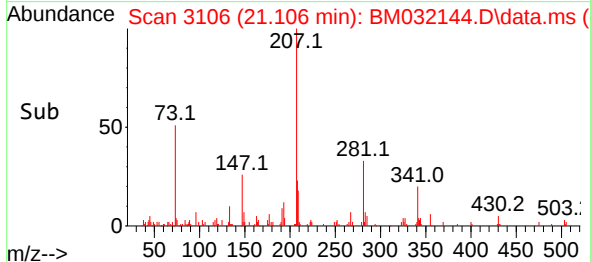

#85
Benzo(a)anthracene
Concen: 0.016 ng/ul
RT: 21.236 min Scan# 3128
Delta R.T. 0.047 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion:228 Resp: 1442
Ion Ratio Lower Upper
228 100
229 20.6 15.9 23.9
226 29.0 21.7 32.5


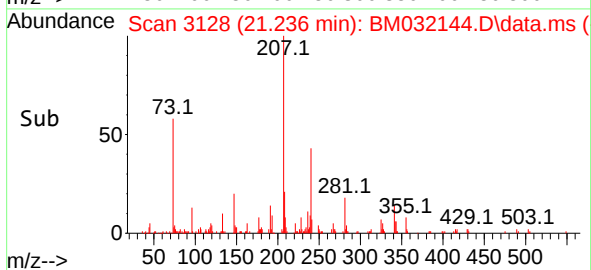






#86
 Bis(2-ethylhexyl)phthalate
 Concen: 0.036 ng/ul
 RT: 21.106 min Scan# 3106
 Delta R.T. -0.006 min
 Lab File: BM032144.D
 Acq: 24 Sep 2021 23:48




Instrument :
 BNA_M
 ClientSampleId :
 DFTPP010


Tgt Ion:149 Resp: 1660
 Ion Ratio Lower Upper
 149 100
 167 0.0 21.6 32.4#
 279 8.5 3.3 4.9#

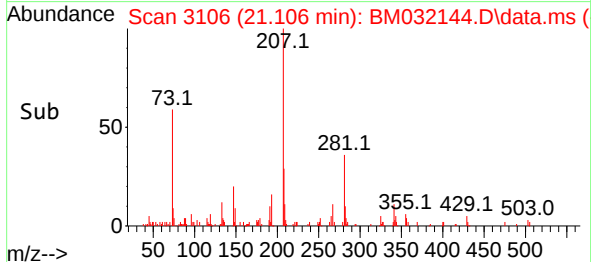

#87
 Chrysene
 Concen: 0.016 ng/ul
 RT: 21.236 min Scan# 3128
 Delta R.T. -0.000 min
 Lab File: BM032144.D
 Acq: 24 Sep 2021 23:48

Tgt Ion:228 Resp: 1442
 Ion Ratio Lower Upper
 228 100
 226 29.0 24.4 36.6
 229 20.6 15.9 23.9




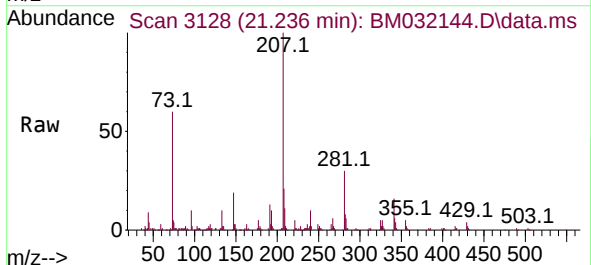




#89
Di-n-octyl phthalate
Concen: 0.004 ng/ul
RT: 21.953 min Scan# 3250
Delta R.T. -0.006 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampleId :
DFTPP010


Tgt Ion:149 Resp: 301

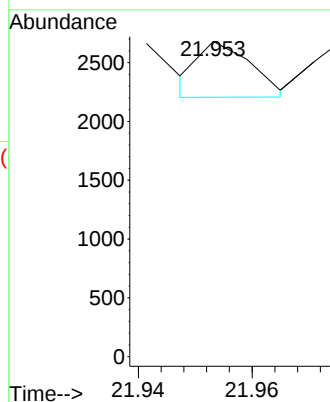

#90
Benzo(b)fluoranthene
Concen: 0.005 ng/ul
RT: 22.712 min Scan# 3379
Delta R.T. -0.012 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion:252 Resp: 402
Ion Ratio Lower Upper
252 100
253 115.7 18.2 27.4#
125 74.8 8.5 12.7#


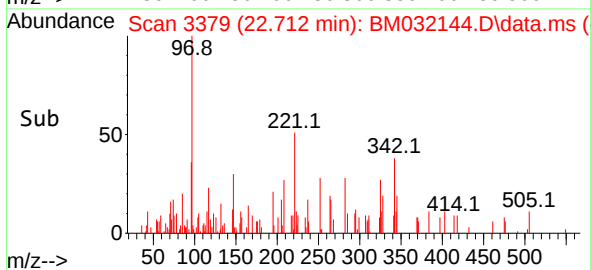






#91
Benzo(k)fluoranthene
Concen: 0.012 ng/ul
RT: 22.759 min Scan# 3387
Delta R.T. -0.006 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48




Instrument :
BNA_M
ClientSampleId :
DFTPP010


Tgt Ion:252 Resp: 969
Ion Ratio Lower Upper
252 100
253 84.0 17.9 26.9#
125 47.6 8.4 12.6#

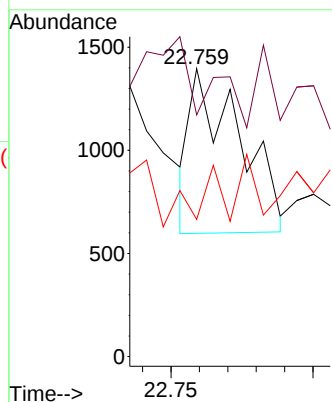

#93
Benzo(a)pyrene
Concen: 0.260 ng/ul
RT: 23.235 min Scan# 3468
Delta R.T. -0.041 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion:252 Resp: 21039
Ion Ratio Lower Upper
252 100
253 35.1 17.8 26.6#
125 21.8 9.2 13.8#


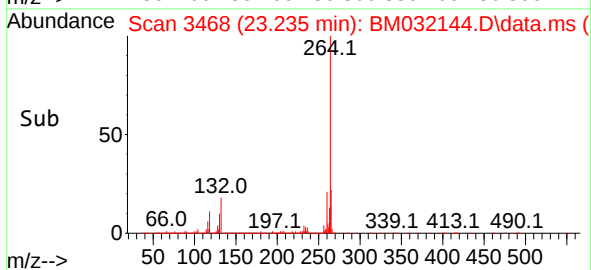






#95
Dibenzo(a,h)anthracene
Concen: 0.004 ng/ul
RT: 25.518 min Scan# 3856
Delta R.T. -0.012 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Instrument :
BNA_M
ClientSampled :
DFTPP010

Tgt Ion:278 Resp: 264
Ion Ratio Lower Upper
278 100
139 0.0 13.5 20.3#
279 116.5 19.4 29.0#

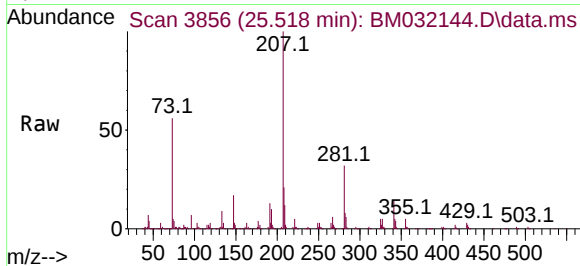

#96
Benzo(g,h,i)perylene
Concen: 0.003 ng/ul
RT: 26.171 min Scan# 3967
Delta R.T. -0.012 min
Lab File: BM032144.D
Acq: 24 Sep 2021 23:48

Tgt Ion:276 Resp: 206
Ion Ratio Lower Upper
276 100
138 0.0 17.9 26.9#
277 0.0 18.6 28.0#

