


Data Path : Z:\HPCHEM1\BNA_M\Data\BM092515\
 Data File : BM002724.D
 Acq On : 25 Sep 2015 09:38
 Operator : UM/IZ
 Sample : DFTPP16
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP16

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM092415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 25 15:05:30 2015

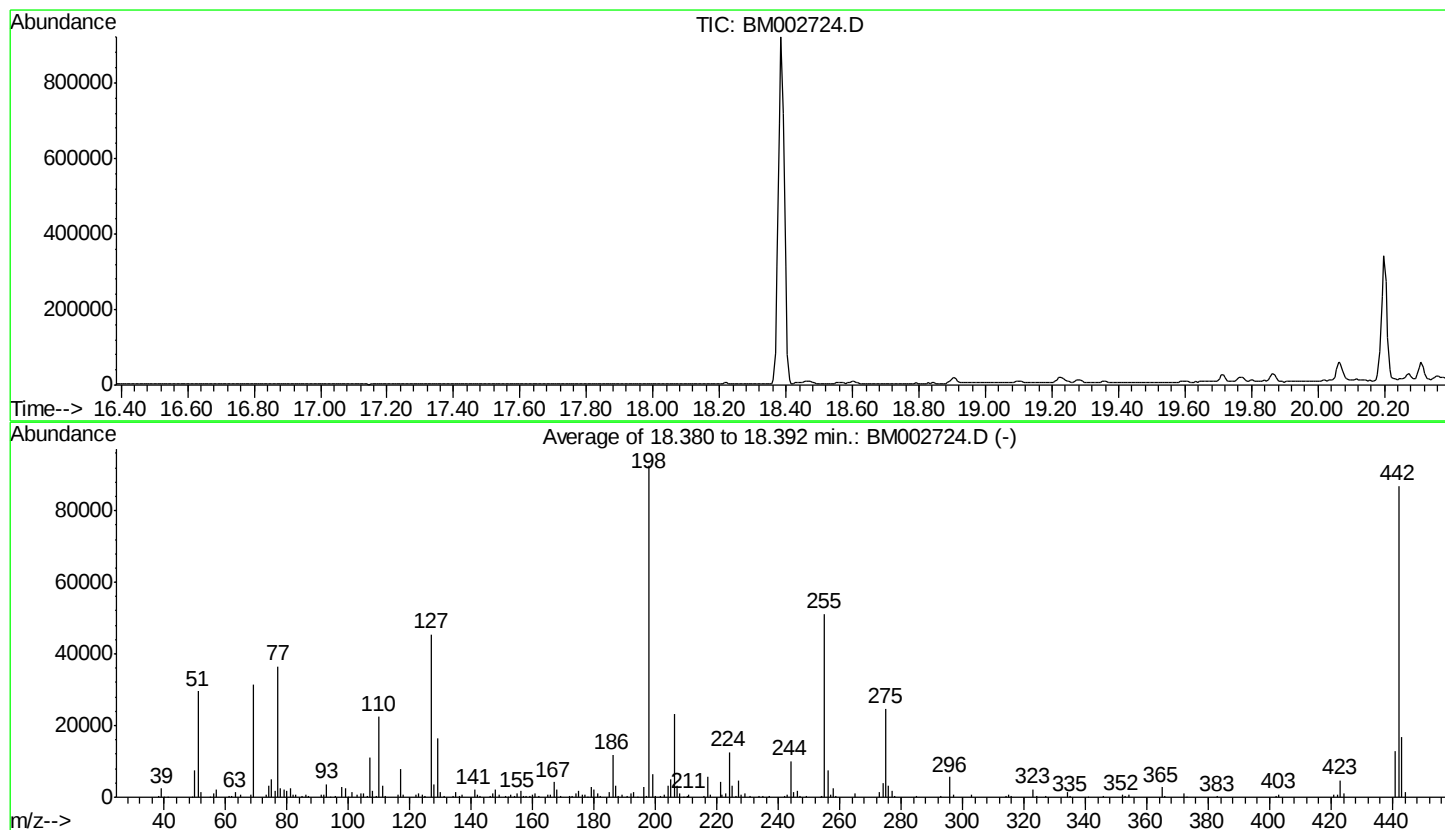

AutoFind: Scans 2600, 2601, 2602; Background Corrected with Scan 2594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	29618	PASS
68	69	0.00	2	1.9	602	PASS
69	198	0.00	100	33.8	31317	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.1	45410	PASS
197	198	0.00	1	0.6	518	PASS
198	198	100	100	100.0	92557	PASS
199	198	5	9	6.8	6276	PASS
275	198	10	60	26.7	24722	PASS
365	198	1	100	3.0	2786	PASS
441	443	0.01	100	77.1	13051	PASS
442	198	50	100	94.0	86986	PASS
443	442	15	24	19.5	16921	PASS

m/z	Abundance
38.00	433.0
39.10	2746.0
40.00	561.0
41.00	413.0
43.00	381.0
44.00	1679.0
50.00	7609.0
51.10	30536.0
52.00	1765.0
55.00	555.0
56.00	1107.0
57.00	2426.0
61.00	446.0
62.00	477.0
63.00	1363.0
65.00	643.0
68.00	612.0
69.00	32528.0
73.00	567.0
74.00	3049.0
75.00	4927.0
76.10	1499.0
77.00	36704.0
78.00	2641.0
79.00	2114.0
80.00	1743.0
81.00	2786.0
82.00	636.0
82.90	751.0
85.00	522.0
85.90	615.0
87.00	465.0
91.00	859.0
92.00	627.0
93.00	3761.0
95.90	305.0
98.00	2828.0
99.00	2648.0
101.00	1536.0
103.00	588.0
104.00	957.0
105.00	995.0
106.10	360.0
107.00	10750.0
108.00	1782.0
109.00	354.0
110.00	22080.0
111.00	3252.0
112.00	438.0
116.00	607.0
117.00	7422.0
117.90	661.0
121.90	892.0
123.00	1173.0
123.90	519.0
125.00	505.0
127.00	43848.0
128.00	3522.0
129.00	15703.0
130.00	1400.0
131.00	362.0
133.90	498.0
134.90	1360.0
135.90	481.0
137.00	826.0
141.00	1999.0
141.90	687.0
143.00	480.0
146.00	344.0
146.90	1199.0
148.00	1966.0
148.90	600.0
150.90	327.0
153.00	820.0
153.90	518.0
155.00	1177.0
156.00	1611.0
157.00	402.0
157.90	456.0
159.00	409.0
160.00	713.0
160.90	772.0
162.10	300.0
165.00	755.0
166.00	626.0
167.00	3738.0
168.00	1917.0
169.00	378.0
171.90	447.0
172.90	523.0
174.00	885.0

Instrument :
BNA_M
ClientSampleId :
DFTPP16

175.00	1571.0
176.10	570.0
176.90	726.0
179.00	2759.0
180.00	2067.0
181.00	1016.0
182.00	323.0
185.00	1420.0
186.00	10886.0
187.00	2992.0
187.90	367.0
189.00	719.0
190.90	385.0
192.00	887.0
193.00	1305.0
196.00	2451.0
197.00	471.0
198.00	82360.0
199.00	5978.0
200.00	484.0
201.60	417.0
202.90	468.0
204.00	2679.0
205.00	4766.0
206.00	20592.0
207.00	3278.0
208.00	833.0
210.20	388.0
210.90	815.0
216.00	452.0
217.00	5049.0
218.00	619.0
221.00	4091.0
223.00	1075.0
224.00	11029.0
225.00	2847.0
226.00	346.0
227.00	3882.0
228.00	563.0
229.00	984.0
231.00	374.0
234.90	356.0
237.00	405.0
242.00	452.0
243.00	579.0
244.00	8704.0
245.00	1149.0
246.00	1334.0
247.00	317.0
253.90	328.0
255.00	43072.0
256.00	6762.0
257.00	579.0
258.00	2179.0
258.90	459.0
265.00	790.0
273.00	1254.0
274.00	3383.0
275.00	20184.0
276.00	2938.0
276.90	1462.0
278.00	306.0
292.90	437.0
296.00	4662.0
296.90	705.0
303.00	637.0
315.00	507.0
315.90	321.0
323.00	1846.0
324.00	367.0
327.00	324.0
334.00	1128.0
335.00	342.0
352.00	455.0
353.00	369.0
354.00	636.0
365.00	2154.0
366.00	341.0
372.00	945.0
401.90	399.0
403.00	589.0
421.00	528.0
422.10	470.0
423.00	3564.0
424.00	897.0
441.00	9407.0
442.00	60256.0
443.00	12221.0
444.10	1204.0

Instrument :
BNA_M
ClientSampleId :
DFTPP16

m/z	Abundance
38.00	433.0
39.10	2866.0
40.00	524.0
41.00	524.0
44.00	1828.0
49.10	327.0
50.00	8767.0
51.10	35344.0
52.00	1797.0
55.00	483.0
56.00	1045.0
57.00	2424.0
61.00	361.0
62.00	510.0
63.00	1466.0
65.00	815.0
68.10	659.0
69.00	36048.0
73.00	627.0
74.00	3594.0
75.00	5756.0
76.00	2044.0
77.00	43040.0
78.00	3050.0
79.00	2825.0
80.00	2191.0
81.00	2984.0
81.90	765.0
83.00	904.0
85.00	656.0
85.90	827.0
86.90	490.0
91.00	953.0
92.00	738.0
93.00	4247.0
93.90	420.0
95.90	341.0
98.00	3268.0
99.00	3120.0
100.00	300.0
101.00	1912.0
102.90	723.0
104.00	1443.0
105.00	1082.0
106.10	425.0
107.00	13558.0
108.00	2262.0
109.00	510.0
110.00	26792.0
111.00	4078.0
112.00	493.0
116.00	795.0
117.00	9453.0
118.00	751.0
122.00	978.0
122.90	1434.0
124.00	763.0
125.00	559.0
127.00	53640.0
128.00	4355.0
129.00	20400.0
130.00	1797.0
131.00	406.0
134.00	563.0
135.00	1794.0
136.00	571.0
137.00	881.0
140.90	2539.0
142.00	927.0
143.00	712.0
145.90	412.0
147.00	1389.0
148.00	2492.0
149.00	690.0
151.00	382.0
151.90	401.0
152.90	770.0
153.90	619.0
155.00	1279.0
156.00	1926.0
157.10	380.0
157.90	399.0
158.90	366.0
159.90	695.0
161.00	1116.0
161.90	375.0
165.00	971.0
165.90	863.0
167.00	5130.0
168.00	2560.0
169.00	424.0

Instrument :
BNA_M
ClientSampleId :
DFTPP16

171.90	432.0
173.00	633.0
173.90	1032.0
175.00	1965.0
176.00	672.0
176.90	1024.0
177.90	366.0
179.00	3447.0
180.00	2514.0
181.00	1269.0
182.00	314.0
185.00	1884.0
186.00	14219.0
187.00	4093.0
188.00	453.0
189.00	887.0
191.00	519.0
191.90	1123.0
193.00	1517.0
196.00	3253.0
197.10	626.0
198.00	109064.0
199.00	7450.0
200.00	640.0
201.50	544.0
202.90	764.0
204.00	3619.0
205.00	6019.0
206.00	27696.0
207.00	4097.0
208.00	1087.0
209.00	331.0
210.20	479.0
211.00	936.0
215.90	449.0
217.00	6815.0
218.00	897.0
221.00	5108.0
221.80	1074.0
223.00	1516.0
224.00	14993.0
225.00	3836.0
226.00	495.0
227.00	5864.0
228.00	711.0
228.90	1182.0
231.00	453.0
233.90	417.0
235.00	354.0
237.00	400.0
242.00	641.0
243.00	808.0
244.00	12190.0
245.00	1661.0
246.00	2067.0
246.90	429.0
249.00	467.0
254.10	475.0
255.00	60920.0
256.00	8847.0
257.00	674.0
258.00	3204.0
258.90	411.0
265.00	1232.0
273.00	1944.0
274.00	5015.0
275.00	29872.0
276.00	3878.0
277.00	2106.0
278.00	329.0
285.00	400.0
292.90	466.0
296.00	6814.0
297.00	869.0
303.00	889.0
314.00	345.0
315.00	689.0
316.00	479.0
323.00	2401.0
324.00	366.0
327.00	513.0
334.00	1591.0
335.00	460.0
341.00	341.0
346.00	559.0
352.00	756.0
353.00	603.0
354.00	903.0
365.00	3449.0
365.90	537.0
372.10	1528.0
373.00	365.0
383.00	394.0
402.00	529.0
403.00	839.0

Instrument :
BNA_M
ClientSampleId :
DFTPP16

421.00	846.0
422.00	768.0
423.00	5828.0
424.00	1190.0
441.00	15287.0
442.00	102416.0
443.00	20000.0
444.00	1693.0

Instrument :
BNA_M
ClientSampleId :
DFTPP16

m/z	Abundance
38.00	358.0
39.00	1877.0
40.00	487.0
41.10	464.0
44.00	1881.0
50.00	5997.0
51.10	22976.0
52.00	1242.0
55.10	356.0
56.00	981.0
57.00	1838.0
60.90	308.0
62.00	374.0
63.00	1019.0
65.00	667.0
68.10	535.0
69.00	25376.0
73.00	484.0
74.00	2544.0
75.00	3887.0
76.10	1552.0
77.10	29968.0
78.00	2248.0
79.00	2047.0
80.00	1350.0
81.00	2163.0
82.00	545.0
83.00	664.0
85.10	393.0
86.00	582.0
87.00	310.0
91.00	718.0
92.00	622.0
93.00	3239.0
98.00	2355.0
99.00	1962.0
101.00	1187.0
103.00	509.0
104.00	949.0
105.00	743.0
106.00	306.0
107.00	9441.0
108.00	1603.0
109.00	403.0
110.00	18424.0
111.00	2668.0
112.00	343.0
116.00	553.0
117.00	6246.0
118.00	452.0
122.00	657.0
123.00	1035.0
123.90	502.0
125.00	443.0
127.00	38744.0
128.00	3078.0
129.00	13763.0
130.00	1182.0
131.00	380.0
133.90	412.0
135.00	1082.0
136.00	535.0
137.00	652.0
141.00	1780.0
142.00	532.0
143.00	419.0
145.90	364.0
147.00	1113.0
148.00	1824.0
149.00	469.0
151.00	320.0
152.90	649.0
153.90	495.0
155.00	1066.0
156.00	1392.0
156.90	433.0
157.90	330.0
158.90	318.0
160.00	642.0
161.00	968.0
164.90	820.0
165.90	607.0
167.00	3544.0
167.90	1844.0
169.00	323.0
171.90	361.0
173.00	368.0
174.00	913.0
175.00	1566.0
176.00	467.0
177.00	740.0

Instrument :
BNA_M
ClientSampleId :
DFTPP16

179.00	2730.0
180.00	1994.0
181.00	933.0
181.90	313.0
184.90	1371.0
186.00	10617.0
187.00	3004.0
188.00	361.0
188.90	731.0
191.00	353.0
192.00	862.0
193.00	1040.0
193.90	314.0
196.00	2553.0
197.10	459.0
198.00	86248.0
198.90	5401.0
200.00	504.0
201.50	406.0
202.90	531.0
204.00	2863.0
205.00	4572.0
206.00	21728.0
207.00	3272.0
207.90	910.0
211.00	729.0
216.00	431.0
217.00	5389.0
218.00	692.0
221.00	3738.0
221.80	868.0
223.00	1112.0
224.00	11520.0
225.00	2815.0
226.00	388.0
227.00	4522.0
227.90	729.0
228.90	1031.0
230.90	441.0
233.80	319.0
235.00	326.0
236.90	431.0
241.90	534.0
243.00	685.0
244.00	9483.0
245.00	1320.0
246.00	1740.0
247.00	334.0
249.00	368.0
254.10	330.0
255.00	49656.0
256.00	7033.0
256.90	567.0
258.00	2412.0
258.90	442.0
265.00	1018.0
273.00	1583.0
274.00	3964.0
275.00	24112.0
276.00	3254.0
276.90	1767.0
285.00	411.0
293.00	481.0
296.00	5644.0
297.00	895.0
303.00	726.0
314.00	308.0
315.00	645.0
316.00	357.0
323.00	2437.0
324.00	433.0
327.00	397.0
334.00	1410.0
346.00	444.0
351.90	687.0
353.00	446.0
354.00	836.0
365.00	2757.0
366.00	389.0
372.00	1182.0
382.90	351.0
402.00	527.0
403.00	825.0
421.00	577.0
422.00	698.0
423.00	5046.0
424.00	1135.0
441.00	14460.0
442.00	98288.0
443.00	18544.0
444.00	1748.0

Instrument :

BNA_M

ClientSampleId :

DFTPP16

Scan 2594 (18.345 min): BM002724.D
DFTPP16

m/z	Abundance
40.00	484.0
41.00	444.0
43.00	326.0
44.00	1888.0
55.10	327.0
207.00	467.0

Instrument :
BNA_M
ClientSampleId :
DFTPP16