

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
 Data File : BM027547.D
 Acq On : 26 Sep 2020 02:42
 Operator : JU/CG
 Sample : L4139-08
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG4A1

Quant Time: Sep 26 05:23:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 24 20:21:51 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	102595	20.00	ng/ul	# 0.00
18) Naphthalene-d8	10.592	136	368004	20.00	ng/ul	# 0.00
36) Acenaphthene-d10	14.433	164	270148	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.174	188	624222	20.00	ng/ul	#-0.01
78) Chrysene-d12	21.350	240	671748	20.00	ng/ul	#-0.01
86) Perylene-d12	23.621	264	716255	20.00	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.316	96	9526	5.28	ng/uL	0.00
5) Phenol-d5	6.969	99	50923	7.61	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.139	67	113344	28.83	ng/ul	0.00
9) 2-Chlorophenol-d4	7.339	132	154502	26.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.504	113	97294	17.35	ng/ul	0.00
19) Nitrobenzene-d5	8.957	128	90579	33.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.674	143	105295	37.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.210	165	224183	30.92	ng/ul	0.00
29) 4-Chloroaniline-d4	10.721	131	18925	2.63	ng/ul	0.00
44) Dimethylphthalate-d6	13.851	166	769954	36.84	ng/ul	0.00
47) Acenaphthylene-d8	14.127	160	880355	35.17	ng/ul	0.00
52) 4-Nitrophenol-d4	14.621	143	22076	7.54	ng/ul	0.00
58) Fluorene-d10	15.427	176	672755	35.78	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.539	200	124027	36.70	ng/ul	0.00
71) Anthracene-d10	17.274	188	1196834	40.65	ng/ul	0.00
79) Pyrene-d10	19.568	212	1424451	40.65	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.474	264	1542776	40.54	ng/ul	-0.02
Target Compounds						
						Qvalue
45) Dimethylphthalate	13.892	163	69264	3.25	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
Data File : BM027547.D
Acq On : 26 Sep 2020 02:42
Operator : JU/CG
Sample : L4139-08
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG4A1


Quant Time: Sep 26 05:23:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 24 20:21:51 2020
Response via : Initial Calibration

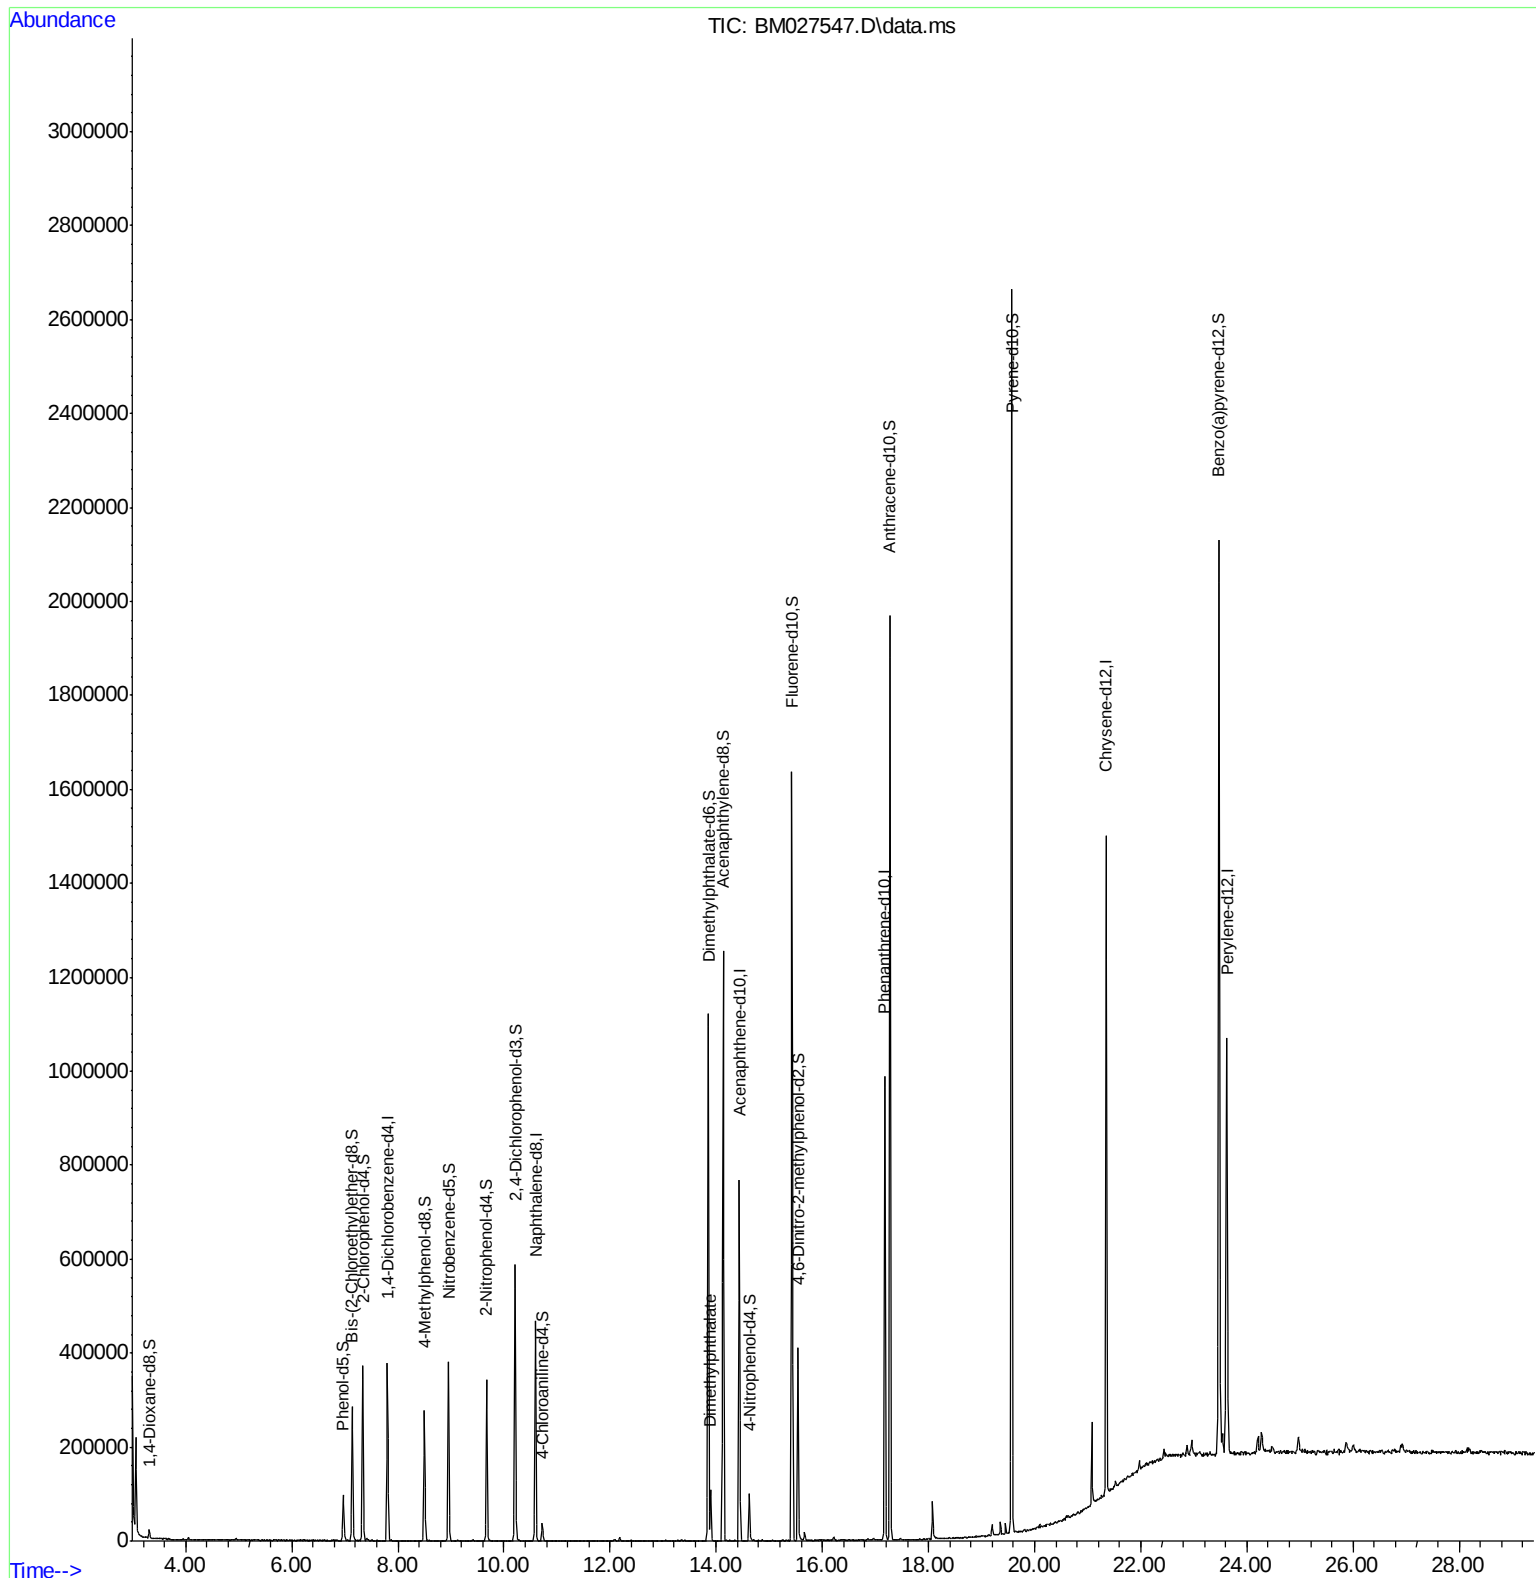

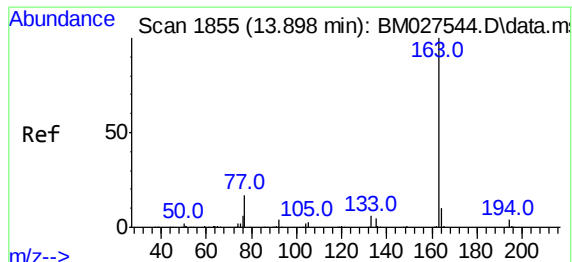

#45
 Dimethylphthalate
 Concen: 3.25 ng/ul
 RT: 13.892 min Scan# 1854
 Delta R.T. -0.012 min
 Lab File: BM027547.D
 Acq: 26 Sep 2020 02:42

Instrument :
 BNA_M
 ClientSampleId :
 BG4A1

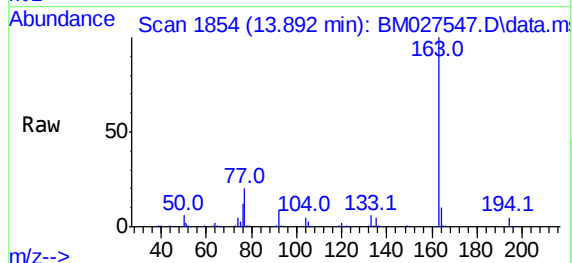

Tgt Ion:163 Resp: 69264

Ion	Ratio	Lower	Upper
163	100		
194	5.3	3.3	4.9#
164	10.3	8.1	12.1

