

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
 Data File : BM027550.D
 Acq On : 26 Sep 2020 04:30
 Operator : JU/CG
 Sample : L4139-10
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG4A2

Quant Time: Sep 26 05:24:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 24 20:21:51 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	92680	20.00	ng/ul	0.00
18) Naphthalene-d8	10.592	136	357058	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.433	164	298113	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.174	188	769683	20.00	ng/ul	#-0.01
78) Chrysene-d12	21.350	240	881664	20.00	ng/ul	#-0.01
86) Perylene-d12	23.621	264	798621	20.00	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.310	96	9843	6.04	ng/uL	0.00
5) Phenol-d5	6.969	99	45289	7.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.139	67	107406	30.24	ng/ul	0.00
9) 2-Chlorophenol-d4	7.339	132	141794	27.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.504	113	94458	18.65	ng/ul	0.00
19) Nitrobenzene-d5	8.951	128	90130	34.25	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.675	143	107682	39.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.210	165	241335	34.30	ng/ul	0.00
29) 4-Chloroaniline-d4	10.722	131	17290	2.48	ng/ul	0.00
44) Dimethylphthalate-d6	13.851	166	964350	41.81	ng/ul	0.00
47) Acenaphthylene-d8	14.127	160	991884	35.90	ng/ul	0.00
52) 4-Nitrophenol-d4	14.621	143	29048	8.99	ng/ul	0.00
58) Fluorene-d10	15.427	176	812734	39.17	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.539	200	173152	41.55	ng/ul	0.00
71) Anthracene-d10	17.274	188	1532772	42.22	ng/ul	0.00
79) Pyrene-d10	19.568	212	1978860	43.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.480	264	1820707	42.91	ng/ul	-0.01
Target Compounds						
45) Dimethylphthalate	13.892	163	84298	3.58	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
Data File : BM027550.D
Acq On : 26 Sep 2020 04:30
Operator : JU/CG
Sample : L4139-10
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG4A2

Quant Time: Sep 26 05:24:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 24 20:21:51 2020
Response via : Initial Calibration

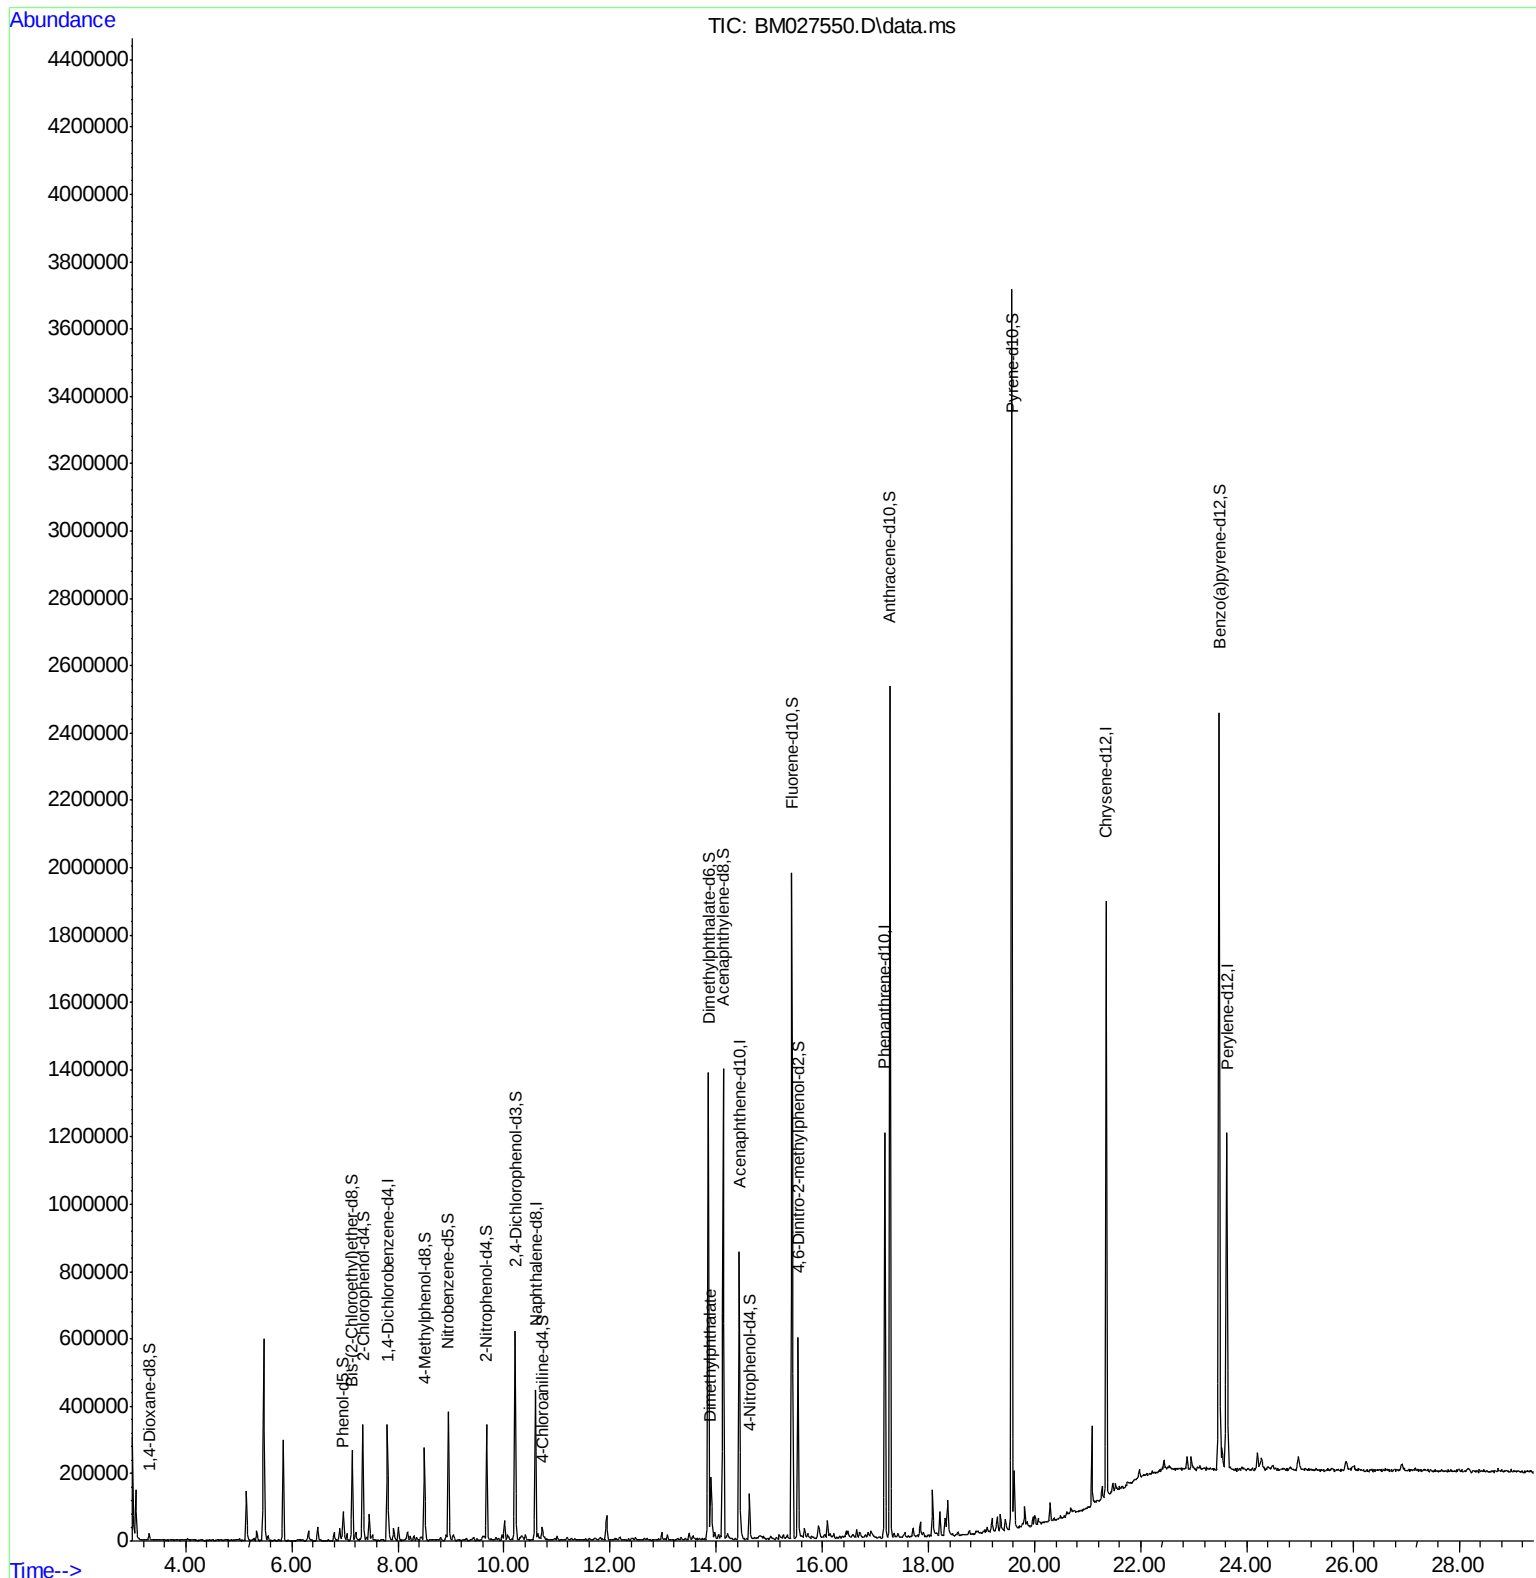

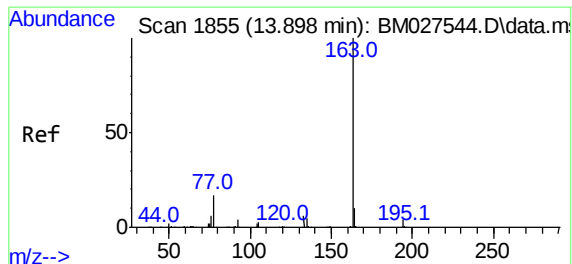

#45
 Dimethylphthalate
 Concen: 3.58 ng/ul
 RT: 13.892 min Scan# 1854
 Delta R.T. -0.012 min
 Lab File: BM027550.D
 Acq: 26 Sep 2020 04:30

Instrument :
 BNA_M
 ClientSampleId :
 BG4A2

Tgt Ion:	163	Resp:	84298
Ion	Ratio	Lower	Upper
163	100		
194	4.9	3.3	4.9
164	10.2	8.1	12.1

