

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
 Data File : BM027553.D
 Acq On : 26 Sep 2020 06:18
 Operator : JU/CG
 Sample : L4139-02
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG4A0

Quant Time: Sep 26 08:45:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 24 20:21:51 2020
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	93434	20.00	ng/ul	0.00
18) Naphthalene-d8	10.592	136	358002	20.00	ng/ul	# 0.00
36) Acenaphthene-d10	14.433	164	287111	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.174	188	708014	20.00	ng/ul	#-0.01
78) Chrysene-d12	21.350	240	701348	20.00	ng/ul	#-0.01
86) Perylene-d12	23.621	264	614117	20.00	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.310	96	9597	5.85	ng/uL	0.00
5) Phenol-d5	6.969	99	48359	7.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.140	67	116710	32.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.340	132	152475	28.93	ng/ul	0.00
13) 4-Methylphenol-d8	8.504	113	100198	19.62	ng/ul	0.00
19) Nitrobenzene-d5	8.951	128	92658	35.11	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.675	143	108900	39.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.210	165	242202	34.34	ng/ul	0.00
29) 4-Chloroaniline-d4	10.722	131	18975	2.71	ng/ul	0.00
44) Dimethylphthalate-d6	13.845	166	903612	40.68	ng/ul	-0.01
47) Acenaphthylene-d8	14.127	160	994589	37.38	ng/ul	0.00
52) 4-Nitrophenol-d4	14.621	143	23814	7.65	ng/ul	0.00
58) Fluorene-d10	15.427	176	784963	39.29	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.539	200	147231	38.41	ng/ul	0.00
71) Anthracene-d10	17.274	188	1419793	42.51	ng/ul	0.00
79) Pyrene-d10	19.568	212	1667637	45.58	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.474	264	1379946	42.30	ng/ul	-0.02
Target Compounds						
45) Dimethylphthalate	13.892	163	55221	2.44	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
Data File : BM027553.D
Acq On : 26 Sep 2020 06:18
Operator : JU/CG
Sample : L4139-02
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG4A0

Quant Time: Sep 26 08:45:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 24 20:21:51 2020
Response via : Initial Calibration

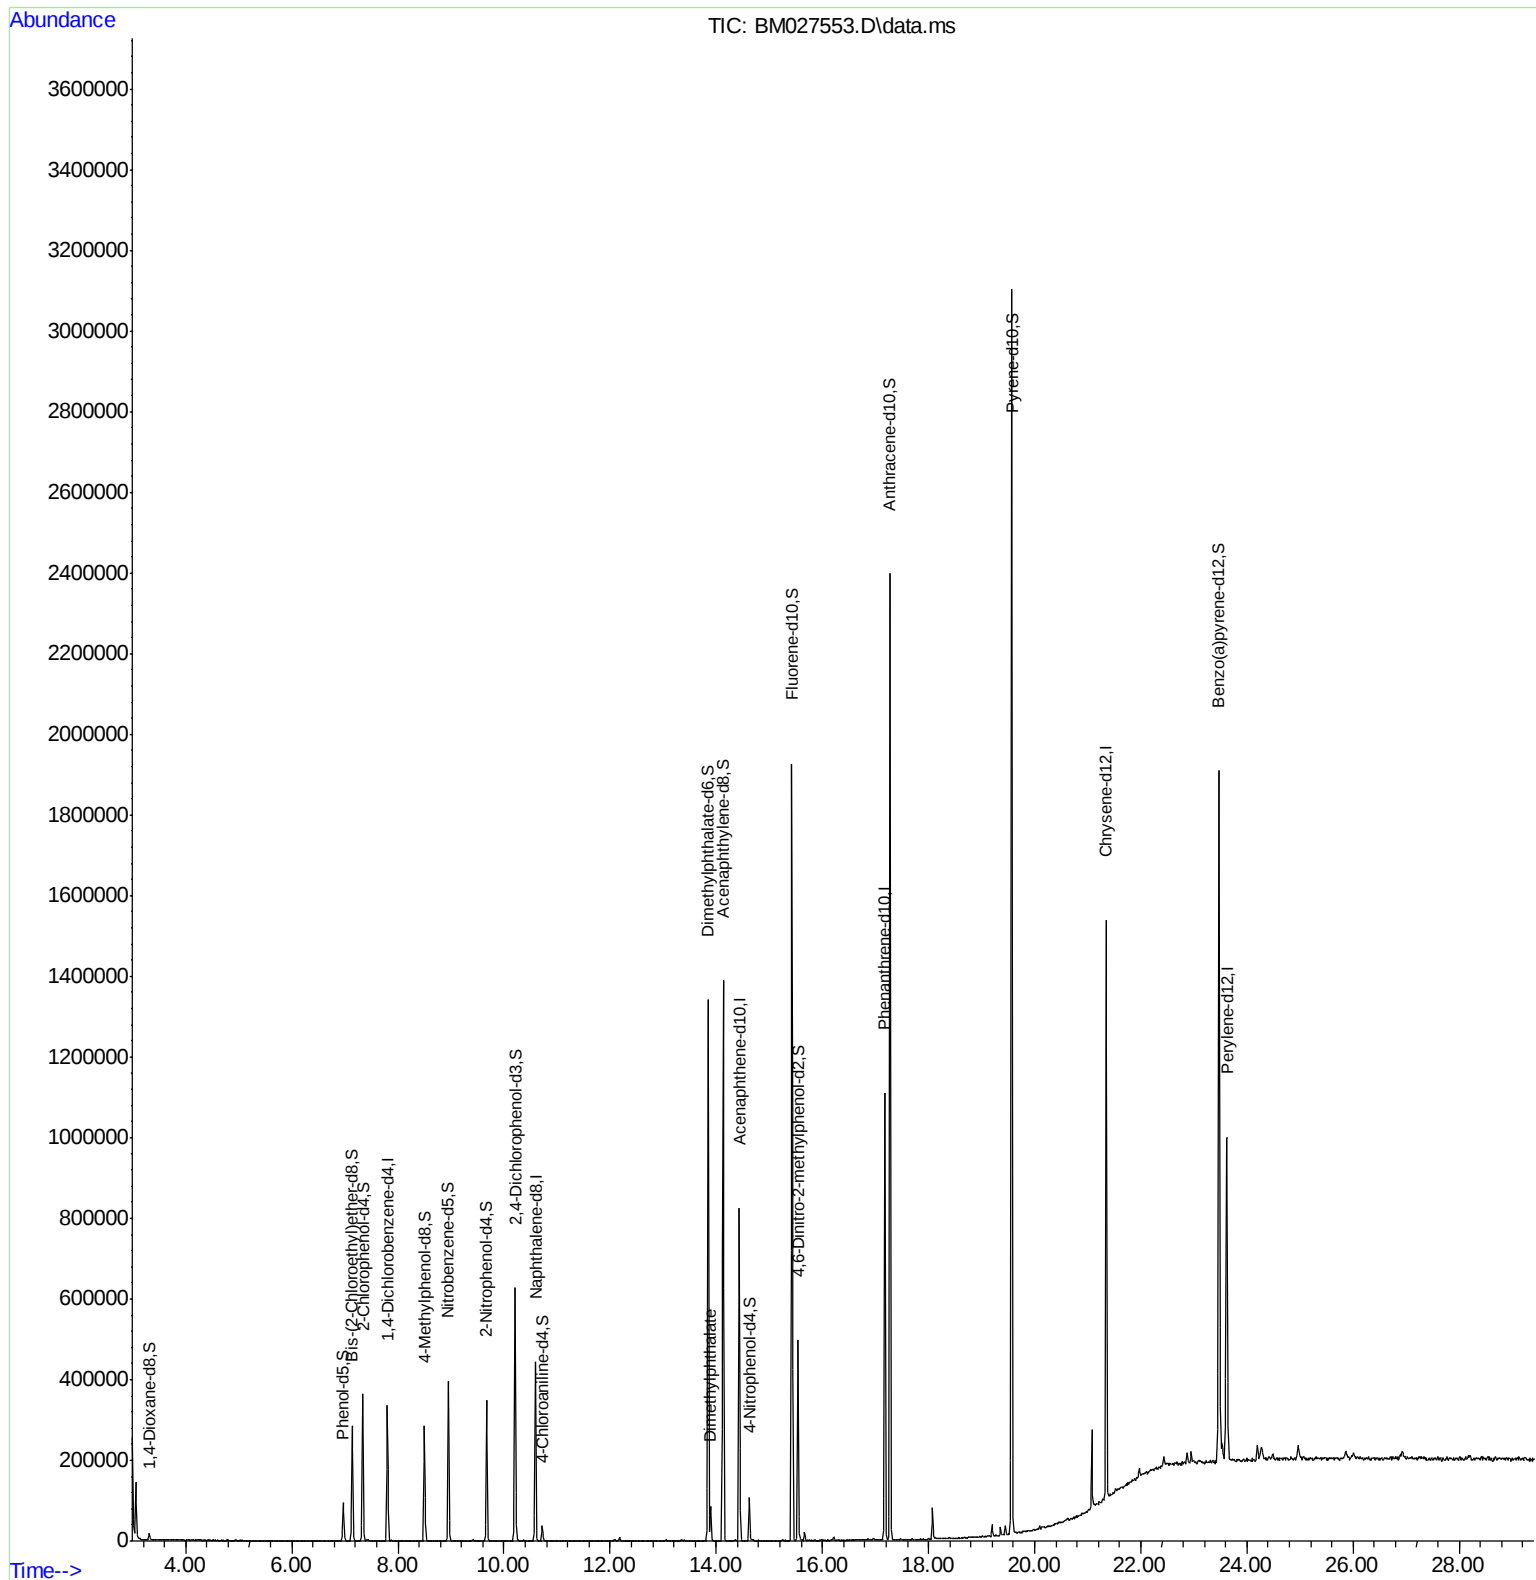

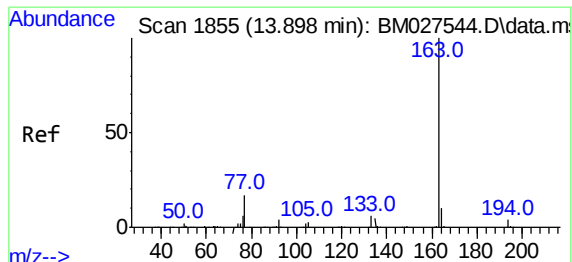

#45
 Dimethylphthalate
 Concen: 2.44 ng/ul
 RT: 13.892 min Scan# 1854
 Delta R.T. -0.012 min
 Lab File: BM027553.D
 Acq: 26 Sep 2020 06:18

Instrument :
 BNA_M
 ClientSampleId :
 BG4A0

Tgt Ion:	163	Resp:	55221
Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.3	4.9
164	10.5	8.1	12.1

