

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
 Data File : BM027523.D
 Acq On : 25 Sep 2020 11:35
 Operator : JU/CG
 Sample : L4135-15
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG487

Quant Time: Sep 25 12:06:50 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 24 20:21:51 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	85072	20.00	ng/ul	0.00
18) Naphthalene-d8	10.598	136	324545	20.00	ng/ul	# 0.00
36) Acenaphthene-d10	14.439	164	257028	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.180	188	605588	20.00	ng/ul	# 0.00
78) Chrysene-d12	21.362	240	552260	20.00	ng/ul	# 0.00
86) Perylene-d12	23.633	264	547552	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	9175	6.14	ng/uL	0.00
5) Phenol-d5	6.969	99	30459	5.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.140	67	82602	25.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.340	132	96519	20.11	ng/ul	0.00
13) 4-Methylphenol-d8	8.504	113	61867	13.31	ng/ul	0.00
19) Nitrobenzene-d5	8.957	128	59441	24.85	ng/ul	0.00
22) 2-Nitrophenol-d4	9.675	143	64175	25.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.210	165	155963	24.39	ng/ul	0.00
29) 4-Chloroaniline-d4	10.728	131	7194	1.14	ng/ul	0.00
44) Dimethylphthalate-d6	13.851	166	620495	31.20	ng/ul	0.00
47) Acenaphthylene-d8	14.133	160	699035	29.35	ng/ul	0.00
52) 4-Nitrophenol-d4	14.622	143	13709	4.92	ng/ul	0.00
58) Fluorene-d10	15.433	176	536668	30.00	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.539	200	91946	28.04	ng/ul	0.00
71) Anthracene-d10	17.280	188	939389	32.88	ng/ul	0.00
79) Pyrene-d10	19.568	212	1046863	36.34	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.492	264	946618	32.54	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.898	163	21210	1.05	ng/ul#	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
Data File : BM027523.D
Acq On : 25 Sep 2020 11:35
Operator : JU/CG
Sample : L4135-15
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG487


Quant Time: Sep 25 12:06:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 24 20:21:51 2020
Response via : Initial Calibration

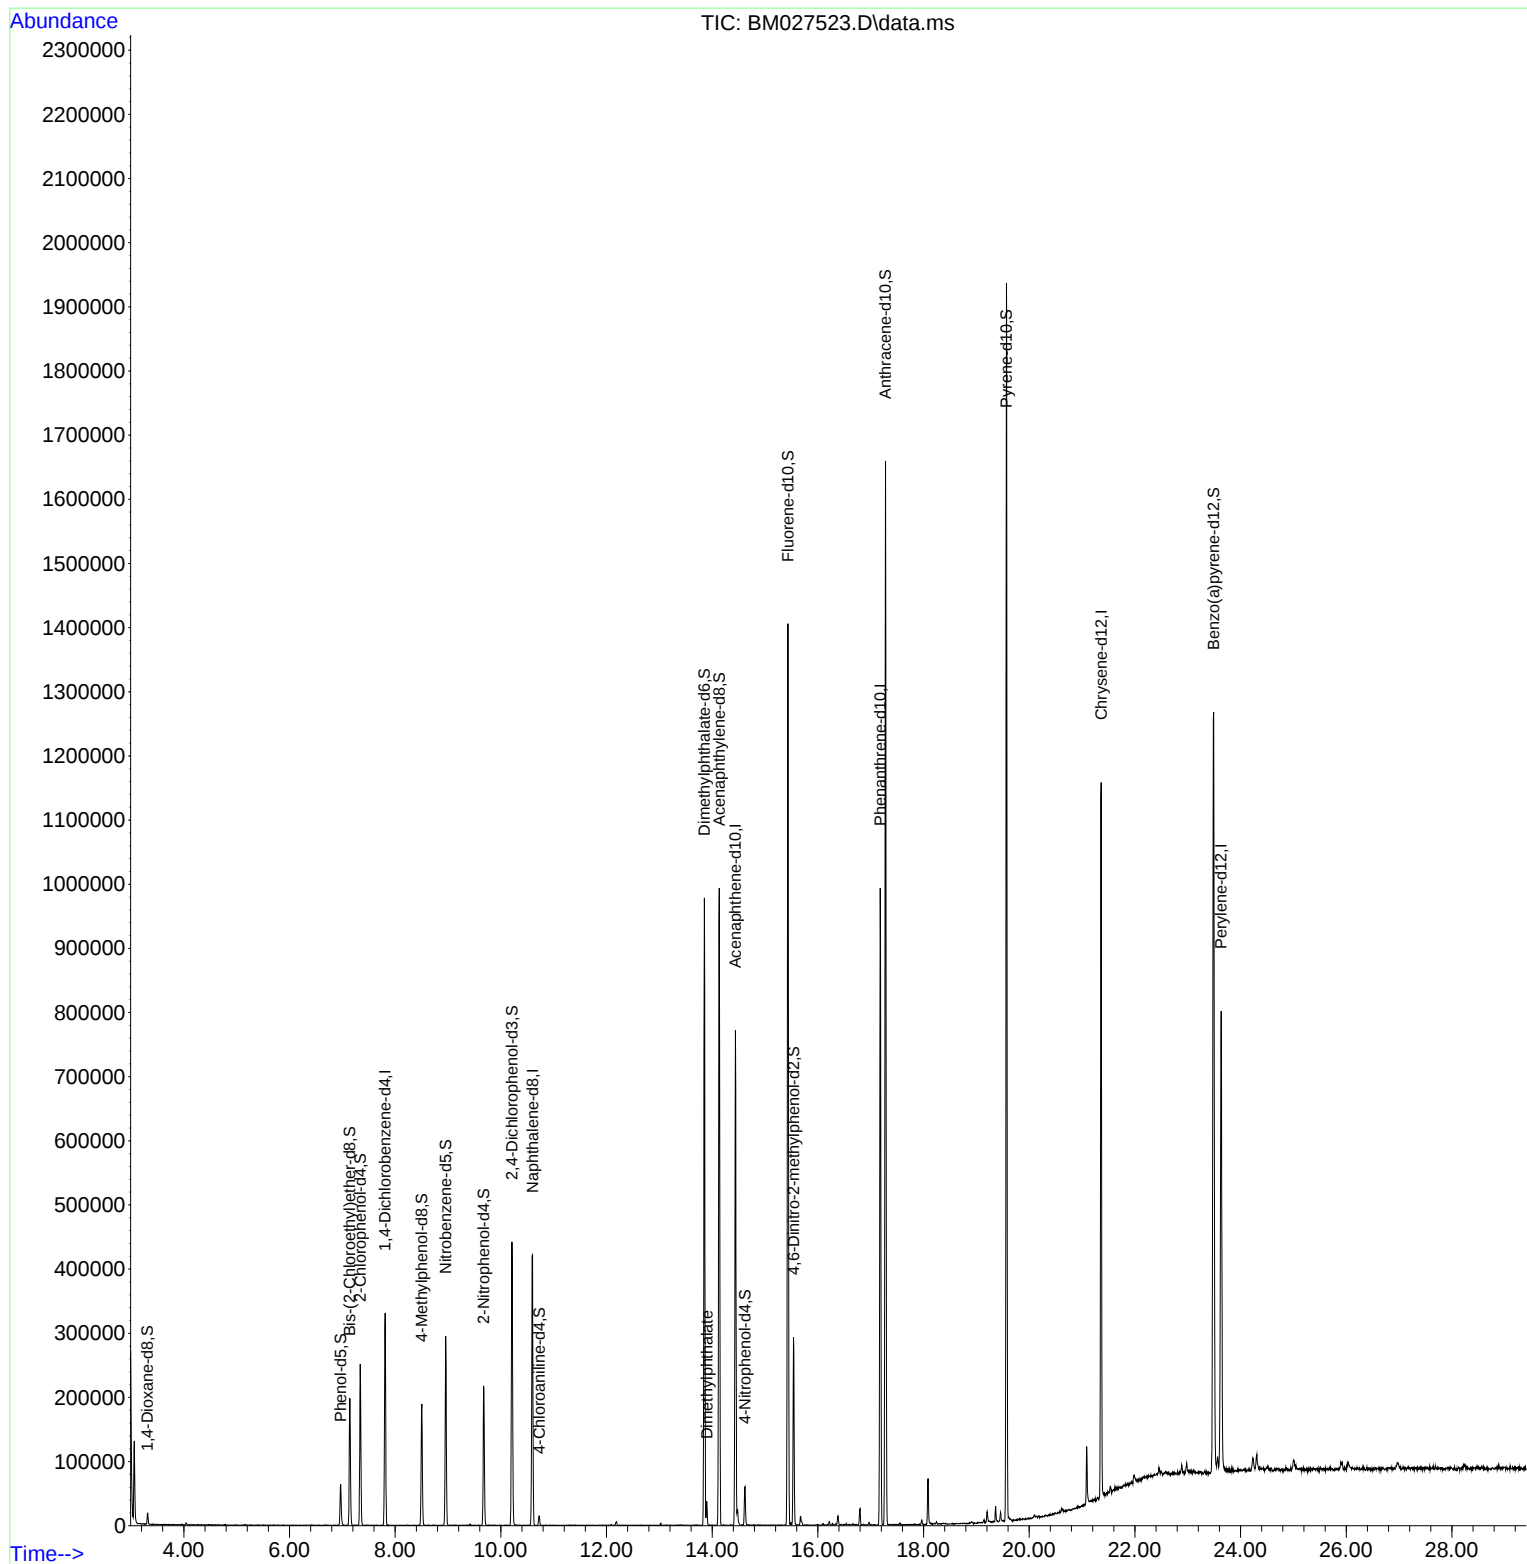

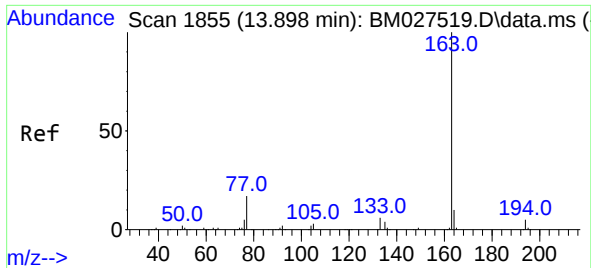

#45
Dimethylphthalate
Concen: 1.05 ng/ul
RT: 13.898 min Scan# 1855
Delta R.T. -0.006 min
Lab File: BM027523.D
Acq: 25 Sep 2020 11:35

Instrument :
BNA_M
ClientSampleId :
BG487

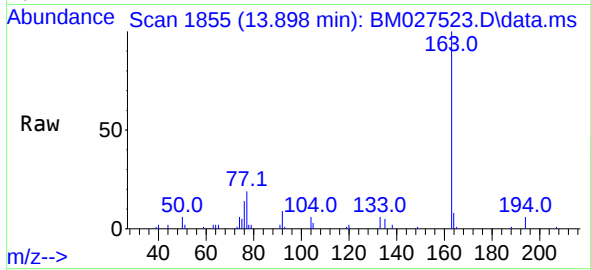

Tgt Ion:163 Resp: 21210
Ion Ratio Lower Upper
163 100
194 5.6 3.3 4.9#
164 8.1 8.1 12.1

