

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM092520\  
 Data File : BM027524.D  
 Acq On : 25 Sep 2020 12:11  
 Operator : JU/CG  
 Sample : L4135-04  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 BG478

Quant Time: Sep 25 12:56:14 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM092420MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Sep 24 20:21:51 2020  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc  | Units  | Dev(Min)  |
|-------------------------------|--------|------|----------|-------|--------|-----------|
| -----                         |        |      |          |       |        |           |
| Internal Standards            |        |      |          |       |        |           |
| 1) 1,4-Dichlorobenzene-d4     | 7.810  | 152  | 88711    | 20.00 | ng/ul  | 0.00      |
| 18) Naphthalene-d8            | 10.598 | 136  | 329206   | 20.00 | ng/ul  | 0.00      |
| 36) Acenaphthene-d10          | 14.439 | 164  | 260048   | 20.00 | ng/ul  | 0.00      |
| 62) Phenanthrene-d10          | 17.180 | 188  | 623846   | 20.00 | ng/ul  | # 0.00    |
| 78) Chrysene-d12              | 21.362 | 240  | 577245   | 20.00 | ng/ul  | # 0.00    |
| 86) Perylene-d12              | 23.632 | 264  | 553145   | 20.00 | ng/ul  | 0.00      |
| System Monitoring Compounds   |        |      |          |       |        |           |
| 3) 1,4-Dioxane-d8             | 3.316  | 96   | 9316     | 5.98  | ng/uL  | 0.00      |
| 5) Phenol-d5                  | 6.969  | 99   | 36559    | 6.32  | ng/ul  | 0.00      |
| 7) Bis-(2-Chloroethyl)eth...  | 7.139  | 67   | 93198    | 27.41 | ng/ul  | 0.00      |
| 9) 2-Chlorophenol-d4          | 7.339  | 132  | 110552   | 22.09 | ng/ul  | 0.00      |
| 13) 4-Methylphenol-d8         | 8.504  | 113  | 70409    | 14.52 | ng/ul  | 0.00      |
| 19) Nitrobenzene-d5           | 8.957  | 128  | 66255    | 27.30 | ng/ul  | 0.00      |
| 22) 2-Nitrophenol-d4          | 9.680  | 143  | 70996    | 27.92 | ng/ul  | 0.00      |
| 26) 2,4-Dichlorophenol-d3     | 10.210 | 165  | 162212   | 25.01 | ng/ul  | 0.00      |
| 29) 4-Chloroaniline-d4        | 10.727 | 131  | 8168     | 1.27  | ng/ul  | 0.00      |
| 44) Dimethylphthalate-d6      | 13.851 | 166  | 622224   | 30.93 | ng/ul  | 0.00      |
| 47) Acenaphthylene-d8         | 14.133 | 160  | 719302   | 29.85 | ng/ul  | 0.00      |
| 52) 4-Nitrophenol-d4          | 14.615 | 143  | 17384    | 6.17  | ng/ul  | -0.01     |
| 58) Fluorene-d10              | 15.433 | 176  | 566136   | 31.28 | ng/ul  | 0.00      |
| 63) 4,6-Dinitro-2-methylph... | 15.539 | 200  | 100657   | 29.80 | ng/ul  | 0.00      |
| 71) Anthracene-d10            | 17.280 | 188  | 1042829  | 35.44 | ng/ul  | 0.00      |
| 79) Pyrene-d10                | 19.574 | 212  | 1202714  | 39.94 | ng/ul  | 0.00      |
| 90) Benzo(a)pyrene-d12        | 23.491 | 264  | 1028597  | 35.00 | ng/ul  | 0.00      |
| Target Compounds              |        |      |          |       |        |           |
| 45) Dimethylphthalate         | 13.898 | 163  | 26515    | 1.29  | ng/ul# | Qvalue 98 |
| -----                         |        |      |          |       |        |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM092520\  
Data File : BM027524.D  
Acq On : 25 Sep 2020 12:11  
Operator : JU/CG  
Sample : L4135-04  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
BG478

Quant Time: Sep 25 12:56:14 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM092420MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Thu Sep 24 20:21:51 2020  
Response via : Initial Calibration

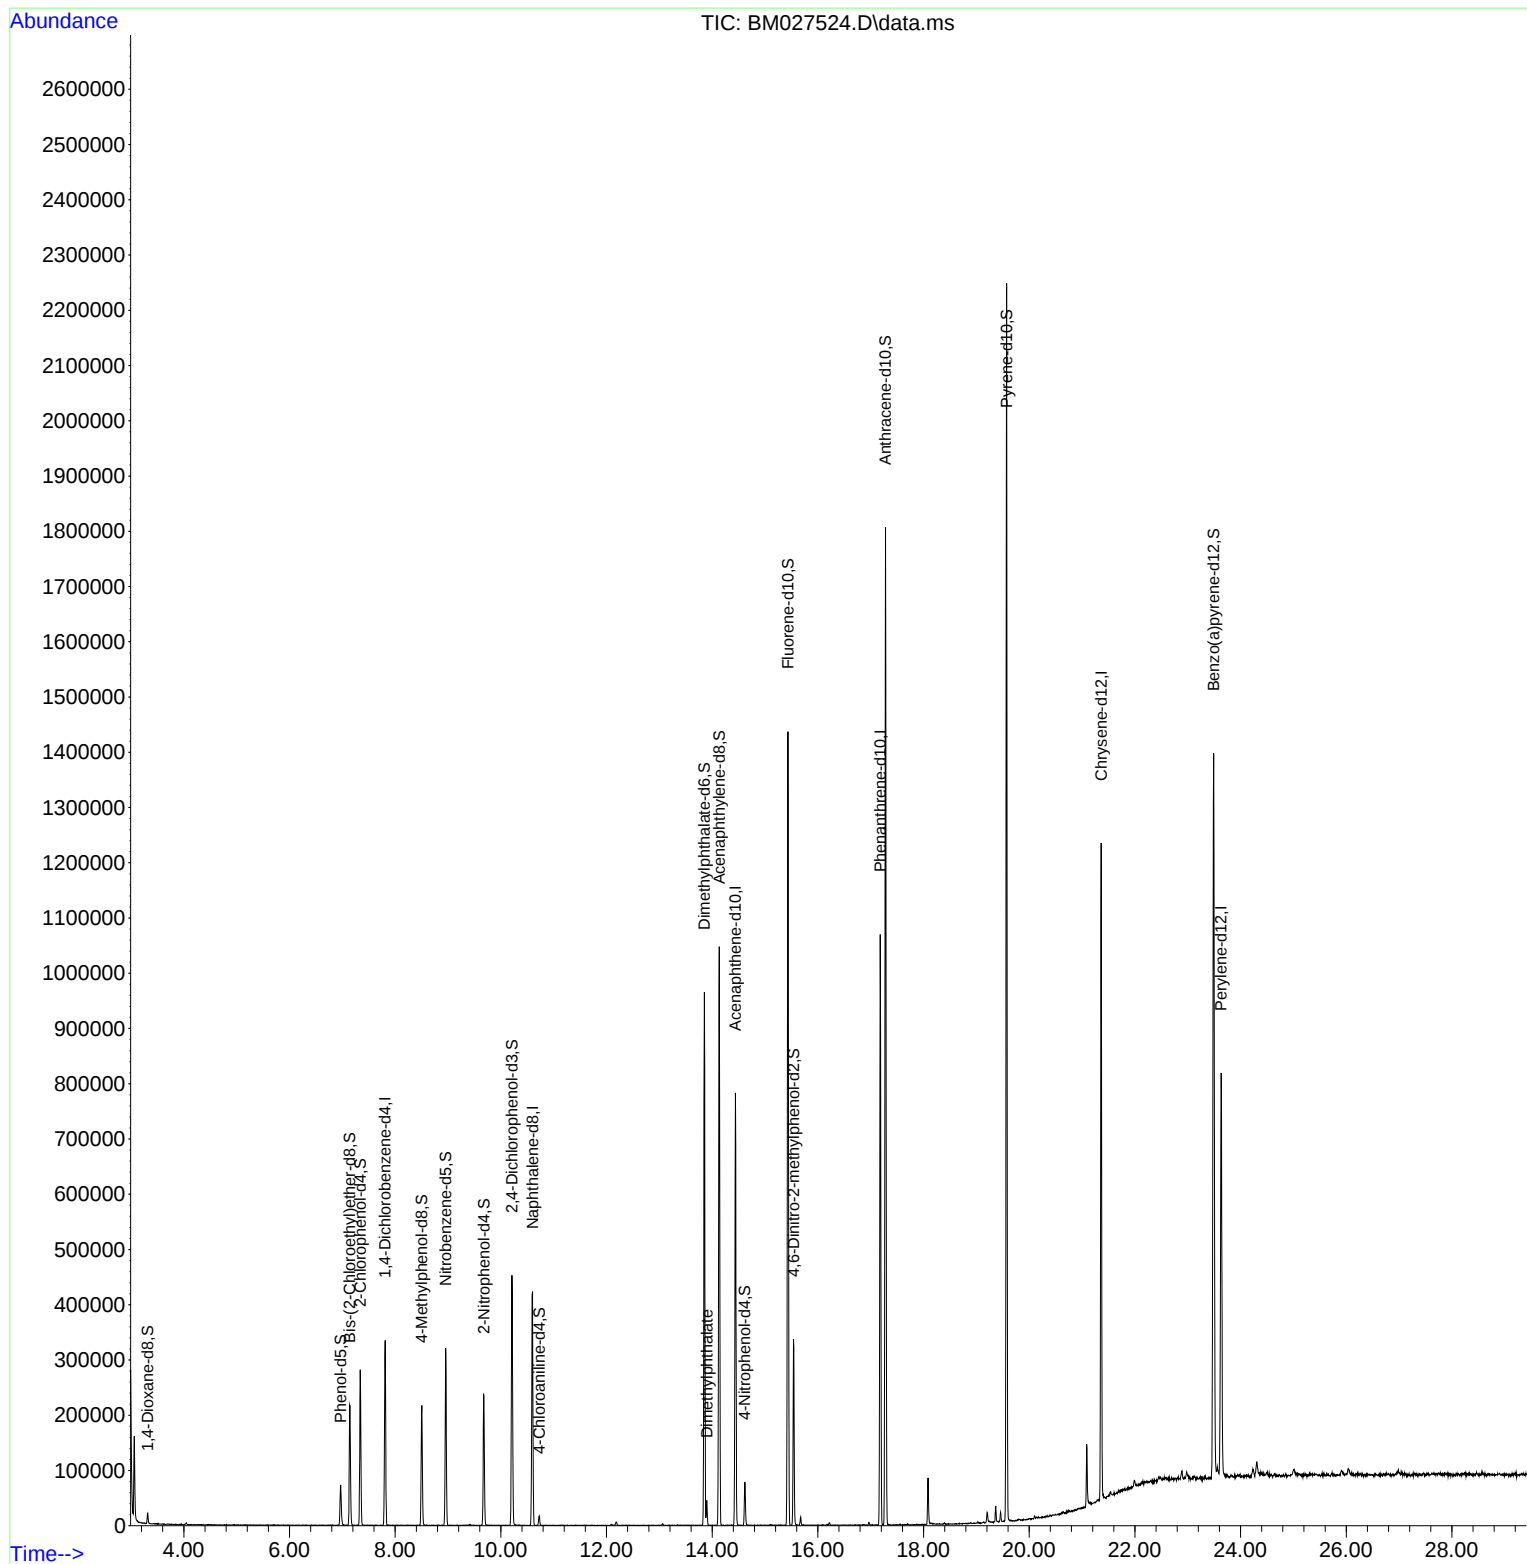

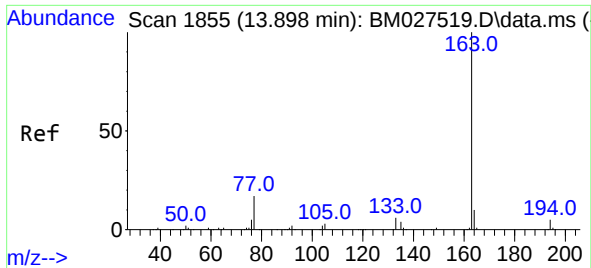

#45  
Dimethylphthalate  
Concen: 1.29 ng/ul  
RT: 13.898 min Scan# 1855  
Delta R.T. -0.006 min  
Lab File: BM027524.D  
Acq: 25 Sep 2020 12:11

Instrument :  
BNA\_M  
ClientSampleId :  
BG478

Tgt Ion:163 Resp: 26515  
Ion Ratio Lower Upper  
163 100  
194 5.2 3.3 4.9#  
164 10.5 8.1 12.1

