

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
 Data File : BM027525.D
 Acq On : 25 Sep 2020 12:48
 Operator : JU/CG
 Sample : L4135-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG482

Quant Time: Sep 25 13:33:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 24 20:21:51 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	84697	20.00	ng/ul	0.00
18) Naphthalene-d8	10.592	136	302018	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.439	164	222170	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.180	188	515493	20.00	ng/ul	# 0.00
78) Chrysene-d12	21.362	240	555368	20.00	ng/ul	# 0.00
86) Perylene-d12	23.633	264	596018	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.316	96	10036	6.74	ng/uL	0.00
5) Phenol-d5	6.969	99	36823	6.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.140	67	94043	28.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.340	132	112254	23.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.504	113	70816	15.30	ng/ul	0.00
19) Nitrobenzene-d5	8.957	128	63717	28.62	ng/ul	0.00
22) 2-Nitrophenol-d4	9.681	143	70064	30.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.210	165	162907	27.38	ng/ul	0.00
29) 4-Chloroaniline-d4	10.722	131	14426	2.45	ng/ul	0.00
44) Dimethylphthalate-d6	13.851	166	570268	33.18	ng/ul	0.00
47) Acenaphthylene-d8	14.133	160	681962	33.12	ng/ul	0.00
52) 4-Nitrophenol-d4	14.621	143	14608	6.07	ng/ul	0.00
58) Fluorene-d10	15.433	176	507195	32.80	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.539	200	83667	29.98	ng/ul	0.00
71) Anthracene-d10	17.280	188	869981	35.78	ng/ul	0.00
79) Pyrene-d10	19.574	212	1030272	35.56	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.491	264	1103631	34.85	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.898	163	25097	1.43	ng/ul	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
Data File : BM027525.D
Acq On : 25 Sep 2020 12:48
Operator : JU/CG
Sample : L4135-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG482

Quant Time: Sep 25 13:33:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 24 20:21:51 2020
Response via : Initial Calibration

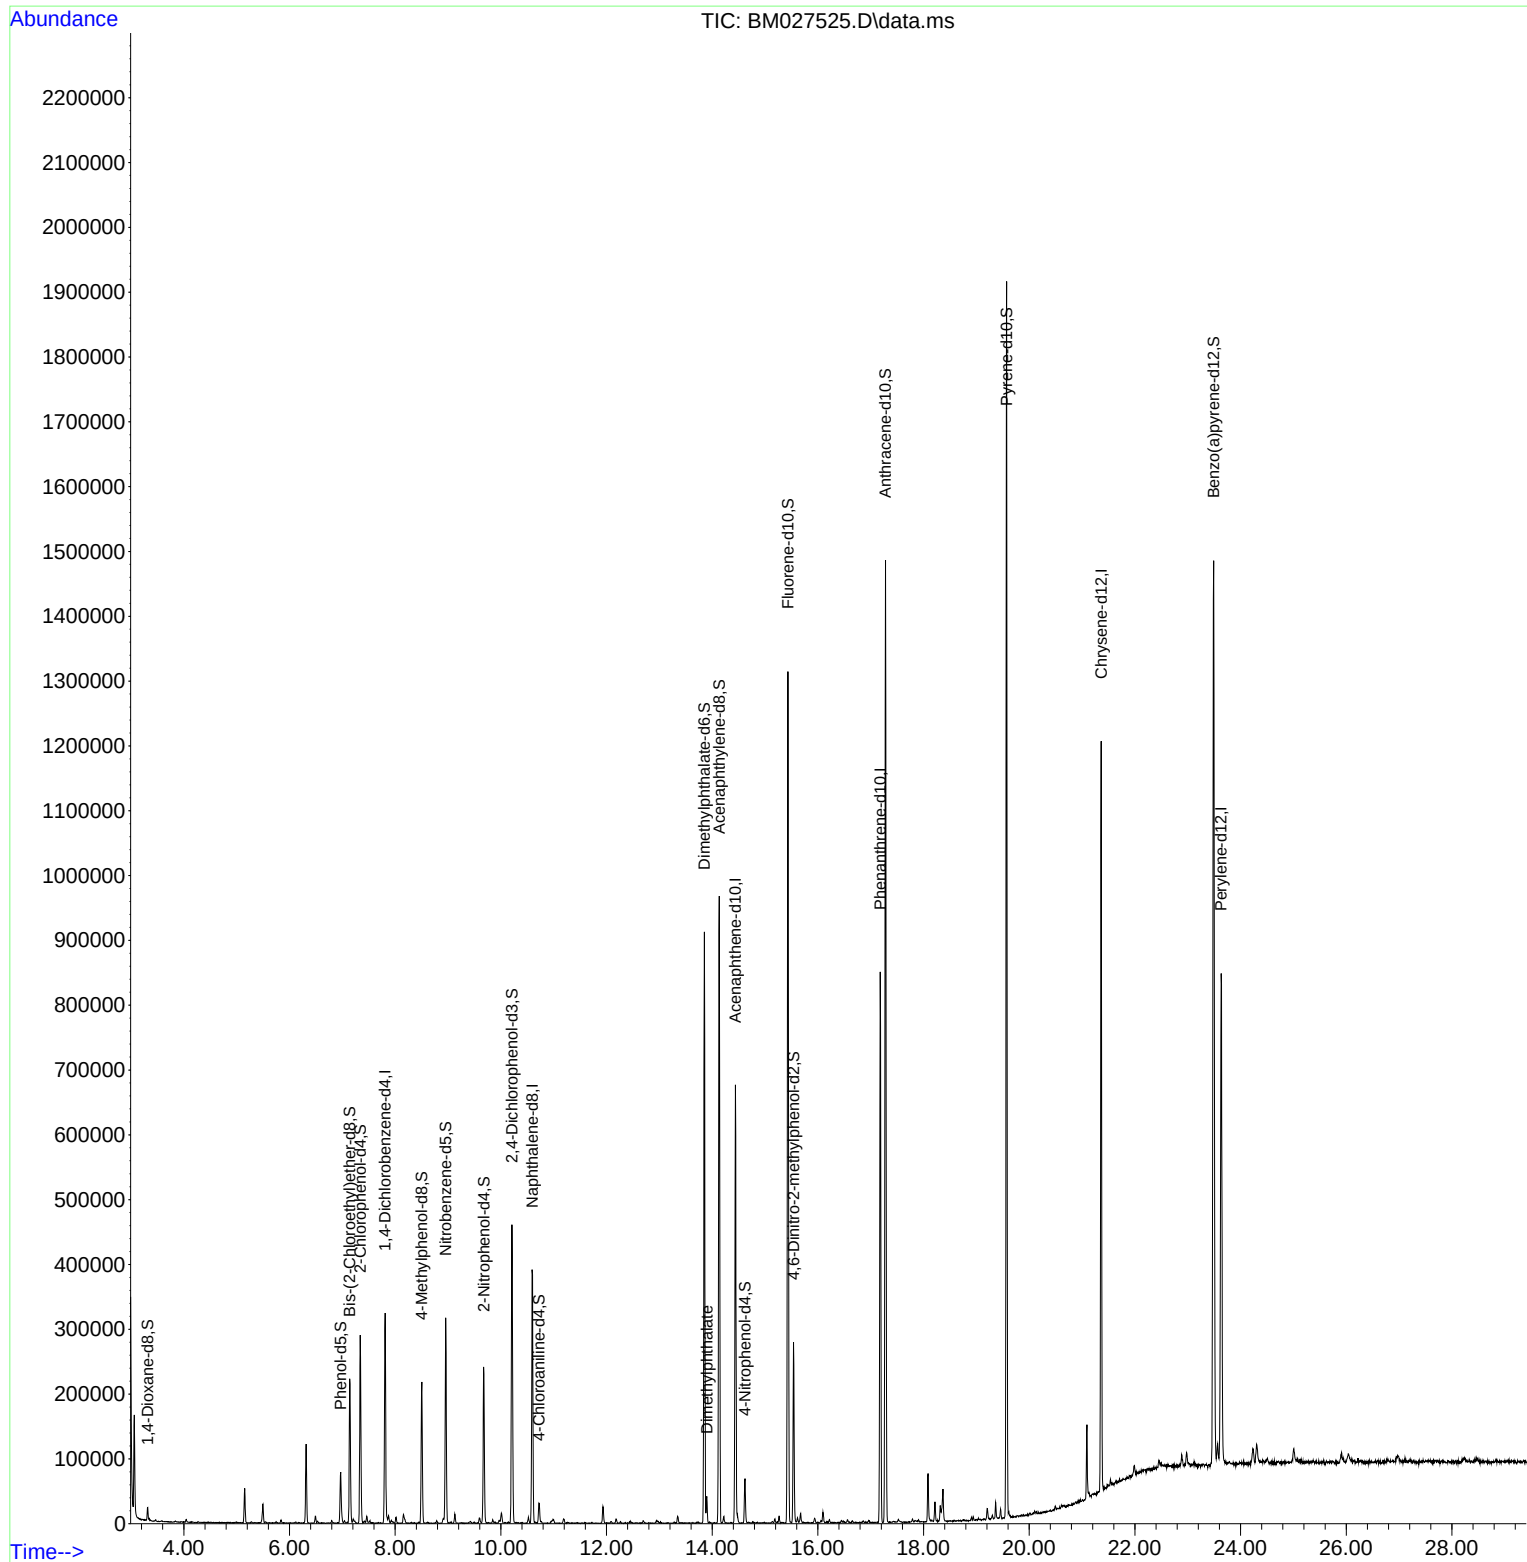

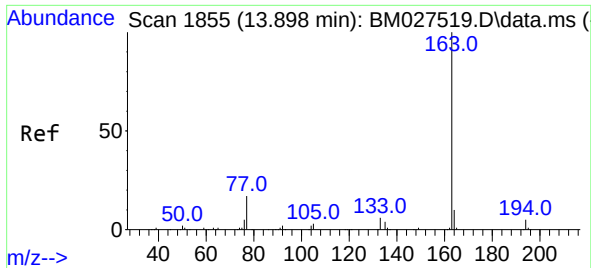

#45
Dimethylphthalate
Concen: 1.43 ng/ul
RT: 13.898 min Scan# 1855
Delta R.T. -0.006 min
Lab File: BM027525.D
Acq: 25 Sep 2020 12:48

Instrument :
BNA_M
ClientSampleId :
BG482

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.8	3.3	4.9
164	12.1	8.1	12.1

