

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
 Data File : BM027527.D
 Acq On : 25 Sep 2020 14:00
 Operator : JU/CG
 Sample : L4135-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG0Q6

Quant Time: Sep 25 14:31:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 24 20:21:51 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	97495	20.00	ng/ul	0.00
18) Naphthalene-d8	10.592	136	357081	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.439	164	279944	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.180	188	638065	20.00	ng/ul	# 0.00
78) Chrysene-d12	21.356	240	603719	20.00	ng/ul	# 0.00
86) Perylene-d12	23.633	264	613415	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	10148	5.92	ng/uL	0.00
5) Phenol-d5	6.969	99	37241	5.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.140	67	92476	24.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.340	132	117925	21.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.504	113	72393	13.58	ng/ul	0.00
19) Nitrobenzene-d5	8.957	128	69013	26.22	ng/ul	0.00
22) 2-Nitrophenol-d4	9.675	143	78506	28.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.210	165	176927	25.15	ng/ul	0.00
29) 4-Chloroaniline-d4	10.722	131	12594	1.81	ng/ul	0.00
44) Dimethylphthalate-d6	13.851	166	625013	28.86	ng/ul	0.00
47) Acenaphthylene-d8	14.133	160	739582	28.51	ng/ul	0.00
52) 4-Nitrophenol-d4	14.622	143	15138	4.99	ng/ul	0.00
58) Fluorene-d10	15.433	176	554553	28.46	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.539	200	90423	26.17	ng/ul	0.00
71) Anthracene-d10	17.280	188	964660	32.05	ng/ul	0.00
79) Pyrene-d10	19.568	212	1078868	34.26	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.486	264	1037800	31.85	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.898	163	29330	1.33	ng/ul#	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
Data File : BM027527.D
Acq On : 25 Sep 2020 14:00
Operator : JU/CG
Sample : L4135-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG0Q6

Quant Time: Sep 25 14:31:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 24 20:21:51 2020
Response via : Initial Calibration

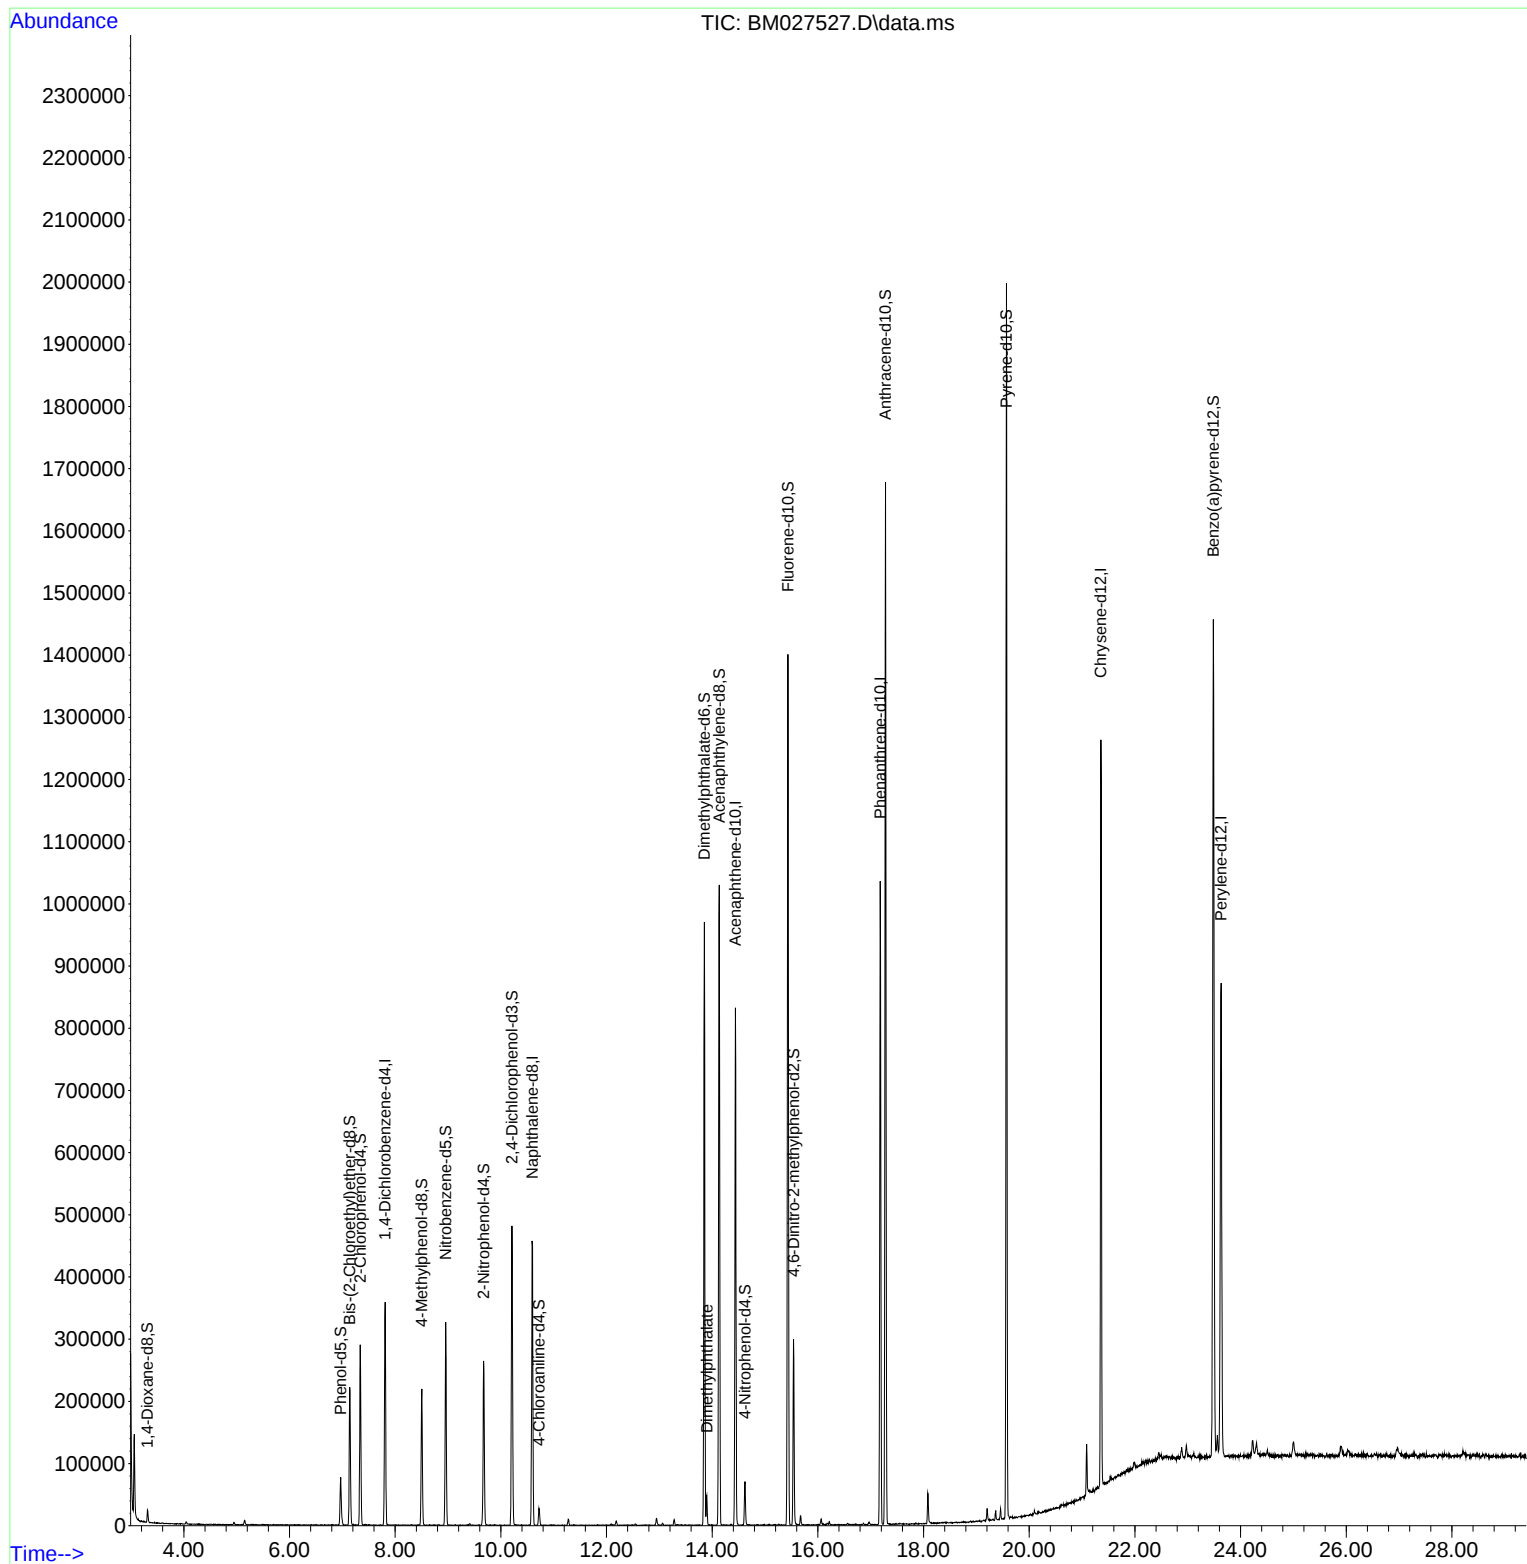

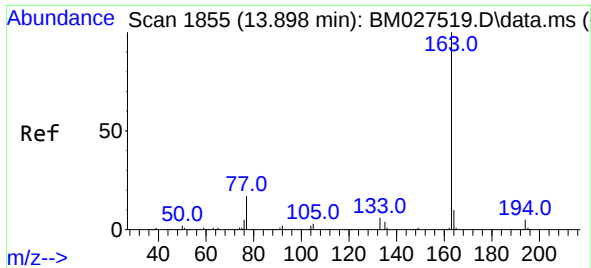

#45
Dimethylphthalate
Concen: 1.33 ng/ul
RT: 13.898 min Scan# 1855
Delta R.T. -0.006 min
Lab File: BM027527.D
Acq: 25 Sep 2020 14:00

Instrument :
BNA_M
ClientSampleId :
BG0Q6

Tgt Ion:	163	Resp:	29330
Ion	Ratio	Lower	Upper
163	100		
194	5.2	3.3	4.9#
164	9.3	8.1	12.1

