

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
 Data File : BM027530.D
 Acq On : 25 Sep 2020 15:49
 Operator : JU/CG
 Sample : L4135-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG484

Quant Time: Sep 25 16:22:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 24 20:21:51 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	99671	20.00	ng/ul	0.00
18) Naphthalene-d8	10.592	136	383609	20.00	ng/ul	# 0.00
36) Acenaphthene-d10	14.439	164	300661	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.180	188	720019	20.00	ng/ul	# 0.00
78) Chrysene-d12	21.362	240	653450	20.00	ng/ul	# 0.00
86) Perylene-d12	23.627	264	631227	20.00	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.310	96	10418	5.95	ng/uL	0.00
5) Phenol-d5	6.969	99	34521	5.31	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.140	67	87958	23.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.340	132	108880	19.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.504	113	68899	12.65	ng/ul	0.00
19) Nitrobenzene-d5	8.957	128	65511	23.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.675	143	76898	25.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.210	165	168777	22.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.722	131	8425	1.12	ng/ul	0.00
44) Dimethylphthalate-d6	13.851	166	604455	25.98	ng/ul	0.00
47) Acenaphthylene-d8	14.133	160	718645	25.79	ng/ul	0.00
52) 4-Nitrophenol-d4	14.621	143	15010	4.61	ng/ul	0.00
58) Fluorene-d10	15.433	176	552654	26.41	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.539	200	88763	22.77	ng/ul	0.00
71) Anthracene-d10	17.280	188	961250	28.30	ng/ul	0.00
79) Pyrene-d10	19.568	212	1064573	31.23	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.486	264	941370	28.07	ng/ul	0.00
Target Compounds						Qvalue
45) Dimethylphthalate	13.898	163	27945	1.18	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
Data File : BM027530.D
Acq On : 25 Sep 2020 15:49
Operator : JU/CG
Sample : L4135-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG484

Quant Time: Sep 25 16:22:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 24 20:21:51 2020
Response via : Initial Calibration

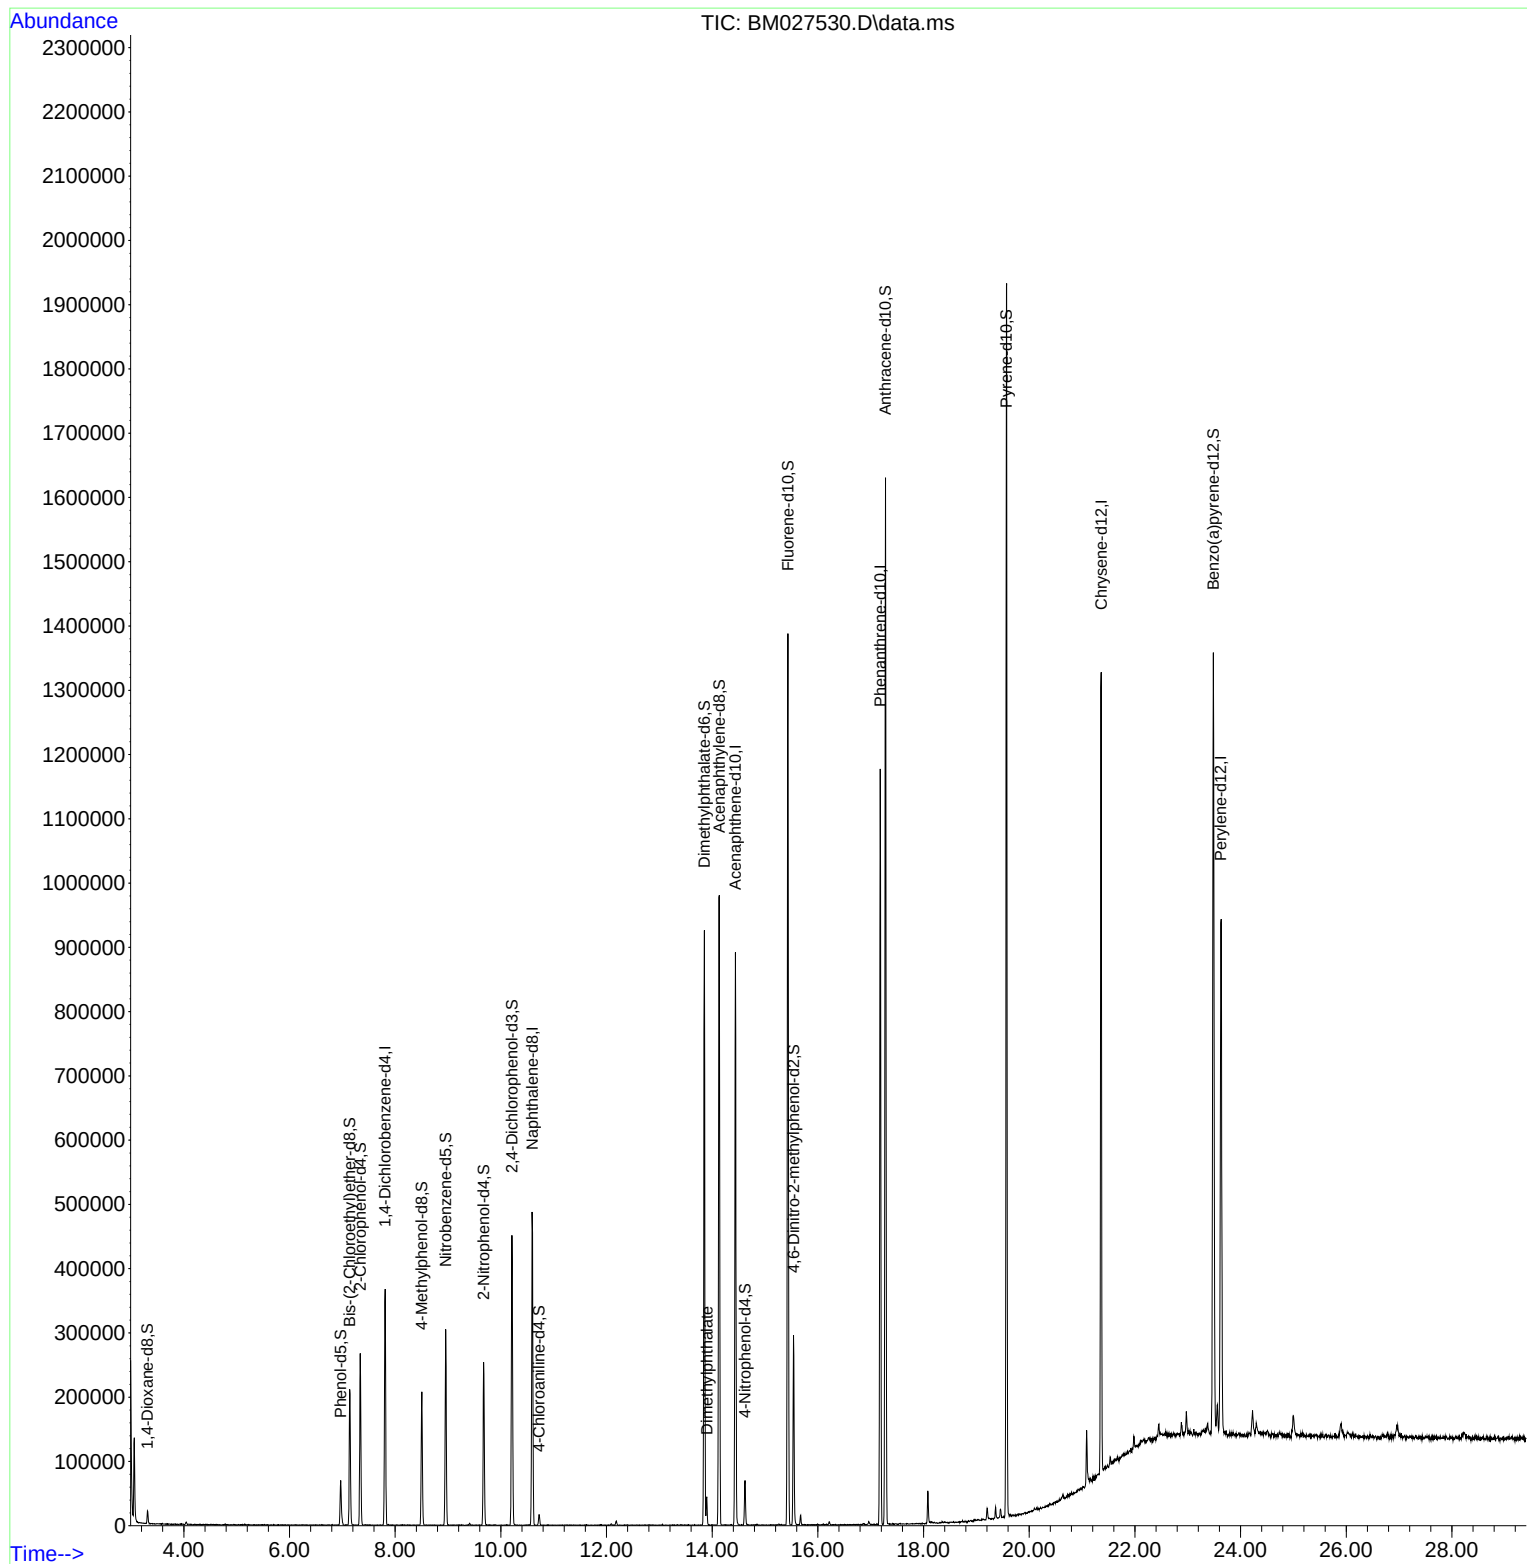

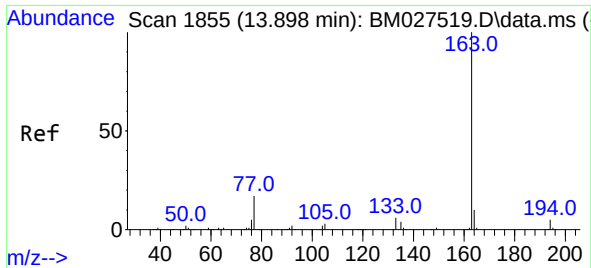

#45
 Dimethylphthalate
 Concen: 1.18 ng/ul
 RT: 13.898 min Scan# 1855
 Delta R.T. -0.006 min
 Lab File: BM027530.D
 Acq: 25 Sep 2020 15:49

Instrument :
 BNA_M
 ClientSampleId :
 BG484

Tgt Ion:	163	Resp:	27945
Ion	Ratio	Lower	Upper
163	100		
194	4.4	3.3	4.9
164	8.2	8.1	12.1

