

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
 Data File : BM027535.D
 Acq On : 25 Sep 2020 18:52
 Operator : JU/CG
 Sample : L4135-14
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG486

Quant Time: Sep 26 00:58:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 24 20:21:51 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	102087	20.00	ng/ul	# 0.00
18) Naphthalene-d8	10.592	136	360774	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.439	164	259738	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.180	188	625518	20.00	ng/ul	# 0.00
78) Chrysene-d12	21.356	240	689889	20.00	ng/ul	# 0.00
86) Perylene-d12	23.627	264	752717	20.00	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.316	96	11650	6.49	ng/uL	0.00
5) Phenol-d5	6.969	99	40370	6.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.140	67	101438	25.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.340	132	128773	22.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.504	113	80061	14.35	ng/ul	0.00
19) Nitrobenzene-d5	8.957	128	75091	28.24	ng/ul	0.00
22) 2-Nitrophenol-d4	9.675	143	84226	30.23	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.210	165	189498	26.66	ng/ul	0.00
29) 4-Chloroaniline-d4	10.728	131	8566	1.22	ng/ul	0.00
44) Dimethylphthalate-d6	13.851	166	672908	33.48	ng/ul	0.00
47) Acenaphthylene-d8	14.127	160	773764	32.15	ng/ul	0.00
52) 4-Nitrophenol-d4	14.621	143	18110	6.43	ng/ul	0.00
58) Fluorene-d10	15.433	176	590582	32.67	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.539	200	102600	30.29	ng/ul	0.00
71) Anthracene-d10	17.280	188	1034772	35.07	ng/ul	0.00
79) Pyrene-d10	19.568	212	1253837	34.84	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.486	264	1395980	34.91	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.898	163	26864	1.31	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
Data File : BM027535.D
Acq On : 25 Sep 2020 18:52
Operator : JU/CG
Sample : L4135-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG486

Quant Time: Sep 26 00:58:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 24 20:21:51 2020
Response via : Initial Calibration

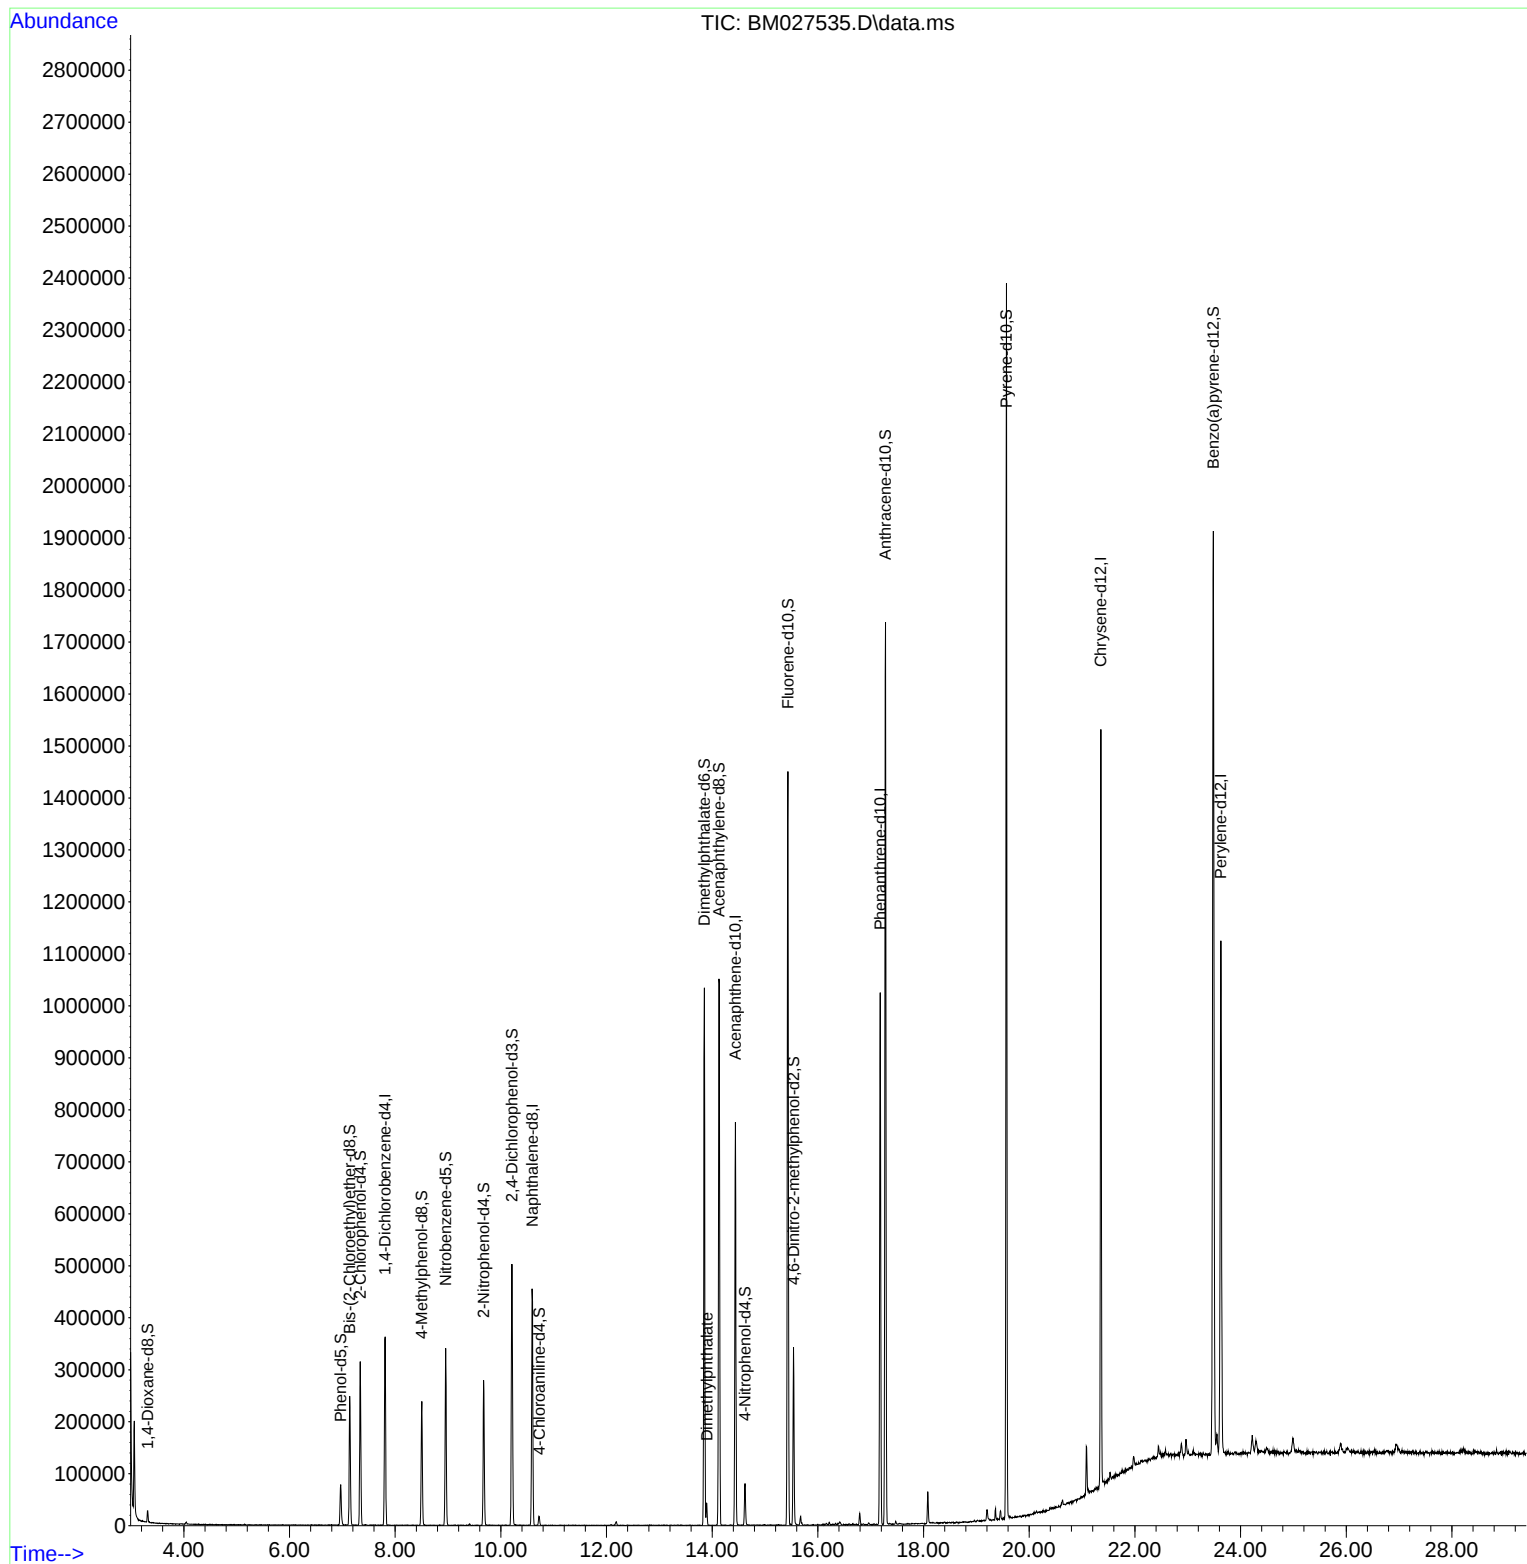

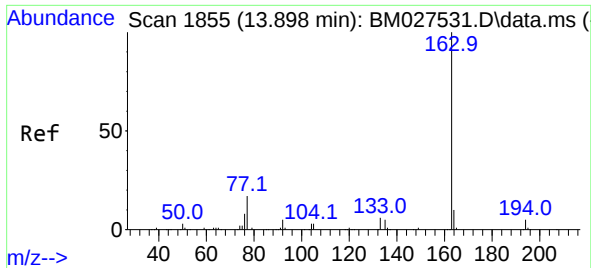

#45
 Dimethylphthalate
 Concen: 1.31 ng/ul
 RT: 13.898 min Scan# 1855
 Delta R.T. -0.006 min
 Lab File: BM027535.D
 Acq: 25 Sep 2020 18:52

Instrument :
 BNA_M
 ClientSampleId :
 BG486

Tgt Ion:163	Resp:	26864
Ion	Ratio	Lower Upper
163	100	
194	4.8	3.3 4.9
164	9.4	8.1 12.1

