

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
 Data File : BM027542.D
 Acq On : 25 Sep 2020 23:06
 Operator : JU/CG
 Sample : L4135-19
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG497

Quant Time: Sep 26 01:01:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 24 20:21:51 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	94165	20.00	ng/ul	0.00
18) Naphthalene-d8	10.592	136	368593	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.439	164	296608	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.180	188	737848	20.00	ng/ul	# 0.00
78) Chrysene-d12	21.356	240	716699	20.00	ng/ul	# 0.00
86) Perylene-d12	23.621	264	623591	20.00	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.316	96	8817	5.33	ng/uL	0.00
5) Phenol-d5	6.969	99	56353	9.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.140	67	111326	30.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.340	132	150830	28.39	ng/ul	0.00
13) 4-Methylphenol-d8	8.504	113	109316	21.24	ng/ul	0.00
19) Nitrobenzene-d5	8.957	128	88656	32.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.675	143	107502	37.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.210	165	248779	34.25	ng/ul	0.00
29) 4-Chloroaniline-d4	10.722	131	11863	1.65	ng/ul	0.00
44) Dimethylphthalate-d6	13.851	166	958036	41.75	ng/ul	0.00
47) Acenaphthylene-d8	14.127	160	1045245	38.03	ng/ul	0.00
52) 4-Nitrophenol-d4	14.622	143	31686	9.85	ng/ul	0.00
58) Fluorene-d10	15.427	176	801962	38.85	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.539	200	155199	38.85	ng/ul	0.00
71) Anthracene-d10	17.280	188	1424735	40.93	ng/ul	0.00
79) Pyrene-d10	19.568	212	1694210	45.32	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.480	264	1377708	41.59	ng/ul	-0.01
Target Compounds						
6) Phenol	6.993	94	10889	1.72	ng/ul	91
45) Dimethylphthalate	13.898	163	45655	1.95	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
Data File : BM027542.D
Acq On : 25 Sep 2020 23:06
Operator : JU/CG
Sample : L4135-19
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG497

Quant Time: Sep 26 01:01:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 24 20:21:51 2020
Response via : Initial Calibration

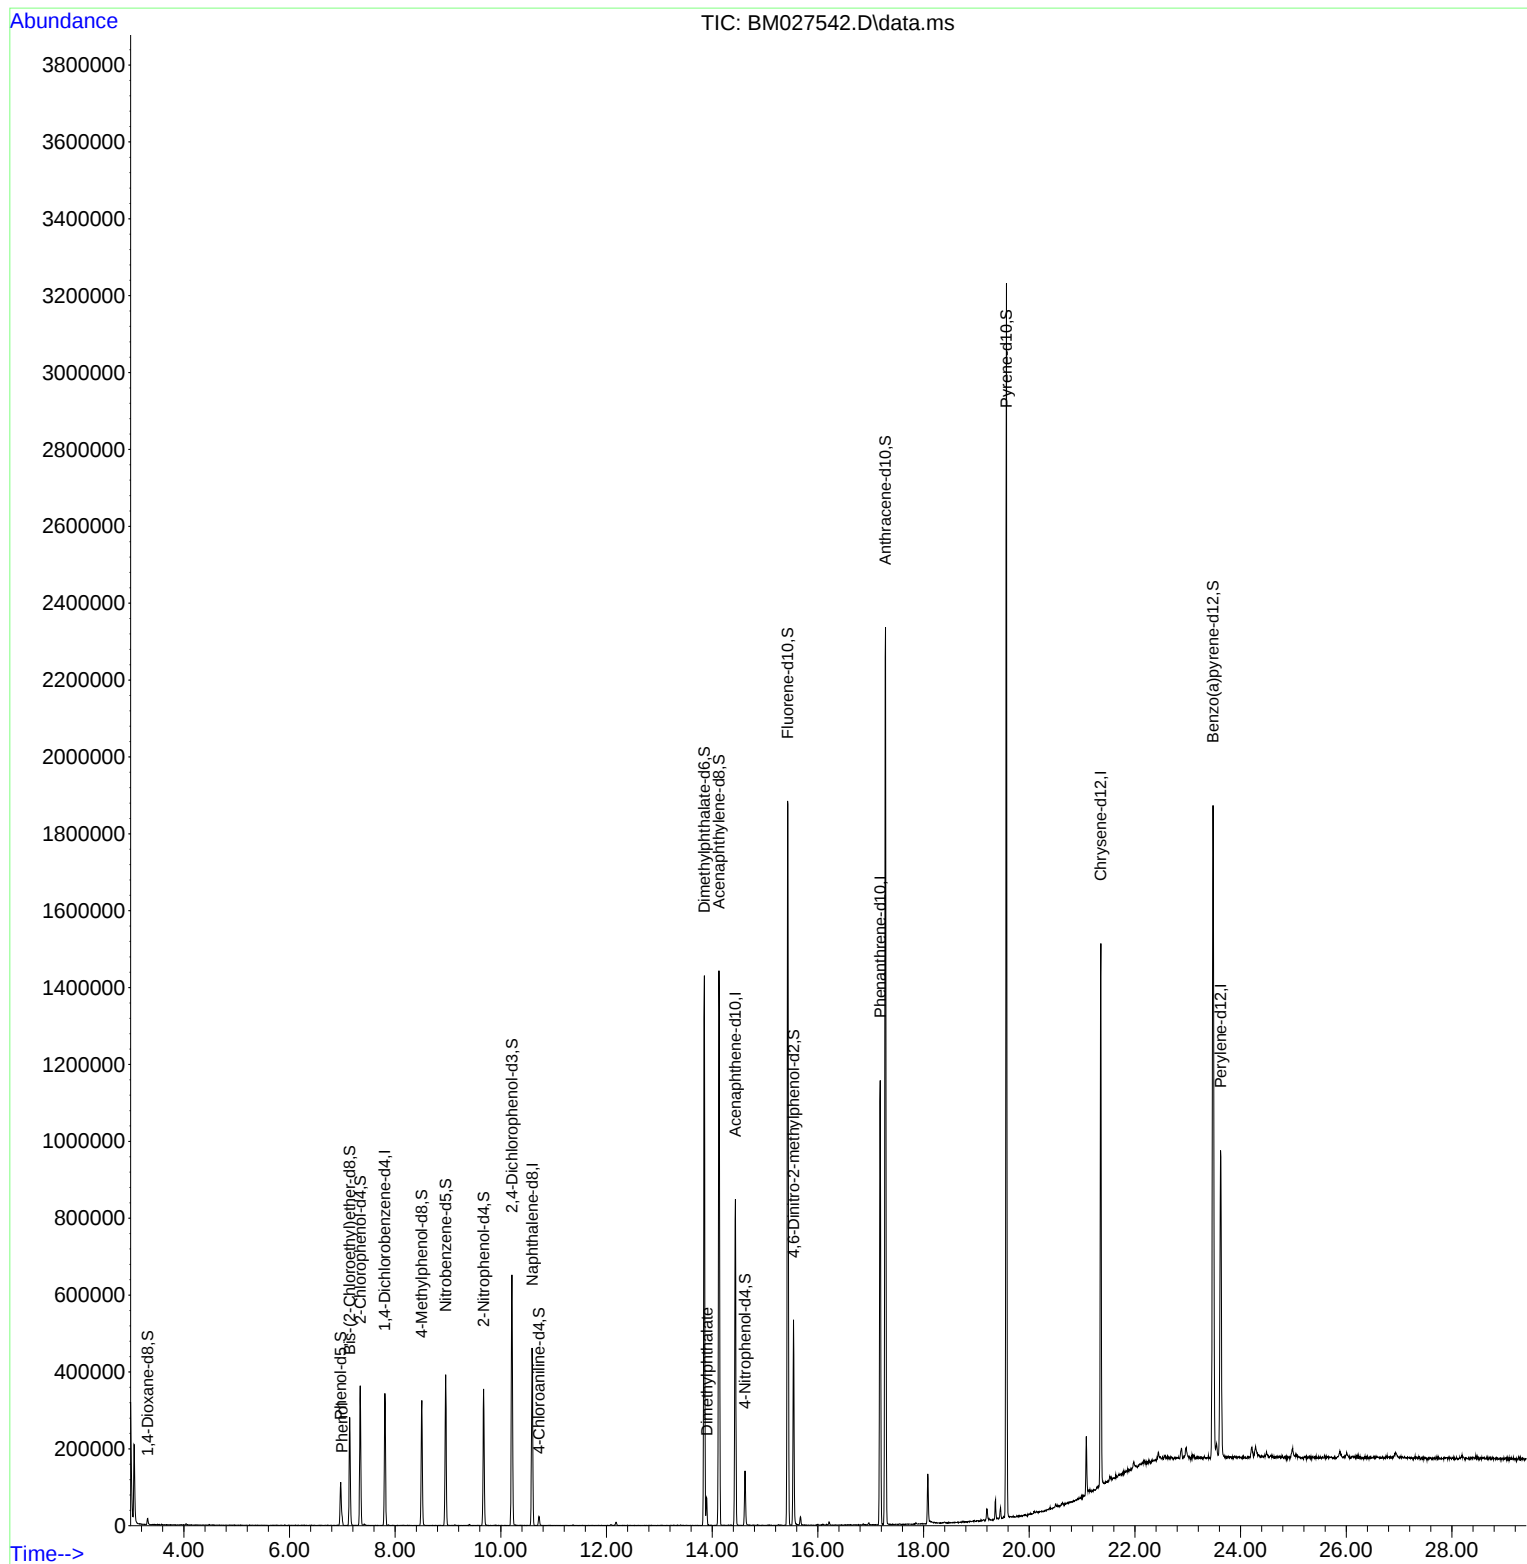




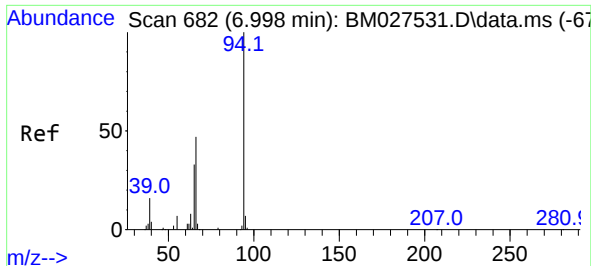


#6
Phenol
Concen: 1.72 ng/ul
RT: 6.993 min Scan# 681
Delta R.T. -0.006 min
Lab File: BM027542.D
Acq: 25 Sep 2020 23:06

Instrument :
BNA_M
ClientSampleId :
BG497

Tgt Ion: 94 Resp: 10889

Ion	Ratio	Lower	Upper
94	100		
65	32.7	30.2	45.4
66	46.5	42.4	63.6

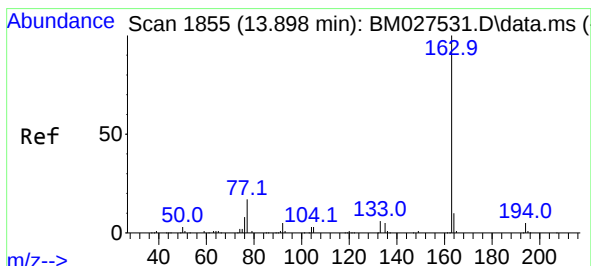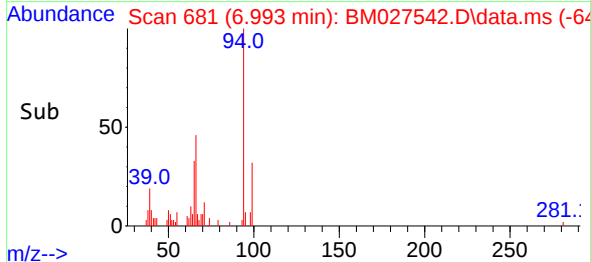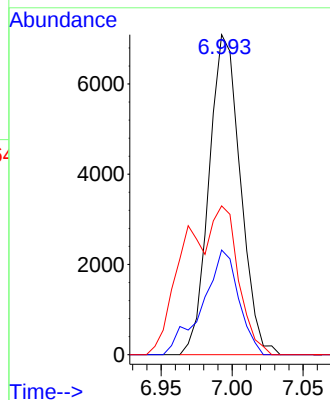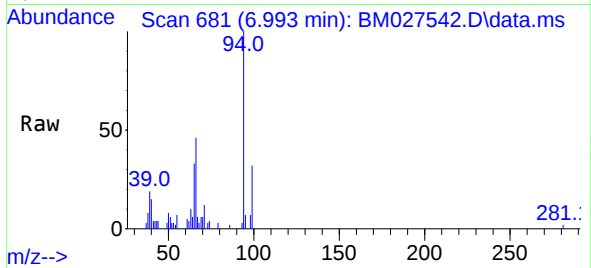

#45
Dimethylphthalate
Concen: 1.95 ng/ul
RT: 13.898 min Scan# 1855
Delta R.T. -0.006 min
Lab File: BM027542.D
Acq: 25 Sep 2020 23:06

Tgt Ion: 163 Resp: 45655

Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.3	4.9
164	9.7	8.1	12.1

