

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
 Data File : BM027521.D
 Acq On : 25 Sep 2020 10:23
 Operator : JU/CG
 Sample : PB131882BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM027521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.063	9	13	19	rVB	20831	24925	0.97%	0.103%
2	3.316	49	56	62	rVB	21575	28153	1.10%	0.117%
3	4.046	176	180	184	rVB2	3526	4277	0.17%	0.018%
4	4.257	213	216	220	rVB2	8631	11086	0.43%	0.046%
5	4.657	280	284	288	rBV4	5449	7289	0.28%	0.030%
6	6.969	670	677	684	rBV	363740	546771	21.31%	2.267%
7	7.145	700	707	716	rVB	266585	402788	15.70%	1.670%
8	7.345	733	741	748	rBV	378826	595850	23.22%	2.471%
9	7.810	813	820	828	rVB	312144	478231	18.64%	1.983%
10	8.504	932	938	948	rBV	449866	701524	27.34%	2.909%
11	8.957	1008	1015	1023	rBV	351856	561832	21.90%	2.330%
12	9.681	1131	1138	1148	rVB	282785	444271	17.32%	1.842%
13	10.216	1222	1229	1239	rBV	542859	858694	33.47%	3.560%
14	10.598	1286	1294	1301	rVB	413713	660412	25.74%	2.738%
15	10.728	1308	1316	1324	rBV	495192	796727	31.05%	3.304%
16	12.186	1558	1564	1569	rVB2	7777	12132	0.47%	0.050%
17	13.851	1841	1847	1856	rBV	1003463	1401318	54.62%	5.810%
18	14.133	1888	1895	1903	rVB	1134995	1624196	63.30%	6.734%
19	14.445	1941	1948	1955	rBV	725888	1065651	41.53%	4.419%
20	14.621	1972	1978	1994	rBV	383347	548734	21.39%	2.275%
21	15.433	2110	2116	2123	rBV	1444292	2042007	79.59%	8.467%
22	15.545	2129	2135	2142	rBV	291492	390987	15.24%	1.621%
23	15.674	2152	2157	2161	rBV	17752	20598	0.80%	0.085%
24	16.221	2243	2250	2253	rBV2	5355	6880	0.27%	0.029%
25	16.968	2372	2377	2380	rBV2	2903	3734	0.15%	0.015%
26	17.180	2407	2413	2420	rBV	902539	1288937	50.24%	5.344%
27	17.280	2424	2430	2439	rVV	1584008	2249945	87.69%	9.329%
28	19.203	2753	2757	2761	rBV2	14258	18385	0.72%	0.076%
29	19.456	2796	2800	2805	rVB	12154	16193	0.63%	0.067%
30	19.574	2814	2820	2827	rVB	1929464	2565797	100.00%	10.639%
31	20.392	2957	2959	2960	rBV2	3799	3255	0.13%	0.013%
32	21.362	3119	3124	3131	rBV	1100530	1324821	51.63%	5.493%
33	23.491	3479	3486	3495	rBV	1244036	2178702	84.91%	9.034%
34	23.633	3504	3510	3523	rVB2	638365	1232501	48.04%	5.110%

Sum of corrected areas: 24117603

Instrument :

BNA_M

ClientSampleId :




SBLK82

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
Data File : BM027521.D
Acq On : 25 Sep 2020 10:23
Operator : JU/CG
Sample : PB131882BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK82

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

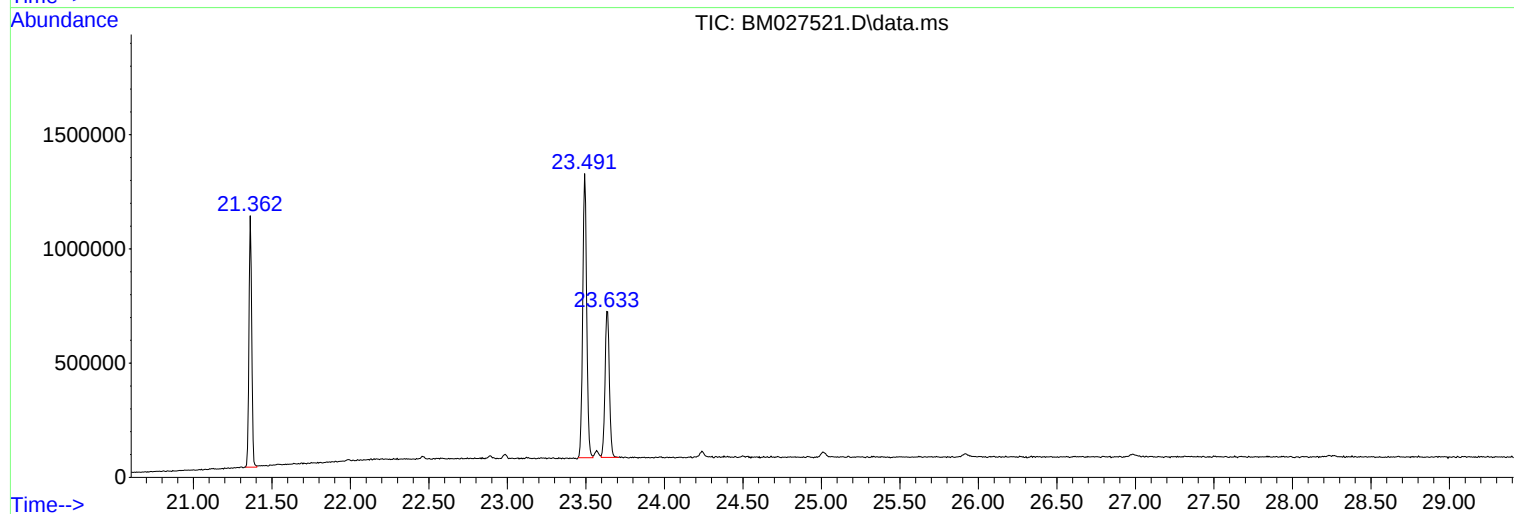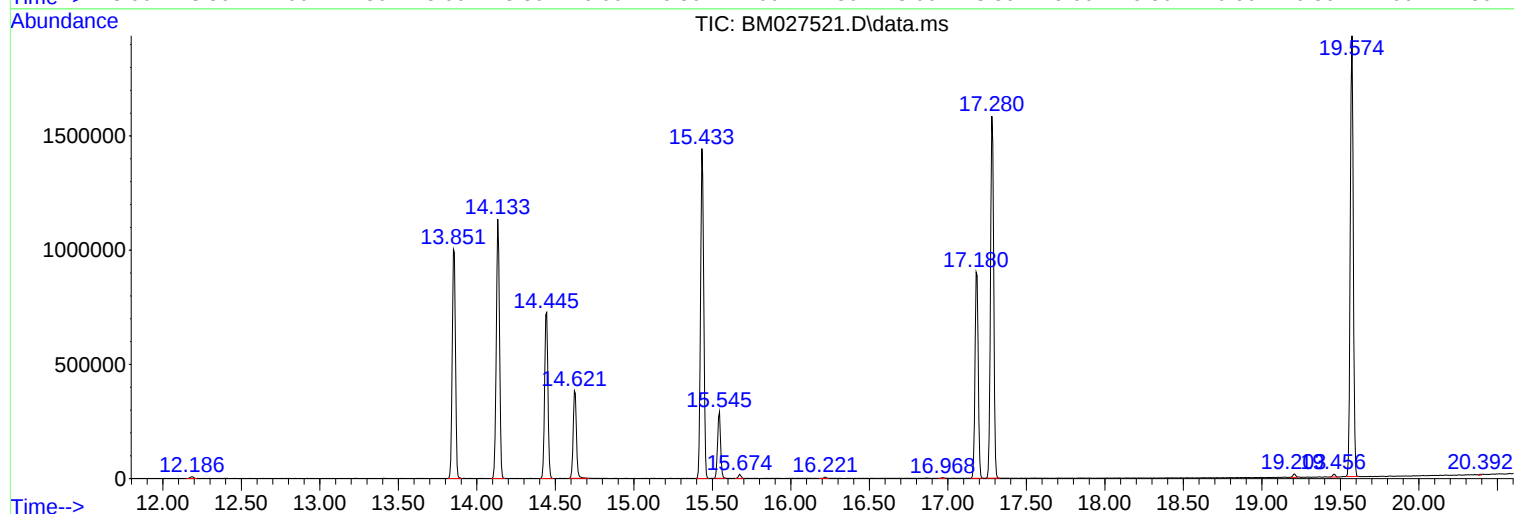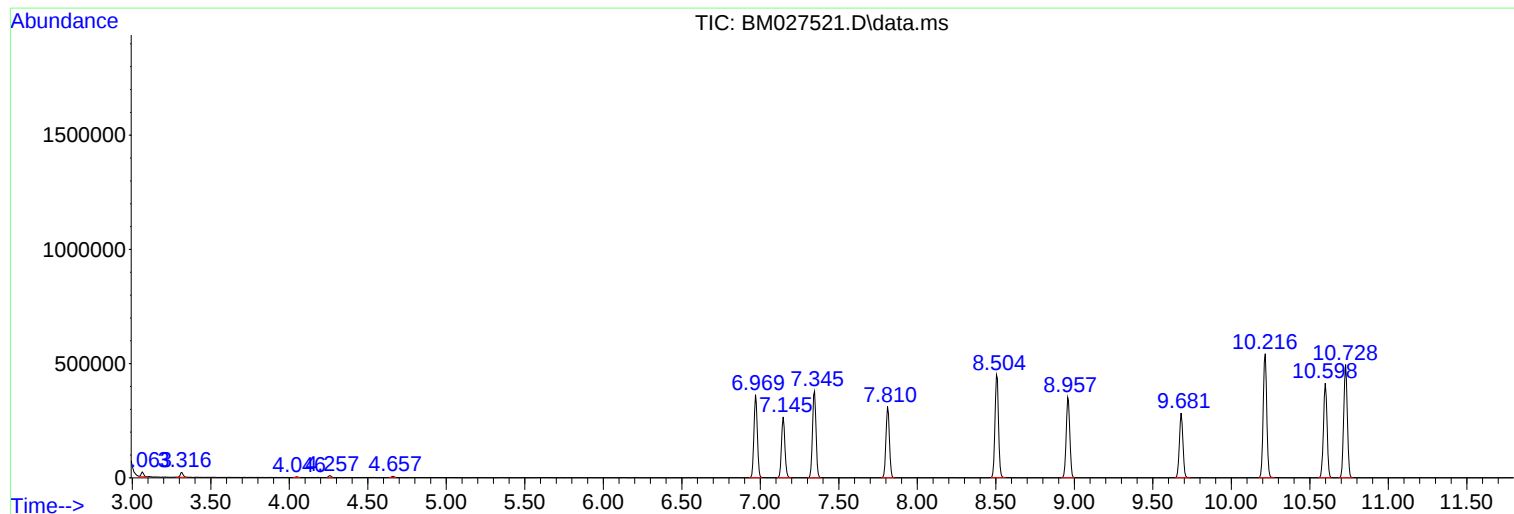

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
Data File : BM027521.D
Acq On : 25 Sep 2020 10:23
Operator : JU/CG
Sample : PB131882BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK82

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092520\
Data File : BM027521.D
Acq On : 25 Sep 2020 10:23
Operator : JU/CG
Sample : PB131882BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK82

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
