

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032148.D
 Acq On : 25 Sep 2021 11:32
 Operator : CG/JU
 Sample : M3919-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Y2

Quant Time: Sep 26 00:19:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 25 01:15:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.666	152	359048	20.000	ng/u1	0.00
20) Naphthalene-d8	10.460	136	1502617	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.312	164	964830	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.036	188	1997307	20.000	ng/u1	0.00
79) Chrysene-d12	21.200	240	1850654	20.000	ng/u1	0.00
88) Perylene-d12	23.371	264	1695865	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.990	96	46905	5.516	ng/uL	0.00
4) Pyridine-d5	3.413	84	302757	12.542	ng/u1	0.00
7) Phenol-d5	6.848	99	241127	8.460	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.989	67	576629	33.648	ng/u1	0.00
11) 2-Chlorophenol-d4	7.201	132	613228	27.715	ng/u1	0.00
15) 4-Methylphenol-d8	8.389	113	426770	19.150	ng/u1	0.00
21) Nitrobenzene-d5	8.819	128	345148	38.457	ng/u1	0.00
24) 2-Nitrophenol-d4	9.548	143	358596	37.787	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.089	165	674989	31.114	ng/u1	0.00
31) 4-Chloroaniline-d4	10.589	131	905756	30.891	ng/u1	0.00
46) Dimethylphthalate-d6	13.712	166	2372310	37.844	ng/u1	0.00
49) Acenaphthylene-d8	14.001	160	2843836	35.707	ng/u1	0.00
54) 4-Nitrophenol-d4	14.507	143	67941	6.662	ng/u1	0.00
60) Fluorene-d10	15.301	176	2020657	37.776	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.412	200	270850	28.694	ng/u1	0.00
73) Anthracene-d10	17.136	188	3235760	38.827	ng/u1	0.00
81) Pyrene-d10	19.424	212	3662007	37.609	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.235	264	3025948	38.020	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.025	88	117502	12.577	ng/uL 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032148.D
Acq On : 25 Sep 2021 11:32
Operator : CG/JU
Sample : M3919-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Y2

Quant Time: Sep 26 00:19:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 25 01:15:33 2021
Response via : Initial Calibration



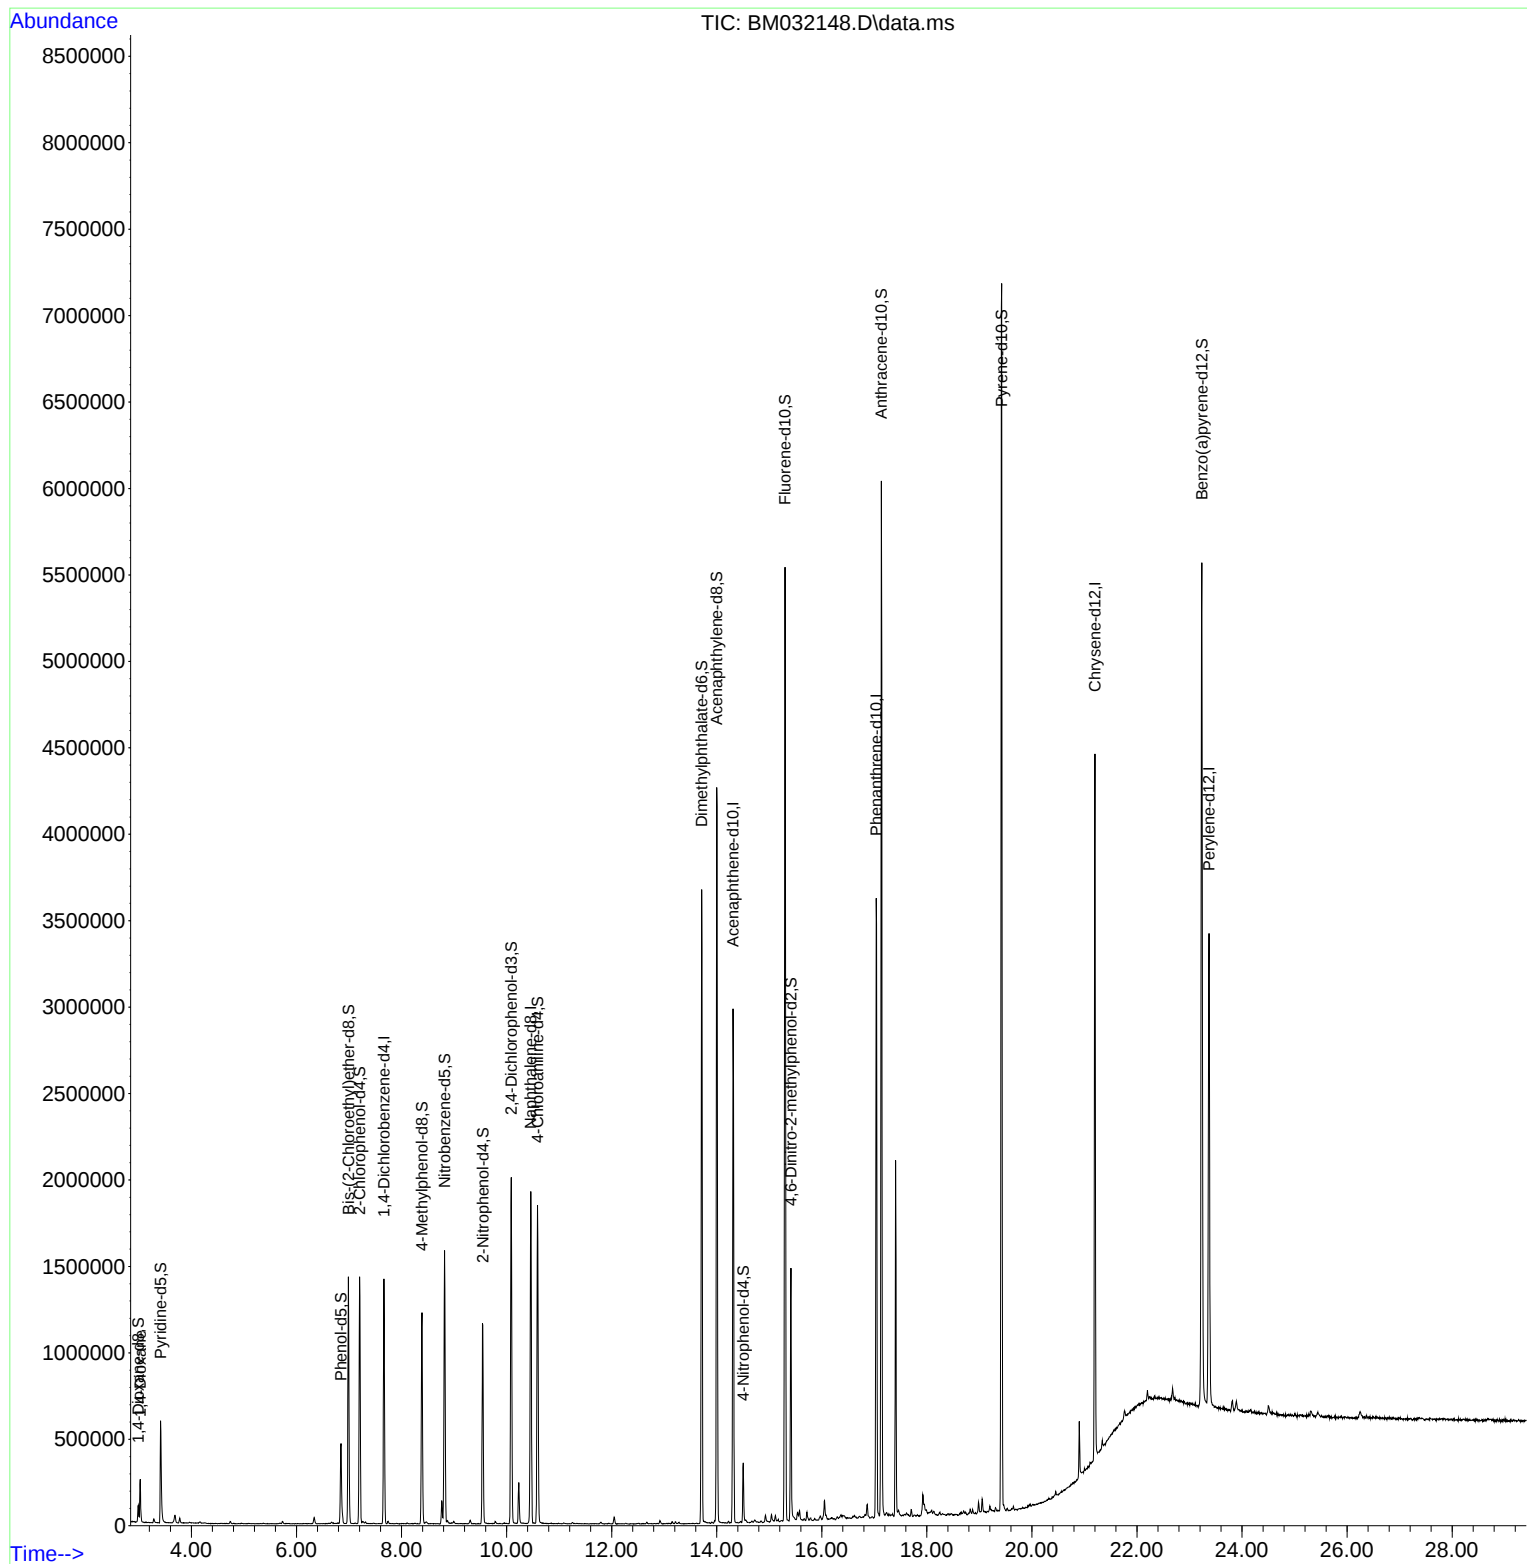


Abundance Scan 32 (3.025 min): BM032145.D\data.ms (-27) #2

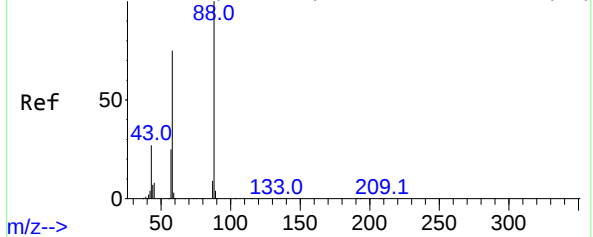

1,4-Dioxane
Concen: 12.577 ng/uL
RT: 3.025 min Scan# 32
Delta R.T. -0.000 min
Lab File: BM032148.D
Acq: 25 Sep 2021 11:32

Tgt Ion:	88	Resp:	117502
Ion	Ratio	Lower	Upper
88	100		
43	27.4	22.3	33.5
58	74.8	62.4	93.6

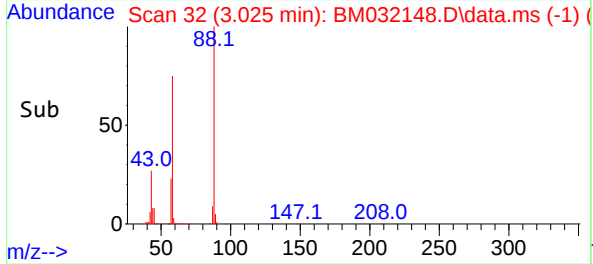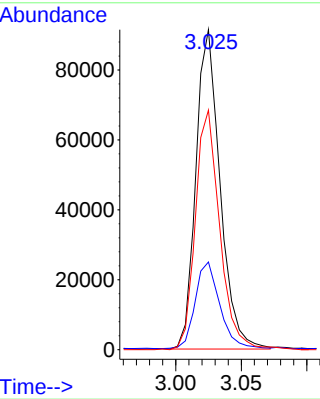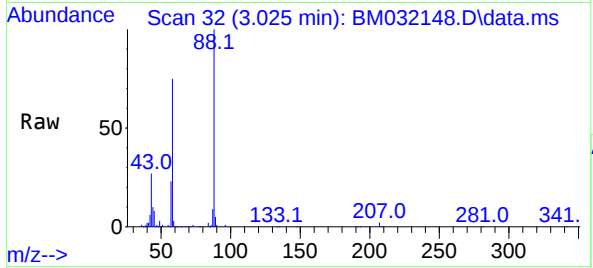

Instrument :
BNA_M
ClientSampleId :
GB6Y2