

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032159.D
 Acq On : 25 Sep 2021 18:11
 Operator : CG/JU
 Sample : M3919-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Z4

Quant Time: Sep 26 00:22:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 25 01:15:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.666	152	318645	20.000	ng/u1	0.00
20) Naphthalene-d8	10.460	136	1337719	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.313	164	859261	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.036	188	1803450	20.000	ng/u1	0.00
79) Chrysene-d12	21.195	240	1849686	20.000	ng/u1	0.00
88) Perylene-d12	23.365	264	1896826	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.984	96	48419	6.416	ng/uL	0.00
4) Pyridine-d5	3.413	84	305545	14.262	ng/u1	0.00
7) Phenol-d5	6.848	99	224923	8.893	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.990	67	584345	38.422	ng/u1	0.00
11) 2-Chlorophenol-d4	7.201	132	619034	31.524	ng/u1	0.00
15) 4-Methylphenol-d8	8.390	113	413671	20.916	ng/u1	0.00
21) Nitrobenzene-d5	8.819	128	368230	46.087	ng/u1	0.00
24) 2-Nitrophenol-d4	9.542	143	383835	45.432	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.089	165	693296	35.897	ng/u1	0.00
31) 4-Chloroaniline-d4	10.589	131	950630	36.418	ng/u1	0.00
46) Dimethylphthalate-d6	13.713	166	2435093	43.618	ng/u1	0.00
49) Acenaphthylene-d8	14.001	160	2903776	40.939	ng/u1	0.00
54) 4-Nitrophenol-d4	14.507	143	73336	8.075	ng/u1	0.00
60) Fluorene-d10	15.301	176	2056385	43.168	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.413	200	303473	35.607	ng/u1	0.00
73) Anthracene-d10	17.136	188	3338598	44.367	ng/u1	0.00
81) Pyrene-d10	19.418	212	3845609	39.515	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.230	264	3786365	42.535	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.019	88	179751	21.679	ng/uL	97
8) Phenol	6.872	94	34660	1.352	ng/u1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032159.D
Acq On : 25 Sep 2021 18:11
Operator : CG/JU
Sample : M3919-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Z4

Quant Time: Sep 26 00:22:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 25 01:15:33 2021
Response via : Initial Calibration




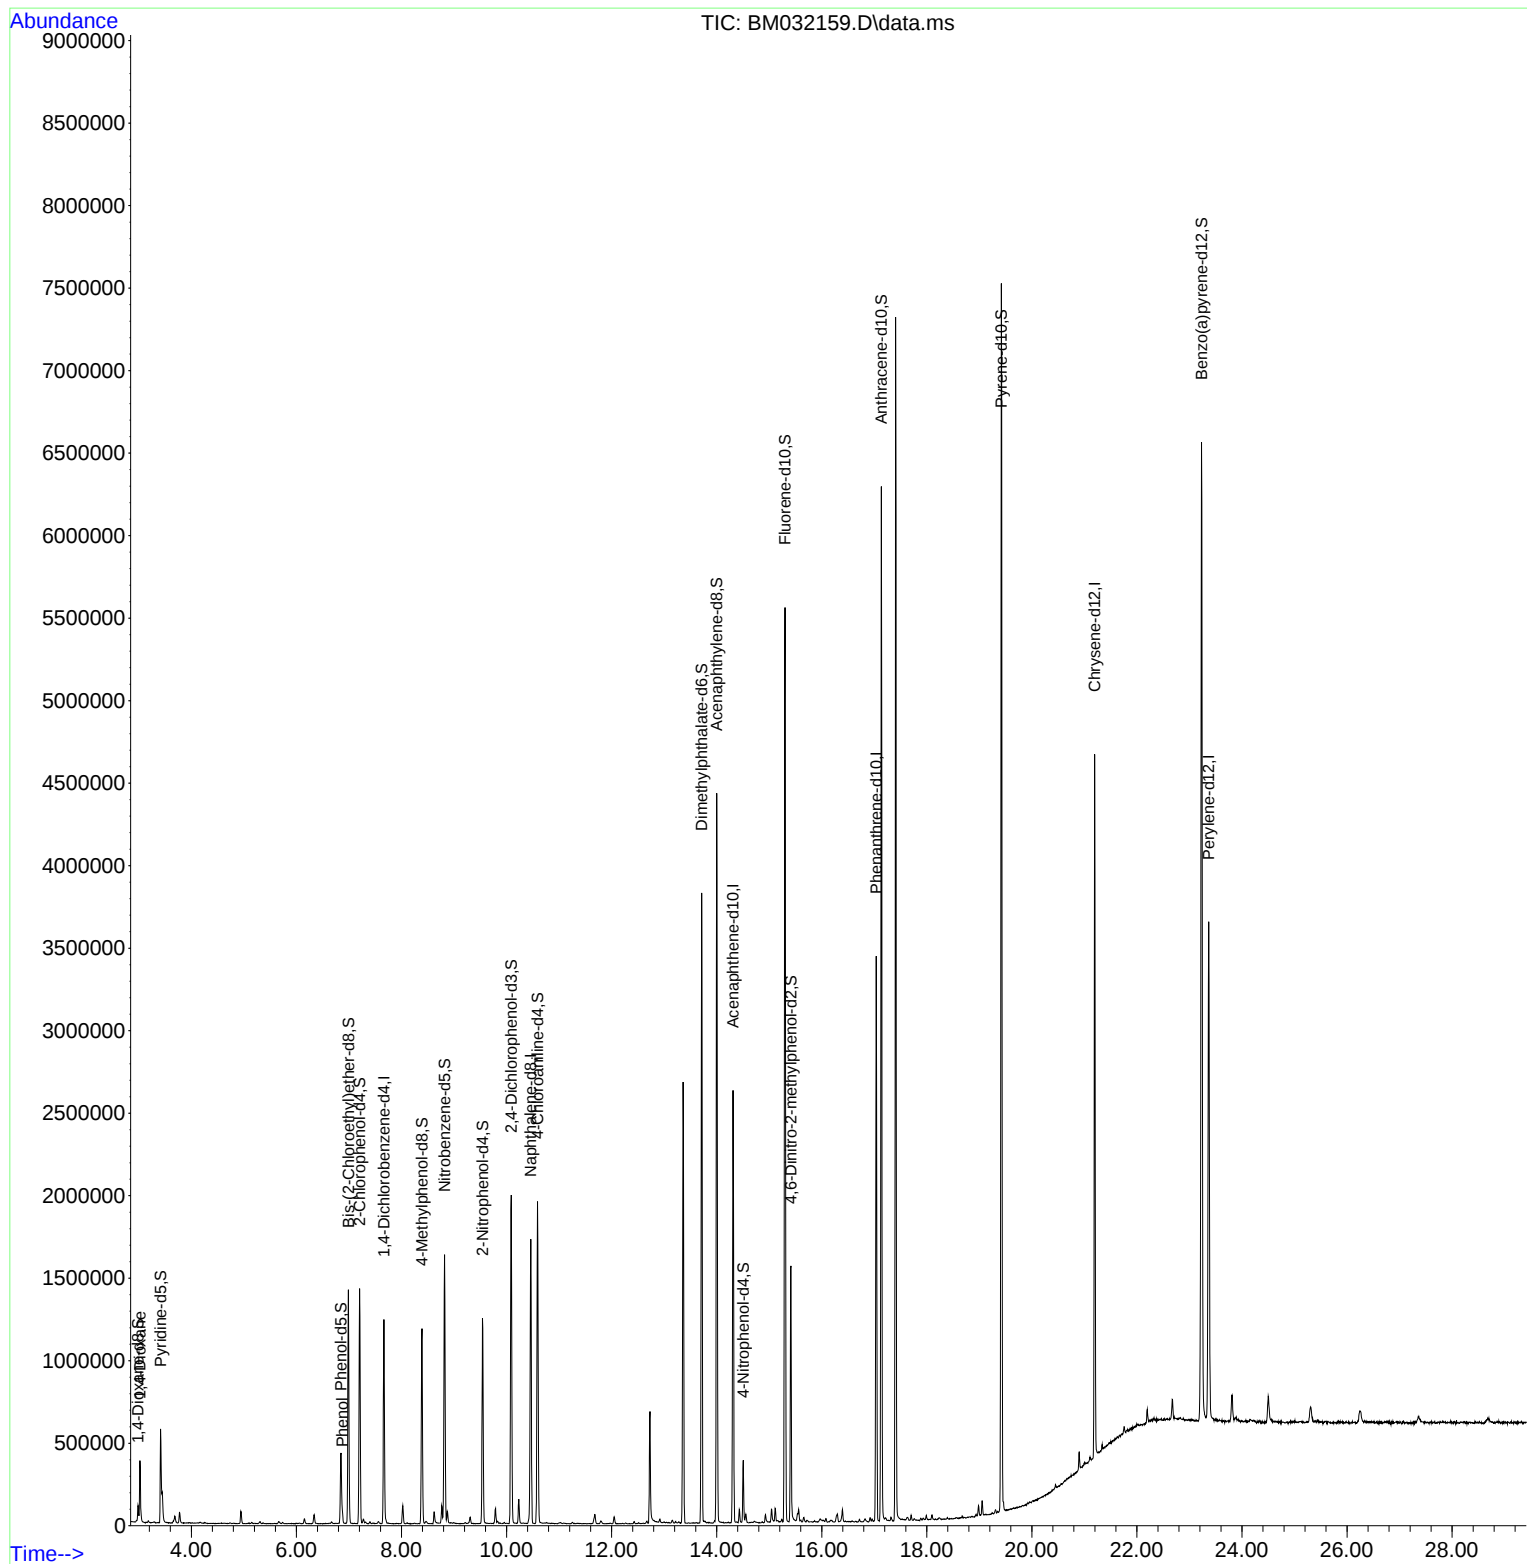


Abundance Scan 32 (3.025 min): BM032145.D\data.ms (-27)

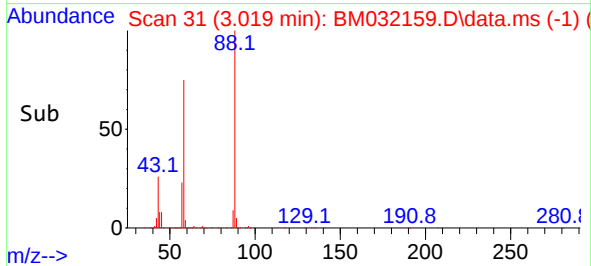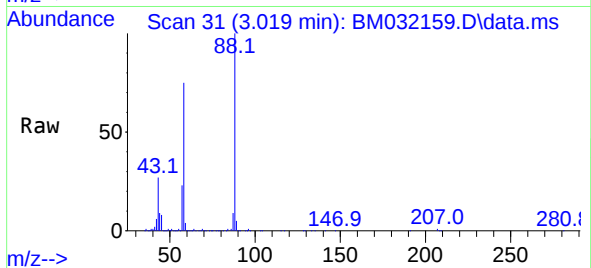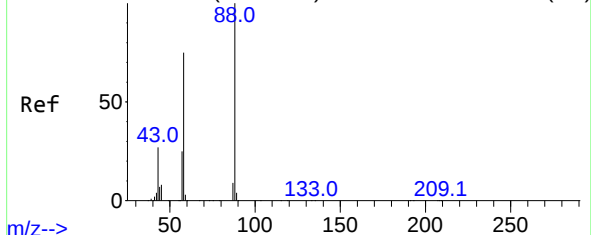


#2
1,4-Dioxane
Concen: 21.679 ng/uL
RT: 3.019 min Scan# 31
Delta R.T. -0.006 min
Lab File: BM032159.D
Acq: 25 Sep 2021 18:11

Tgt Ion:	88	Resp:	179751
Ion	Ratio	Lower	Upper
88	100		
43	26.9	22.3	33.5
58	75.1	62.4	93.6

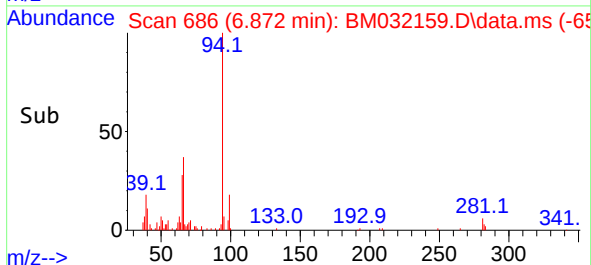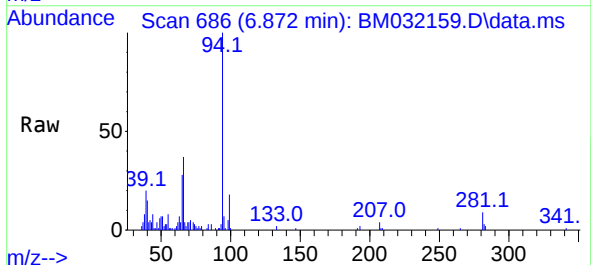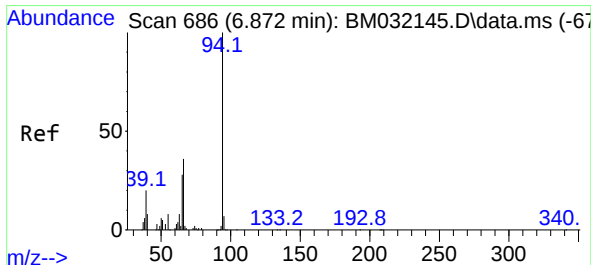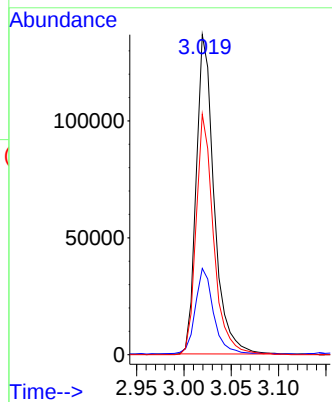

#8
Phenol
Concen: 1.352 ng/uL
RT: 6.872 min Scan# 686
Delta R.T. -0.006 min
Lab File: BM032159.D
Acq: 25 Sep 2021 18:11

Tgt Ion:	94	Resp:	34660
Ion	Ratio	Lower	Upper
94	100		
65	28.0	22.4	33.6
66	36.7	29.9	44.9

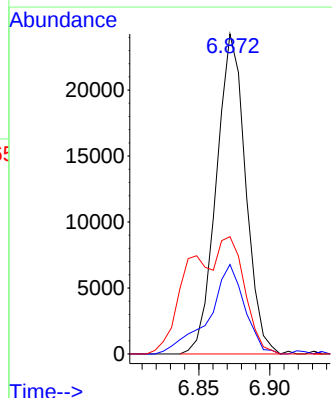

Instrument :
BNA_M
ClientSampled :
GB6Z4