

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032183.D
 Acq On : 26 Sep 2021 09:52
 Operator : CG/JU
 Sample : PB139380BS
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS380

Quant Time: Sep 27 01:08:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 25 01:15:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.660	152	295234	20.000	ng/u1	0.00
20) Naphthalene-d8	10.454	136	1130687	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.307	164	634388	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.036	188	1161556	20.000	ng/u1	0.00
79) Chrysene-d12	21.195	240	1043857	20.000	ng/u1	0.00
88) Perylene-d12	23.359	264	1044475	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.990	96	63406	9.068	ng/uL	0.00
4) Pyridine-d5	3.413	84	815594	41.089	ng/u1	0.00
7) Phenol-d5	6.848	99	983313	41.959	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.990	67	583155	41.384	ng/u1	0.00
11) 2-Chlorophenol-d4	7.201	132	807631	44.390	ng/u1	0.00
15) 4-Methylphenol-d8	8.390	113	763646	41.673	ng/u1	0.00
21) Nitrobenzene-d5	8.819	128	363444	53.817	ng/u1	0.00
24) 2-Nitrophenol-d4	9.542	143	383707	53.733	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.084	165	744695	45.619	ng/u1	0.00
31) 4-Chloroaniline-d4	10.589	131	943784	42.776	ng/u1	0.00
46) Dimethylphthalate-d6	13.713	166	1886967	45.781	ng/u1	0.00
49) Acenaphthylene-d8	14.001	160	2450084	46.787	ng/u1	0.00
54) 4-Nitrophenol-d4	14.507	143	328614	49.010	ng/u1	0.00
60) Fluorene-d10	15.295	176	1633473	46.445	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.413	200	267662	48.760	ng/u1	0.00
73) Anthracene-d10	17.130	188	2346504	48.415	ng/u1	0.00
81) Pyrene-d10	19.418	212	2487329	45.288	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.224	264	2297894	46.879	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.025	88	133033	17.317	ng/uL	93
5) Pyridine	3.431	79	853524	43.368	ng/u1	98
6) Benzaldehyde	6.790	77	595994	45.140	ng/u1	95
8) Phenol	6.872	94	1063476	44.763	ng/u1	97
10) Bis(2-Chloroethyl)ether	7.078	93	852661	45.044	ng/u1	96
12) 2-Chlorophenol	7.231	128	879247	46.329	ng/u1	97
13) 2-Methylphenol	8.125	108	788493	43.852	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.201	45	1043284	40.045	ng/u1	97
16) Acetophenone	8.478	105	1212808	43.666	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.472	70	576097	40.667	ng/u1	95
18) 4-Methylphenol	8.454	108	839847	44.439	ng/u1	97
19) Hexachloroethane	8.754	117	360309	46.256	ng/u1	99
22) Nitrobenzene	8.860	77	881474	50.606	ng/u1	97
23) Isophorone	9.378	82	1545016	42.610	ng/u1	100
25) 2-Nitrophenol	9.572	139	445407	54.598	ng/u1	96
26) 2,4-Dimethylphenol	9.648	107	900975	46.375	ng/u1	98
27) Bis(2-Chloroethoxy)met...	9.866	93	1066365	46.005	ng/u1	100
29) 2,4-Dichlorophenol	10.113	162	778839	48.498	ng/u1	100
30) Naphthalene	10.507	128	2614998	47.115	ng/u1	99
32) 4-Chloroaniline	10.613	127	956130	42.480	ng/u1	100
33) Hexachlorobutadiene	10.813	225	508130	46.026	ng/u1	99
34) Caprolactam	11.342	113	201480	41.131	ng/u1	89
35) 4-Chloro-3-methylphenol	11.754	107	769164	44.469	ng/u1	97
36) 2-Methylnaphthalene	12.119	142	1790268	48.051	ng/u1	98


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032183.D
 Acq On : 26 Sep 2021 09:52
 Operator : CG/JU
 Sample : PB139380BS
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS380

Quant Time: Sep 27 01:08:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 25 01:15:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.342	142	1706001	44.986	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.501	216	896170	49.489	ng/ul	99
40) Hexachlorocyclopentadiene	12.495	237	470824	48.516	ng/ul	98
41) 2,4,6-Trichlorophenol	12.742	196	568074	50.154	ng/ul	100
42) 2,4,5-Trichlorophenol	12.813	196	598819	49.802	ng/ul	99
43) 1,1'-Biphenyl	13.136	154	2199130	48.948	ng/ul	99
44) 2-Chloronaphthalene	13.177	162	1682621	49.641	ng/ul	99
45) 2-Nitroaniline	13.377	65	419291	54.727	ng/ul	93
47) Dimethylphthalate	13.760	163	1940137	47.181	ng/ul	100
48) 2,6-Dinitrotoluene	13.872	165	368759	54.009	ng/ul	99
50) Acenaphthylene	14.030	152	2480362	45.097	ng/ul	99
51) 3-Nitroaniline	14.201	138	376909	50.474	ng/ul	96
52) Acenaphthene	14.371	153	1746046	48.801	ng/ul	99
53) 2,4-Dinitrophenol	14.401	184	180145	48.263	ng/ul	98
55) 4-Nitrophenol	14.524	109	273428	49.995	ng/ul	93
56) Dibenzofuran	14.707	168	2445818	47.627	ng/ul	99
57) 2,4-Dinitrotoluene	14.660	165	521223	54.725	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	14.936	232	480004	48.934	ng/ul	99
59) Diethylphthalate	15.124	149	1889995	47.019	ng/ul	100
61) Fluorene	15.354	166	1878171	47.136	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.342	204	940231	46.666	ng/ul	99
63) 4-Nitroaniline	15.366	138	352514	53.857	ng/ul	99
66) 4,6-Dinitro-2-methylph...	15.424	198	287009	52.966	ng/ul	100
67) N-Nitrosodiphenylamine	15.554	169	1622810	50.128	ng/ul	100
68) 4-Bromophenyl-phenylether	16.230	248	558697	50.372	ng/ul	98
69) Hexachlorobenzene	16.365	284	642568	47.655	ng/ul	99
70) Atrazine	16.495	200	542844	47.435	ng/ul	99
71) Pentachlorophenol	16.701	266	373296	48.197	ng/ul	100
72) Phenanthrene	17.077	178	2864907	49.404	ng/ul	100
74) Anthracene	17.165	178	2924988	50.325	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.113	216	917502	51.243	ng/ul	99
76) Pentachlorobenzene	14.642	250	810824	46.766	ng/ul	99
77) Carbazole	17.430	167	2561626	52.105	ng/ul	100
78) Di-n-butylphthalate	17.989	149	2893360	51.226	ng/ul	100
80) Fluoranthene	19.083	202	3134731	45.993	ng/ul	100
82) Pyrene	19.448	202	3229584	46.208	ng/ul	99
83) Butylbenzylphthalate	20.330	149	1135848	56.516	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.112	252	940629	54.334	ng/ul	99
85) Benzo(a)anthracene	21.177	228	2929421	49.809	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.106	149	1649797	55.450	ng/ul	98
87) Chrysene	21.230	228	2886135	48.701	ng/ul	100
89) Di-n-octyl phthalate	21.953	149	2838929	53.493	ng/ul	100
90) Benzo(b)fluoranthene	22.718	252	3010480	48.803	ng/ul	99
91) Benzo(k)fluoranthene	22.759	252	3018189	51.628	ng/ul	99
93) Benzo(a)pyrene	23.271	252	2744108	47.111	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	25.512	276	3373050	56.817	ng/ul	99
95) Dibenzo(a,h)anthracene	25.518	278	2856239	58.010	ng/ul	99
96) Benzo(g,h,i)perylene	26.177	276	2904493	55.197	ng/ul	99





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 17.317 ng/uL
RT: 3.025 min Scan# 32
Delta R.T. 0.000 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion: 88 Resp: 133033
Ion Ratio Lower Upper
88 100
43 25.4 22.3 33.5
58 71.7 62.4 93.6



#5
Pyridine
Concen: 43.368 ng/uL
RT: 3.431 min Scan# 101
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion: 79 Resp: 853524
Ion Ratio Lower Upper
79 100
52 71.7 58.3 87.5
51 34.0 29.1 43.7



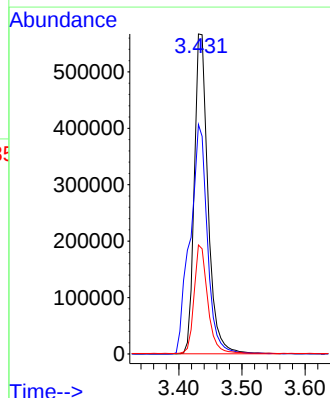





#6
Benzaldehyde
Concen: 45.140 ng/ul
RT: 6.790 min Scan# 672
Delta R.T. -0.000 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion: 77 Resp: 595994
Ion Ratio Lower Upper
77 100
105 101.3 77.0 115.4
106 97.0 74.2 111.2



#8
Phenol
Concen: 44.763 ng/ul
RT: 6.872 min Scan# 686
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion: 94 Resp: 1063476
Ion Ratio Lower Upper
94 100
65 26.8 22.4 33.6
66 35.3 29.9 44.9









#10
Bis(2-Chloroethyl)ether
Concen: 45.044 ng/ul
RT: 7.078 min Scan# 721
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Instrument :
BNA_M
ClientSampleId :
SLCS380

Tgt Ion: 93 Resp: 852661




Ion	Ratio	Lower	Upper
93	100		
63	74.8	63.4	95.2
95	32.2	25.5	38.3




#12
2-Chlorophenol
Concen: 46.329 ng/ul
RT: 7.231 min Scan# 747
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:128 Resp: 879247

Ion	Ratio	Lower	Upper
128	100		
64	44.2	38.3	57.5
130	32.5	25.8	38.8









#13
2-Methylphenol
Concen: 43.852 ng/ul
RT: 8.125 min Scan# 899
Delta R.T. -0.000 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:108 Resp: 788493
Ion Ratio Lower Upper
108 100
107 89.0 71.6 107.4



#14
2,2'-oxybis(1-Chloropropane)
Concen: 40.045 ng/ul
RT: 8.201 min Scan# 912
Delta R.T. -0.000 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion: 45 Resp: 1043284
Ion Ratio Lower Upper
45 100
77 15.7 11.2 16.8
79 12.3 9.1 13.7


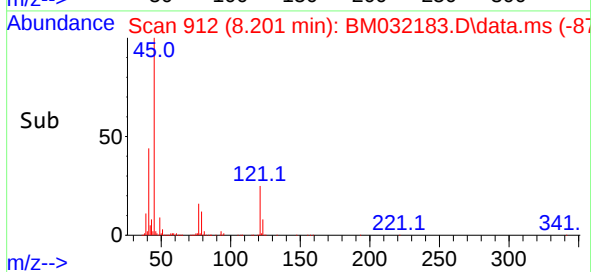






#16
Acetophenone
Concen: 43.666 ng/ul
RT: 8.478 min Scan# 959
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:105 Resp: 1212808
Ion Ratio Lower Upper
105 100
77 77.0 63.0 94.4
51 25.6 22.2 33.2

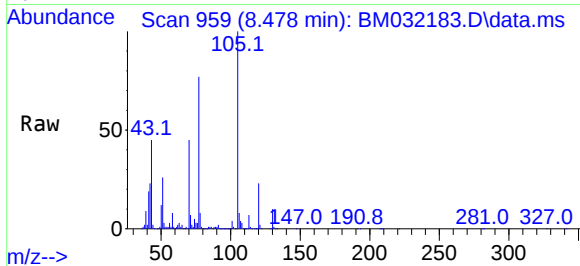

#17
N-Nitroso-di-n-propylamine
Concen: 40.667 ng/ul
RT: 8.472 min Scan# 958
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion: 70 Resp: 576097
Ion Ratio Lower Upper
70 100
42 53.2 46.2 69.4
101 10.3 7.5 11.3
130 22.1 16.2 24.2


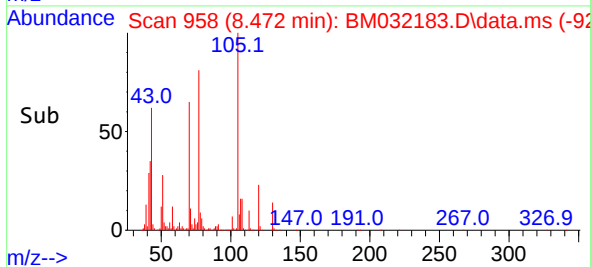

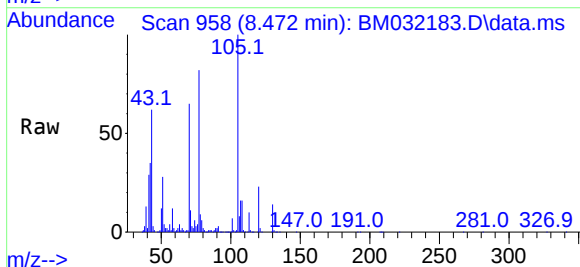




#18
4-Methylphenol
Concen: 44.439 ng/ul
RT: 8.454 min Scan# 955
Delta R.T. -0.000 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:108 Resp: 839847
Ion Ratio Lower Upper
108 100
107 108.4 89.1 133.7



#19
Hexachloroethane
Concen: 46.256 ng/ul
RT: 8.754 min Scan# 1006
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:117 Resp: 360309
Ion Ratio Lower Upper
117 100
201 99.6 79.5 119.3
199 63.7 49.1 73.7



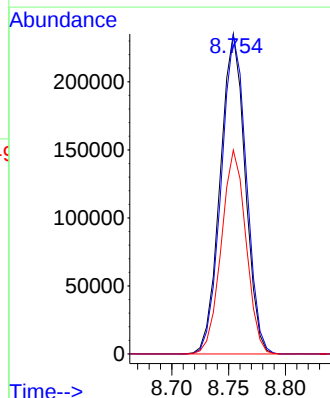





#22
Nitrobenzene
Concen: 50.606 ng/ul
RT: 8.860 min Scan# 1024
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion: 77 Resp: 881474
Ion Ratio Lower Upper
77 100
123 47.1 36.1 54.1
65 13.2 11.0 16.6



#23
Isophorone
Concen: 42.610 ng/ul
RT: 9.378 min Scan# 1112
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion: 82 Resp: 1545016
Ion Ratio Lower Upper
82 100
95 7.1 5.8 8.6
138 17.8 14.1 21.1









#25
2-Nitrophenol
Concen: 54.598 ng/ul
RT: 9.572 min Scan# 1145
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:	139	Resp:	445407
Ion	Ratio	Lower	Upper
139	100		
65	49.0	42.0	63.0
109	30.6	25.8	38.8



#26
2,4-Dimethylphenol
Concen: 46.375 ng/ul
RT: 9.648 min Scan# 1158
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:	107	Resp:	900975
Ion	Ratio	Lower	Upper
107	100		
121	50.8	40.4	60.6
122	86.7	67.6	101.4









#27
Bis(2-Chloroethoxy)methane
Concen: 46.005 ng/ul
RT: 9.866 min Scan# 1195
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Instrument :
BNA_M
ClientSampleId :
SLCS380

Tgt Ion: 93 Resp: 1066365




Ion	Ratio	Lower	Upper
93	100		
95	33.2	26.2	39.4
123	11.3	9.0	13.6

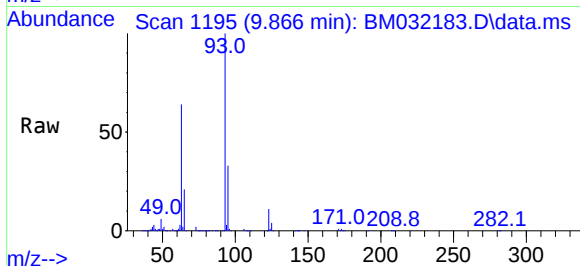


#29
2,4-Dichlorophenol
Concen: 48.498 ng/ul
RT: 10.113 min Scan# 1237
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion: 162 Resp: 778839

Ion	Ratio	Lower	Upper
162	100		
164	64.9	51.6	77.4
98	35.6	28.6	42.8


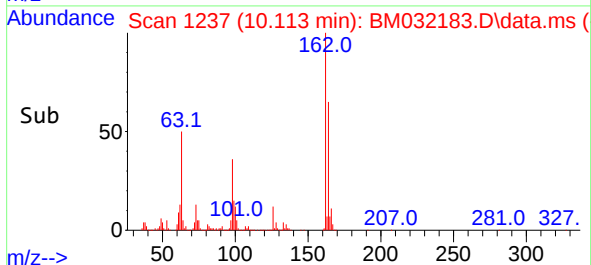

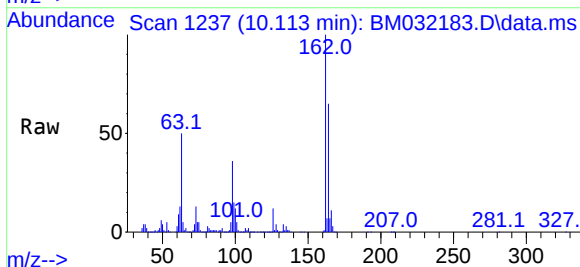




#30
Naphthalene
Concen: 47.115 ng/ul
RT: 10.507 min Scan# 1304
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:128 Resp: 2614998
Ion Ratio Lower Upper
128 100
129 11.1 8.7 13.1
127 13.1 10.2 15.4



#32
4-Chloroaniline
Concen: 42.480 ng/ul
RT: 10.613 min Scan# 1322
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:127 Resp: 956130
Ion Ratio Lower Upper
127 100
129 32.2 25.8 38.6









#33
Hexachlorobutadiene
Concen: 46.026 ng/ul
RT: 10.813 min Scan# 1356
Delta R.T. -0.012 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampled :
SLCS380


Tgt Ion:225 Resp: 508130
Ion Ratio Lower Upper
225 100
223 62.8 50.6 76.0
227 63.7 52.2 78.4



#34
Caprolactam
Concen: 41.131 ng/ul
RT: 11.342 min Scan# 1446
Delta R.T. -0.000 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:113 Resp: 201480
Ion Ratio Lower Upper
113 100
55 157.8 138.1 207.1
56 118.5 106.0 159.0









#35
4-Chloro-3-methylphenol
Concen: 44.469 ng/ul
RT: 11.754 min Scan# 1516
Delta R.T. -0.000 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Instrument :
BNA_M
ClientSampleId :
SLCS380

Tgt Ion:107 Resp: 769164




Ion	Ratio	Lower	Upper
107	100		
144	26.7	20.3	30.5
142	81.5	62.8	94.2




#36
2-Methylnaphthalene
Concen: 48.051 ng/ul
RT: 12.119 min Scan# 1578
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:142 Resp: 1790268

Ion	Ratio	Lower	Upper
142	100		
141	89.2	70.2	105.2



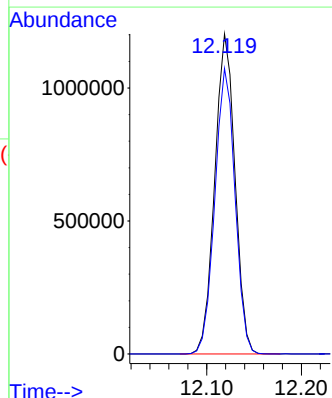





#37
1-Methylnaphthalene
Concen: 44.986 ng/ul
RT: 12.342 min Scan# 1616
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:142 Resp: 1706001
Ion Ratio Lower Upper
142 100
141 91.1 74.3 111.5
116 3.7 3.0 4.6



#39
1,2,4,5-Tetrachlorobenzene
Concen: 49.489 ng/ul
RT: 12.501 min Scan# 1643
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:216 Resp: 896170
Ion Ratio Lower Upper
216 100
214 79.1 64.2 96.4
179 21.0 17.1 25.7
108 19.9 16.0 24.0


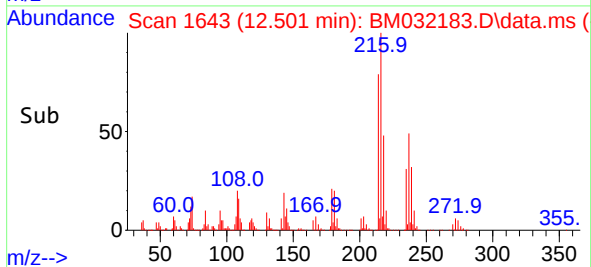

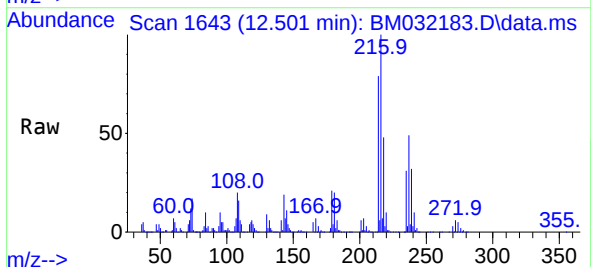




#40
Hexachlorocyclopentadiene
Concen: 48.516 ng/ul
RT: 12.495 min Scan# 1642
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:237 Resp: 470824
Ion Ratio Lower Upper
237 100
235 63.1 49.4 74.0
272 12.7 10.1 15.1



#41
2,4,6-Trichlorophenol
Concen: 50.154 ng/ul
RT: 12.742 min Scan# 1684
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:196 Resp: 568074
Ion Ratio Lower Upper
196 100
198 97.6 77.8 116.6
200 30.8 24.6 36.8









#42
2,4,5-Trichlorophenol
Concen: 49.802 ng/ul
RT: 12.813 min Scan# 1696
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampled :
SLCS380


Tgt Ion:196 Resp: 598819
Ion Ratio Lower Upper
196 100
198 95.3 77.4 116.2
200 30.9 24.3 36.5

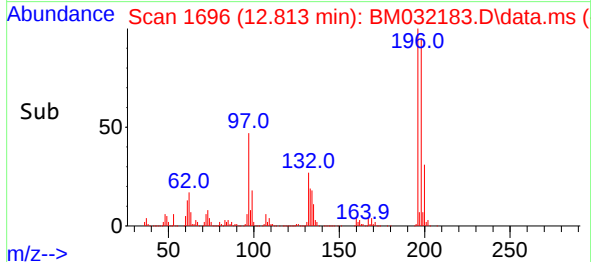

#43
1,1'-Biphenyl
Concen: 48.948 ng/ul
RT: 13.136 min Scan# 1751
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:154 Resp: 2199130
Ion Ratio Lower Upper
154 100
153 40.3 31.9 47.9
76 12.7 10.7 16.1









#44
2-Chloronaphthalene
Concen: 49.641 ng/ul
RT: 13.177 min Scan# 1758
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:162 Resp: 1682621
Ion Ratio Lower Upper
162 100
164 32.9 25.9 38.9
127 40.1 32.0 48.0



#45
2-Nitroaniline
Concen: 54.727 ng/ul
RT: 13.377 min Scan# 1792
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion: 65 Resp: 419291
Ion Ratio Lower Upper
65 100
92 72.4 54.5 81.7
138 113.5 84.1 126.1









#47
Dimethylphthalate
Concen: 47.181 ng/ul
RT: 13.760 min Scan# 1857
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:163 Resp: 1940137
Ion Ratio Lower Upper
163 100
194 4.1 3.3 4.9
164 10.0 8.1 12.1



#48
2,6-Dinitrotoluene
Concen: 54.009 ng/ul
RT: 13.872 min Scan# 1876
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:165 Resp: 368759
Ion Ratio Lower Upper
165 100
89 57.5 46.8 70.2
121 21.6 17.3 25.9









#50
Acenaphthylene
Concen: 45.097 ng/ul
RT: 14.030 min Scan# 1903
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:152 Resp: 2480362
Ion Ratio Lower Upper
152 100
151 19.7 15.7 23.5
153 12.8 10.6 15.8



#51
3-Nitroaniline
Concen: 50.474 ng/ul
RT: 14.201 min Scan# 1932
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:138 Resp: 376909
Ion Ratio Lower Upper
138 100
108 10.8 10.5 15.7
92 113.5 94.0 141.0









#52
Acenaphthene
Concen: 48.801 ng/ul
RT: 14.371 min Scan# 1961
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:153 Resp: 1746046
Ion Ratio Lower Upper
153 100
152 47.6 38.4 57.6
154 88.0 71.0 106.6



#53
2,4-Dinitrophenol
Concen: 48.263 ng/ul
RT: 14.401 min Scan# 1966
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:184 Resp: 180145
Ion Ratio Lower Upper
184 100
63 69.2 56.7 85.1
154 71.0 57.5 86.3









#55
4-Nitrophenol
Concen: 49.995 ng/ul
RT: 14.524 min Scan# 1987
Delta R.T. -0.000 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:109 Resp: 273428
Ion Ratio Lower Upper
109 100
139 135.2 103.7 155.5
65 125.6 109.4 164.2

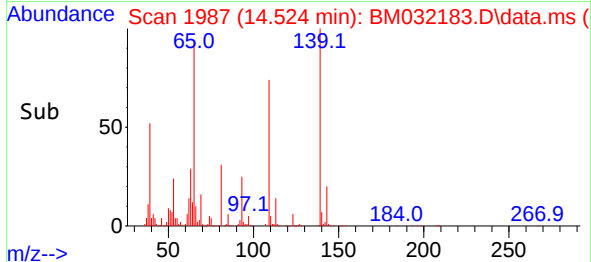

#56
Dibenzofuran
Concen: 47.627 ng/ul
RT: 14.707 min Scan# 2018
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:168 Resp: 2445818
Ion Ratio Lower Upper
168 100
139 36.7 29.8 44.6









#57
2,4-Dinitrotoluene
Concen: 54.725 ng/ul
RT: 14.660 min Scan# 2010
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:165 Resp: 521223
Ion Ratio Lower Upper
165 100
63 41.7 34.2 51.2
182 3.1 2.3 3.5



#58
2,3,4,6-Tetrachlorophenol
Concen: 48.934 ng/ul
RT: 14.936 min Scan# 2057
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:232 Resp: 480004
Ion Ratio Lower Upper
232 100
131 46.5 36.2 54.2
130 2.3 1.9 2.9
166 30.8 24.8 37.2









#59
Diethylphthalate
Concen: 47.019 ng/ul
RT: 15.124 min Scan# 2089
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:149 Resp: 1889995
Ion Ratio Lower Upper
149 100
177 22.5 17.9 26.9
150 12.6 10.0 15.0



#61
Fluorene
Concen: 47.136 ng/ul
RT: 15.354 min Scan# 2128
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:166 Resp: 1878171
Ion Ratio Lower Upper
166 100
165 97.1 77.7 116.5
167 13.0 10.7 16.1









#62
4-Chlorophenyl-phenylether
Concen: 46.666 ng/ul
RT: 15.342 min Scan# 2126
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:204 Resp: 940231
Ion Ratio Lower Upper
204 100
206 32.8 25.8 38.6
141 59.6 47.9 71.9

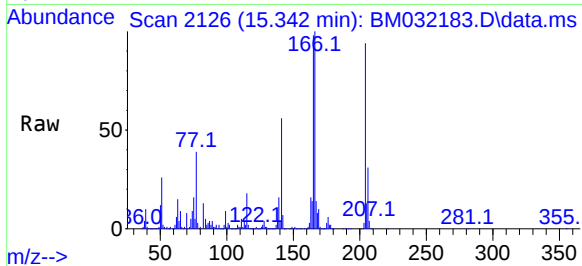

#63
4-Nitroaniline
Concen: 53.857 ng/ul
RT: 15.366 min Scan# 2130
Delta R.T. -0.000 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:138 Resp: 352514
Ion Ratio Lower Upper
138 100
92 50.4 41.4 62.2
108 79.1 63.8 95.6



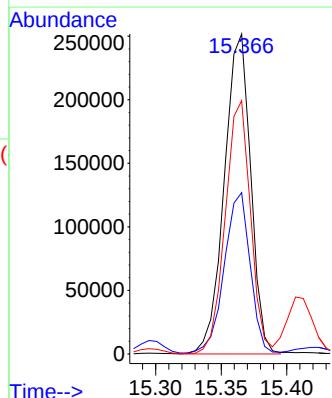
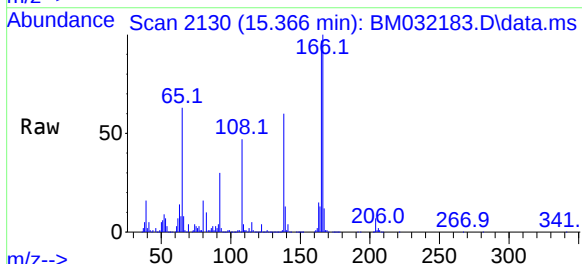




#66
4,6-Dinitro-2-methylphenol
Concen: 52.966 ng/ul
RT: 15.424 min Scan# 2140
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:198 Resp: 287009
Ion Ratio Lower Upper
198 100
182 4.4 3.8 5.8
77 24.9 19.8 29.8

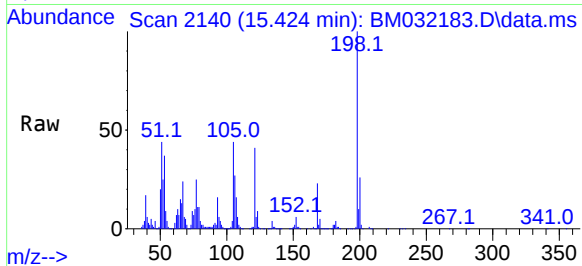

#67
N-Nitrosodiphenylamine
Concen: 50.128 ng/ul
RT: 15.554 min Scan# 2162
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:169 Resp: 1622810
Ion Ratio Lower Upper
169 100
168 65.9 52.3 78.5
167 35.8 28.6 42.8




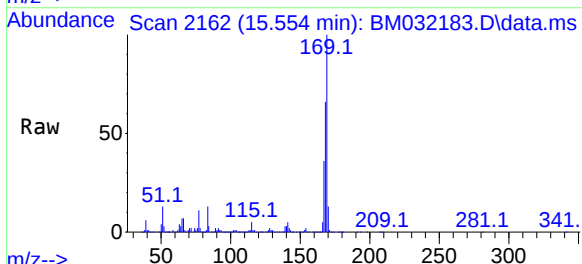




#68
4-Bromophenyl-phenylether
Concen: 50.372 ng/ul
RT: 16.230 min Scan# 2277
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:248 Resp: 558697
Ion Ratio Lower Upper
248 100
250 96.6 77.0 115.6
141 75.6 57.6 86.4

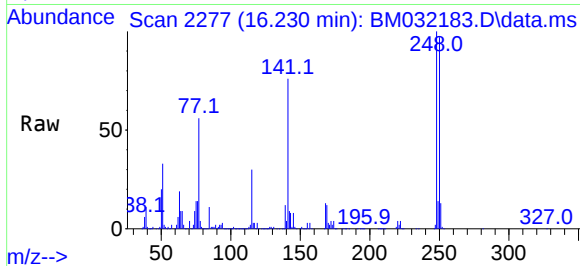

#69
Hexachlorobenzene
Concen: 47.655 ng/ul
RT: 16.365 min Scan# 2300
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:284 Resp: 642568
Ion Ratio Lower Upper
284 100
142 35.0 28.4 42.6
249 31.4 24.7 37.1


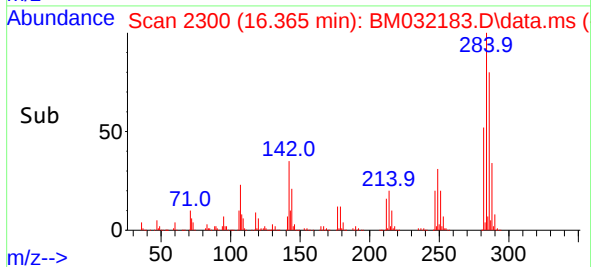

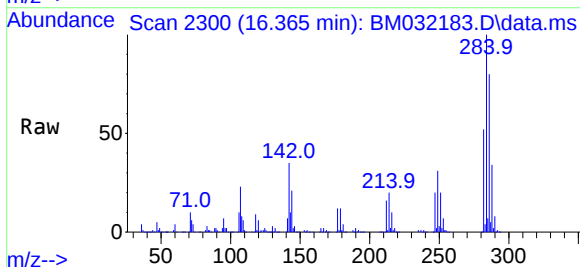




#70
Atrazine
Concen: 47.435 ng/ul
RT: 16.495 min Scan# 2322
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:200 Resp: 542844
Ion Ratio Lower Upper
200 100
173 27.0 21.4 32.0
215 48.2 39.4 59.2



#71
Pentachlorophenol
Concen: 48.197 ng/ul
RT: 16.701 min Scan# 2357
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:266 Resp: 373296
Ion Ratio Lower Upper
266 100
264 62.9 50.2 75.2
268 63.8 51.0 76.6









#72
Phenanthrene
Concen: 49.404 ng/u1
RT: 17.077 min Scan# 2421
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:178 Resp: 2864907
Ion Ratio Lower Upper
178 100
179 15.3 12.3 18.5
176 19.4 15.4 23.0

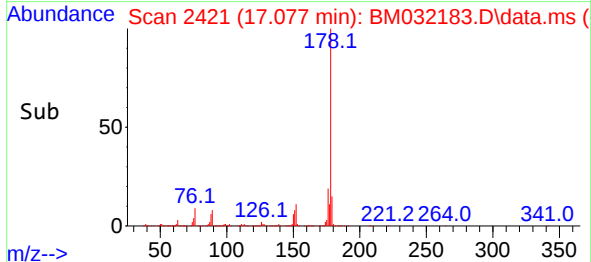

#74
Anthracene
Concen: 50.325 ng/u1
RT: 17.165 min Scan# 2436
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:178 Resp: 2924988
Ion Ratio Lower Upper
178 100
179 15.6 12.6 19.0
176 18.8 14.8 22.2









#75
1,2,3,4-Tetrachlorobenzene
Concen: 51.243 ng/uL
RT: 13.113 min Scan# 1747
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:216 Resp: 917502
Ion Ratio Lower Upper
216 100
214 79.0 62.7 94.1
218 48.7 38.7 58.1

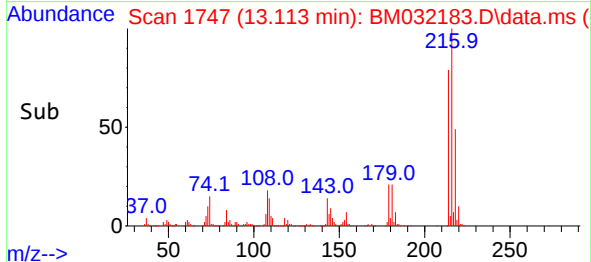

#76
Pentachlorobenzene
Concen: 46.766 ng/uL
RT: 14.642 min Scan# 2007
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:250 Resp: 810824
Ion Ratio Lower Upper
250 100
248 62.2 50.0 75.0
252 63.8 51.6 77.4

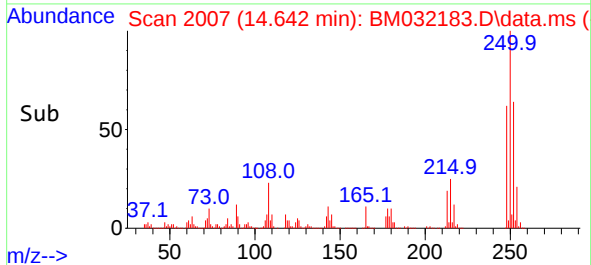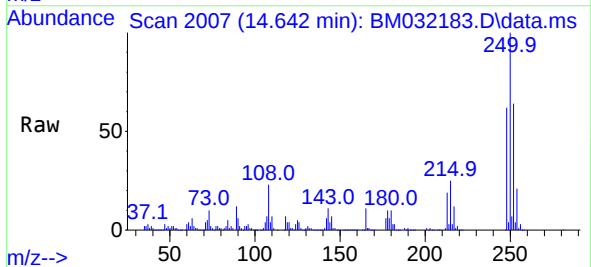







#77
 Carbazole
 Concen: 52.105 ng/ul
 RT: 17.430 min Scan# 2481
 Delta R.T. -0.006 min
 Lab File: BM032183.D
 Acq: 26 Sep 2021 09:52

Instrument :
 BNA_M
 ClientSampleId :
 SLCS380

Tgt Ion:167 Resp: 2561626




Ion	Ratio	Lower	Upper
167	100		
166	21.8	17.3	25.9
139	13.0	10.3	15.5

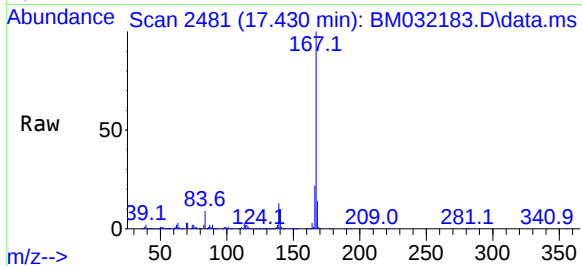


#78
 Di-n-butylphthalate
 Concen: 51.226 ng/ul
 RT: 17.989 min Scan# 2576
 Delta R.T. -0.006 min
 Lab File: BM032183.D
 Acq: 26 Sep 2021 09:52

Tgt Ion:149 Resp: 2893360

Ion	Ratio	Lower	Upper
149	100		
150	9.1	7.4	11.0
104	5.1	4.2	6.2




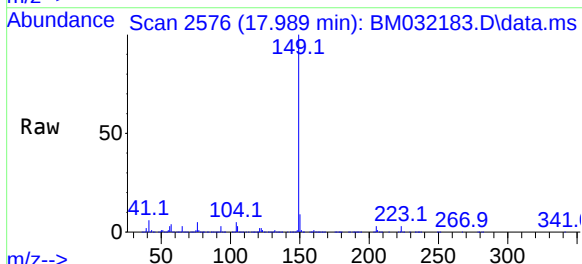




#80
Fluoranthene
Concen: 45.993 ng/u1
RT: 19.083 min Scan# 2762
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:202 Resp: 3134731
Ion Ratio Lower Upper
202 100
101 11.4 9.2 13.8
100 8.6 6.9 10.3

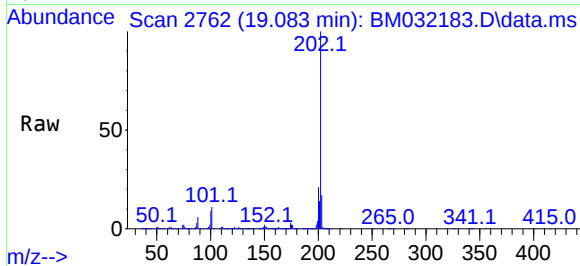

#82
Pyrene
Concen: 46.208 ng/u1
RT: 19.448 min Scan# 2824
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:202 Resp: 3229584
Ion Ratio Lower Upper
202 100
101 13.2 10.1 15.1
100 10.6 8.4 12.6




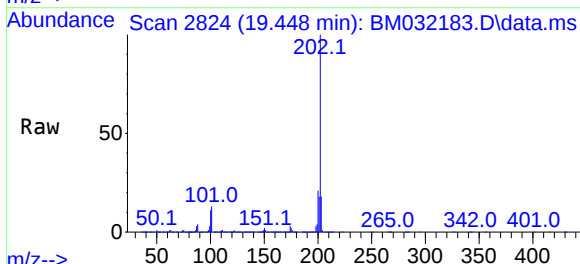




#83
Butylbenzylphthalate
Concen: 56.516 ng/ul
RT: 20.330 min Scan# 2974
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:149 Resp: 1135848
Ion Ratio Lower Upper
149 100
91 73.3 61.8 92.8
206 20.4 16.2 24.4

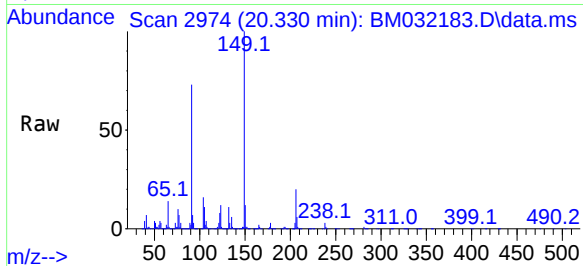

#84
3,3'-Dichlorobenzidine
Concen: 54.334 ng/ul
RT: 21.112 min Scan# 3107
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:252 Resp: 940629
Ion Ratio Lower Upper
252 100
254 64.7 52.2 78.2
126 11.5 8.8 13.2



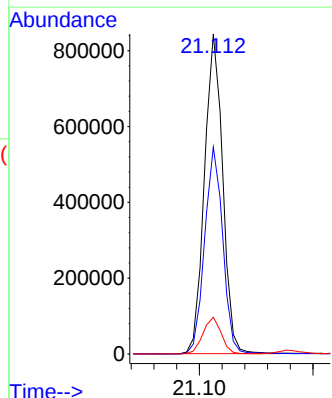
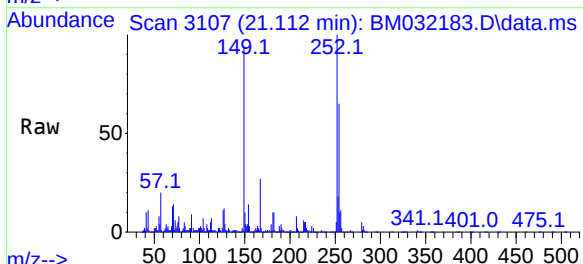




#85
Benzo(a)anthracene
Concen: 49.809 ng/ul
RT: 21.177 min Scan# 3118
Delta R.T. -0.012 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:228 Resp: 2929421
Ion Ratio Lower Upper
228 100
229 20.2 15.9 23.9
226 27.8 21.7 32.5

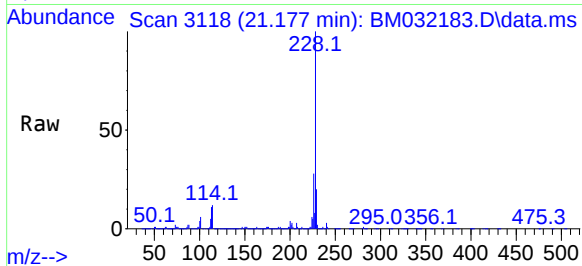

#86
Bis(2-ethylhexyl)phthalate
Concen: 55.450 ng/ul
RT: 21.106 min Scan# 3106
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:149 Resp: 1649797
Ion Ratio Lower Upper
149 100
167 28.0 21.6 32.4
279 4.5 3.3 4.9




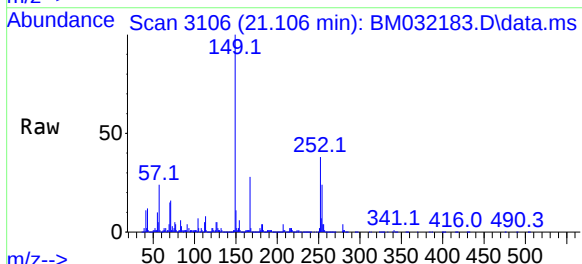




#87
Chrysene
Concen: 48.701 ng/ul
RT: 21.230 min Scan# 3127
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:228 Resp: 2886135
Ion Ratio Lower Upper
228 100
226 30.4 24.4 36.6
229 20.1 15.9 23.9



#89
Di-n-octyl phthalate
Concen: 53.493 ng/ul
RT: 21.953 min Scan# 3250
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:149 Resp: 2838929



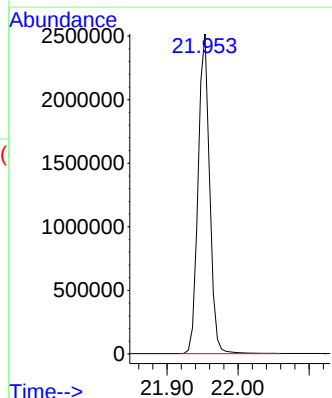





#90
Benzo(b)fluoranthene
Concen: 48.803 ng/ul
RT: 22.718 min Scan# 3380
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampleId :
SLCS380


Tgt Ion:252 Resp: 3010480
Ion Ratio Lower Upper
252 100
253 22.1 18.2 27.4
125 10.1 8.5 12.7



#91
Benzo(k)fluoranthene
Concen: 51.628 ng/ul
RT: 22.759 min Scan# 3387
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:252 Resp: 3018189
Ion Ratio Lower Upper
252 100
253 22.0 17.9 26.9
125 10.4 8.4 12.6









#93
Benzo(a)pyrene
Concen: 47.111 ng/ul
RT: 23.271 min Scan# 3474
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52




Instrument :
BNA_M
ClientSampled :
SLCS380


Tgt Ion:252 Resp: 2744108
Ion Ratio Lower Upper
252 100
253 21.7 17.8 26.6
125 11.0 9.2 13.8

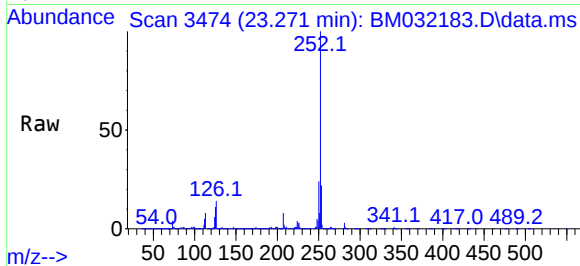

#94
Indeno(1,2,3-cd)pyrene
Concen: 56.817 ng/ul
RT: 25.512 min Scan# 3855
Delta R.T. -0.012 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:276 Resp: 3373050
Ion Ratio Lower Upper
276 100
138 27.0 21.5 32.3
277 25.5 21.0 31.6




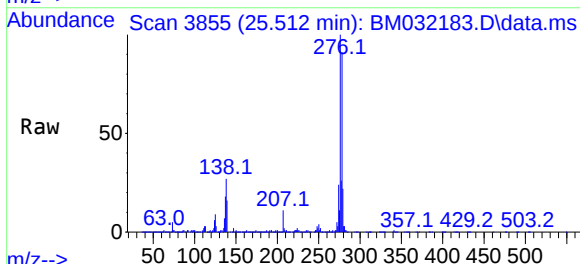




#95
Dibenzo(a,h)anthracene
Concen: 58.010 ng/ul
RT: 25.518 min Scan# 3856
Delta R.T. -0.012 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Instrument :
BNA_M
ClientSampled :
SLCS380

Tgt Ion:278 Resp: 2856239
Ion Ratio Lower Upper
278 100
139 17.2 13.5 20.3
279 23.8 19.4 29.0

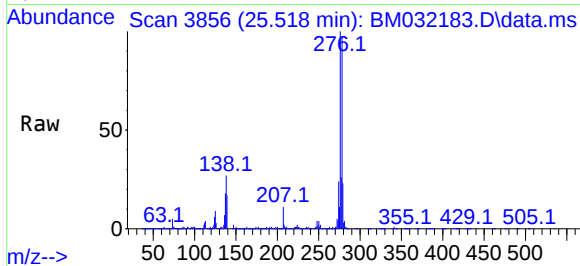

#96
Benzo(g,h,i)perylene
Concen: 55.197 ng/ul
RT: 26.177 min Scan# 3968
Delta R.T. -0.006 min
Lab File: BM032183.D
Acq: 26 Sep 2021 09:52

Tgt Ion:276 Resp: 2904493
Ion Ratio Lower Upper
276 100
138 22.6 17.9 26.9
277 24.2 18.6 28.0

