

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032154.D
 Acq On : 25 Sep 2021 15:09
 Operator : CG/JU
 Sample : M3919-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Y4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032154.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.990	21	26	33	rVB	112233	143900	1.28%	0.133%
2	3.284	73	76	80	rBV	15936	18684	0.17%	0.017%
3	3.413	94	98	116	rBV	509749	742025	6.59%	0.688%
4	3.684	136	144	150	rBV3	48257	92245	0.82%	0.085%
5	3.778	155	160	165	rBV	29824	41003	0.36%	0.038%
6	4.160	221	225	231	rBV7	8664	15799	0.14%	0.015%
7	5.737	489	493	499	rVB	9604	15370	0.14%	0.014%
8	6.672	647	652	658	rBV2	11642	18431	0.16%	0.017%
9	6.843	676	681	695	rVB	591450	958288	8.51%	0.888%
10	6.990	699	706	715	rVB	1783495	2668825	23.69%	2.473%
11	7.201	735	742	749	rBV	1851004	2754062	24.45%	2.552%
12	7.260	749	752	757	rVV	10402	18022	0.16%	0.017%
13	7.313	757	761	765	rVB2	10534	14049	0.12%	0.013%
14	7.666	814	821	828	rBV	1585200	2353235	20.89%	2.180%
15	7.748	832	835	842	rVB2	12262	17052	0.15%	0.016%
16	8.113	890	897	900	rVB5	8180	13854	0.12%	0.013%
17	8.390	936	944	952	rBV	1608014	2418638	21.47%	2.241%
18	8.819	1009	1017	1030	rBV	2052523	3082633	27.36%	2.856%
19	8.995	1043	1047	1053	rVB5	12008	18158	0.16%	0.017%
20	9.307	1094	1100	1109	rVB	20859	37367	0.33%	0.035%
21	9.542	1132	1140	1154	rBV	1571755	2473161	21.95%	2.291%
22	9.790	1175	1182	1187	rVB7	7550	15643	0.14%	0.014%
23	10.090	1225	1233	1244	rBV	2544803	4029730	35.77%	3.734%
24	10.231	1251	1257	1265	rBV	319530	473533	4.20%	0.439%
25	10.460	1285	1296	1303	rBV	2244810	3500482	31.07%	3.243%
26	10.589	1310	1318	1328	rBV	2280642	3662838	32.51%	3.394%
27	11.248	1427	1430	1437	rBV6	8090	12673	0.11%	0.012%
28	11.789	1516	1522	1526	rBV4	13805	21272	0.19%	0.020%
29	12.048	1561	1566	1575	rVB2	52238	84787	0.75%	0.079%
30	12.272	1597	1604	1608	rBV8	7011	12310	0.11%	0.011%
31	12.672	1667	1672	1677	rVB3	12096	17367	0.15%	0.016%
32	12.919	1709	1714	1718	rBV4	15128	23843	0.21%	0.022%
33	13.154	1749	1754	1757	rBV3	11045	15787	0.14%	0.015%
34	13.213	1761	1764	1768	rVV4	10391	14651	0.13%	0.014%
35	13.272	1771	1774	1781	rVB2	9728	15886	0.14%	0.015%
36	13.713	1842	1849	1855	rBV	4685974	6290195	55.83%	5.828%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032154.D
 Acq On : 25 Sep 2021 15:09
 Operator : CG/JU
 Sample : M3919-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Y4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Title : SVOA CALIBRATION

37	13.960	1887	1891	1892	rBV2	15189	16937	0.15%	0.016%
38	14.001	1892	1898	1909	rVB	5452533	7547856	67.00%	6.993%
39	14.225	1933	1936	1940	rVB5	9328	11829	0.10%	0.011%
40	14.313	1944	1951	1964	rVV	3320113	4671802	41.47%	4.329%
41	14.454	1972	1975	1978	rBV2	10902	12945	0.11%	0.012%
42	14.507	1978	1984	1994	rVV	467388	641570	5.69%	0.594%
43	14.719	2016	2020	2026	rBV8	8423	13138	0.12%	0.012%
44	15.113	2082	2087	2093	rBV	31197	45823	0.41%	0.042%
45	15.166	2093	2096	2101	rVB4	9400	12735	0.11%	0.012%
46	15.301	2112	2119	2130	rBV	6843830	9411998	83.54%	8.721%
47	15.413	2132	2138	2154	rBV	1878887	2478936	22.00%	2.297%
48	15.536	2154	2159	2165	rVB	49451	74849	0.66%	0.069%
49	15.713	2184	2189	2198	rVB2	42659	69535	0.62%	0.064%
50	15.966	2229	2232	2238	rVV6	11281	19214	0.17%	0.018%
51	16.077	2247	2251	2257	rVB4	24610	31286	0.28%	0.029%
52	16.195	2264	2271	2274	rBV8	7841	15064	0.13%	0.014%
53	16.719	2357	2360	2364	rBV4	12990	15663	0.14%	0.015%
54	16.824	2371	2378	2383	rBV2	22940	41734	0.37%	0.039%
55	17.036	2407	2414	2424	rBV	4019382	5379161	47.75%	4.984%
56	17.136	2424	2431	2443	rVV	7371835	10092441	89.58%	9.351%
57	17.224	2443	2446	2452	rVB7	11786	23175	0.21%	0.021%
58	17.401	2473	2476	2483	rVB4	12014	18202	0.16%	0.017%
59	17.707	2524	2528	2533	rVB	34905	43767	0.39%	0.041%
60	17.924	2561	2565	2572	rBV4	29047	54013	0.48%	0.050%
61	17.989	2573	2576	2581	rVB	17151	23647	0.21%	0.022%
62	18.812	2713	2716	2719	rVB4	11757	12958	0.12%	0.012%
63	18.983	2740	2745	2751	rBV2	69480	106242	0.94%	0.098%
64	19.054	2753	2757	2765	rVB	97803	130061	1.15%	0.121%
65	19.307	2797	2800	2804	rVB	29546	34051	0.30%	0.032%
66	19.342	2804	2806	2813	rBV8	9857	16713	0.15%	0.015%
67	19.418	2813	2819	2829	rBV	8424849	11265793	100.00%	10.438%
68	20.901	3067	3071	3076	rBV2	284161	355774	3.16%	0.330%
69	21.195	3116	3121	3128	rBV	4286670	5174808	45.93%	4.795%
70	23.230	3460	3467	3481	rVV	5180941	9309678	82.64%	8.626%
71	23.365	3484	3490	3502	rVB2	2632588	4648976	41.27%	4.307%


Sum of corrected areas: 107928172

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032154.D
Acq On : 25 Sep 2021 15:09
Operator : CG/JU
Sample : M3919-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Y4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

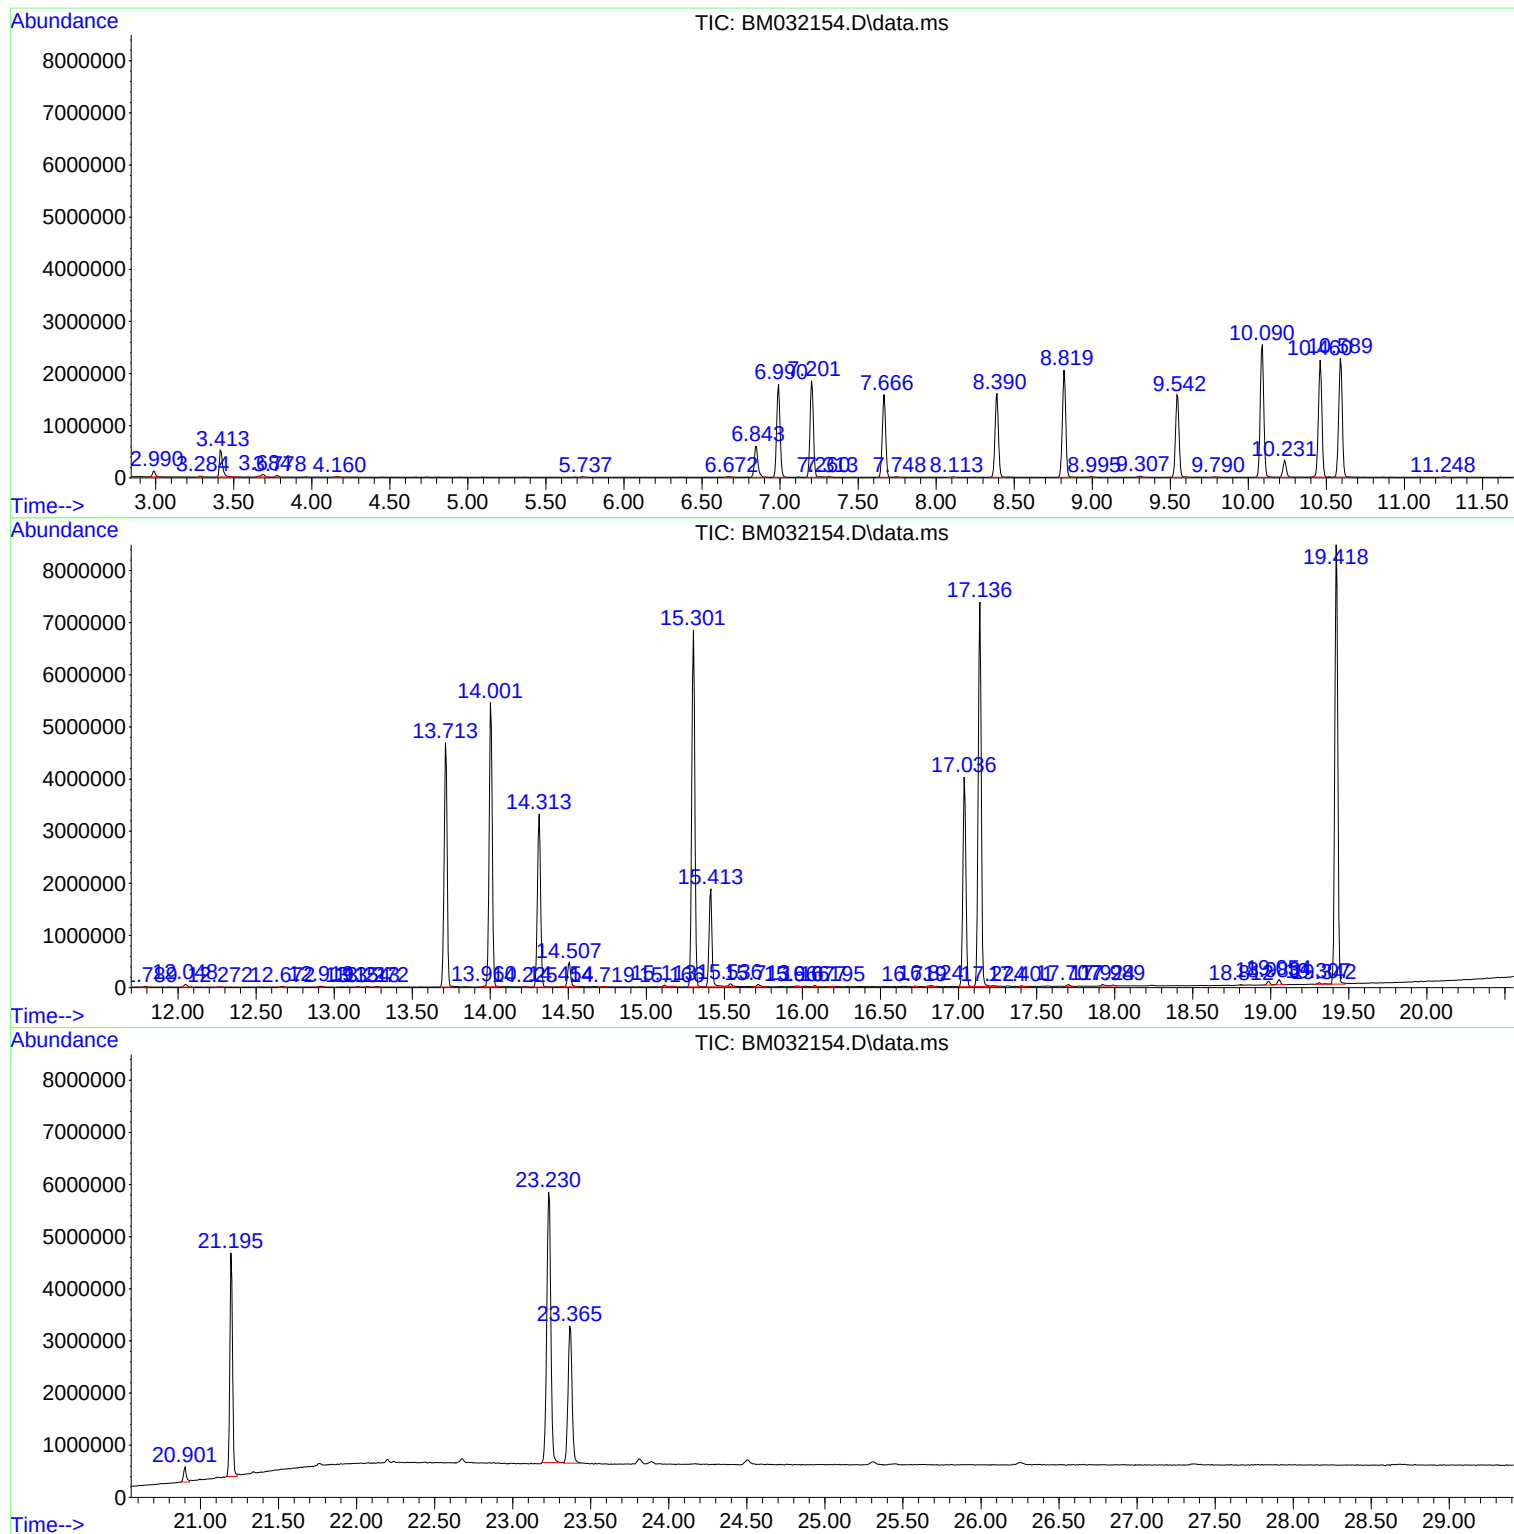

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032154.D
Acq On : 25 Sep 2021 15:09
Operator : CG/JU
Sample : M3919-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Y4










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.231	2.71 ng/ul	473533	Naphthalene-d8	10.460

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
5			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83

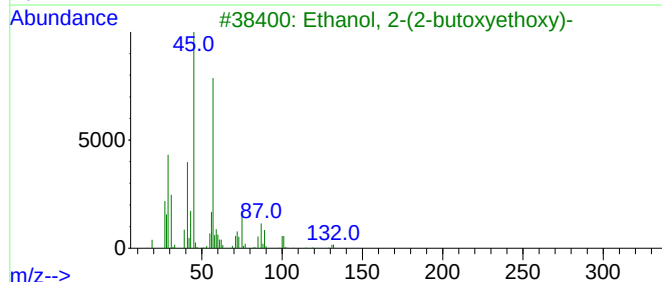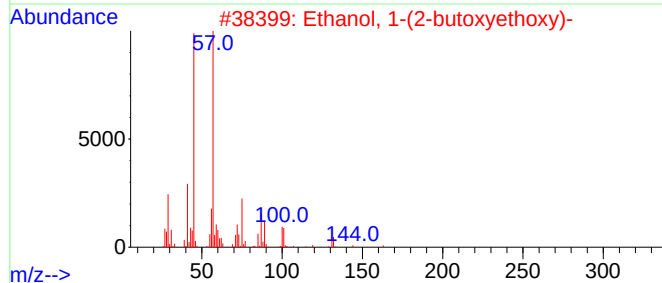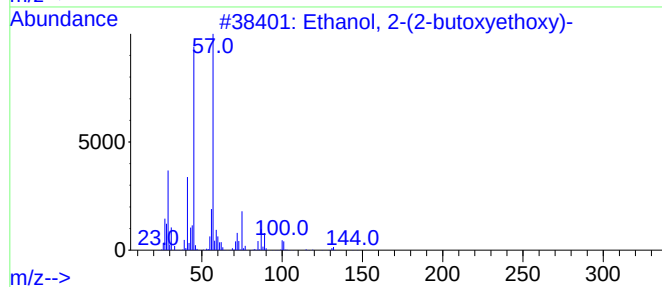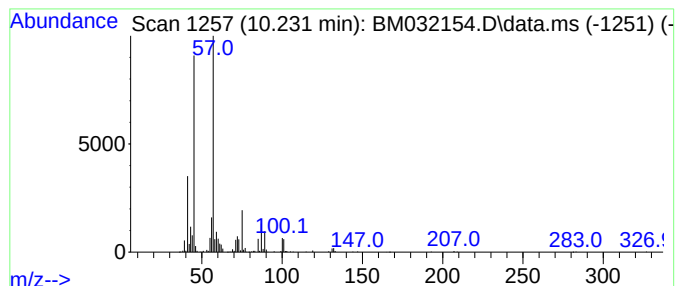

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032154.D
Acq On : 25 Sep 2021 15:09
Operator : CG/JU
Sample : M3919-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Y4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.231	2.7	ng/u1	473533	2	10.460	3500480	20.0