

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032157.D
 Acq On : 25 Sep 2021 16:58
 Operator : CG/JU
 Sample : M3919-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Z2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032157.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.990	22	26	28	rBV	115313	139468	1.36%	0.146%
2	3.025	28	32	43	rVB	327472	429186	4.19%	0.451%
3	3.413	94	98	116	rBV	583978	865301	8.44%	0.908%
4	3.684	140	144	150	rVB	38666	61674	0.60%	0.065%
5	3.778	156	160	165	rVB	22583	33180	0.32%	0.035%
6	4.172	220	227	230	rBV8	5731	11877	0.12%	0.012%
7	5.107	381	386	389	rBV2	9542	12828	0.13%	0.013%
8	5.731	489	492	499	rVB	10780	18941	0.18%	0.020%
9	6.848	676	682	692	rVB	487262	730323	7.12%	0.767%
10	6.990	699	706	715	rVB	1522238	2262198	22.06%	2.375%
11	7.113	724	727	734	rVB7	7410	11286	0.11%	0.012%
12	7.201	734	742	750	rBV	1564988	2320599	22.63%	2.436%
13	7.313	757	761	766	rVB5	9794	12501	0.12%	0.013%
14	7.666	813	821	829	rBV	1359409	2016340	19.66%	2.116%
15	7.742	829	834	842	rVB6	7297	13579	0.13%	0.014%
16	8.389	936	944	953	rBV	1299511	1981365	19.32%	2.080%
17	8.466	953	957	968	rVB10	8403	20140	0.20%	0.021%
18	8.766	1003	1008	1010	rBV3	10013	16209	0.16%	0.017%
19	8.819	1010	1017	1023	rVV	1718703	2567153	25.03%	2.695%
20	8.878	1023	1027	1030	rVB2	17497	26862	0.26%	0.028%
21	8.989	1043	1046	1052	rVB8	7675	13156	0.13%	0.014%
22	9.307	1096	1100	1106	rVB2	19013	31278	0.31%	0.033%
23	9.542	1134	1140	1153	rBV	1280972	2001287	19.52%	2.101%
24	9.789	1174	1182	1188	rBV2	41428	63971	0.62%	0.067%
25	10.089	1224	1233	1244	rBV	2133825	3349829	32.67%	3.516%
26	10.236	1252	1258	1265	rVB4	15841	28089	0.27%	0.029%
27	10.460	1286	1296	1303	rBV	1884702	2990588	29.16%	3.139%
28	10.589	1309	1318	1327	rBV	2083261	3312650	32.30%	3.477%
29	11.095	1400	1404	1412	rVB8	6443	14175	0.14%	0.015%
30	11.683	1495	1504	1511	rVB5	26390	56397	0.55%	0.059%
31	11.795	1518	1523	1533	rVB7	11444	28250	0.28%	0.030%
32	12.048	1559	1566	1573	rVB	46748	77357	0.75%	0.081%
33	12.672	1665	1672	1676	rBV3	12433	18990	0.19%	0.020%
34	12.724	1676	1681	1688	rVB	19835	29012	0.28%	0.030%
35	12.919	1708	1714	1718	rVB	13993	21606	0.21%	0.023%
36	13.154	1750	1754	1759	rVB6	11993	18325	0.18%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032157.D
 Acq On : 25 Sep 2021 16:58
 Operator : CG/JU
 Sample : M3919-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Z2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Title : SVOA CALIBRATION

37	13.277	1771	1775	1780	rVV3	10096	14204	0.14%	0.015%
38	13.360	1782	1789	1796	rVB7	6255	10499	0.10%	0.011%
39	13.713	1841	1849	1855	rBV	4207649	5551560	54.14%	5.827%
40	13.760	1855	1857	1866	rVB7	11354	26444	0.26%	0.028%
41	14.001	1887	1898	1911	rBV	4684930	6541002	63.78%	6.866%
42	14.313	1944	1951	1963	rVV	2913272	3984822	38.86%	4.183%
43	14.507	1978	1984	1989	rBV	408180	552376	5.39%	0.580%
44	14.554	1989	1992	1997	rVB2	44066	65724	0.64%	0.069%
45	14.724	2017	2021	2024	rBV6	11580	15500	0.15%	0.016%
46	14.924	2051	2055	2058	rBV	11554	14450	0.14%	0.015%
47	15.042	2071	2075	2082	rVB4	15782	27421	0.27%	0.029%
48	15.118	2083	2088	2092	rVV2	42081	56743	0.55%	0.060%
49	15.301	2112	2119	2132	rBV	6081474	8415342	82.06%	8.833%
50	15.413	2132	2138	2154	rVV	1680324	2180957	21.27%	2.289%
51	15.536	2155	2159	2167	rVV	51741	104129	1.02%	0.109%
52	15.595	2167	2169	2175	rVV5	14471	23009	0.22%	0.024%
53	15.660	2175	2180	2186	rVV	18701	33080	0.32%	0.035%
54	15.718	2186	2190	2198	rVB10	4447	11521	0.11%	0.012%
55	15.965	2225	2232	2239	rBV10	14757	34662	0.34%	0.036%
56	16.030	2239	2243	2247	rVV6	10271	20732	0.20%	0.022%
57	16.077	2247	2251	2256	rVB3	21613	31015	0.30%	0.033%
58	16.301	2284	2289	2293	rVB3	18634	24564	0.24%	0.026%
59	16.395	2296	2305	2309	rVV3	19415	44421	0.43%	0.047%
60	16.448	2311	2314	2319	rVB6	7949	11106	0.11%	0.012%
61	16.718	2357	2360	2365	rVB6	13509	15605	0.15%	0.016%
62	16.824	2372	2378	2382	rBV	16588	31207	0.30%	0.033%
63	17.036	2406	2414	2422	rBV	3418993	4543559	44.31%	4.769%
64	17.136	2424	2431	2443	rBV	6912709	9222028	89.93%	9.680%
65	17.312	2459	2461	2466	rVB	10201	12475	0.12%	0.013%
66	17.407	2473	2477	2483	rVB5	11159	20738	0.20%	0.022%
67	17.701	2524	2527	2531	rBV5	10383	14578	0.14%	0.015%
68	17.924	2561	2565	2568	rBV2	43277	53591	0.52%	0.056%
69	17.989	2573	2576	2580	rVB	37603	47315	0.46%	0.050%
70	18.783	2707	2711	2714	rBV6	9082	18141	0.18%	0.019%
71	18.983	2741	2745	2749	rBV	66791	86705	0.85%	0.091%
72	19.053	2753	2757	2762	rVV	87643	115506	1.13%	0.121%
73	19.306	2797	2800	2804	rVB	23716	27445	0.27%	0.029%
74	19.418	2813	2819	2830	rBV	7752751	10254954	100.00%	10.764%
75	20.448	2992	2994	2998	rVB3	41815	45985	0.45%	0.048%
76	20.900	3068	3071	3077	rBV3	179810	244194	2.38%	0.256%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032157.D
Acq On : 25 Sep 2021 16:58
Operator : CG/JU
Sample : M3919-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Z2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Title : SVOA CALIBRATION

77	21.106	3103	3106	3110	rBV	493409	510225	4.98%	0.536%
78	21.195	3116	3121	3130	rBV	3487968	4323358	42.16%	4.538%
79	23.230	3460	3467	3482	rVB	4760634	8460248	82.50%	8.880%
80	23.365	3485	3490	3503	rVB2	2172241	3819227	37.24%	4.009%




Sum of corrected areas: 95268337

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032157.D
Acq On : 25 Sep 2021 16:58
Operator : CG/JU
Sample : M3919-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Z2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

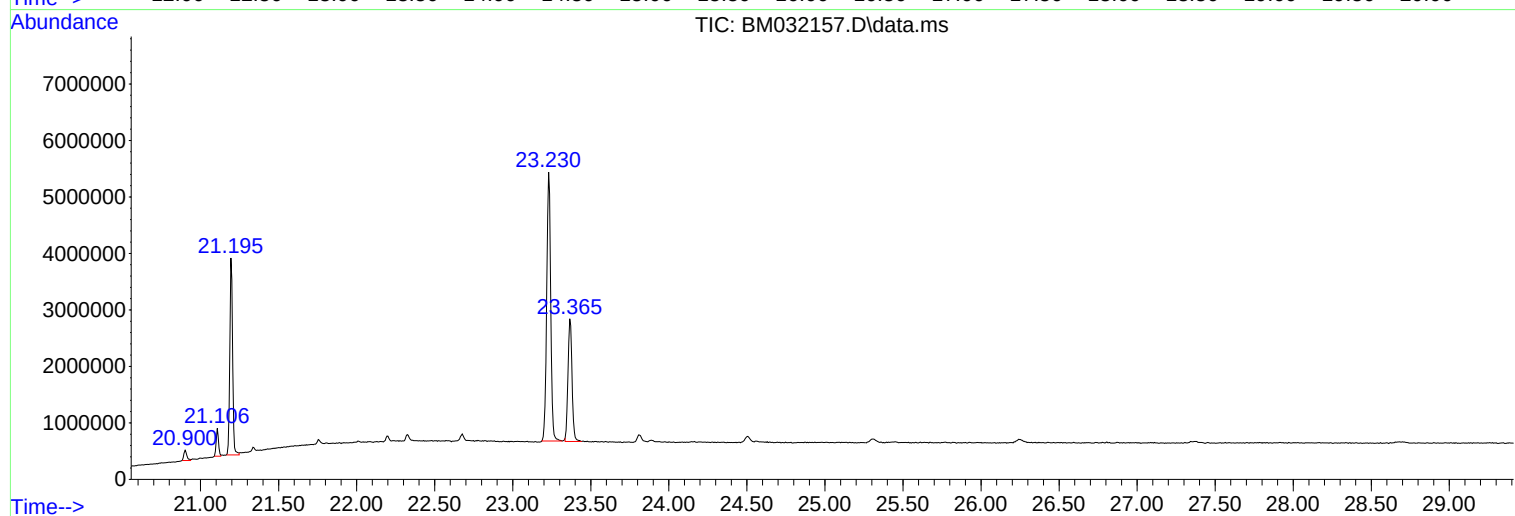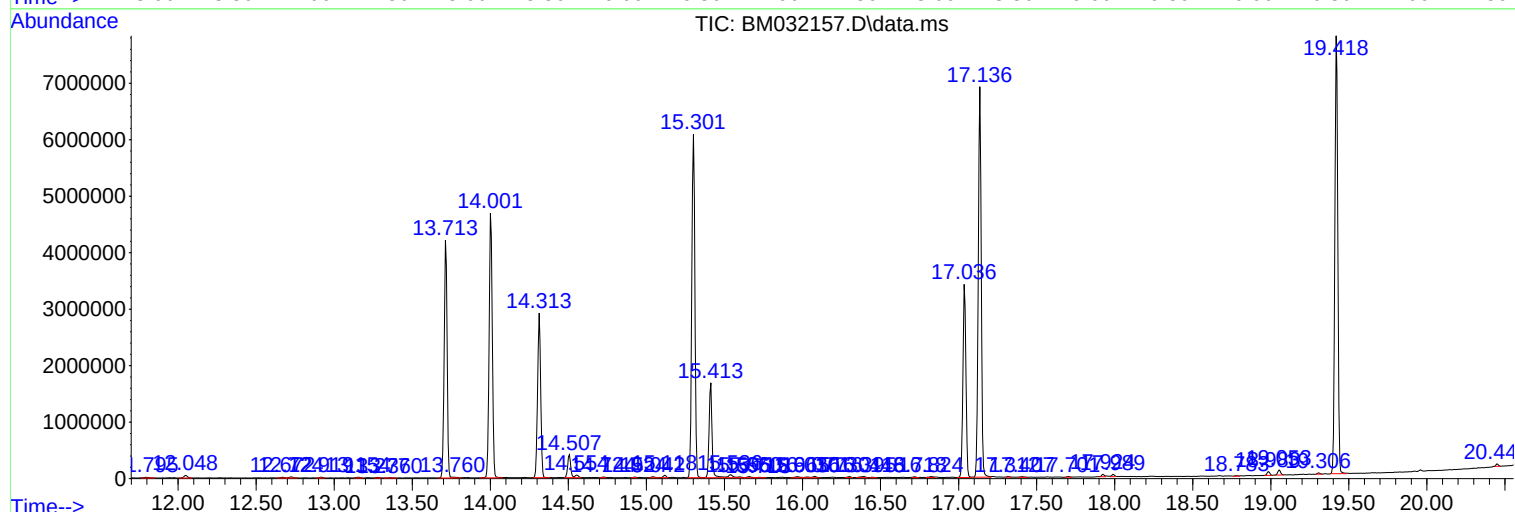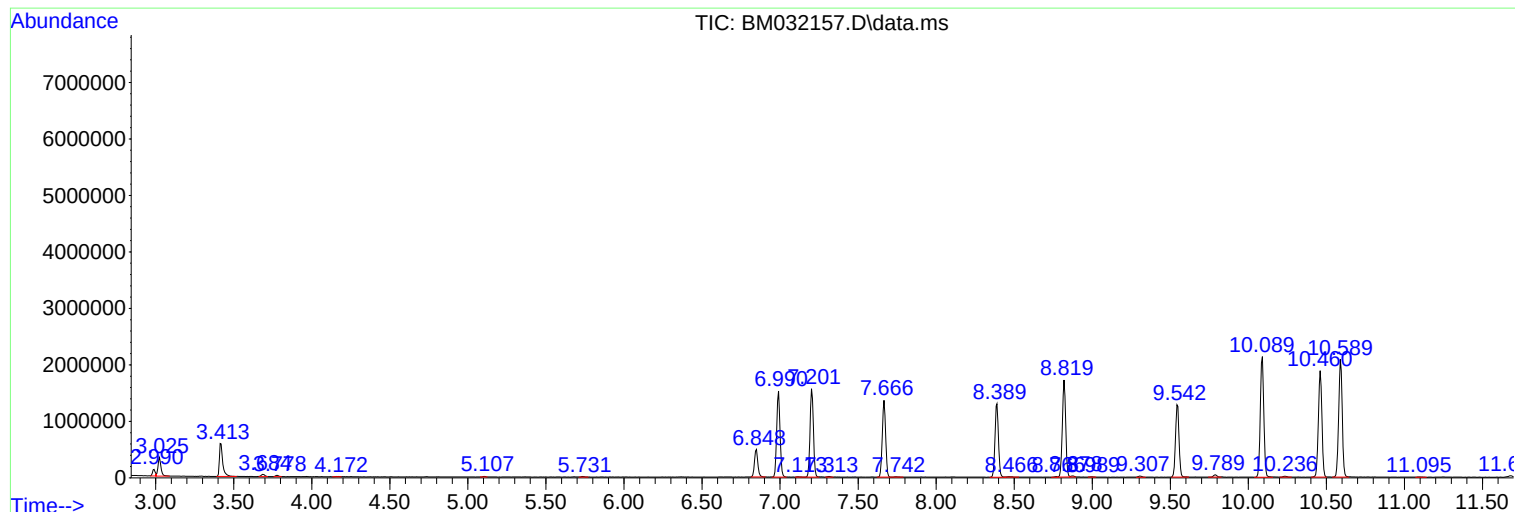

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032157.D
Acq On : 25 Sep 2021 16:58
Operator : CG/JU
Sample : M3919-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Z2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032157.D
Acq On : 25 Sep 2021 16:58
Operator : CG/JU
Sample : M3919-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Z2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------