

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032162.D
 Acq On : 25 Sep 2021 20:36
 Operator : CG/JU
 Sample : PB139361BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK361

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.984	21	25	39	rVB	102149	146244	1.54%	0.154%
2	3.413	94	98	120	rBV	1393769	2014108	21.23%	2.126%
3	3.778	154	160	166	rBV	25421	38795	0.41%	0.041%
4	4.807	330	335	340	rVB4	6306	11519	0.12%	0.012%
5	6.848	675	682	689	rBV	1641850	2421029	25.51%	2.555%
6	6.989	698	706	716	rVB	1302008	1977140	20.84%	2.087%
7	7.201	733	742	754	rBV	1640857	2495577	26.30%	2.634%
8	7.666	813	821	828	rVB	1291859	1947930	20.53%	2.056%
9	8.389	936	944	956	rBV	2040864	3082084	32.48%	3.253%
10	8.819	1010	1017	1028	rBV	1475273	2266527	23.89%	2.392%
11	9.542	1133	1140	1155	rBV	1196666	1850367	19.50%	1.953%
12	10.089	1222	1233	1245	rBV	1982886	3160286	33.31%	3.336%
13	10.460	1289	1296	1306	rVB	1816967	2904267	30.61%	3.066%
14	10.589	1310	1318	1326	rBV	2079022	3279027	34.56%	3.461%
15	12.048	1558	1566	1573	rVB2	38763	63841	0.67%	0.067%
16	13.277	1772	1775	1780	rVB3	6799	9960	0.10%	0.011%
17	13.713	1843	1849	1855	rBV	3568596	4663118	49.14%	4.922%
18	13.754	1855	1856	1861	rVB5	9628	9740	0.10%	0.010%
19	14.001	1891	1898	1918	rBV	4243355	5686846	59.93%	6.003%
20	14.313	1944	1951	1959	rBV	2875509	3976520	41.91%	4.197%
21	14.507	1977	1984	1997	rBV	1677304	2212919	23.32%	2.336%
22	15.301	2111	2119	2127	rBV	5139883	7055504	74.36%	7.447%
23	15.407	2132	2137	2148	rBV	1294205	1709142	18.01%	1.804%
24	15.536	2155	2159	2163	rVB	38851	54583	0.58%	0.058%
25	15.965	2227	2232	2237	rBV8	8048	14291	0.15%	0.015%
26	16.077	2247	2251	2255	rBV5	14065	18820	0.20%	0.020%
27	16.824	2374	2378	2383	rVB	13886	18274	0.19%	0.019%
28	17.036	2408	2414	2421	rBV	3509803	4679978	49.32%	4.940%
29	17.136	2424	2431	2443	rBV	5524520	7684723	80.99%	8.111%
30	18.983	2741	2745	2750	rBV	53675	64040	0.67%	0.068%
31	19.053	2752	2757	2766	rVB	69873	99409	1.05%	0.105%
32	19.306	2797	2800	2803	rBV	16285	17373	0.18%	0.018%
33	19.418	2813	2819	2829	rBV	6951416	8985889	94.70%	9.485%
34	21.194	3116	3121	3129	rBV	4482062	5242797	55.25%	5.534%
35	23.230	3459	3467	3482	rVB	5367398	9488668	100.00%	10.015%
36	23.365	3484	3490	3505	rVB2	3025889	5388990	56.79%	5.688%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032162.D
Acq On : 25 Sep 2021 20:36
Operator : CG/JU
Sample : PB139361BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK361

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Title : SVOA CALIBRATION




Sum of corrected areas: 94740325

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032162.D
Acq On : 25 Sep 2021 20:36
Operator : CG/JU
Sample : PB139361BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK361

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

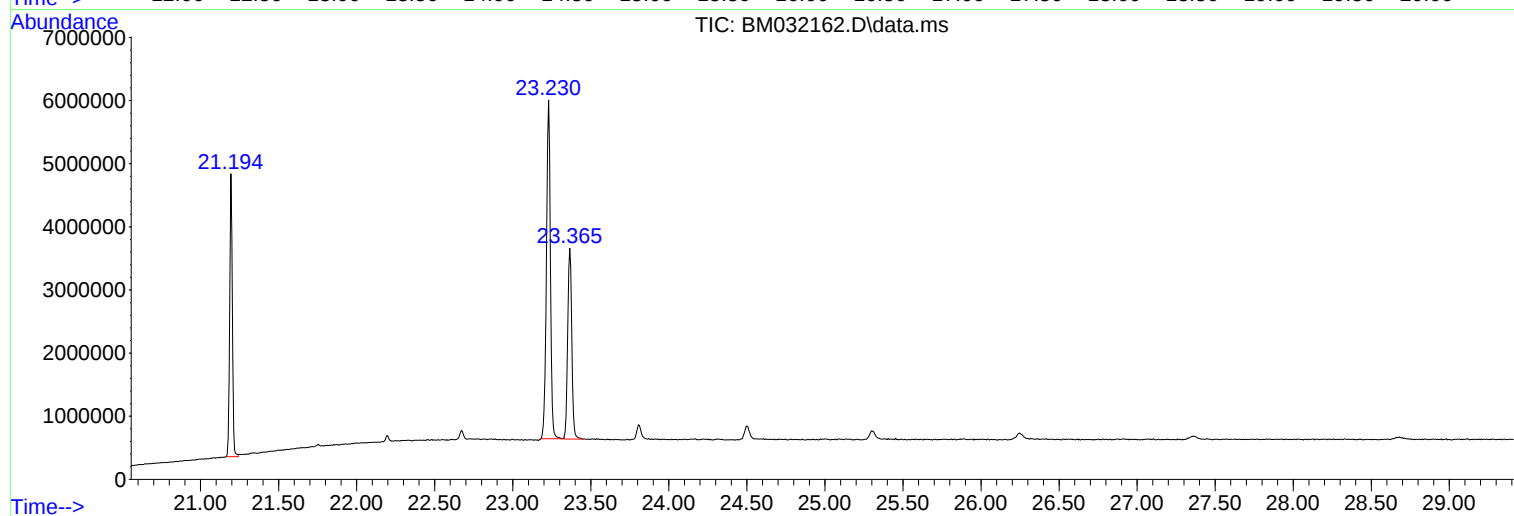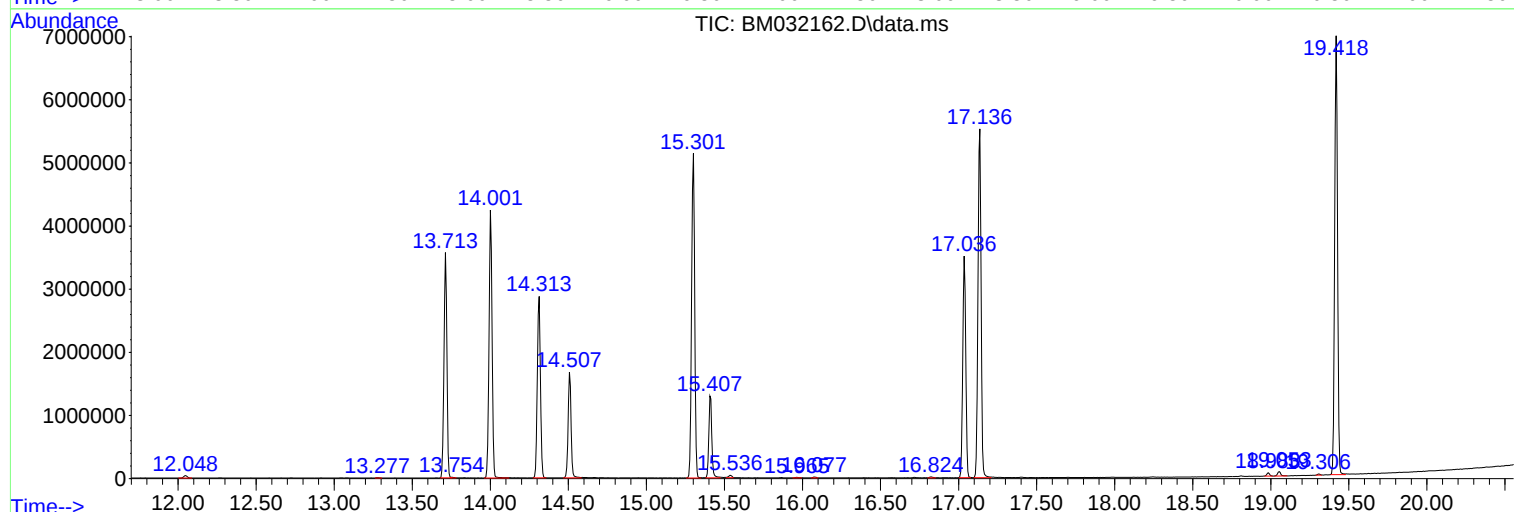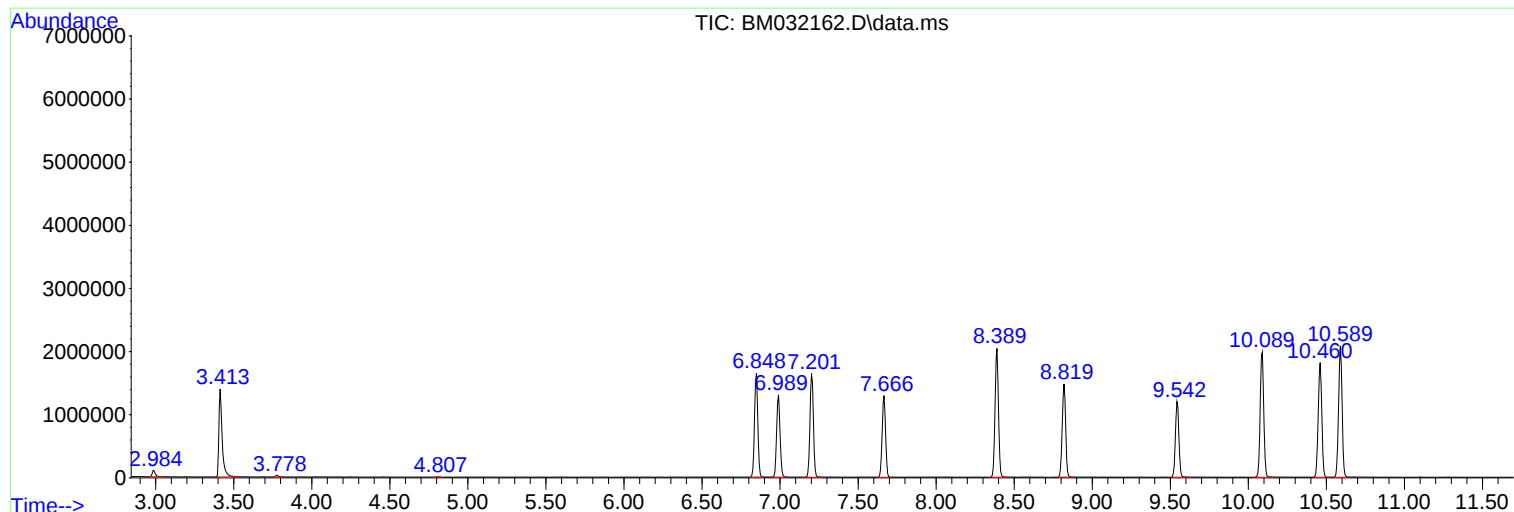

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032162.D
Acq On : 25 Sep 2021 20:36
Operator : CG/JU
Sample : PB139361BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK361

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032162.D
Acq On : 25 Sep 2021 20:36
Operator : CG/JU
Sample : PB139361BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK361

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
