

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032163.D
 Acq On : 25 Sep 2021 21:12
 Operator : CG/JU
 Sample : PB139144BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK144

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.984	21	25	34	rVB	127223	171746	1.55%	0.156%
2	3.413	94	98	116	rBV	1681763	2451226	22.18%	2.233%
3	3.778	154	160	168	rVB	27413	41480	0.38%	0.038%
4	6.848	675	682	693	rBV	1988180	2970467	26.88%	2.707%
5	6.990	697	706	716	rVB	1601941	2421679	21.91%	2.207%
6	7.201	735	742	752	rBV	2029769	3029211	27.41%	2.760%
7	7.666	814	821	829	rVB	1290391	1946367	17.61%	1.773%
8	8.389	936	944	953	rBV	2488787	3771339	34.13%	3.436%
9	8.819	1009	1017	1025	rBV	1824583	2789313	25.24%	2.542%
10	9.542	1133	1140	1155	rBV	1476069	2279627	20.63%	2.077%
11	10.083	1225	1232	1243	rBV	2403533	3861053	34.94%	3.518%
12	10.460	1289	1296	1305	rVB	1809955	2891339	26.16%	2.635%
13	10.589	1309	1318	1329	rBV	2528489	4009331	36.28%	3.653%
14	12.048	1560	1566	1574	rVB	51101	76492	0.69%	0.070%
15	13.277	1768	1775	1782	rVB3	7704	13198	0.12%	0.012%
16	13.713	1842	1849	1855	rBV	4456731	5720872	51.77%	5.213%
17	13.754	1855	1856	1863	rVB4	11308	16356	0.15%	0.015%
18	14.001	1891	1898	1909	rBV	4863210	6917627	62.60%	6.303%
19	14.313	1944	1951	1960	rBV	2830364	3938663	35.64%	3.589%
20	14.507	1977	1984	1998	rBV	2013941	2764543	25.02%	2.519%
21	15.301	2112	2119	2130	rBV	6330836	8548510	77.35%	7.789%
22	15.413	2132	2138	2150	rBV	1671514	2188274	19.80%	1.994%
23	15.536	2155	2159	2168	rVB	50338	72134	0.65%	0.066%
24	15.965	2227	2232	2236	rBV7	9533	16923	0.15%	0.015%
25	16.083	2246	2252	2256	rBV5	22433	33462	0.30%	0.030%
26	16.718	2355	2360	2367	rBV5	9548	14557	0.13%	0.013%
27	16.824	2375	2378	2383	rVB2	14234	18158	0.16%	0.017%
28	17.036	2408	2414	2422	rBV	3474346	4650599	42.08%	4.238%
29	17.136	2424	2431	2449	rBV	6716765	9440052	85.42%	8.602%
30	17.401	2471	2476	2481	rBV3	9594	12226	0.11%	0.011%
31	17.701	2524	2527	2534	rVB7	16252	22090	0.20%	0.020%
32	18.812	2712	2716	2721	rBV5	13771	19423	0.18%	0.018%
33	18.983	2741	2745	2750	rBV2	65249	82881	0.75%	0.076%
34	19.053	2752	2757	2764	rVV	86577	121205	1.10%	0.110%
35	19.306	2797	2800	2804	rBV	24287	32744	0.30%	0.030%
36	19.418	2813	2819	2829	rBV	8154255	10898701	98.62%	9.931%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032163.D
Acq On : 25 Sep 2021 21:12
Operator : CG/JU
Sample : PB139144BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK144

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Title : SVOA CALIBRATION

37	21.195	3116	3121	3129	rBV	4321802	5163254	46.72%	4.705%
38	23.230	3460	3467	3479	rVB2	6213704	11051123	100.00%	10.070%
39	23.365	3484	3490	3507	rVB2	3034511	5280038	47.78%	4.811%




Sum of corrected areas: 109748283

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032163.D
Acq On : 25 Sep 2021 21:12
Operator : CG/JU
Sample : PB139144BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK144

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

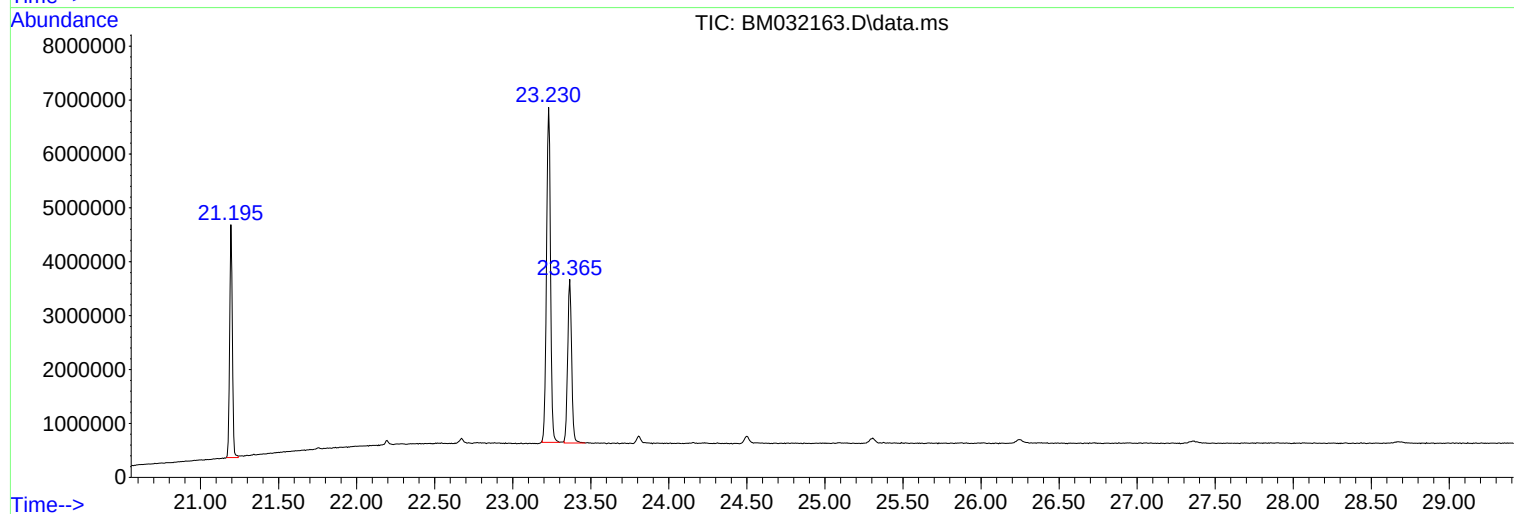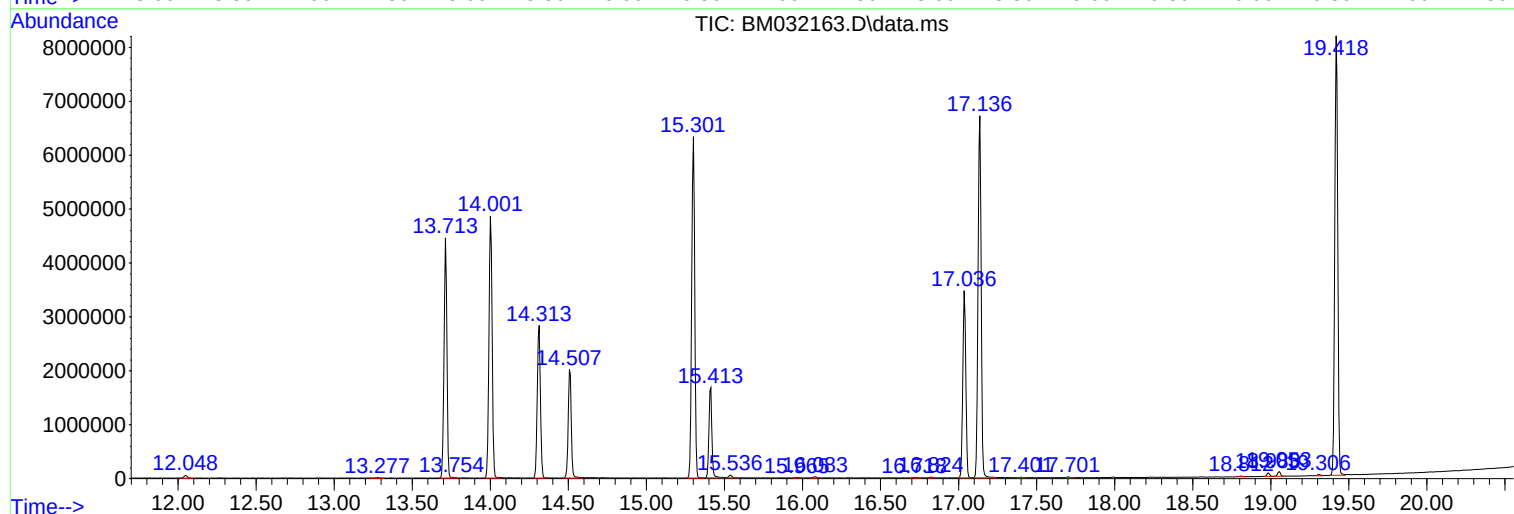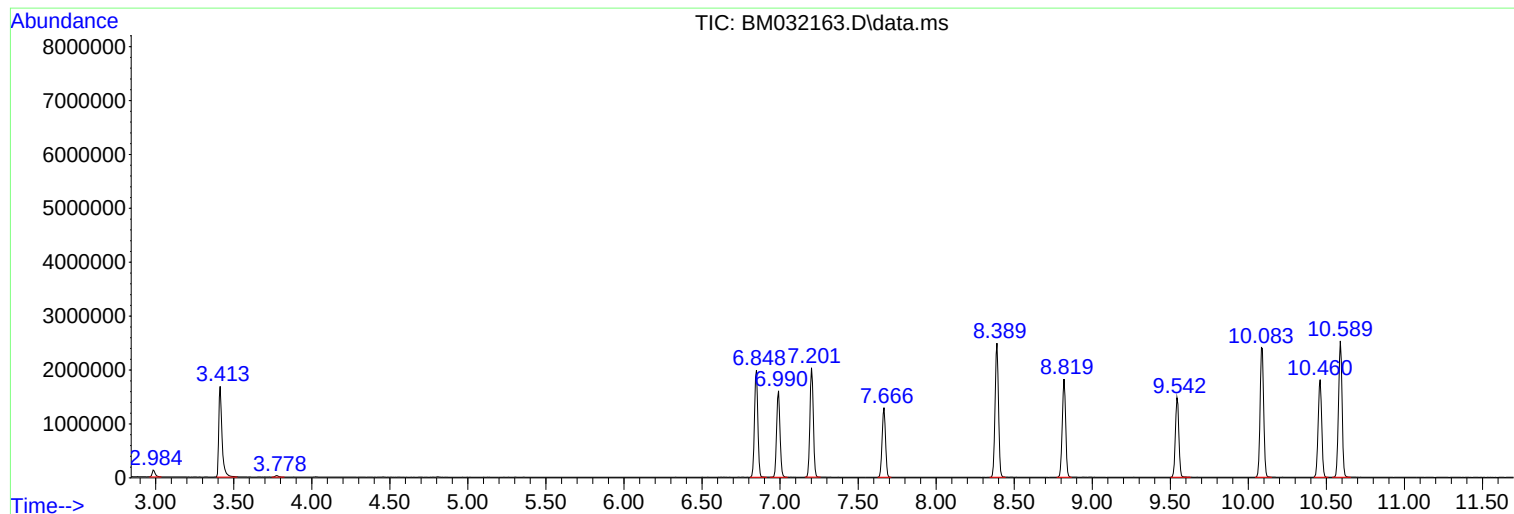

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032163.D
Acq On : 25 Sep 2021 21:12
Operator : CG/JU
Sample : PB139144BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK144

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032163.D
Acq On : 25 Sep 2021 21:12
Operator : CG/JU
Sample : PB139144BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK144

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
