

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032175.D
 Acq On : 26 Sep 2021 04:29
 Operator : CG/JU
 Sample : M3919-17
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Z6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032175.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.990	22	26	32	rVB	111090	136081	1.74%	0.181%
2	3.419	95	99	118	rBV	269194	398580	5.09%	0.530%
3	3.690	138	145	153	rVB	43593	71635	0.91%	0.095%
4	3.778	156	160	166	rVB	26035	34471	0.44%	0.046%
5	6.842	675	681	690	rVB	411950	615357	7.85%	0.818%
6	6.989	698	706	715	rBV	1457428	2231008	28.47%	2.964%
7	7.201	735	742	751	rBV	1484644	2205743	28.14%	2.931%
8	7.313	756	761	765	rVB3	9982	14185	0.18%	0.019%
9	7.666	814	821	828	rBV	1369997	2079453	26.53%	2.763%
10	8.383	937	943	953	rBV	1130821	1684891	21.50%	2.239%
11	8.478	954	959	967	rVB2	10441	18135	0.23%	0.024%
12	8.819	1008	1017	1024	rBV	1564977	2438401	31.11%	3.240%
13	8.995	1041	1047	1049	rVB6	6912	9668	0.12%	0.013%
14	9.066	1053	1059	1065	rVB	18264	29310	0.37%	0.039%
15	9.136	1065	1071	1077	rBV	25178	36377	0.46%	0.048%
16	9.301	1094	1099	1106	rVB2	18034	31304	0.40%	0.042%
17	9.542	1132	1140	1150	rBV	885972	1318952	16.83%	1.752%
18	10.083	1225	1232	1241	rBV	1878966	2905800	37.08%	3.861%
19	10.460	1284	1296	1305	rBV	1743304	2817675	35.95%	3.744%
20	10.589	1310	1318	1328	rBV	1223535	1940747	24.76%	2.579%
21	11.083	1397	1402	1411	rVB6	10753	23605	0.30%	0.031%
22	11.183	1414	1419	1424	rBV2	8822	16184	0.21%	0.022%
23	11.242	1428	1429	1436	rVV7	7135	10102	0.13%	0.013%
24	11.307	1436	1440	1445	rVB2	11286	17006	0.22%	0.023%
25	11.783	1515	1521	1528	rBV4	8046	16264	0.21%	0.022%
26	12.048	1560	1566	1571	rVB	39499	64613	0.82%	0.086%
27	12.266	1598	1603	1610	rVB7	5022	8098	0.10%	0.011%
28	12.666	1666	1671	1675	rVV7	8836	12852	0.16%	0.017%
29	12.913	1707	1713	1717	rBV3	10651	15237	0.19%	0.020%
30	13.036	1729	1734	1739	rBV7	4572	7948	0.10%	0.011%
31	13.218	1757	1765	1767	rBV9	5391	9816	0.13%	0.013%
32	13.271	1771	1774	1781	rVB4	7379	12503	0.16%	0.017%
33	13.713	1842	1849	1855	rBV	3075890	4156981	53.04%	5.523%
34	14.001	1887	1898	1911	rBV	3795066	5230170	66.73%	6.949%
35	14.312	1944	1951	1958	rBV	2316887	3384459	43.18%	4.497%
36	14.501	1978	1983	1995	rBV	136148	203943	2.60%	0.271%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032175.D
 Acq On : 26 Sep 2021 04:29
 Operator : CG/JU
 Sample : M3919-17
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Z6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Title : SVOA CALIBRATION

37	14.712	2017	2019	2024	rBV6	6869	10400	0.13%	0.014%
38	15.112	2082	2087	2092	rBV	37663	47599	0.61%	0.063%
39	15.295	2112	2118	2127	rBV	4610840	6404677	81.72%	8.510%
40	15.407	2132	2137	2149	rBV	451367	605462	7.73%	0.804%
41	15.536	2154	2159	2163	rVV	37693	57903	0.74%	0.077%
42	15.595	2163	2169	2173	rVV8	6105	11631	0.15%	0.015%
43	15.654	2175	2179	2186	rVV2	14119	20537	0.26%	0.027%
44	15.748	2189	2195	2201	rVB5	9596	14897	0.19%	0.020%
45	15.965	2227	2232	2238	rBV9	8007	15083	0.19%	0.020%
46	16.077	2246	2251	2257	rVB4	12844	17226	0.22%	0.023%
47	16.518	2320	2326	2329	rBV6	3855	9866	0.13%	0.013%
48	16.642	2341	2347	2352	rBV2	20054	28562	0.36%	0.038%
49	16.718	2356	2360	2363	rBV5	8287	9198	0.12%	0.012%
50	16.824	2373	2378	2384	rVB	12984	18841	0.24%	0.025%
51	17.036	2408	2414	2424	rVB	2693938	3606147	46.01%	4.791%
52	17.130	2424	2430	2441	rBV2	5197960	7150718	91.24%	9.501%
53	17.318	2458	2462	2466	rVB4	7929	11861	0.15%	0.016%
54	17.406	2473	2477	2480	rVB4	8319	10929	0.14%	0.015%
55	17.700	2522	2527	2533	rBV2	74382	93157	1.19%	0.124%
56	17.989	2572	2576	2580	rBV2	11499	16599	0.21%	0.022%
57	18.983	2741	2745	2751	rVB2	43394	55782	0.71%	0.074%
58	19.053	2752	2757	2761	rBV	59470	82962	1.06%	0.110%
59	19.418	2813	2819	2830	rBV	6106835	7837448	100.00%	10.414%
60	21.194	3116	3121	3130	rBV	2966081	3619537	46.18%	4.809%
61	23.224	3460	3466	3480	rVB2	4317032	7639435	97.47%	10.150%
62	23.359	3484	3489	3502	rVB2	2091452	3657735	46.67%	4.860%




Sum of corrected areas: 75261746

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032175.D
Acq On : 26 Sep 2021 04:29
Operator : CG/JU
Sample : M3919-17
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Z6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

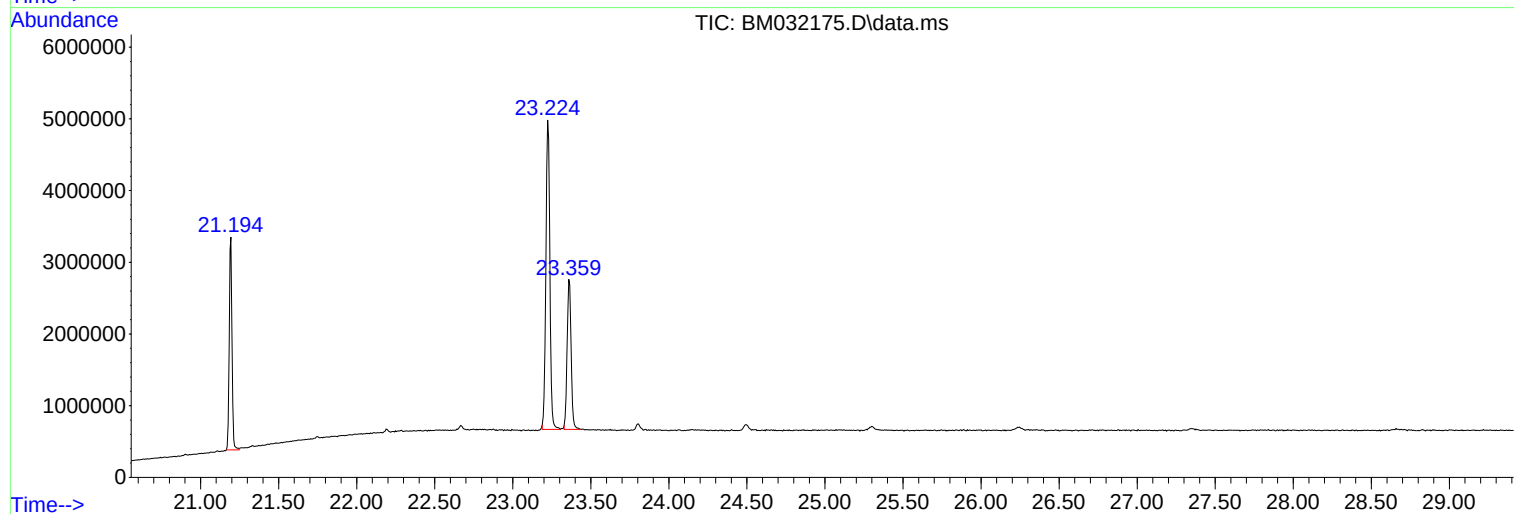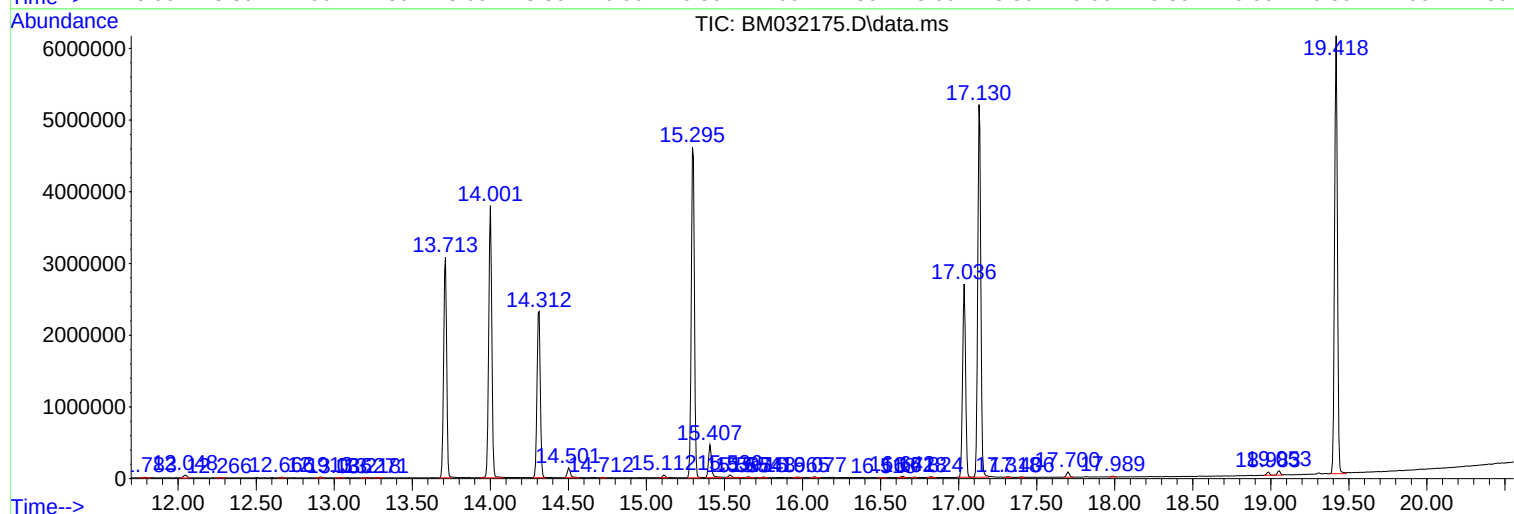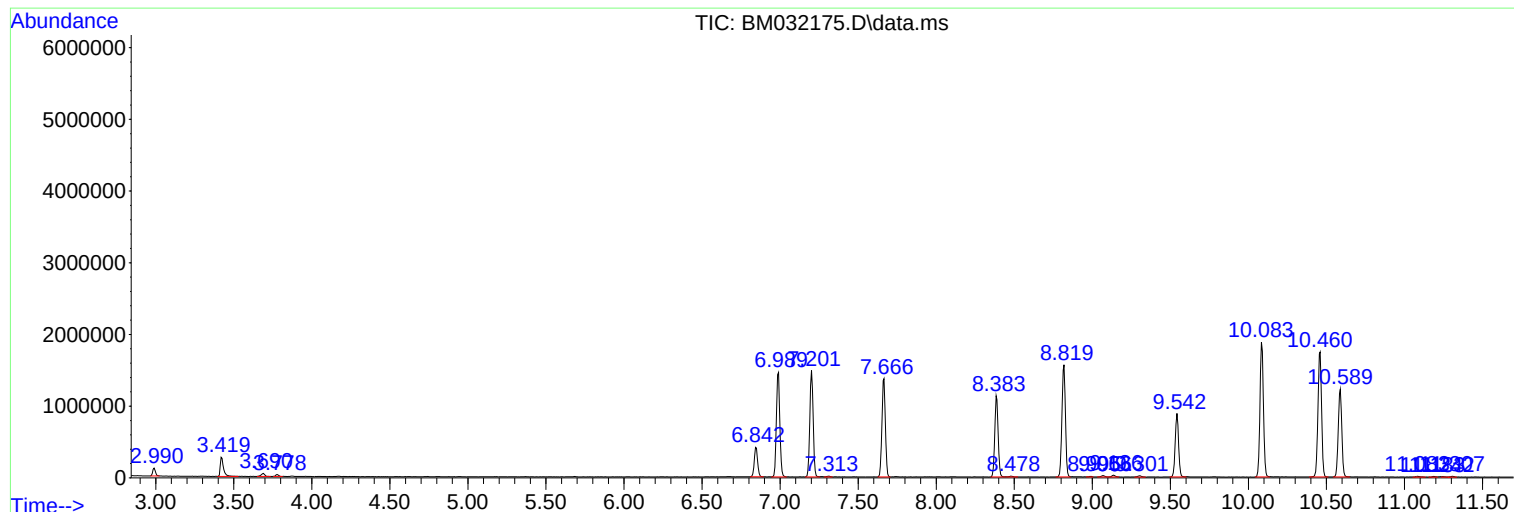

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032175.D
Acq On : 26 Sep 2021 04:29
Operator : CG/JU
Sample : M3919-17
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Z6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032175.D
Acq On : 26 Sep 2021 04:29
Operator : CG/JU
Sample : M3919-17
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Z6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc