

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032179.D
 Acq On : 26 Sep 2021 07:29
 Operator : CG/JU
 Sample : PB139167BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK167

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032179.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.990	22	26	35	rVB	132759	165508	2.36%	0.194%
2	3.413	94	98	116	rBV	1687734	2255339	32.13%	2.644%
3	3.778	154	160	166	rBV	27656	40348	0.57%	0.047%
4	4.807	332	335	341	rVB6	5618	8145	0.12%	0.010%
5	6.843	674	681	690	rBV	1753653	2618173	37.29%	3.069%
6	6.984	698	705	715	rVB	1404186	2128177	30.31%	2.495%
7	7.201	734	742	751	rBV	1844725	2735658	38.97%	3.207%
8	7.660	813	820	828	rVB	1624542	2473804	35.24%	2.900%
9	8.384	936	943	952	rBV	2142993	3176916	45.25%	3.724%
10	8.813	1009	1016	1025	rBV	1491038	2324934	33.12%	2.726%
11	9.542	1132	1140	1150	rBV	1212776	1846555	26.30%	2.165%
12	10.084	1225	1232	1241	rBV	2084068	3176693	45.25%	3.724%
13	10.454	1287	1295	1304	rVB	2110388	3330713	47.44%	3.905%
14	10.589	1309	1318	1334	rBV	2000973	3195934	45.52%	3.747%
15	12.042	1559	1565	1571	rVB	38375	58955	0.84%	0.069%
16	13.278	1770	1775	1779	rBV5	5990	8743	0.12%	0.010%
17	13.707	1842	1848	1854	rBV	3012935	4047821	57.66%	4.745%
18	13.754	1854	1856	1861	rVB4	8840	10380	0.15%	0.012%
19	14.001	1891	1898	1912	rBV	3565948	5090241	72.51%	5.967%
20	14.307	1943	1950	1960	rBV	2862657	4018288	57.24%	4.711%
21	14.507	1977	1984	1998	rBV	1338282	1777428	25.32%	2.084%
22	15.295	2111	2118	2128	rBV	4533385	6163691	87.80%	7.226%
23	15.407	2131	2137	2150	rBV	1069421	1384976	19.73%	1.624%
24	15.536	2155	2159	2168	rVB	33594	49985	0.71%	0.059%
25	15.960	2226	2231	2236	rBV8	7408	10888	0.16%	0.013%
26	16.071	2246	2250	2255	rBV8	8950	14706	0.21%	0.017%
27	16.713	2356	2359	2363	rBV6	6160	8289	0.12%	0.010%
28	16.818	2372	2377	2383	rVB	13136	20348	0.29%	0.024%
29	17.036	2407	2414	2423	rBV	3124535	4291716	61.13%	5.031%
30	17.130	2423	2430	2445	rBV	4771590	6378206	90.85%	7.477%
31	17.395	2472	2475	2478	rBV3	7437	9395	0.13%	0.011%
32	18.977	2741	2744	2750	rBV2	38330	57834	0.82%	0.068%
33	19.048	2752	2756	2761	rBV	52546	72937	1.04%	0.086%
34	19.418	2813	2819	2831	rBV	5254388	7020365	100.00%	8.230%
35	21.195	3116	3121	3127	rBV	3485809	4275442	60.90%	5.012%
36	23.224	3460	3466	3481	rVB	4000534	6668799	94.99%	7.818%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032179.D
Acq On : 26 Sep 2021 07:29
Operator : CG/JU
Sample : PB139167BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK167

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Title : SVOA CALIBRATION

37 23.359 3483 3489 3503 rVB2 2532530 4385374 62.47% 5.141%




Sum of corrected areas: 85301704

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032179.D
Acq On : 26 Sep 2021 07:29
Operator : CG/JU
Sample : PB139167BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK167

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

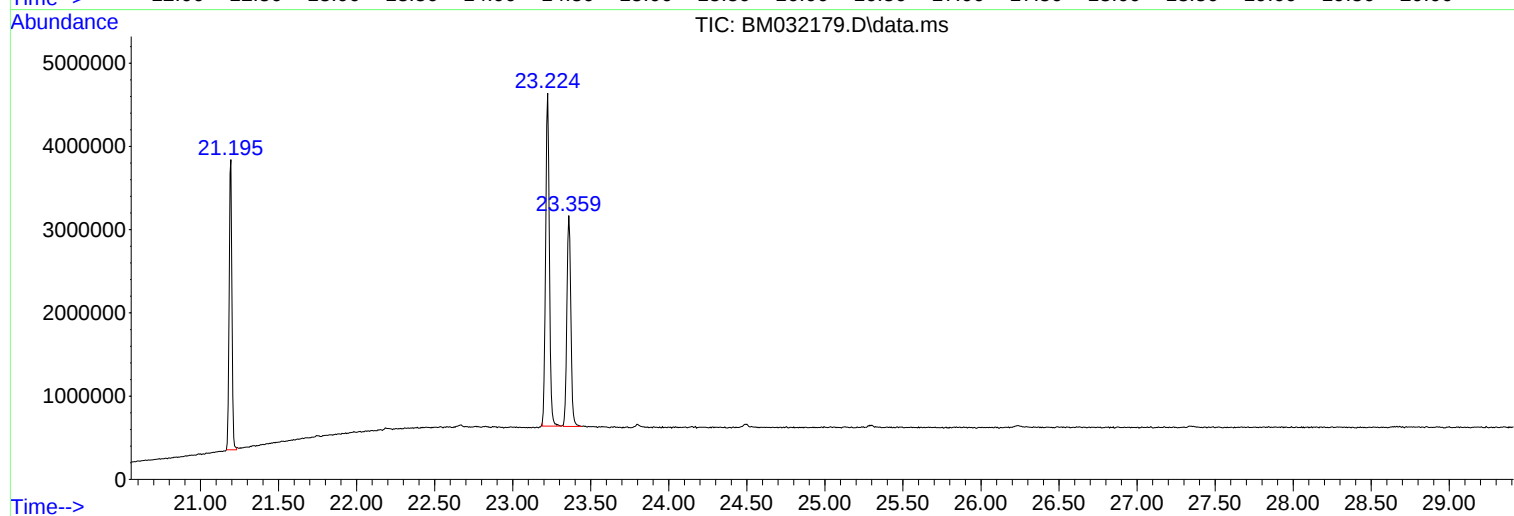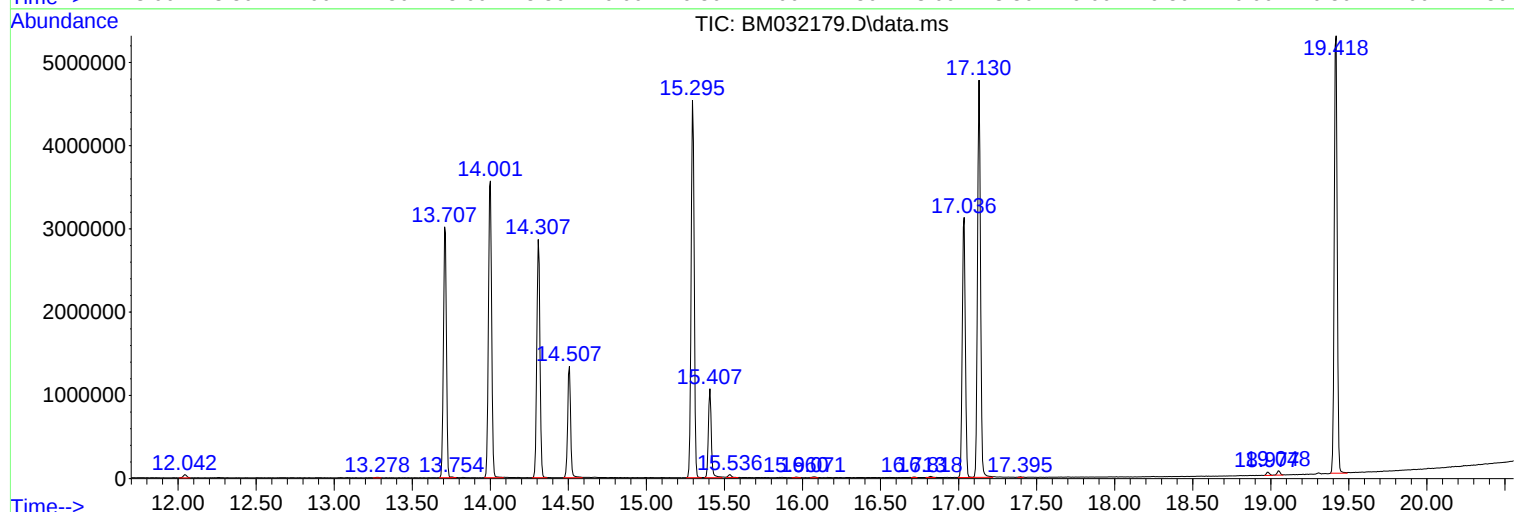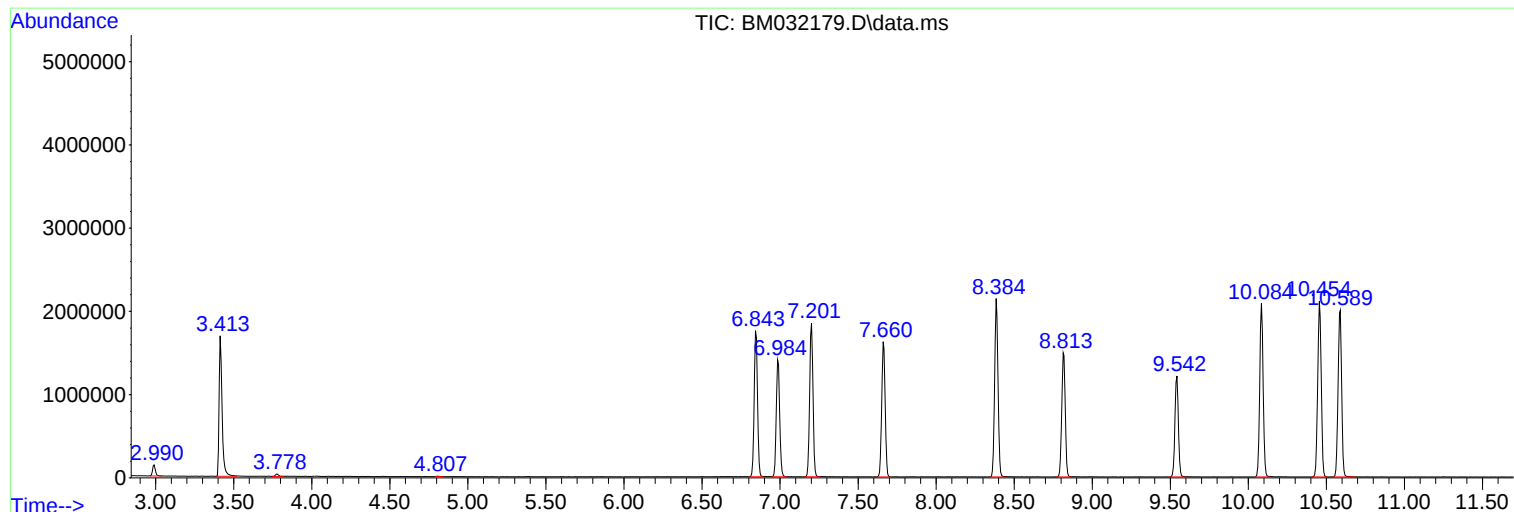

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032179.D
Acq On : 26 Sep 2021 07:29
Operator : CG/JU
Sample : PB139167BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK167

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032179.D
Acq On : 26 Sep 2021 07:29
Operator : CG/JU
Sample : PB139167BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK167

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
