

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032180.D
 Acq On : 26 Sep 2021 08:04
 Operator : CG/JU
 Sample : PB139380BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK380

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032180.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.990	21	26	33	rBV	127598	160472	2.32%	0.197%
2	3.413	94	98	120	rBV	1581455	2124949	30.78%	2.604%
3	3.778	155	160	168	rVB	26454	35929	0.52%	0.044%
4	4.807	331	335	340	rVB5	6816	10392	0.15%	0.013%
5	6.843	674	681	690	rBV	1690204	2464257	35.69%	3.020%
6	6.984	698	705	716	rVB	1360695	2020586	29.27%	2.476%
7	7.201	732	742	751	rBV	1740609	2590360	37.52%	3.174%
8	7.660	813	820	828	rVB	1510734	2272815	32.92%	2.785%
9	8.384	936	943	958	rBV	2006272	3018623	43.72%	3.699%
10	8.813	1009	1016	1025	rBV	1431999	2180256	31.58%	2.672%
11	9.542	1133	1140	1150	rBV	1128203	1724682	24.98%	2.113%
12	10.084	1224	1232	1242	rBV	1959986	2983377	43.21%	3.656%
13	10.454	1286	1295	1304	rBV	1973397	3078897	44.60%	3.773%
14	10.584	1309	1317	1334	rBV	1902631	3027584	43.85%	3.710%
15	12.042	1560	1565	1571	rVB	35868	57577	0.83%	0.071%
16	13.277	1768	1775	1780	rBV3	5069	8461	0.12%	0.010%
17	13.707	1842	1848	1854	rBV	2901259	3872914	56.10%	4.746%
18	13.754	1854	1856	1861	rVB3	8019	8895	0.13%	0.011%
19	14.001	1891	1898	1917	rBV	3375461	4798050	69.50%	5.880%
20	14.307	1942	1950	1962	rBV	2640896	3733745	54.08%	4.575%
21	14.507	1977	1984	1998	rBV	1292499	1703821	24.68%	2.088%
22	15.295	2112	2118	2131	rBB	4382472	5958711	86.31%	7.302%
23	15.407	2131	2137	2147	rBV	1036673	1282401	18.58%	1.571%
24	15.536	2154	2159	2164	rVB	50406	73339	1.06%	0.090%
25	15.954	2228	2230	2236	rVB6	5235	8492	0.12%	0.010%
26	16.071	2246	2250	2258	rVB7	9701	14999	0.22%	0.018%
27	16.713	2356	2359	2364	rVB5	5894	7155	0.10%	0.009%
28	16.818	2373	2377	2382	rBV	11680	15147	0.22%	0.019%
29	17.036	2407	2414	2424	rBV	2950834	4106555	59.48%	5.032%
30	17.130	2424	2430	2451	rVV	4698442	6210113	89.95%	7.610%
31	17.701	2524	2527	2533	rBV7	6181	9475	0.14%	0.012%
32	18.983	2740	2745	2749	rBV	45159	58767	0.85%	0.072%
33	19.054	2752	2757	2762	rBV	48626	69141	1.00%	0.085%
34	19.412	2812	2818	2832	rBV	5122949	6903704	100.00%	8.460%
35	21.195	3116	3121	3127	rBV	3485160	4172313	60.44%	5.113%
36	23.224	3460	3466	3479	rVB	3899833	6542277	94.76%	8.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032180.D
Acq On : 26 Sep 2021 08:04
Operator : CG/JU
Sample : PB139380BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK380

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Title : SVOA CALIBRATION

37 23.359 3483 3489 3501 rVB2 2497938 4294535 62.21% 5.263%




Sum of corrected areas: 81603766

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032180.D
Acq On : 26 Sep 2021 08:04
Operator : CG/JU
Sample : PB139380BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK380

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

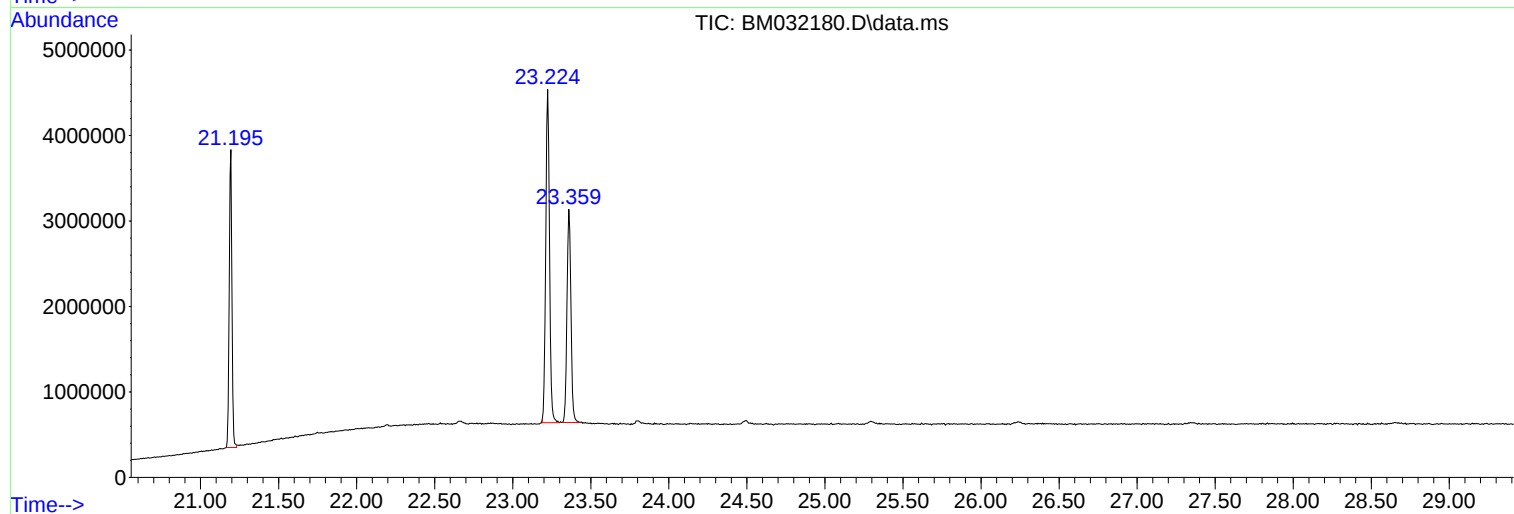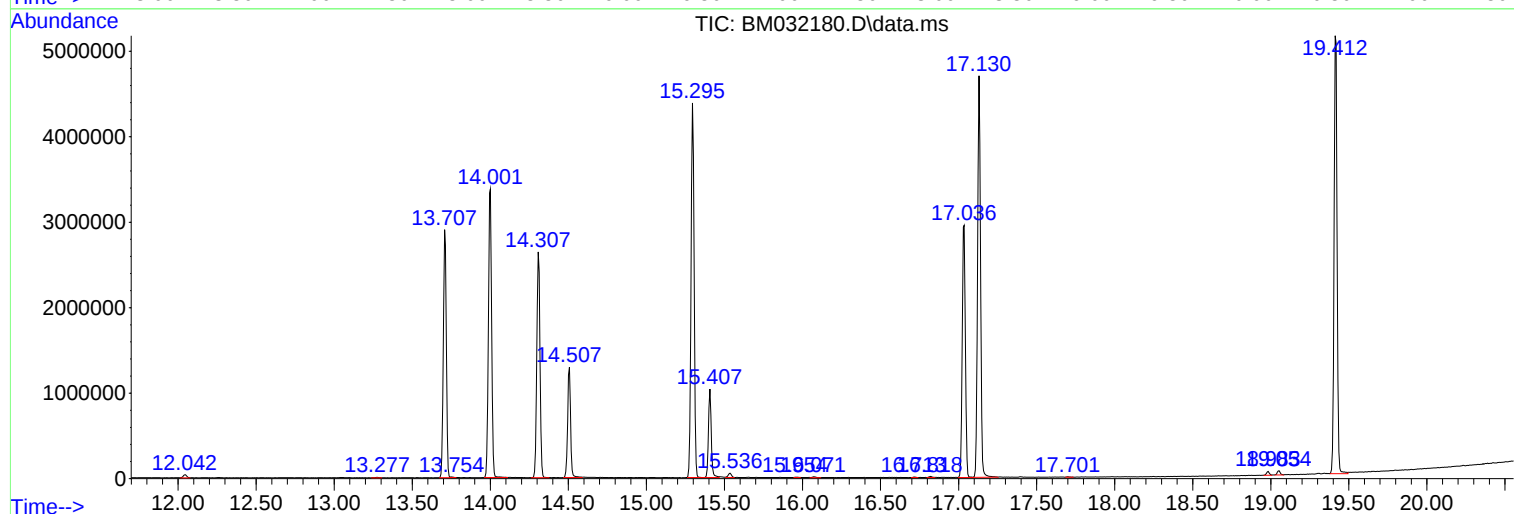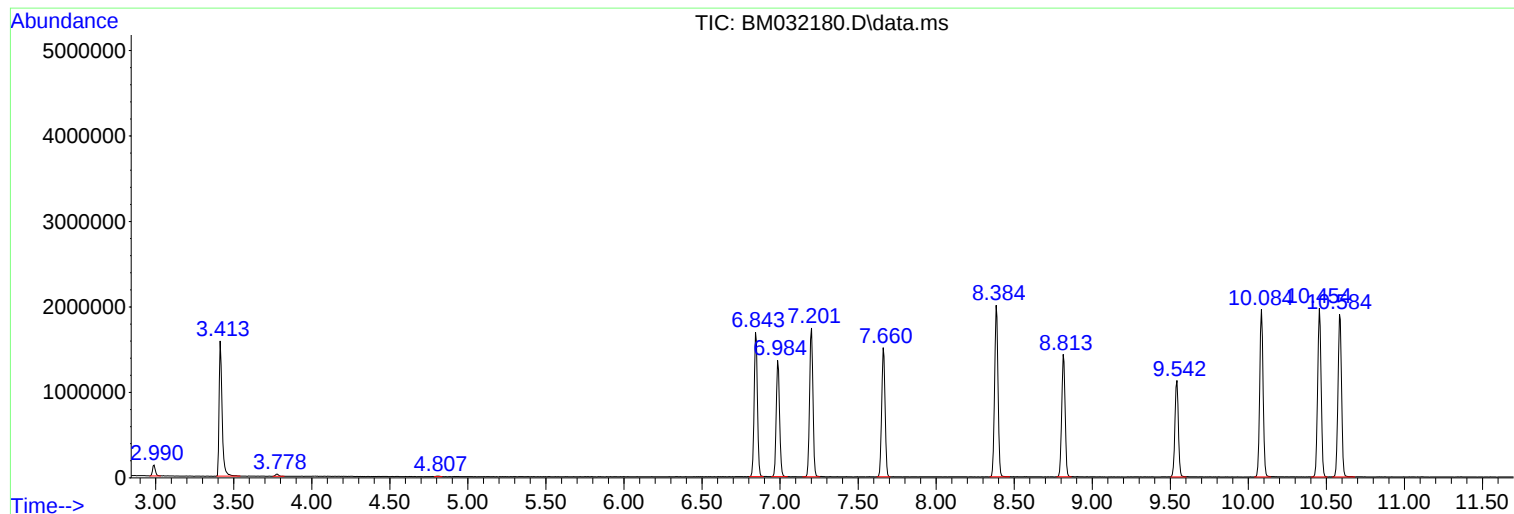

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032180.D
Acq On : 26 Sep 2021 08:04
Operator : CG/JU
Sample : PB139380BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK380

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032180.D
Acq On : 26 Sep 2021 08:04
Operator : CG/JU
Sample : PB139380BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK380

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
