

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032181.D
 Acq On : 26 Sep 2021 08:40
 Operator : CG/JU
 Sample : PB139378BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK378

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032181.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.990	22	26	36	rVB	131901	166358	2.48%	0.207%
2	3.413	94	98	113	rBV	1652654	2202922	32.79%	2.737%
3	3.778	155	160	164	rVB	24088	34835	0.52%	0.043%
4	4.807	332	335	340	rVB6	5896	8595	0.13%	0.011%
5	6.842	674	681	689	rBV	1715729	2584525	38.47%	3.211%
6	6.984	699	705	716	rVB	1400372	2132814	31.74%	2.650%
7	7.201	732	742	754	rBV	1823947	2716854	40.44%	3.376%
8	7.660	814	820	828	rBV	1403536	2103716	31.31%	2.614%
9	8.383	936	943	953	rBV	2109419	3147330	46.84%	3.911%
10	8.813	1010	1016	1027	rBV	1513728	2309299	34.37%	2.869%
11	9.542	1133	1140	1150	rBV	1190321	1810829	26.95%	2.250%
12	10.083	1225	1232	1242	rBV	2061807	3152459	46.92%	3.917%
13	10.454	1288	1295	1304	rBV	1810174	2849344	42.41%	3.540%
14	10.583	1309	1317	1330	rBV	1911896	3155423	46.96%	3.921%
15	12.042	1558	1565	1571	rVB2	36146	60547	0.90%	0.075%
16	12.260	1598	1602	1606	rBV5	3678	6983	0.10%	0.009%
17	13.036	1731	1734	1737	rBV3	4745	6865	0.10%	0.009%
18	13.271	1771	1774	1778	rVB3	5625	9029	0.13%	0.011%
19	13.713	1842	1849	1854	rBV	2856013	3865967	57.54%	4.804%
20	13.748	1854	1855	1859	rVB4	8257	9009	0.13%	0.011%
21	14.001	1890	1898	1913	rBV	3509792	5014174	74.63%	6.230%
22	14.307	1943	1950	1963	rVB	2448353	3429684	51.04%	4.262%
23	14.507	1975	1984	1997	rBV	1249811	1668689	24.84%	2.073%
24	15.295	2111	2118	2126	rBV	4510102	6032541	89.78%	7.496%
25	15.407	2131	2137	2153	rVV	1027426	1281897	19.08%	1.593%
26	15.536	2155	2159	2165	rVB	32763	48443	0.72%	0.060%
27	15.959	2226	2231	2235	rBV8	5966	9076	0.14%	0.011%
28	16.077	2246	2251	2256	rVB5	10903	16178	0.24%	0.020%
29	16.712	2355	2359	2365	rVB7	5562	9065	0.13%	0.011%
30	16.824	2372	2378	2382	rBV	13272	20985	0.31%	0.026%
31	17.036	2407	2414	2420	rBV	2764001	3702981	55.11%	4.601%
32	17.130	2424	2430	2450	rVB	4561726	6102227	90.82%	7.582%
33	17.695	2522	2526	2531	rBV7	5531	8730	0.13%	0.011%
34	18.983	2740	2745	2749	rBV3	36161	48821	0.73%	0.061%
35	19.053	2752	2757	2764	rVV	45855	65698	0.98%	0.082%
36	19.300	2797	2799	2805	rBV3	10576	13418	0.20%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032181.D
Acq On : 26 Sep 2021 08:40
Operator : CG/JU
Sample : PB139378BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK378

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Title : SVOA CALIBRATION

37	19.418	2813	2819	2828	rBV	5145559	6718993	100.00%	8.349%
38	21.194	3116	3121	3127	rBV	3015643	3724426	55.43%	4.628%
39	23.224	3459	3466	3480	rVB	3822537	6470178	96.30%	8.039%
40	23.359	3483	3489	3500	rVB2	2167324	3759987	55.96%	4.672%




Sum of corrected areas: 80479894

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032181.D
Acq On : 26 Sep 2021 08:40
Operator : CG/JU
Sample : PB139378BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK378

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

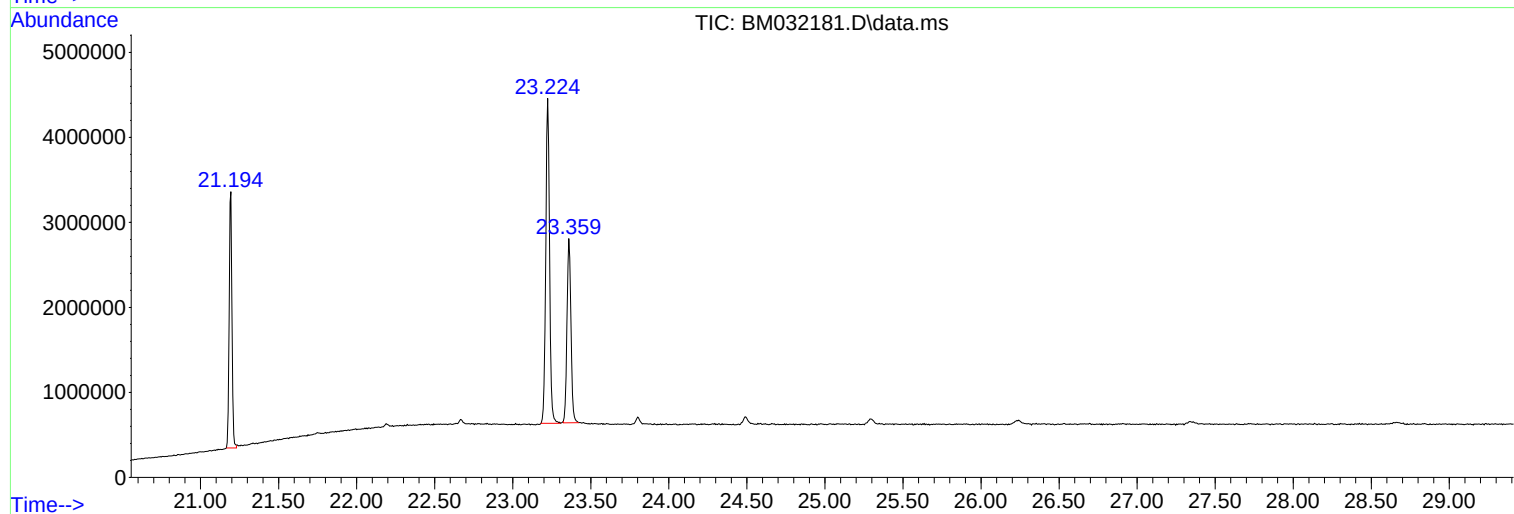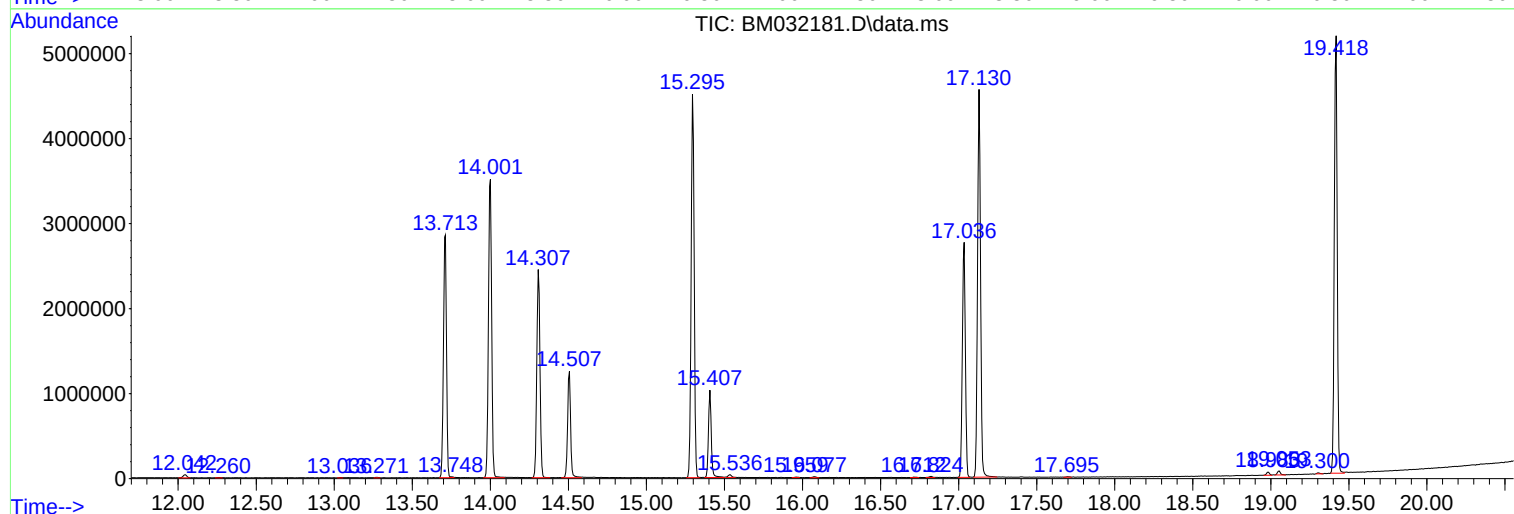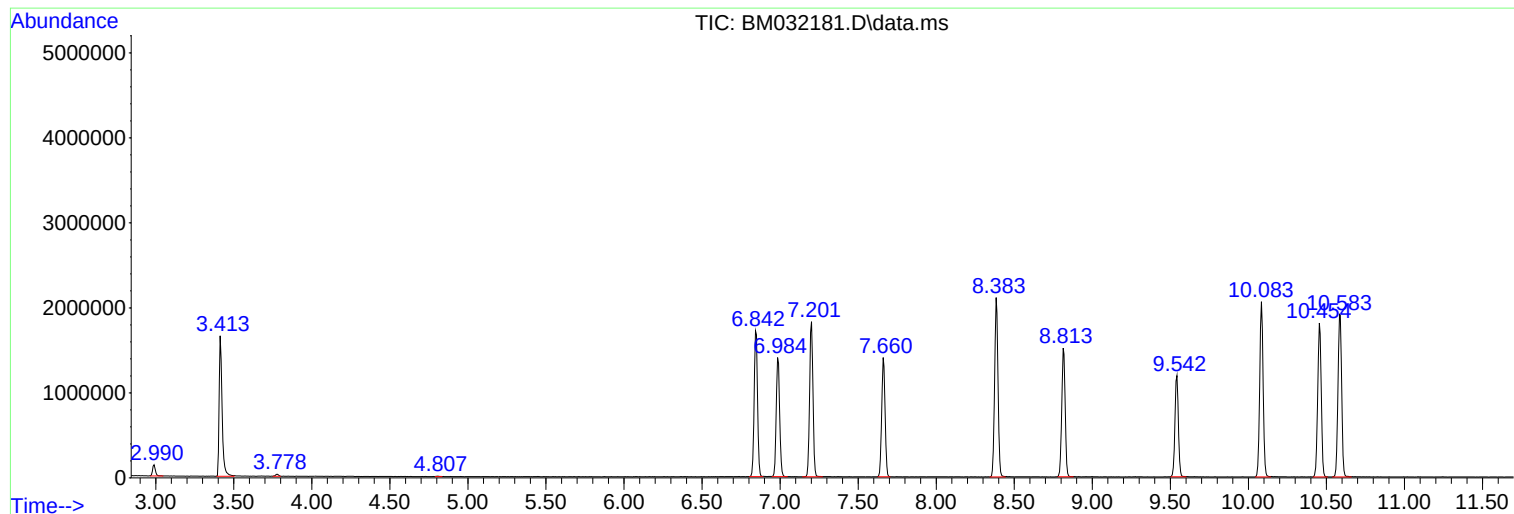

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032181.D
Acq On : 26 Sep 2021 08:40
Operator : CG/JU
Sample : PB139378BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK378

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032181.D
Acq On : 26 Sep 2021 08:40
Operator : CG/JU
Sample : PB139378BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK378

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
