

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032185.D
 Acq On : 26 Sep 2021 11:03
 Operator : CG/JU
 Sample : M3739-05
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.990	21	26	32	rVB	107352	133160	1.40%	0.143%
2	3.278	72	75	85	rBV	176136	224538	2.35%	0.241%
3	3.419	95	99	112	rBV	527862	739970	7.75%	0.793%
4	3.684	139	144	151	rVB	40204	65880	0.69%	0.071%
5	3.778	155	160	167	rVB	28055	39394	0.41%	0.042%
6	5.684	476	484	488	rBV10	8409	15179	0.16%	0.016%
7	5.731	488	492	497	rBV	14296	19175	0.20%	0.021%
8	6.843	675	681	691	rVB	474756	721612	7.56%	0.774%
9	6.984	697	705	715	rBV	1520877	2289623	23.99%	2.454%
10	7.201	734	742	748	rBV	1580501	2393241	25.07%	2.566%
11	7.254	748	751	757	rVV	27679	45404	0.48%	0.049%
12	7.307	757	760	767	rVB6	8441	14167	0.15%	0.015%
13	7.660	814	820	828	rVB	1625825	2410127	25.25%	2.584%
14	7.742	828	834	840	rVB2	11598	17688	0.19%	0.019%
15	7.919	859	864	870	rBV6	6997	11526	0.12%	0.012%
16	8.248	914	920	927	rBV3	28297	52926	0.55%	0.057%
17	8.384	934	943	955	rBV	1296363	1914436	20.06%	2.052%
18	8.478	955	959	965	rVB7	5355	10143	0.11%	0.011%
19	8.813	1009	1016	1025	rBV	1701675	2584117	27.07%	2.770%
20	8.960	1037	1041	1043	rBV3	6207	9640	0.10%	0.010%
21	8.989	1043	1046	1050	rVB5	10339	14199	0.15%	0.015%
22	9.301	1094	1099	1105	rVB	13653	21401	0.22%	0.023%
23	9.542	1131	1140	1151	rBV	1284129	2036063	21.33%	2.183%
24	10.083	1224	1232	1244	rBV	2104402	3264912	34.21%	3.500%
25	10.231	1250	1257	1266	rBV	1035752	1488158	15.59%	1.595%
26	10.454	1284	1295	1303	rBV	2089499	3288071	34.45%	3.525%
27	10.583	1307	1317	1327	rBV	1022309	1613290	16.90%	1.729%
28	10.801	1349	1354	1361	rBV	12522	20305	0.21%	0.022%
29	11.783	1513	1521	1526	rVB9	5557	10414	0.11%	0.011%
30	12.042	1560	1565	1571	rVB	41744	64511	0.68%	0.069%
31	12.666	1666	1671	1674	rBV3	6355	10609	0.11%	0.011%
32	12.913	1709	1713	1718	rVB6	9768	14687	0.15%	0.016%
33	13.148	1746	1753	1759	rBV6	10716	16477	0.17%	0.018%
34	13.207	1759	1763	1769	rVV6	10223	16583	0.17%	0.018%
35	13.272	1769	1774	1779	rVB5	9981	14956	0.16%	0.016%
36	13.707	1838	1848	1854	rBV	3756885	5040789	52.81%	5.404%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032185.D
 Acq On : 26 Sep 2021 11:03
 Operator : CG/JU
 Sample : M3739-05
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B79

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Title : SVOA CALIBRATION

37	13.954	1887	1890	1891	rBV2	10475	10757	0.11%	0.012%
38	13.995	1891	1897	1908	rVB	4042265	5855374	61.35%	6.277%
39	14.307	1944	1950	1957	rVV	2851504	4024391	42.16%	4.314%
40	14.448	1969	1974	1978	rBV	14907	21551	0.23%	0.023%
41	14.501	1978	1983	1997	rVV	358697	482603	5.06%	0.517%
42	14.718	2014	2020	2026	rVB10	7355	13180	0.14%	0.014%
43	15.113	2084	2087	2092	rBV5	8147	11601	0.12%	0.012%
44	15.295	2111	2118	2131	rBV	5721000	7789179	81.61%	8.350%
45	15.407	2131	2137	2151	rVV	1641725	2068928	21.68%	2.218%
46	15.536	2154	2159	2169	rVB2	45163	80090	0.84%	0.086%
47	15.730	2186	2192	2197	rVB3	25536	39116	0.41%	0.042%
48	15.965	2224	2232	2238	rBV10	14483	29996	0.31%	0.032%
49	16.018	2238	2241	2244	rVV4	7500	10642	0.11%	0.011%
50	16.071	2244	2250	2255	rVB5	19475	36404	0.38%	0.039%
51	16.171	2264	2267	2273	rVB8	7206	12879	0.13%	0.014%
52	16.648	2342	2348	2352	rVB6	7824	11846	0.12%	0.013%
53	16.718	2356	2360	2365	rVV6	8795	14696	0.15%	0.016%
54	16.824	2368	2378	2381	rBV3	20523	43248	0.45%	0.046%
55	16.854	2381	2383	2387	rVB5	10476	11404	0.12%	0.012%
56	17.036	2407	2414	2420	rBV	3163774	4436589	46.48%	4.756%
57	17.130	2423	2430	2443	rVV2	6346824	8533253	89.40%	9.148%
58	17.224	2443	2446	2451	rVB7	10941	16883	0.18%	0.018%
59	17.401	2472	2476	2480	rVV2	8166	11746	0.12%	0.013%
60	17.565	2501	2504	2508	rVB4	8065	11041	0.12%	0.012%
61	17.701	2522	2527	2532	rBV	126804	151526	1.59%	0.162%
62	17.918	2560	2564	2568	rBV4	29236	44371	0.46%	0.048%
63	18.218	2612	2615	2624	rVB7	10871	18982	0.20%	0.020%
64	18.548	2667	2671	2676	rBV7	8908	15852	0.17%	0.017%
65	18.865	2719	2725	2728	rBV3	26730	46009	0.48%	0.049%
66	18.983	2740	2745	2749	rBV	61930	89037	0.93%	0.095%
67	19.048	2752	2756	2764	rVV	79675	117141	1.23%	0.126%
68	19.301	2797	2799	2803	rVB	18765	23906	0.25%	0.026%
69	19.418	2813	2819	2825	rBV	7164341	9544761	100.00%	10.232%
70	19.648	2855	2858	2865	rVB4	37990	61338	0.64%	0.066%
71	20.895	3067	3070	3074	rBV3	150919	185119	1.94%	0.198%
72	21.195	3116	3121	3127	rBV	3814689	4558700	47.76%	4.887%
73	23.224	3459	3466	3476	rVB2	5312421	9494385	99.47%	10.178%
74	23.359	3483	3489	3500	rVB2	2692878	4708804	49.33%	5.048%

Sum of corrected areas: 93284699

Instrument :

BNA_M

ClientSampleId :




C0B79

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032185.D
Acq On : 26 Sep 2021 11:03
Operator : CG/JU
Sample : M3739-05
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B79

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

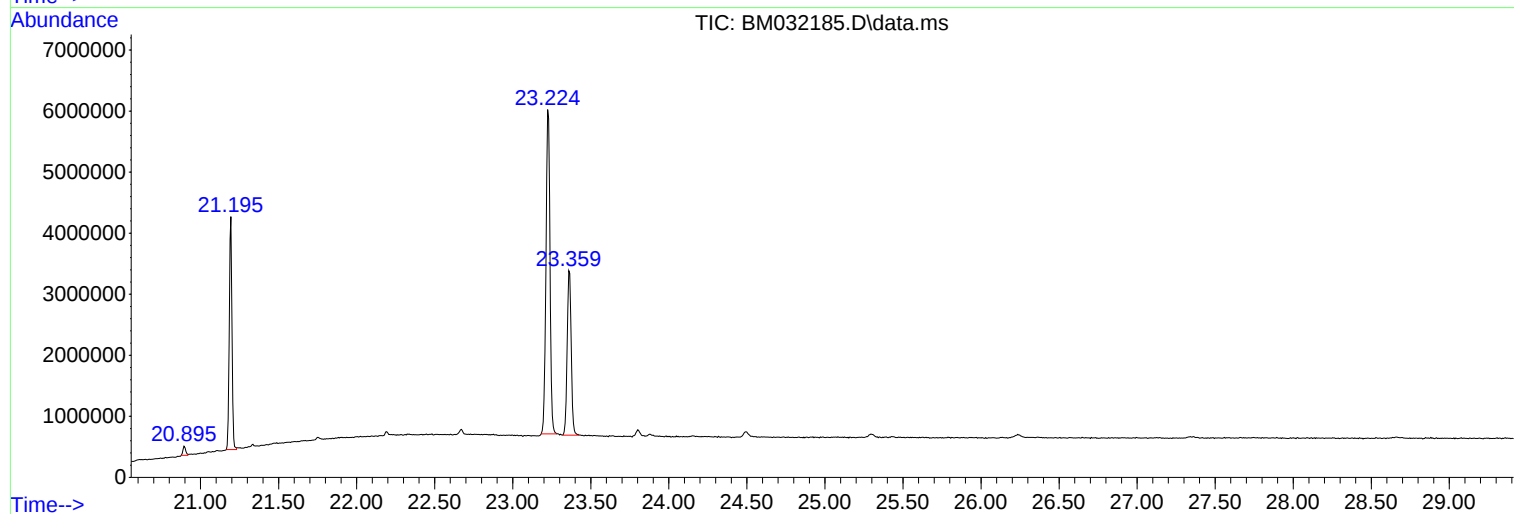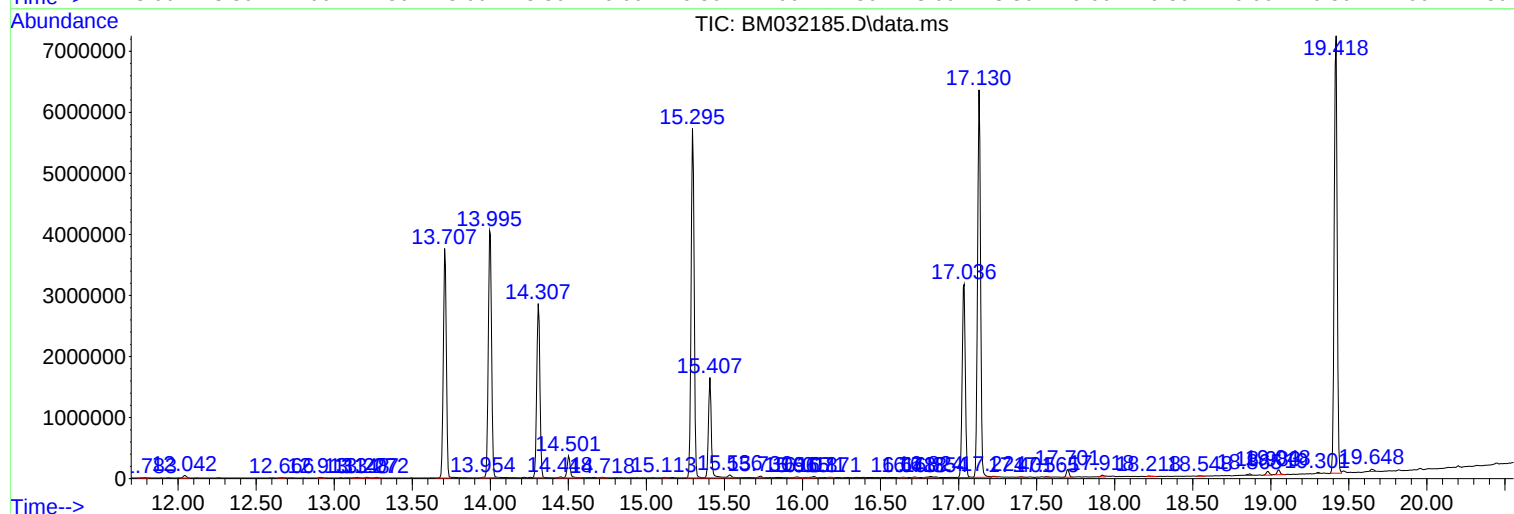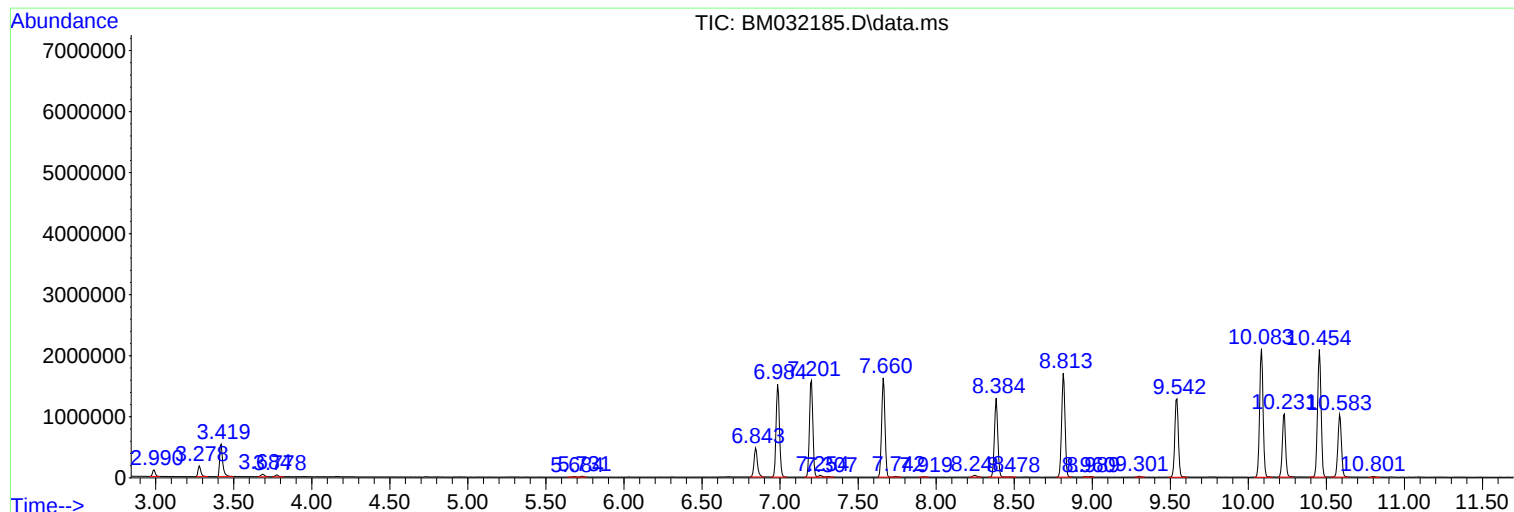

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032185.D
Acq On : 26 Sep 2021 11:03
Operator : CG/JU
Sample : M3739-05
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B79










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.230	9.05 ng/ul	1488160	Naphthalene-d8	10.454

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	72

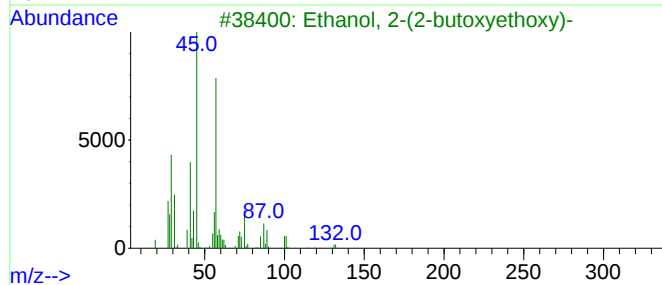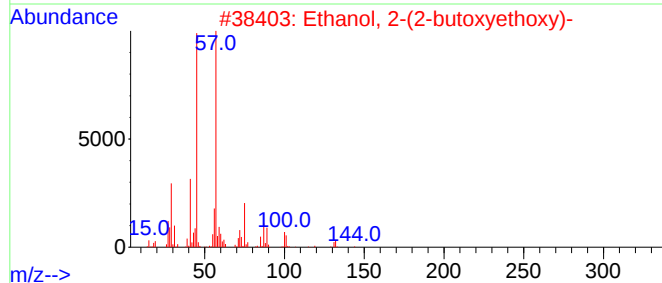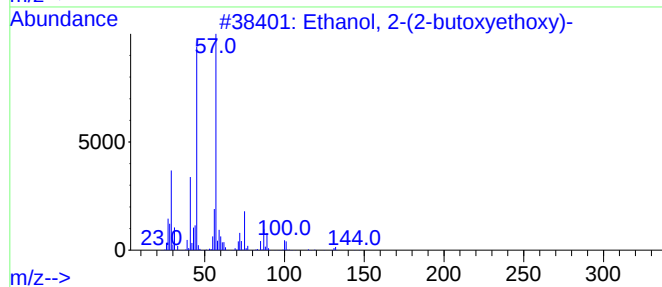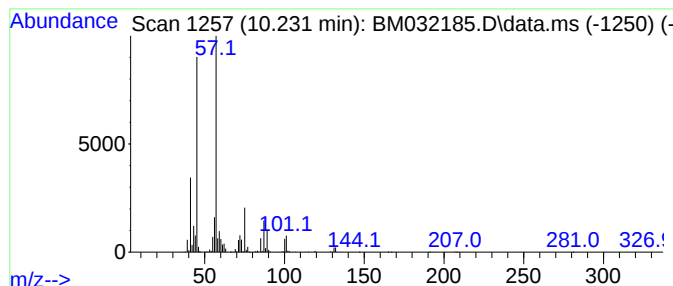

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032185.D
Acq On : 26 Sep 2021 11:03
Operator : CG/JU
Sample : M3739-05
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B79

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.230	9.1	ng/ul	1488160	2	10.454	3288070	20.0