

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032195.D
 Acq On : 26 Sep 2021 17:03
 Operator : CG/JU
 Sample : M3873-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW7X2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032195.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.960	16	21	25	rBV	421091	655541	7.98%	0.750%
2	3.419	95	99	111	rBV	272265	386337	4.71%	0.442%
3	3.684	138	144	150	rVB	48030	79920	0.97%	0.091%
4	3.772	155	159	165	rVB	28855	42180	0.51%	0.048%
5	3.960	187	191	197	rVB8	5376	12391	0.15%	0.014%
6	4.154	220	224	230	rVB5	19996	31774	0.39%	0.036%
7	5.678	479	483	488	rVB6	5665	8647	0.11%	0.010%
8	5.731	489	492	496	rVB3	7257	9514	0.12%	0.011%
9	6.607	637	641	645	rBV6	5837	8803	0.11%	0.010%
10	6.672	647	652	659	rVV	24551	37934	0.46%	0.043%
11	6.843	675	681	691	rBV	527227	794461	9.68%	0.908%
12	6.984	696	705	714	rBV	1576007	2366143	28.82%	2.706%
13	7.195	733	741	749	rBV	1607196	2497484	30.42%	2.856%
14	7.307	757	760	764	rVB4	11937	16551	0.20%	0.019%
15	7.660	813	820	829	rBV	1645483	2461442	29.98%	2.815%
16	7.742	829	834	839	rVB	16681	26346	0.32%	0.030%
17	7.913	859	863	868	rVB7	5449	9085	0.11%	0.010%
18	8.242	914	919	923	rBV7	6076	11935	0.15%	0.014%
19	8.384	936	943	953	rBV	1383656	2031523	24.74%	2.323%
20	8.813	1009	1016	1024	rBV	1752572	2662990	32.43%	3.045%
21	9.301	1092	1099	1102	rVB7	8894	15862	0.19%	0.018%
22	9.542	1132	1140	1148	rBV	1325406	2070156	25.21%	2.367%
23	9.783	1174	1181	1185	rBV4	11390	21737	0.26%	0.025%
24	10.083	1225	1232	1243	rBV	2139137	3298381	40.17%	3.772%
25	10.225	1251	1256	1264	rVB	154742	232782	2.84%	0.266%
26	10.454	1287	1295	1302	rBV	2103184	3321945	40.46%	3.798%
27	10.583	1309	1317	1327	rBV	1613214	2605223	31.73%	2.979%
28	11.095	1398	1404	1408	rBV6	9400	18352	0.22%	0.021%
29	11.248	1423	1430	1439	rBV5	15923	28447	0.35%	0.033%
30	12.042	1559	1565	1572	rVB2	42091	64291	0.78%	0.074%
31	12.913	1708	1713	1718	rBV6	7479	12653	0.15%	0.014%
32	13.148	1747	1753	1759	rBV7	9441	16675	0.20%	0.019%
33	13.207	1759	1763	1770	rVV4	14134	21470	0.26%	0.025%
34	13.272	1770	1774	1779	rVB2	7646	11315	0.14%	0.013%
35	13.707	1841	1848	1854	rBV	3340567	4450549	54.21%	5.089%
36	13.748	1854	1855	1865	rVB6	13944	26595	0.32%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
 Data File : BM032195.D
 Acq On : 26 Sep 2021 17:03
 Operator : CG/JU
 Sample : M3873-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW7X2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
 Title : SVOA CALIBRATION

37	13.954	1886	1890	1891	rBV3	10110	11171	0.14%	0.013%
38	13.995	1891	1897	1908	rVB	3865667	5607136	68.29%	6.411%
39	14.307	1943	1950	1960	rVV	2972759	4038879	49.19%	4.618%
40	14.460	1970	1976	1977	rBV6	6536	8563	0.10%	0.010%
41	14.501	1977	1983	1994	rVV	337674	462102	5.63%	0.528%
42	14.718	2015	2020	2026	rBV9	10146	20771	0.25%	0.024%
43	15.042	2069	2075	2081	rVB	22256	32833	0.40%	0.038%
44	15.118	2081	2088	2092	rBV2	88382	119490	1.46%	0.137%
45	15.295	2111	2118	2129	rBV	4965809	6854366	83.48%	7.838%
46	15.407	2131	2137	2150	rVV	1384148	1745395	21.26%	1.996%
47	15.536	2154	2159	2171	rVB2	43513	82613	1.01%	0.094%
48	15.660	2175	2180	2184	rVB8	6500	12619	0.15%	0.014%
49	15.713	2184	2189	2191	rBV5	6416	9477	0.12%	0.011%
50	15.965	2226	2232	2238	rBV10	10895	23467	0.29%	0.027%
51	16.077	2247	2251	2256	rVB4	17932	25300	0.31%	0.029%
52	16.183	2264	2269	2271	rBV5	7008	11913	0.15%	0.014%
53	16.636	2343	2346	2351	rBV4	12159	18175	0.22%	0.021%
54	16.718	2355	2360	2363	rBV5	9682	12906	0.16%	0.015%
55	16.818	2370	2377	2381	rBV2	27093	46196	0.56%	0.053%
56	16.954	2396	2400	2404	rVB6	8230	9816	0.12%	0.011%
57	17.036	2407	2414	2420	rBV	3163048	4406584	53.67%	5.039%
58	17.130	2423	2430	2445	rBV	5450319	7345897	89.47%	8.400%
59	17.318	2458	2462	2465	rVB2	11019	14449	0.18%	0.017%
60	17.395	2472	2475	2482	rBV4	9802	17954	0.22%	0.021%
61	17.701	2523	2527	2534	rVB	41304	52307	0.64%	0.060%
62	17.918	2561	2564	2571	rBV8	22348	43844	0.53%	0.050%
63	17.983	2573	2575	2581	rVB	17049	22145	0.27%	0.025%
64	18.859	2722	2724	2727	rBV4	9149	11031	0.13%	0.013%
65	18.983	2741	2745	2750	rBV2	48267	67770	0.83%	0.077%
66	19.048	2752	2756	2760	rBV	67680	90972	1.11%	0.104%
67	19.301	2797	2799	2803	rVB2	17307	19316	0.24%	0.022%
68	19.412	2813	2818	2824	rBV	5909855	8210573	100.00%	9.388%
69	20.895	3067	3070	3076	rBV3	79888	124518	1.52%	0.142%
70	21.100	3103	3105	3109	rVB	118951	110975	1.35%	0.127%
71	21.195	3116	3121	3130	rBV	3660935	4535918	55.24%	5.187%
72	23.224	3459	3466	3476	rVB2	4686046	8175163	99.57%	9.348%
73	23.359	3483	3489	3502	rVB2	2739193	4684857	57.06%	5.357%


Sum of corrected areas: 87454895

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032195.D
Acq On : 26 Sep 2021 17:03
Operator : CG/JU
Sample : M3873-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW7X2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

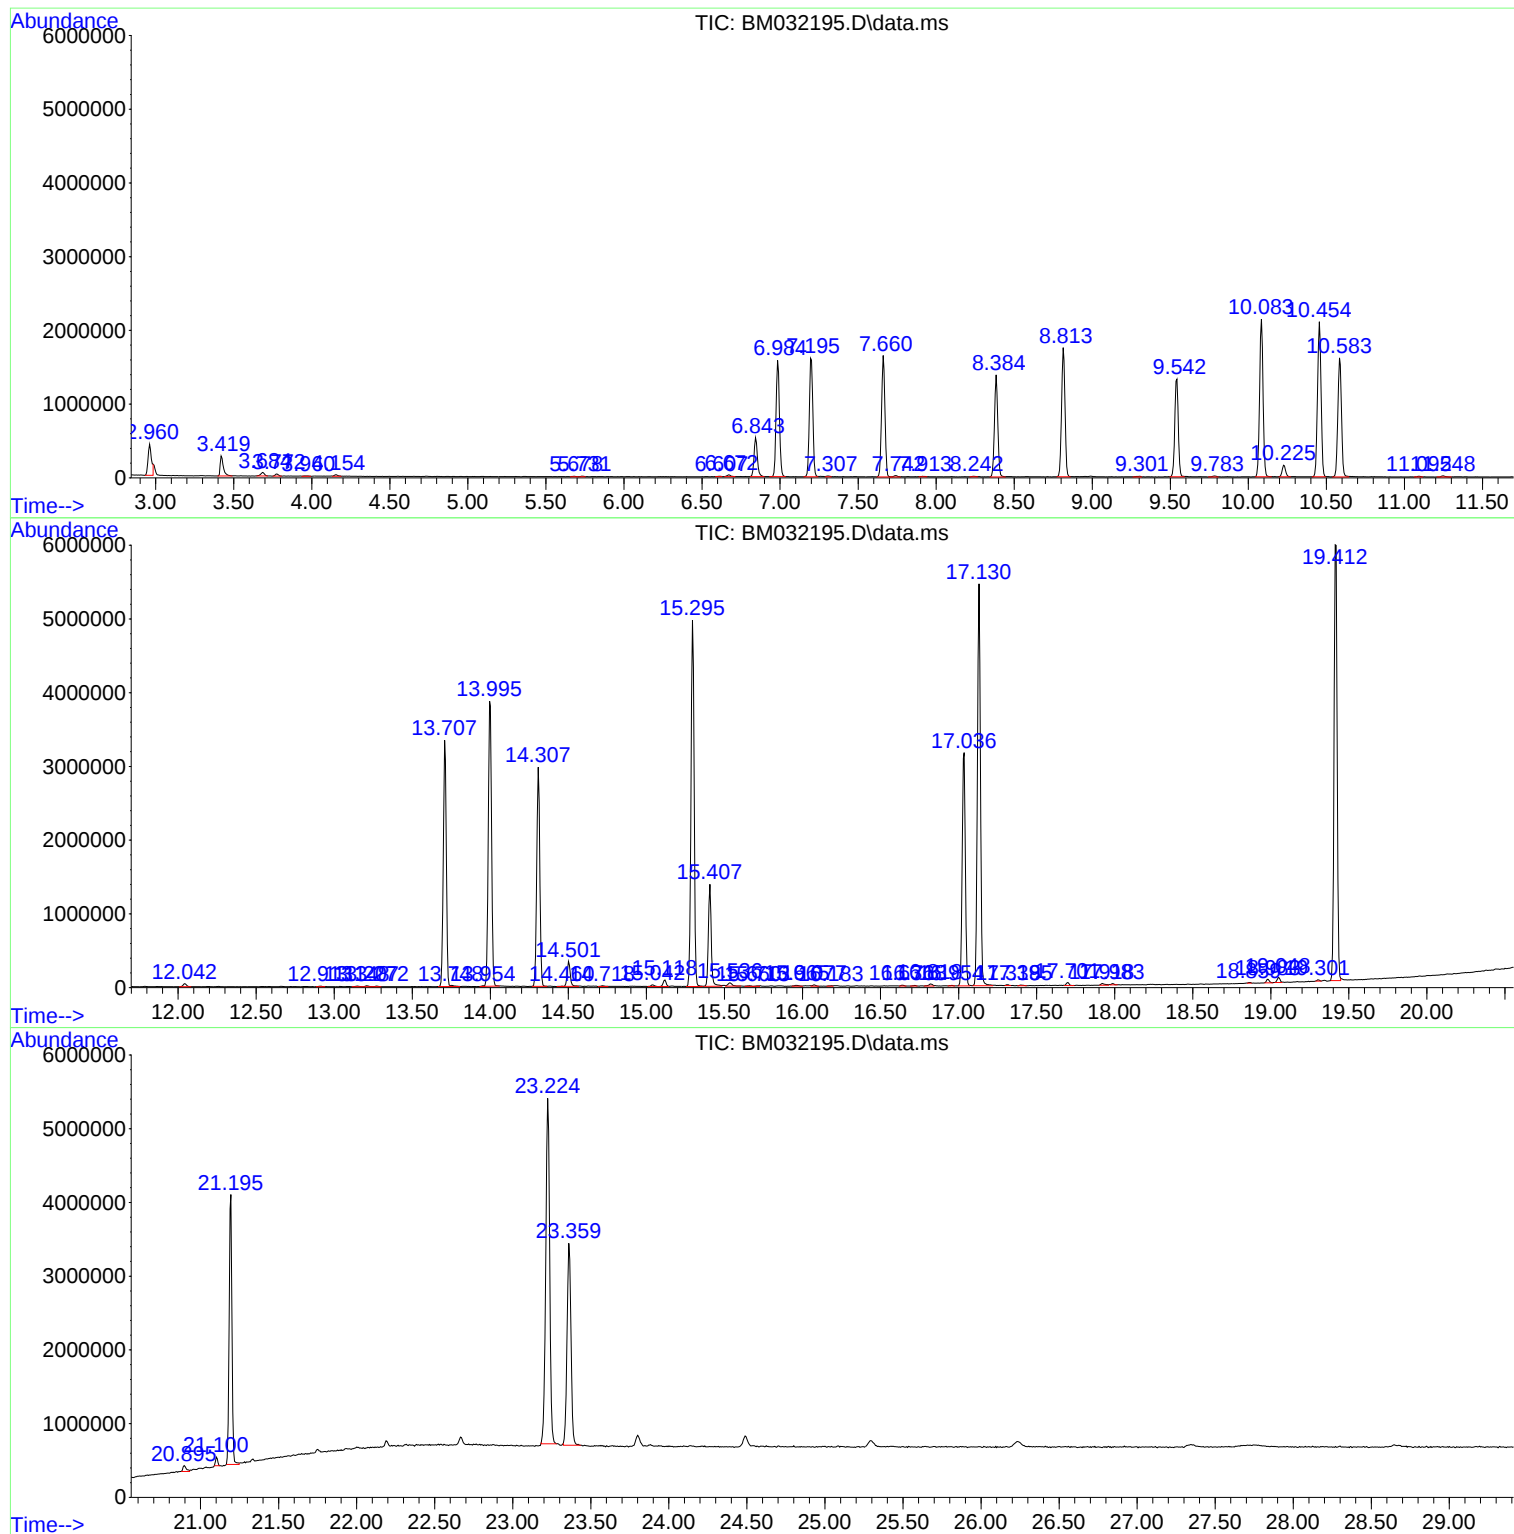

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032195.D
Acq On : 26 Sep 2021 17:03
Operator : CG/JU
Sample : M3873-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW7X2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092521\
Data File : BM032195.D
Acq On : 26 Sep 2021 17:03
Operator : CG/JU
Sample : M3873-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW7X2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------