

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092616\
 Data File : BM007578.D
 Acq On : 26 Sep 2016 19:18
 Operator : UM/SJ
 Sample : PB93623BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK23

Quant Time: Sep 27 02:00:31 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 27 01:59:49 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.78	152	196132	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	934769	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	761094	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	1800302	20.00	ng/ul	0.00
75) Chrysene-d12	21.34	240	2506566	20.00	ng/ul	0.00
83) Perylene-d12	23.60	264	2342991	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	26867	6.73	ng/uL	0.00
5) Phenol-d5	6.95	99	505317	29.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	306545	32.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	393165	31.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.48	113	445332	29.97	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	215015	32.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	248414	32.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.19	165	448173	29.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	634301	39.94	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	1839470	33.23	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	2061231	32.09	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	302186	30.92	ng/ul	0.00
57) Fluorene-d10	15.40	176	1592133	32.79	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	305238	27.79	ng/ul	0.00
70) Anthracene-d10	17.25	188	2740115	33.12	ng/ul	0.00
76) Pyrene-d10	19.54	212	3477620	34.96	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.46	264	3459659	33.37	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.48	70	12474	1.09	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092616\
Data File : BM007578.D
Acq On : 26 Sep 2016 19:18
Operator : UM/SJ
Sample : PB93623BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK23

Quant Time: Sep 27 02:00:31 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 27 01:59:49 2016
Response via : Initial Calibration

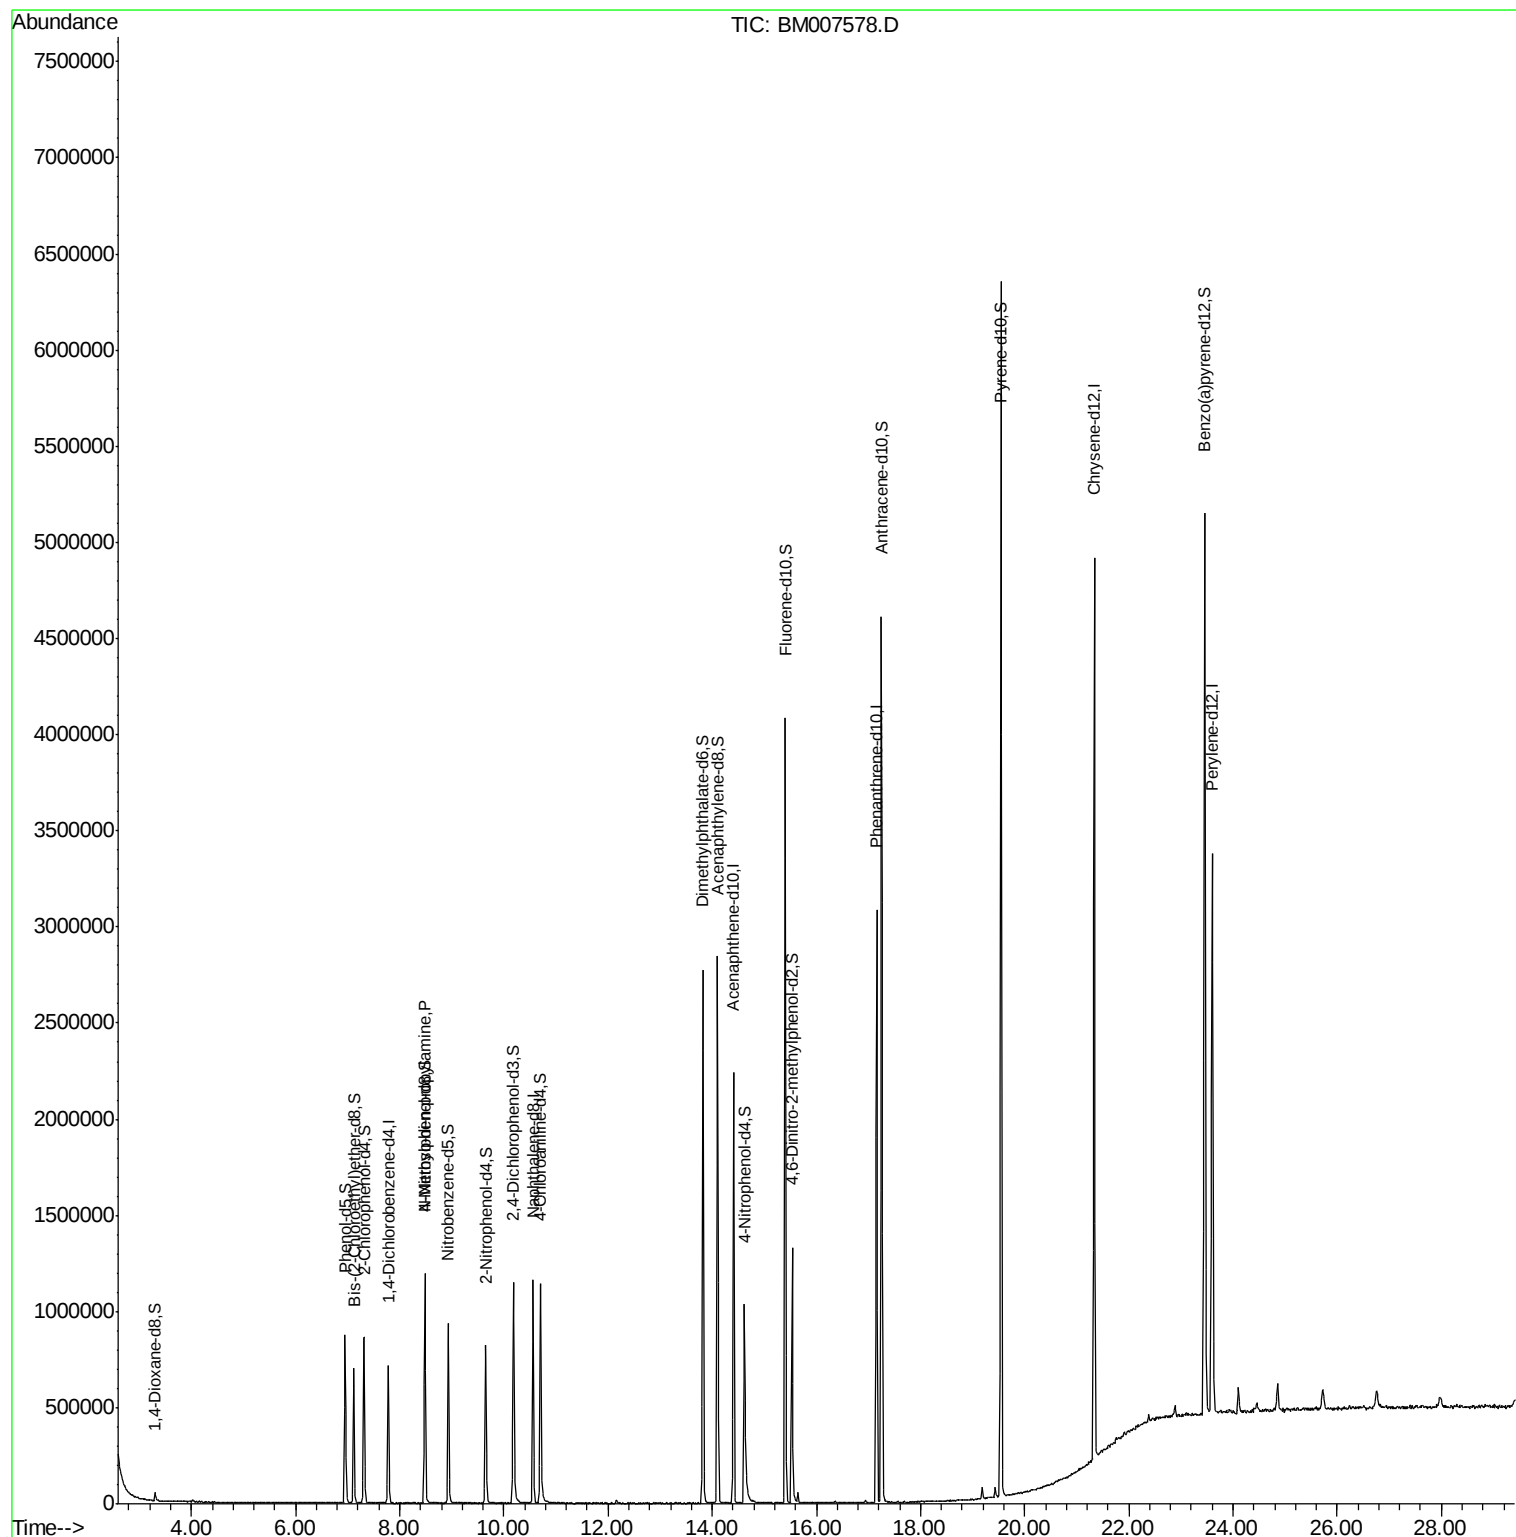

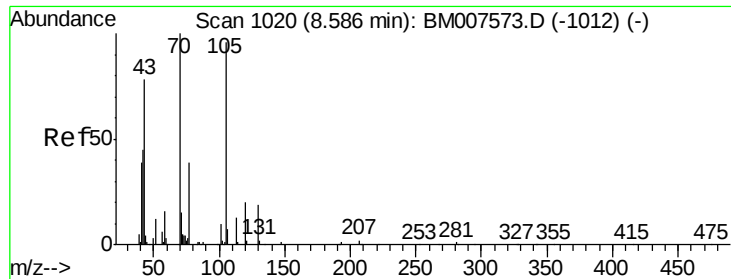

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.09 ng/ul
 RT: 8.48 min Scan# 1002
 Delta R.T. -0.11 min
 Lab File: BM007578.D
 Acq: 26 Sep 2016 19:18

Instrument :
 BNA_M
 ClientSampleId :
 SBLK23

Tgt Ion: 70 Resp: 12474
 Ion Ratio Lower Upper
 70 100
 42 306.1 43.4 65.2#
 101 0.0 7.8 11.6#
 130 0.0 16.2 24.4#

