

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
 Data File : BM036765.D
 Acq On : 27 Sep 2022 03:16
 Operator : CG/JU
 Sample : N4746-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8M5

Quant Time: Sep 27 03:48:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 26 23:10:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.998	152	431213	20.000	ng/u1	0.00
20) Naphthalene-d8	10.810	136	1887776	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.627	164	1178951	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.362	188	2297435	20.000	ng/u1	0.00
79) Chrysene-d12	21.527	240	1753288	20.000	ng/u1	0.00
88) Perylene-d12	23.956	264	1505404	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	51100	4.442	ng/uL	0.00
4) Pyridine-d5	3.816	84	242056	7.215	ng/u1	0.00
7) Phenol-d5	7.157	99	240608	6.244	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	723150	30.901	ng/u1	0.00
11) 2-Chlorophenol-d4	7.528	132	700367	25.244	ng/u1	0.00
15) 4-Methylphenol-d8	8.704	113	469681	16.495	ng/u1	-0.01
21) Nitrobenzene-d5	9.163	128	474143	37.108	ng/u1	0.00
24) 2-Nitrophenol-d4	9.892	143	451237	39.426	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.428	165	803392	30.290	ng/u1	0.00
31) 4-Chloroaniline-d4	10.945	131	940337	21.323	ng/u1	0.00
46) Dimethylphthalate-d6	14.039	166	2875462	36.163	ng/u1	0.00
49) Acenaphthylene-d8	14.322	160	3346192	35.478	ng/u1	0.00
54) 4-Nitrophenol-d4	14.816	143	68932	4.470	ng/u1	0.00
60) Fluorene-d10	15.616	176	2549752	35.783	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.727	200	271710	29.892	ng/u1	0.00
73) Anthracene-d10	17.462	188	3835004	36.508	ng/u1	0.00
81) Pyrene-d10	19.745	212	4204251	48.742	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.803	264	2846221	38.699	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.439	149	80291	1.296	ng/u1	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036765.D
Acq On : 27 Sep 2022 03:16
Operator : CG/JU
Sample : N4746-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8M5


Quant Time: Sep 27 03:48:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 26 23:10:22 2022
Response via : Initial Calibration

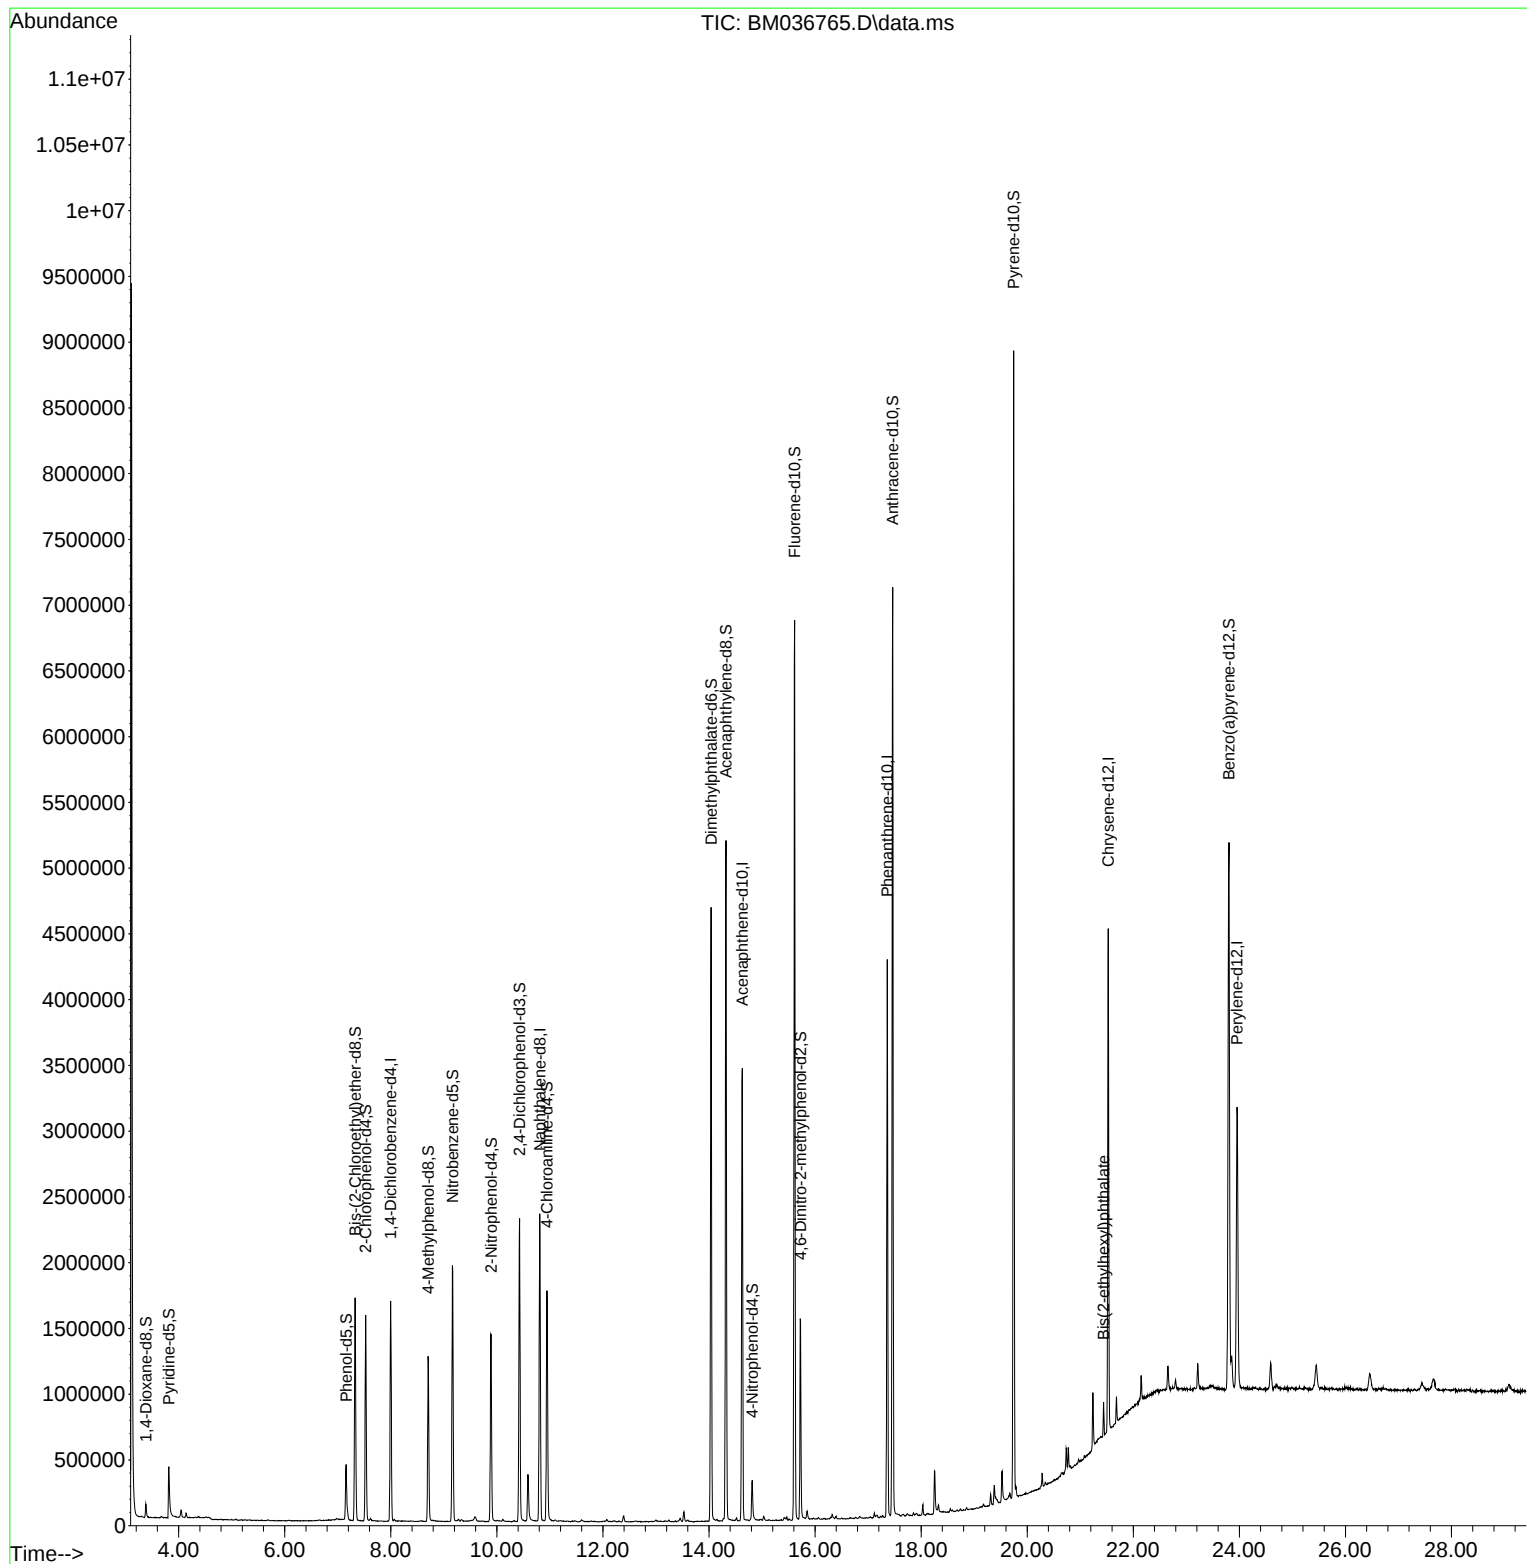

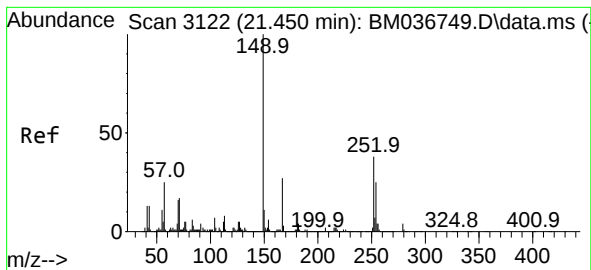

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.296 ng/ul
 RT: 21.439 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BM036765.D
 Acq: 27 Sep 2022 03:16

Instrument :
 BNA_M
 ClientSampleId :
 CB8M5

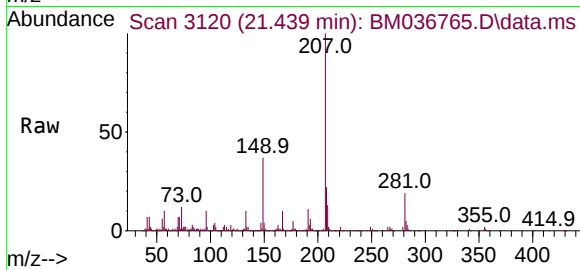

Tgt Ion:149	Resp:	80291
Ion	Ratio	Lower Upper
149	100	
167	25.9	22.0 33.0
279	4.1	3.3 4.9

