

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
 Data File : BM036766.D
 Acq On : 27 Sep 2022 03:52
 Operator : CG/JU
 Sample : N4746-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8M7

Quant Time: Sep 27 04:37:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 26 23:10:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.998	152	428271	20.000	ng/u1	0.00
20) Naphthalene-d8	10.810	136	1864132	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.621	164	1143460	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.363	188	2202310	20.000	ng/u1	0.00
79) Chrysene-d12	21.527	240	1645826	20.000	ng/u1	0.00
88) Perylene-d12	23.956	264	1384816	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	48332	4.231	ng/uL	0.00
4) Pyridine-d5	3.810	84	408506	12.261	ng/u1	0.00
7) Phenol-d5	7.157	99	112857	2.949	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	581093	25.001	ng/u1	0.00
11) 2-Chlorophenol-d4	7.528	132	303925	11.030	ng/u1	0.00
15) 4-Methylphenol-d8	8.704	113	240900	8.519	ng/u1	-0.01
21) Nitrobenzene-d5	9.163	128	371282	29.426	ng/u1	0.00
24) 2-Nitrophenol-d4	9.887	143	177560	15.711	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.428	165	355312	13.566	ng/u1	0.00
31) 4-Chloroaniline-d4	10.945	131	1045605	24.011	ng/u1	0.00
46) Dimethylphthalate-d6	14.039	166	2298936	29.810	ng/u1	0.00
49) Acenaphthylene-d8	14.322	160	2482560	27.139	ng/u1	0.00
54) 4-Nitrophenol-d4	14.827	143	23822	1.593	ng/u1	0.00
60) Fluorene-d10	15.610	176	1876959	27.158	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.721	200	77322	8.874	ng/u1	-0.01
73) Anthracene-d10	17.462	188	2797321	27.780	ng/u1	0.00
81) Pyrene-d10	19.745	212	3065519	37.861	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.797	264	2019093	29.843	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.416	88	19835	1.612	ng/uL	92
8) Phenol	7.181	94	57678	1.404	ng/u1	99
86) Bis(2-ethylhexyl)phtha...	21.439	149	265529	4.568	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036766.D
Acq On : 27 Sep 2022 03:52
Operator : CG/JU
Sample : N4746-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8M7

Quant Time: Sep 27 04:37:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 26 23:10:22 2022
Response via : Initial Calibration




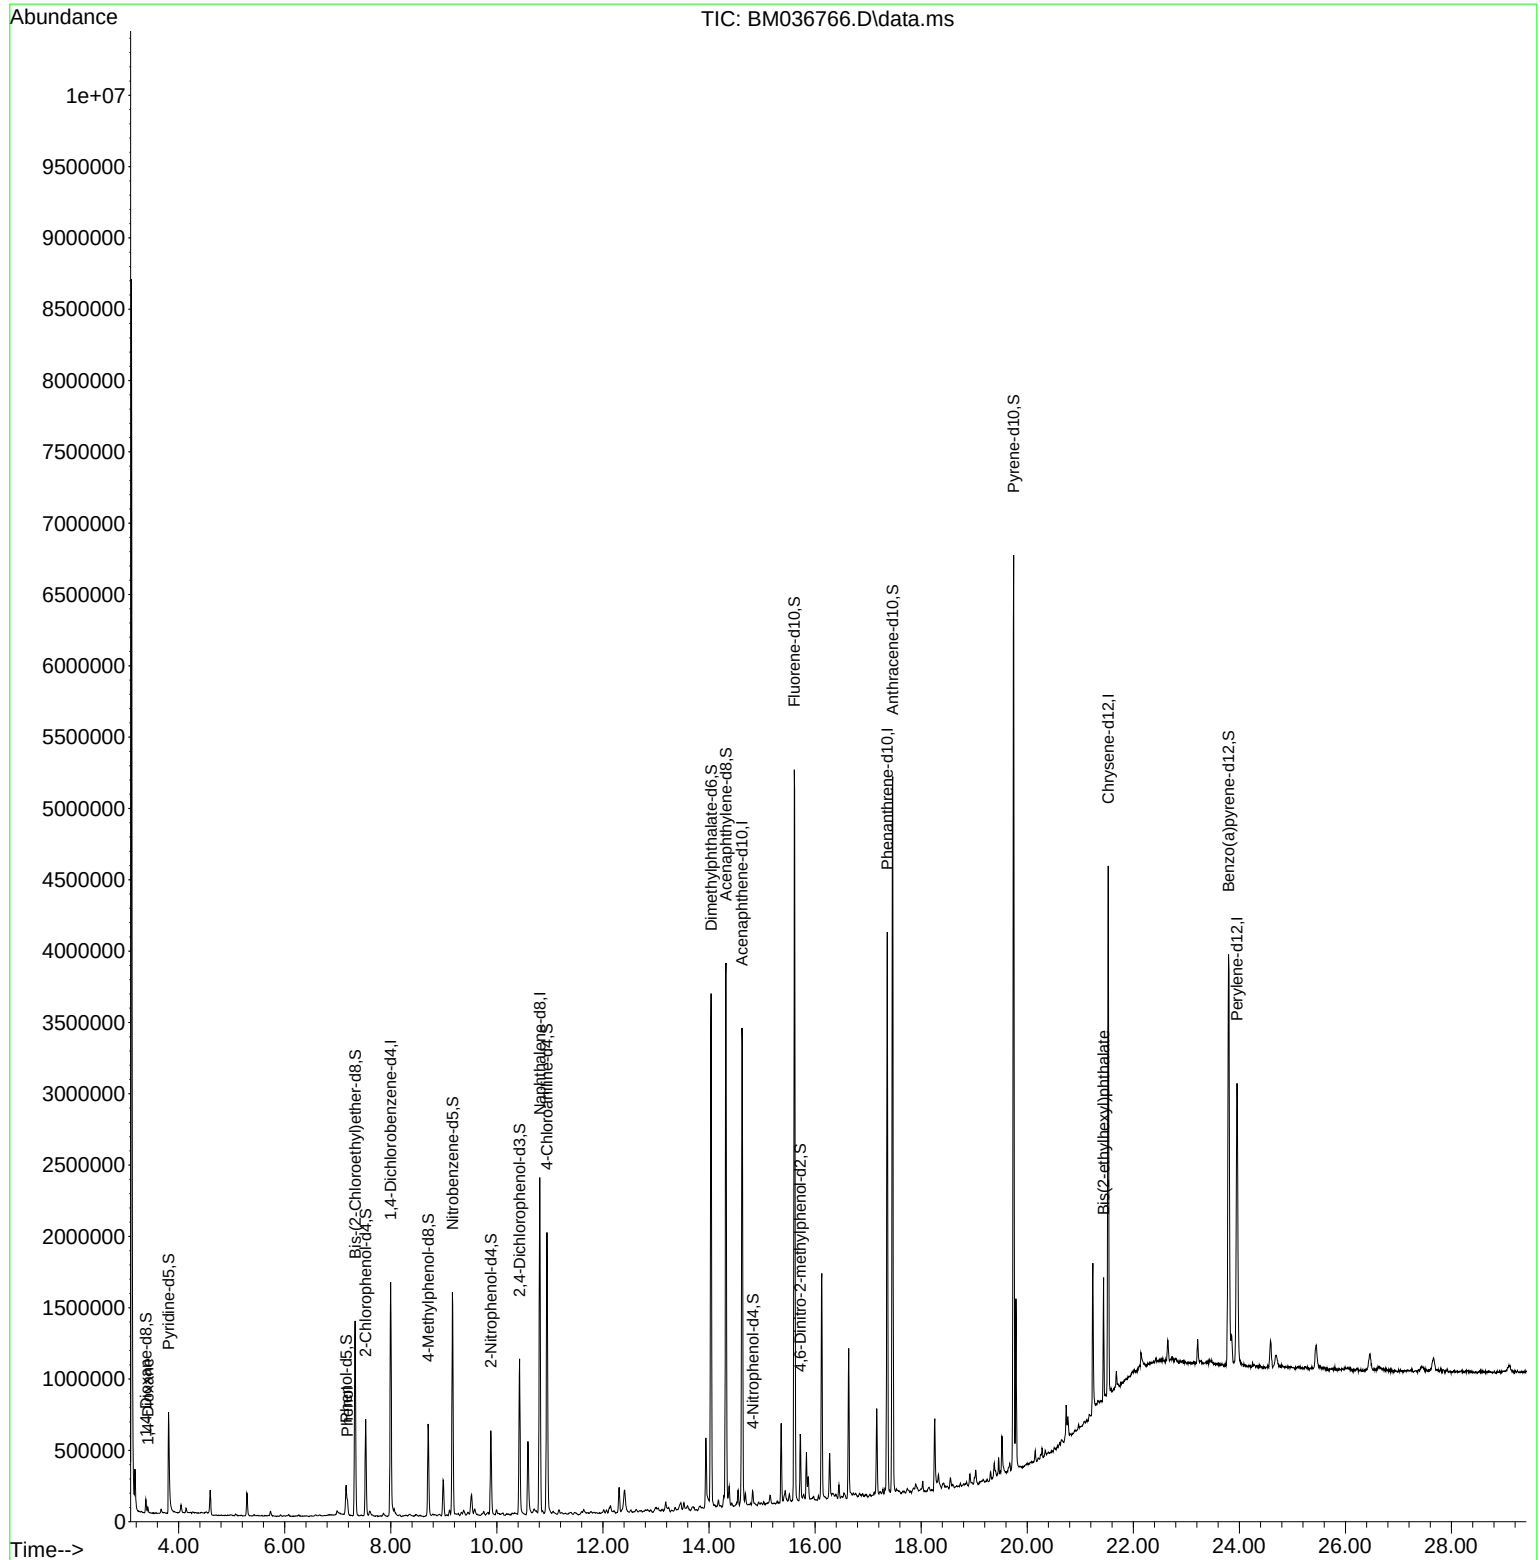


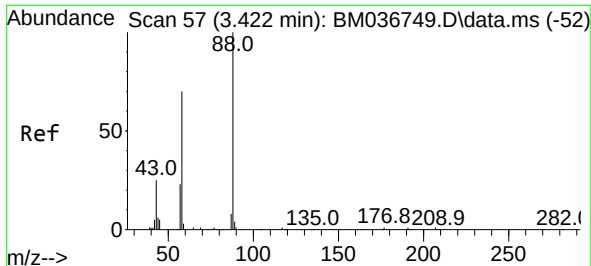

#2
 1,4-Dioxane
 Concen: 1.612 ng/uL
 RT: 3.416 min Scan# 50
 Delta R.T. -0.006 min
 Lab File: BM036766.D
 Acq: 27 Sep 2022 03:52




Instrument :
 BNA_M
 ClientSampleId :
 CB8M7


Tgt Ion: 88	Resp: 19835
Ion Ratio	Lower Upper
88 100	
43 30.0	23.1 34.7
58 62.7	56.6 85.0

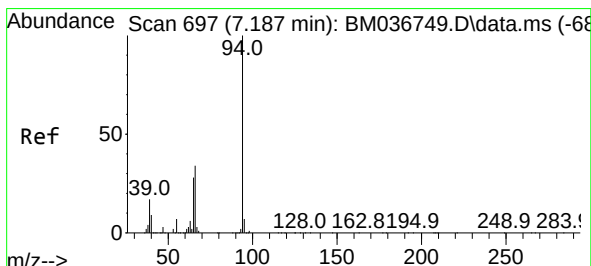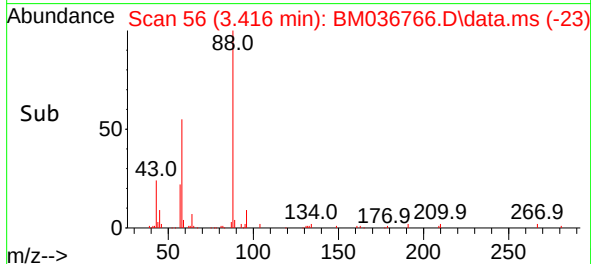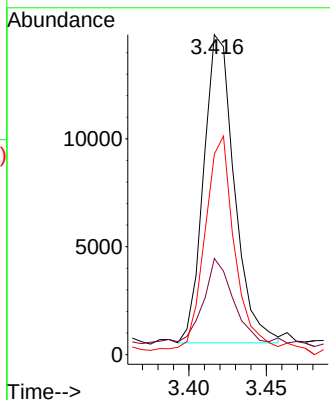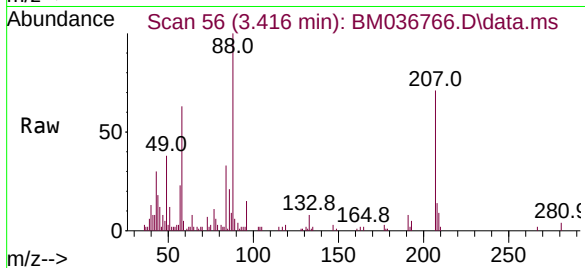

#8
 Phenol
 Concen: 1.404 ng/uL
 RT: 7.181 min Scan# 696
 Delta R.T. -0.006 min
 Lab File: BM036766.D
 Acq: 27 Sep 2022 03:52

Tgt Ion: 94	Resp: 57678
Ion Ratio	Lower Upper
94 100	
65 28.3	22.2 33.4
66 35.5	28.9 43.3

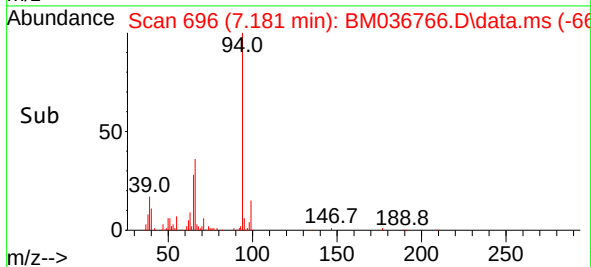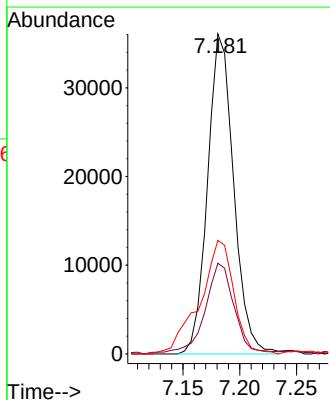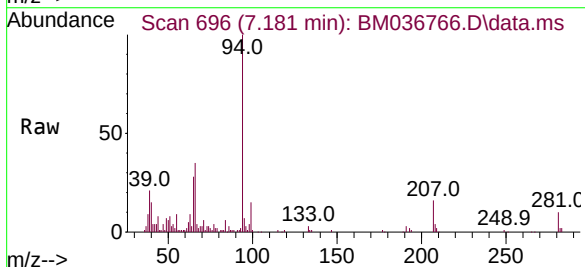

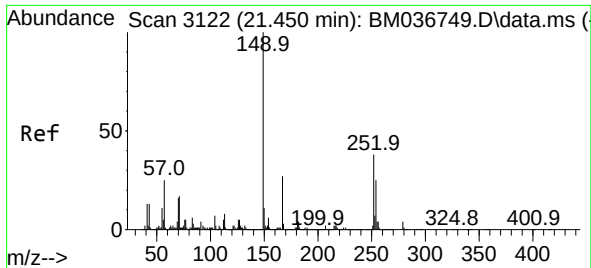

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 4.568 ng/ul
 RT: 21.439 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BM036766.D
 Acq: 27 Sep 2022 03:52

Instrument :
 BNA_M
 ClientSampleId :
 CB8M7

Tgt Ion:149 Resp: 265529
 Ion Ratio Lower Upper
 149 100
 167 26.3 22.0 33.0
 279 3.8 3.3 4.9

