

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
 Data File : BM036740.D
 Acq On : 26 Sep 2022 11:50
 Operator : CG/JU
 Sample : PB147814BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK814

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036740.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	3	5	20	rVB	325249	469223	5.59%	0.513%
2	3.387	47	51	59	rVB	105223	155029	1.85%	0.170%
3	3.811	121	123	145	rBV	1115317	1791035	21.35%	1.960%
4	4.146	176	180	185	rVB	30013	42268	0.50%	0.046%
5	7.157	686	692	708	rVB	1600452	2555665	30.47%	2.796%
6	7.334	715	722	733	rVB	1361152	2142849	25.55%	2.345%
7	7.534	748	756	766	rBV	1615628	2604368	31.05%	2.850%
8	8.004	829	836	846	rBV	1414759	2213166	26.38%	2.422%
9	8.710	949	956	966	rBV	2079408	3283698	39.15%	3.593%
10	9.169	1026	1034	1044	rBV	1613600	2553358	30.44%	2.794%
11	9.893	1150	1157	1171	rBV	1174491	1922430	22.92%	2.103%
12	10.428	1241	1248	1261	rBV	1914711	3240504	38.63%	3.546%
13	10.816	1305	1314	1323	rBV	1976132	3285582	39.17%	3.595%
14	10.951	1328	1337	1349	rBV	1933350	3297881	39.32%	3.608%
15	12.392	1576	1582	1590	rBV2	38269	63839	0.76%	0.070%
16	13.533	1768	1776	1781	rBV	42824	67140	0.80%	0.073%
17	13.604	1783	1788	1793	rVB2	7536	10511	0.13%	0.012%
18	14.039	1853	1862	1878	rBV	3599340	4798956	57.21%	5.251%
19	14.322	1903	1910	1925	rBV	3964736	5688712	67.82%	6.224%
20	14.628	1952	1962	1972	rBV	3153077	4392734	52.37%	4.806%
21	14.816	1988	1994	2012	rBV	1472916	2187369	26.08%	2.393%
22	15.286	2072	2074	2079	rVB6	6164	8602	0.10%	0.009%
23	15.616	2121	2130	2143	rBV	5469801	7404974	88.28%	8.102%
24	15.727	2143	2149	2161	rBV	1068824	1485978	17.72%	1.626%
25	15.857	2166	2171	2176	rVB	44114	69549	0.83%	0.076%
26	16.398	2259	2263	2267	rVB4	15272	20134	0.24%	0.022%
27	16.851	2333	2340	2347	rBV2	12266	23311	0.28%	0.026%
28	17.045	2369	2373	2380	rVB9	8408	12731	0.15%	0.014%
29	17.157	2387	2392	2393	rBV5	9764	10078	0.12%	0.011%
30	17.363	2421	2427	2436	rBV	3661320	4975502	59.32%	5.444%
31	17.463	2438	2444	2465	rVB	5808127	7925125	94.48%	8.671%
32	17.921	2518	2522	2528	rVB	14688	21801	0.26%	0.024%
33	19.315	2755	2759	2764	rBV	55403	74368	0.89%	0.081%
34	19.380	2767	2770	2775	rVB	54646	75812	0.90%	0.083%
35	19.745	2826	2832	2843	rBV	6428248	8388239	100.00%	9.178%
36	20.739	2998	3001	3007	rBV	128199	148111	1.77%	0.162%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036740.D
Acq On : 26 Sep 2022 11:50
Operator : CG/JU
Sample : PB147814BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK814

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Title : SVOA CALIBRATION

37	21.533	3131	3136	3142	rBV	3290831	4232964	50.46%	4.632%
38	23.809	3516	3523	3531	rBV2	3076921	6095000	72.66%	6.669%
39	23.962	3544	3549	3561	rVB2	1824527	3654973	43.57%	3.999%




Sum of corrected areas: 91393569

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036740.D
Acq On : 26 Sep 2022 11:50
Operator : CG/JU
Sample : PB147814BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK814

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

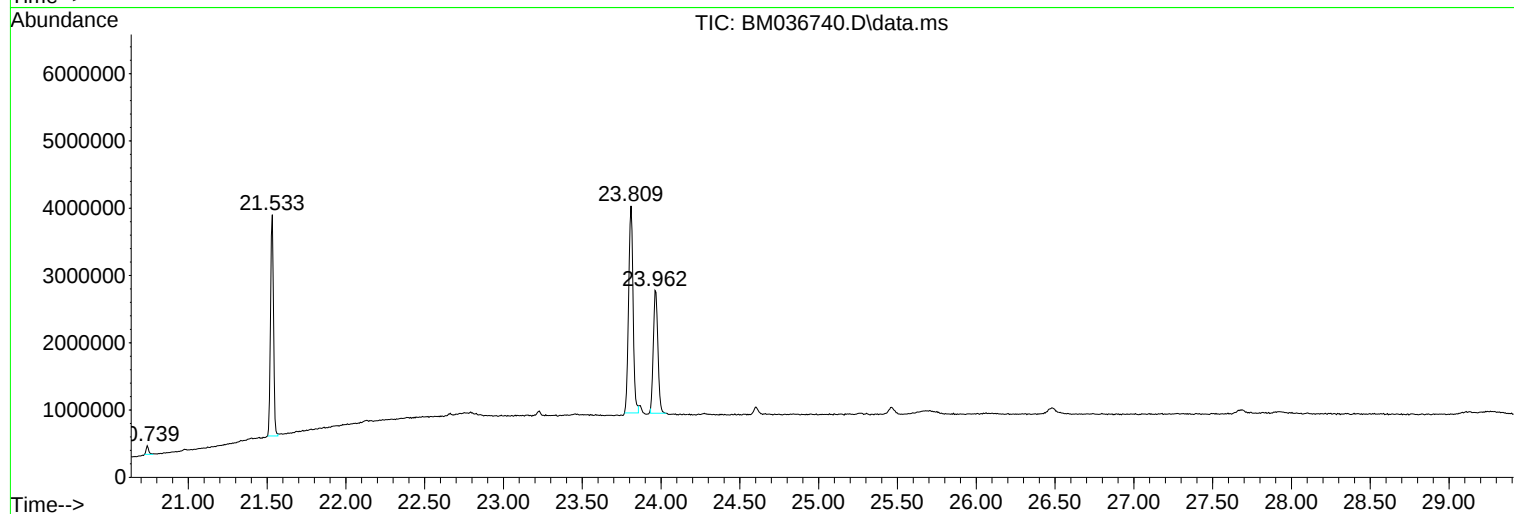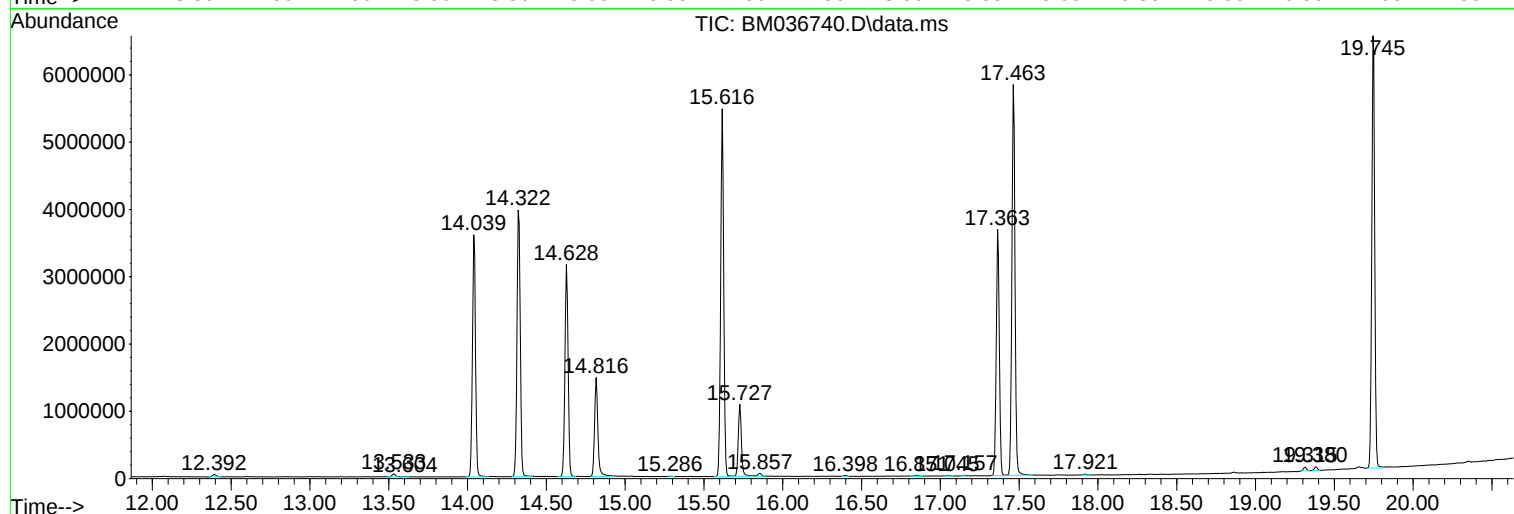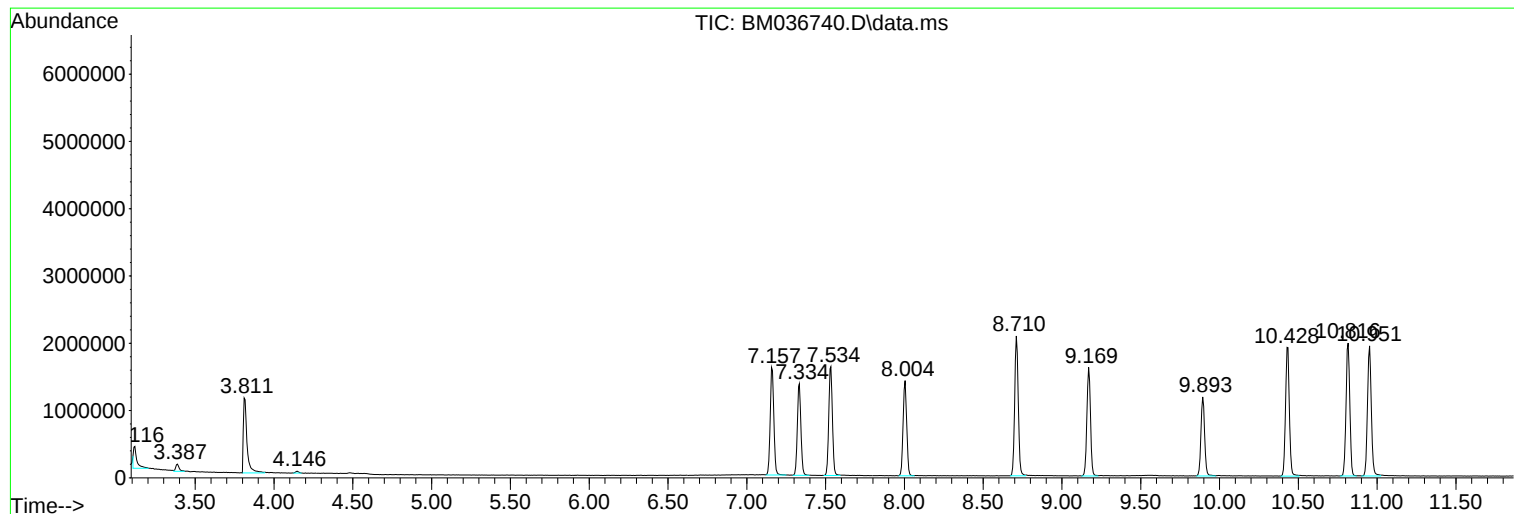

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036740.D
Acq On : 26 Sep 2022 11:50
Operator : CG/JU
Sample : PB147814BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK814










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.116	4.24 ng/ul	469223	1,4-Dichlorobenzene-d4	8.004

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	25
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

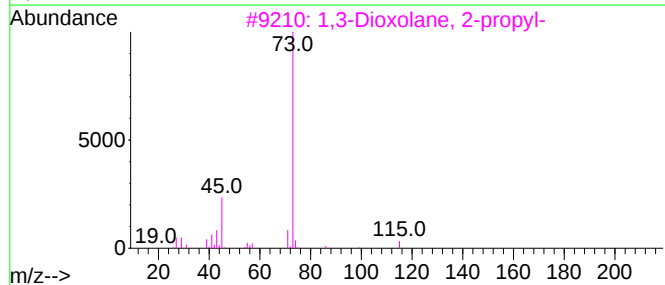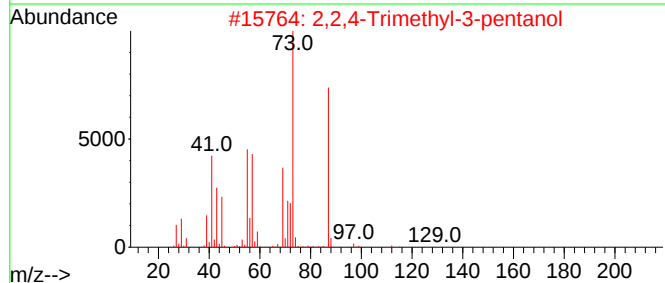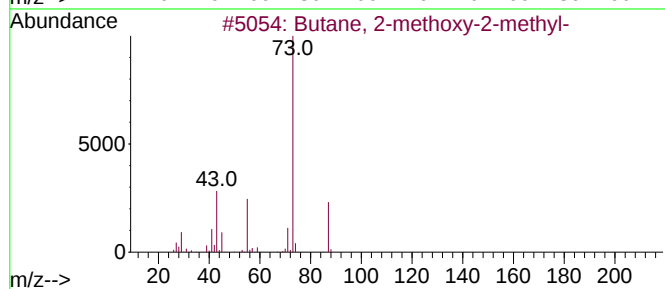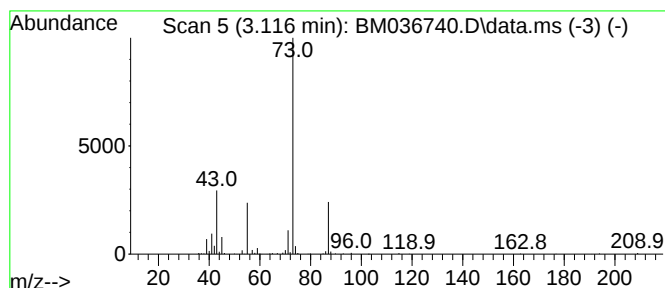

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036740.D
Acq On : 26 Sep 2022 11:50
Operator : CG/JU
Sample : PB147814BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK814

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.116	4.2	ng/u1	469223	1	8.004	2213170	20.0