

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
 Data File : BM036741.D
 Acq On : 26 Sep 2022 12:27
 Operator : CG/JU
 Sample : PB147828BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK828

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	3	5	21	rVB	213708	320075	3.83%	0.349%
2	3.387	47	51	62	rVB	107967	155897	1.87%	0.170%
3	3.810	121	123	140	rBV	1120695	1793761	21.48%	1.956%
4	4.146	176	180	187	rVB	29048	40445	0.48%	0.044%
5	7.163	686	693	704	rVB	1564400	2503791	29.98%	2.730%
6	7.334	715	722	734	rVB	1363233	2116939	25.35%	2.308%
7	7.534	748	756	771	rBV	1633550	2576567	30.85%	2.810%
8	8.004	828	836	845	rBV	1420400	2221916	26.60%	2.423%
9	8.710	947	956	974	rBV	2049841	3240676	38.80%	3.534%
10	9.169	1026	1034	1044	rBV	1591026	2519743	30.17%	2.748%
11	9.892	1149	1157	1166	rBV	1158099	1867624	22.36%	2.037%
12	10.433	1241	1249	1258	rBV	1869887	3149458	37.71%	3.434%
13	10.816	1305	1314	1326	rBV	1987367	3319457	39.75%	3.620%
14	10.951	1328	1337	1357	rBV	1916897	3216263	38.51%	3.507%
15	12.392	1574	1582	1590	rVB2	36376	64950	0.78%	0.071%
16	13.527	1770	1775	1782	rBV4	15167	25039	0.30%	0.027%
17	13.604	1782	1788	1791	rBV7	7344	10897	0.13%	0.012%
18	14.039	1854	1862	1874	rBV	3394772	4698828	56.26%	5.124%
19	14.327	1903	1911	1922	rBV	3879216	5669179	67.88%	6.182%
20	14.627	1954	1962	1970	rBV	3148463	4530966	54.25%	4.941%
21	14.815	1987	1994	2011	rBV	1453783	2178383	26.08%	2.375%
22	14.986	2021	2023	2028	rVB6	6566	9187	0.11%	0.010%
23	15.033	2028	2031	2037	rVB7	7219	11505	0.14%	0.013%
24	15.615	2121	2130	2143	rBV	5371995	7322083	87.67%	7.984%
25	15.727	2143	2149	2162	rVV	1090141	1479122	17.71%	1.613%
26	15.857	2166	2171	2177	rVB2	43848	70868	0.85%	0.077%
27	16.398	2259	2263	2269	rBV8	11286	18839	0.23%	0.021%
28	16.851	2335	2340	2345	rBV5	10638	17223	0.21%	0.019%
29	17.045	2370	2373	2377	rVB6	8002	9573	0.11%	0.010%
30	17.145	2388	2390	2396	rVB5	7970	12612	0.15%	0.014%
31	17.368	2421	2428	2436	rBV	3736735	5218276	62.48%	5.690%
32	17.462	2438	2444	2459	rVV	5689500	7772630	93.07%	8.476%
33	17.915	2518	2521	2525	rVB4	15026	19334	0.23%	0.021%
34	18.862	2679	2682	2686	rBV2	16639	22845	0.27%	0.025%
35	19.315	2755	2759	2766	rBV4	60512	87602	1.05%	0.096%
36	19.386	2767	2771	2775	rVB	53135	74184	0.89%	0.081%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036741.D
Acq On : 26 Sep 2022 12:27
Operator : CG/JU
Sample : PB147828BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK828

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Title : SVOA CALIBRATION

37	19.745	2827	2832	2842	rBV	6169051	8351720	100.00%	9.107%
38	20.739	2998	3001	3006	rBV2	131857	157749	1.89%	0.172%
39	21.533	3131	3136	3144	rBV	3616122	4671967	55.94%	5.095%
40	23.809	3516	3523	3530	rBV2	3146512	6131160	73.41%	6.686%
41	23.968	3544	3550	3563	rVB2	2014257	4024798	48.19%	4.389%




Sum of corrected areas: 91704131

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036741.D
Acq On : 26 Sep 2022 12:27
Operator : CG/JU
Sample : PB147828BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK828

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

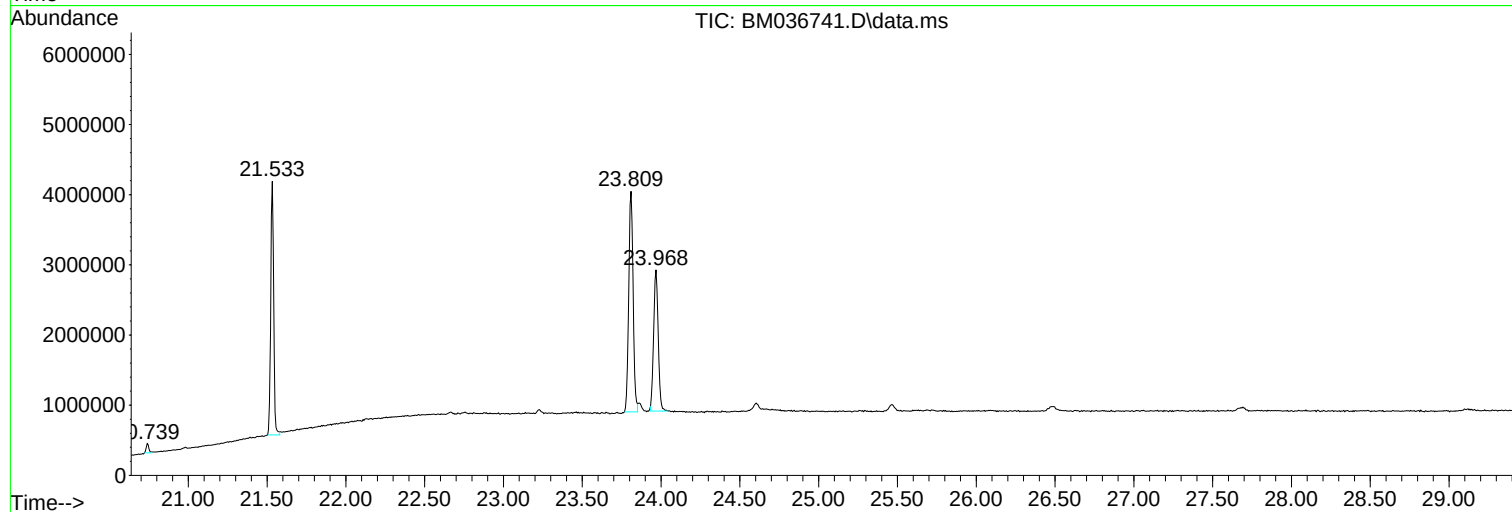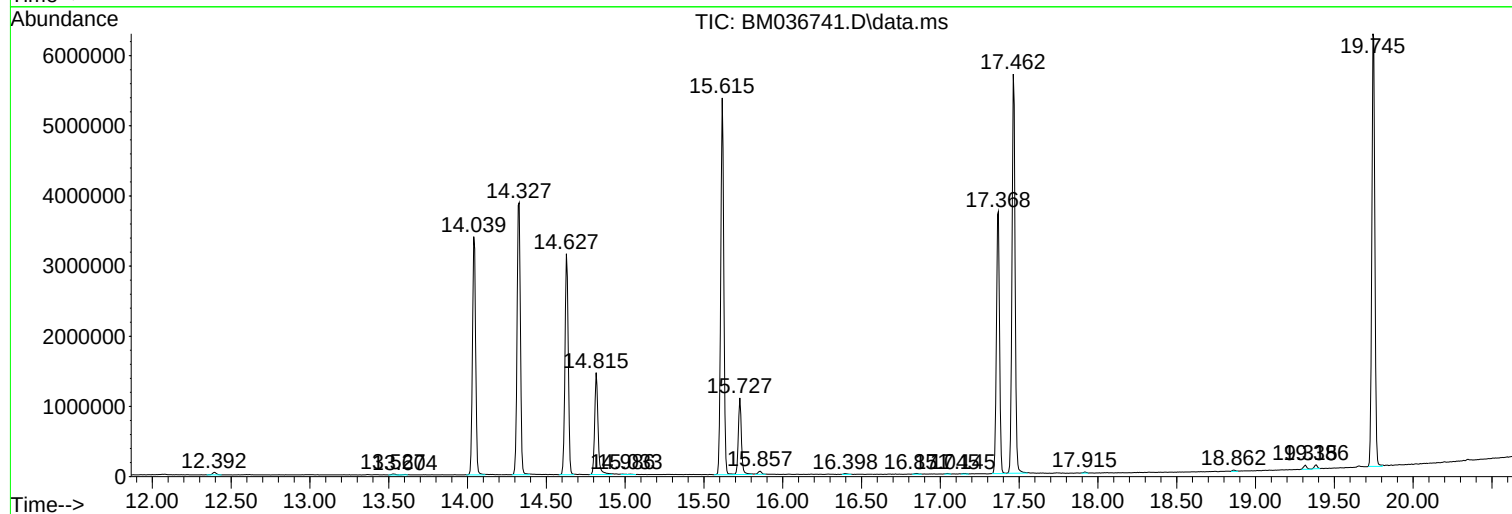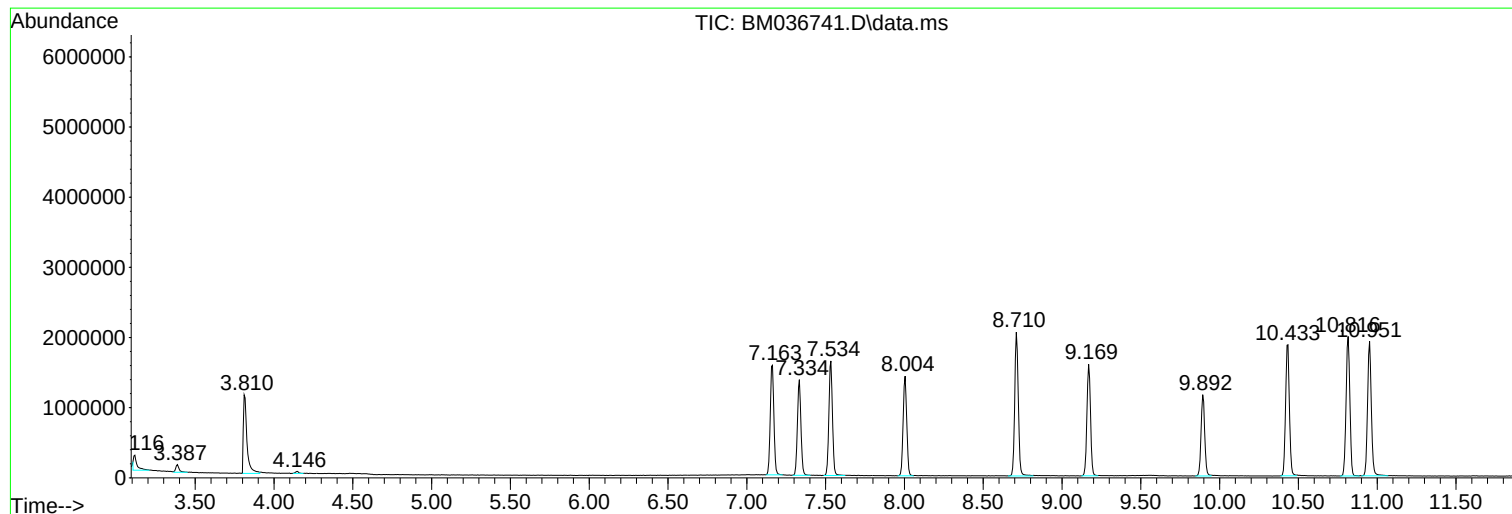

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036741.D
Acq On : 26 Sep 2022 12:27
Operator : CG/JU
Sample : PB147828BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK828










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.116	2.88 ng/ul	320075	1,4-Dichlorobenzene-d4	8.004

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	56
3			N-Ethylformamide	73	C3H7NO	000627-45-2	9
4			Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	9
5			1-(2-Methoxyethoxy)-2-methyl-2-p...	162	C8H18O3	1000364-24-4	9

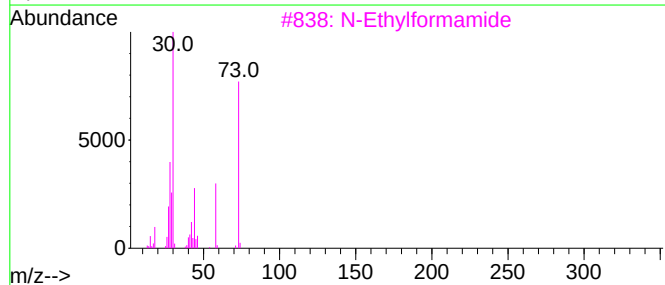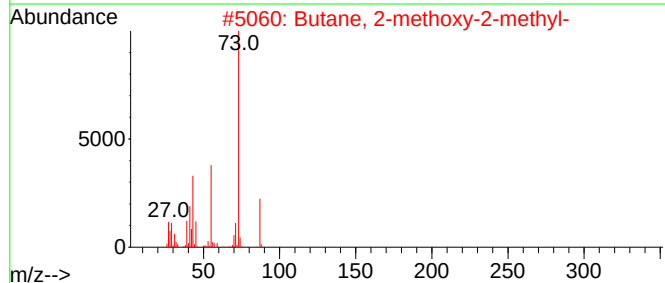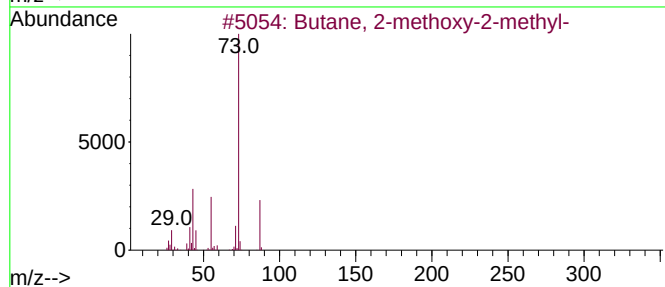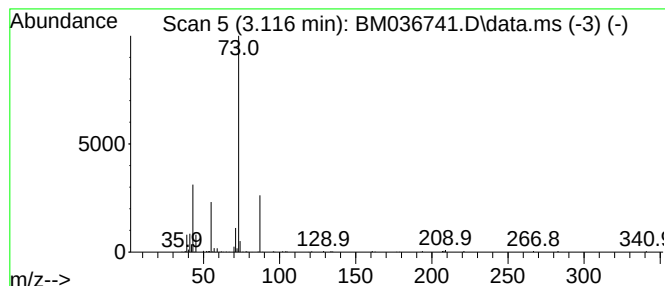

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036741.D
Acq On : 26 Sep 2022 12:27
Operator : CG/JU
Sample : PB147828BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK828

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.116	2.9	ng/u1	320075	1	8.004	2221920	20.0