

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
 Data File : BM036752.D
 Acq On : 26 Sep 2022 19:21
 Operator : CG/JU
 Sample : PB147885BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK885

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036752.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	3	5	21	rVB	271526	329647	3.82%	0.347%
2	3.387	47	51	57	rVB	113136	152787	1.77%	0.161%
3	3.810	120	123	140	rBV	1313706	2050426	23.76%	2.161%
4	4.146	176	180	184	rVB	25561	36801	0.43%	0.039%
5	7.163	686	693	706	rVB	1798188	2894514	33.54%	3.051%
6	7.334	715	722	733	rVB	1579437	2452876	28.42%	2.585%
7	7.534	747	756	774	rVB	1892239	2962559	34.33%	3.122%
8	8.004	829	836	845	rVB	1261434	2000765	23.18%	2.109%
9	8.710	949	956	967	rBV	2328085	3731842	43.24%	3.933%
10	9.169	1025	1034	1047	rBV	1860527	2944530	34.12%	3.103%
11	9.892	1149	1157	1166	rBV	1375216	2201120	25.50%	2.320%
12	10.433	1239	1249	1264	rBV	2196027	3682956	42.67%	3.882%
13	10.816	1306	1314	1323	rBV	1830334	3013037	34.91%	3.175%
14	10.951	1328	1337	1353	rBV	2189294	3697110	42.84%	3.896%
15	12.069	1520	1527	1529	rBV8	7441	14104	0.16%	0.015%
16	12.392	1576	1582	1592	rBV	41743	76037	0.88%	0.080%
17	13.527	1771	1775	1781	rBV3	19619	32930	0.38%	0.035%
18	13.598	1784	1787	1793	rVB3	6201	10596	0.12%	0.011%
19	14.039	1856	1862	1872	rBV	3808439	5381214	62.35%	5.671%
20	14.327	1903	1911	1926	rBV	4528999	6537537	75.75%	6.890%
21	14.627	1955	1962	1970	rBV	2869268	4012810	46.50%	4.229%
22	14.815	1987	1994	2010	rBV	1567825	2395574	27.76%	2.525%
23	15.039	2028	2032	2037	rVB7	7722	14755	0.17%	0.016%
24	15.421	2091	2097	2100	rBV8	5720	9153	0.11%	0.010%
25	15.615	2123	2130	2143	rBV	6054434	8268485	95.81%	8.714%
26	15.727	2143	2149	2158	rBV	1252516	1641130	19.02%	1.730%
27	15.857	2166	2171	2180	rVB	49054	80302	0.93%	0.085%
28	16.398	2257	2263	2268	rBV6	14255	24032	0.28%	0.025%
29	16.845	2336	2339	2345	rVB2	12057	16924	0.20%	0.018%
30	17.045	2370	2373	2377	rBV5	9402	12357	0.14%	0.013%
31	17.151	2387	2391	2397	rVB5	8211	12014	0.14%	0.013%
32	17.362	2421	2427	2438	rBV	3072603	4442486	51.47%	4.682%
33	17.462	2438	2444	2460	rVV	5907890	8325596	96.47%	8.774%
34	17.921	2519	2522	2527	rVB3	13275	16160	0.19%	0.017%
35	18.856	2678	2681	2685	rBV3	18566	27192	0.32%	0.029%
36	19.315	2755	2759	2764	rBV2	61566	83556	0.97%	0.088%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036752.D
Acq On : 26 Sep 2022 19:21
Operator : CG/JU
Sample : PB147885BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK885

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Title : SVOA CALIBRATION

37	19.386	2767	2771	2776	rVV	56133	78057	0.90%	0.082%
38	19.750	2827	2833	2841	rBV	6677557	8630394	100.00%	9.096%
39	20.739	2998	3001	3007	rBV2	161930	221378	2.57%	0.233%
40	21.533	3131	3136	3143	rBV	2911711	3641688	42.20%	3.838%
41	23.809	3517	3523	3530	rBV2	2977695	5736394	66.47%	6.046%
42	23.968	3544	3550	3558	rVB	1485315	2990833	34.65%	3.152%




Sum of corrected areas: 94884658

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036752.D
Acq On : 26 Sep 2022 19:21
Operator : CG/JU
Sample : PB147885BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK885

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

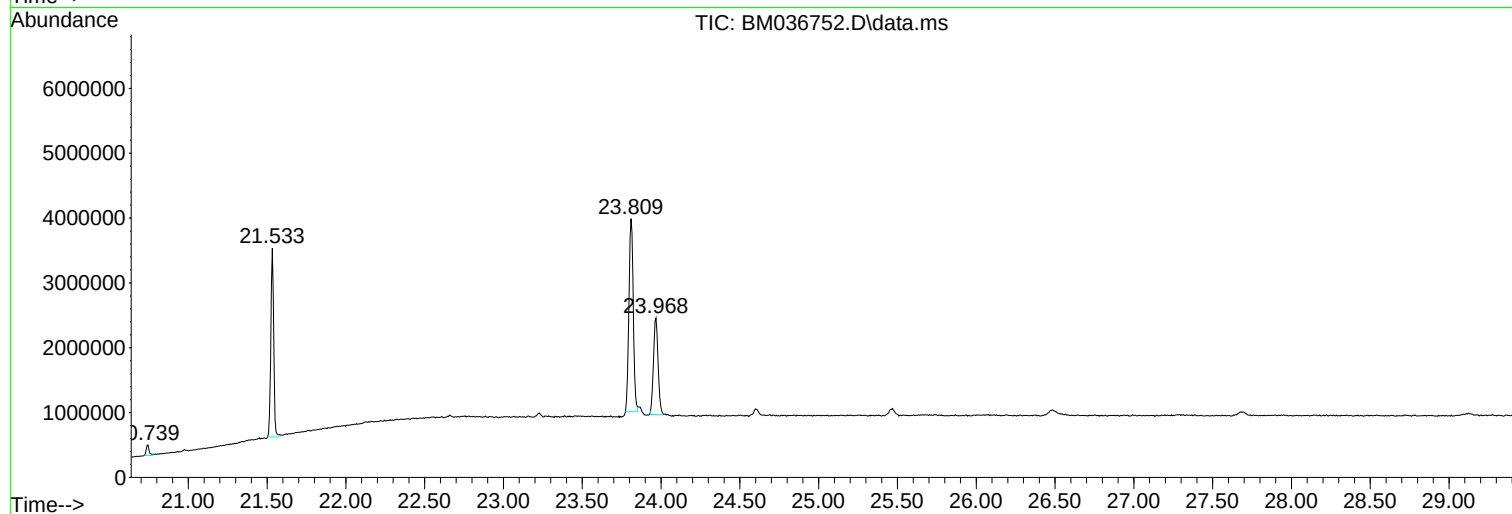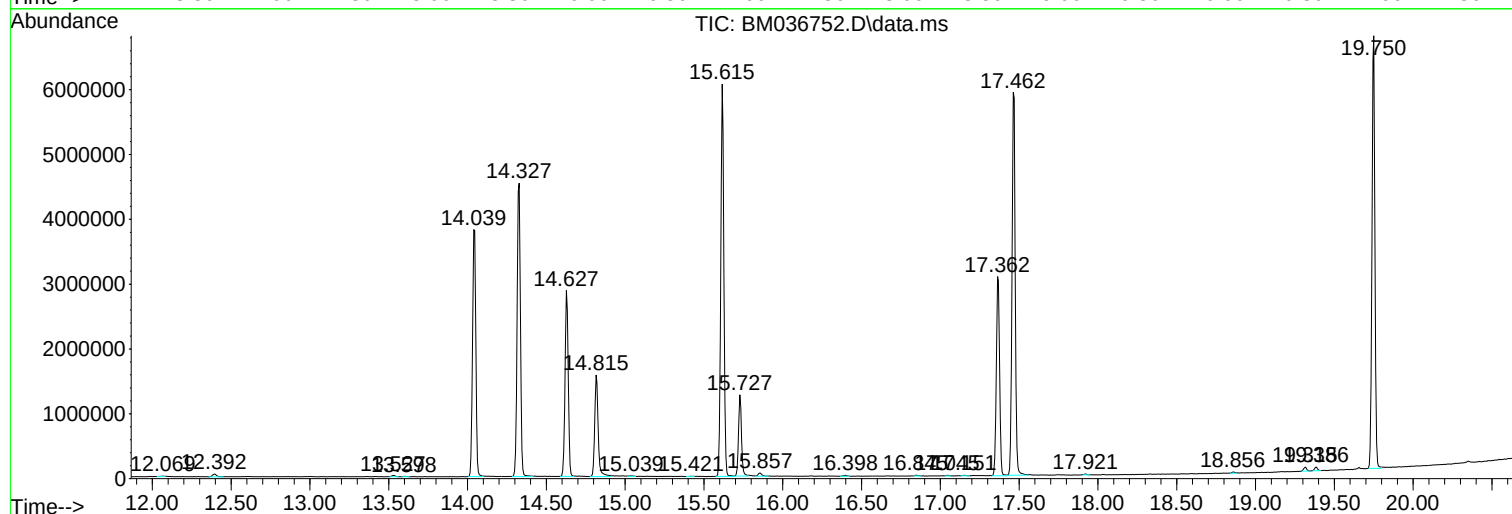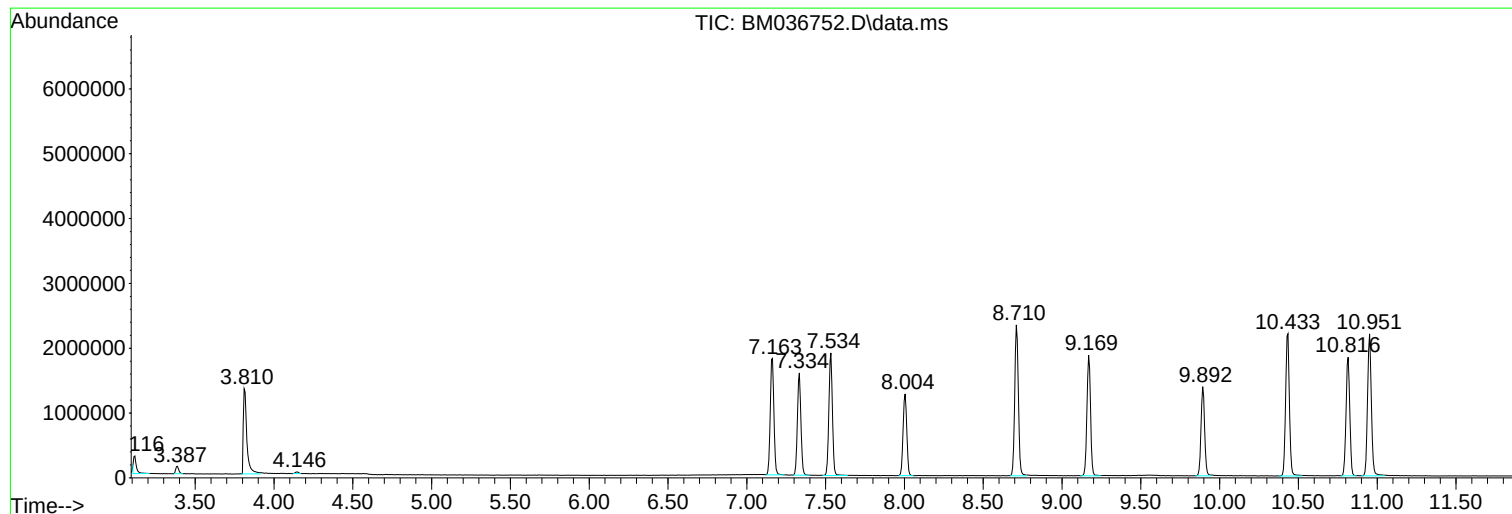

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036752.D
Acq On : 26 Sep 2022 19:21
Operator : CG/JU
Sample : PB147885BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK885










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.116	3.30 ng/ul	329647	1,4-Dichlorobenzene-d4	8.004

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
4			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	25
5			1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	12

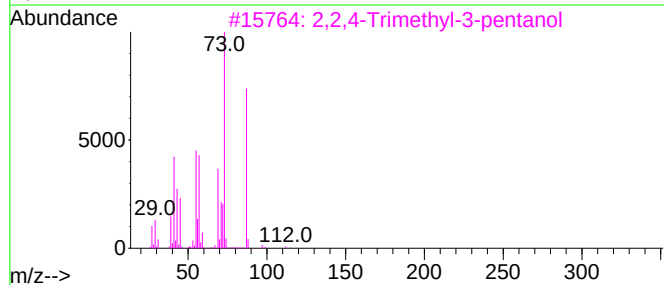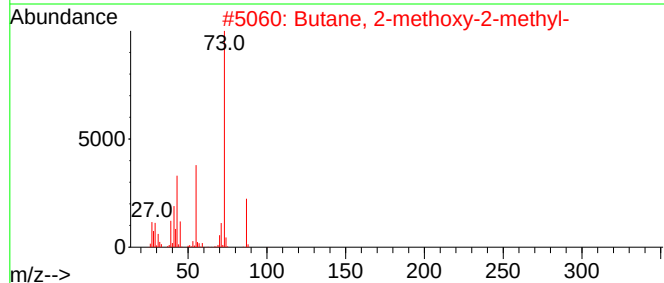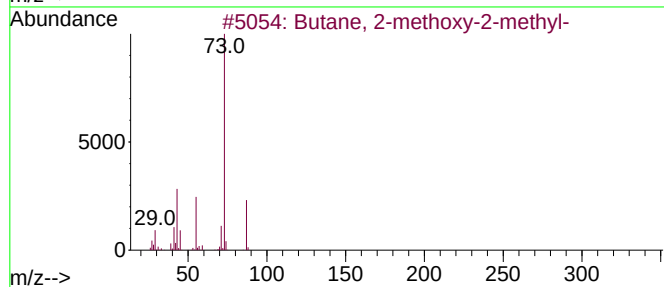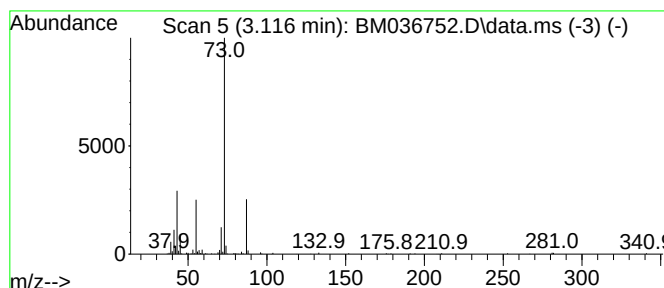

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036752.D
Acq On : 26 Sep 2022 19:21
Operator : CG/JU
Sample : PB147885BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK885

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.116	3.3	ng/u1	329647	1	8.004	2000770	20.0