

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
 Data File : BM036754.D
 Acq On : 26 Sep 2022 20:35
 Operator : CG/JU
 Sample : PB147882BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK882

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036754.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.110	3	4	15	rVB	321874	362501	3.80%	0.342%
2	3.381	46	50	57	rBV	105394	148810	1.56%	0.140%
3	3.810	120	123	139	rBV	1295831	1965672	20.61%	1.854%
4	4.146	175	180	186	rBV	31293	47525	0.50%	0.045%
5	7.157	685	692	704	rVB	1818996	2859715	29.98%	2.697%
6	7.328	715	721	731	rVB	1529525	2417455	25.35%	2.280%
7	7.528	747	755	764	rBV	1794595	2890285	30.31%	2.726%
8	8.004	827	836	843	rBV	1671220	2671957	28.02%	2.520%
9	8.710	949	956	971	rBV	2360399	3726345	39.07%	3.515%
10	9.169	1026	1034	1044	rBV	1822784	2910700	30.52%	2.745%
11	9.892	1149	1157	1170	rBV	1364589	2225155	23.33%	2.099%
12	10.428	1241	1248	1264	rBV	2232915	3664719	38.43%	3.457%
13	10.816	1306	1314	1323	rBV	2399655	4032854	42.29%	3.804%
14	10.951	1328	1337	1353	rBV	2191737	3794193	39.78%	3.579%
15	12.074	1521	1528	1534	rBV7	10584	24933	0.26%	0.024%
16	12.392	1575	1582	1588	rBV	43033	78215	0.82%	0.074%
17	13.533	1770	1776	1784	rBV	64830	103566	1.09%	0.098%
18	14.039	1856	1862	1881	rBV	4176407	5800128	60.82%	5.471%
19	14.321	1903	1910	1920	rBV	4588228	6721559	70.48%	6.340%
20	14.627	1955	1962	1973	rBV	3952768	5456468	57.21%	5.147%
21	14.815	1987	1994	2010	rBV	1701602	2614729	27.42%	2.466%
22	15.039	2029	2032	2038	rVB7	9104	14074	0.15%	0.013%
23	15.615	2123	2130	2142	rBV	6367051	8642379	90.62%	8.152%
24	15.727	2143	2149	2161	rVV	1394059	1885162	19.77%	1.778%
25	15.857	2166	2171	2180	rVB2	45890	84672	0.89%	0.080%
26	16.180	2223	2226	2232	rVB7	5808	12104	0.13%	0.011%
27	16.398	2259	2263	2268	rVB5	13620	16635	0.17%	0.016%
28	16.851	2335	2340	2344	rBV3	14439	20117	0.21%	0.019%
29	17.039	2369	2372	2377	rVB7	10068	16135	0.17%	0.015%
30	17.151	2388	2391	2397	rBV8	8904	15602	0.16%	0.015%
31	17.368	2421	2428	2438	rBV	4044598	5991401	62.82%	5.651%
32	17.462	2438	2444	2458	rVV	6558672	9175076	96.20%	8.654%
33	17.921	2519	2522	2526	rVB3	14061	17609	0.18%	0.017%
34	19.315	2755	2759	2763	rBV3	61477	79653	0.84%	0.075%
35	19.380	2767	2770	2775	rVV2	62188	82240	0.86%	0.078%
36	19.750	2827	2833	2846	rBV	7347603	9537308	100.00%	8.996%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036754.D
Acq On : 26 Sep 2022 20:35
Operator : CG/JU
Sample : PB147882BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK882

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Title : SVOA CALIBRATION

37	20.745	2998	3002	3006	rBV2	162851	210950	2.21%	0.199%
38	21.533	3131	3136	3143	rBV	3729843	4908559	51.47%	4.630%
39	23.815	3517	3524	3531	rBV2	3325520	6620056	69.41%	6.244%
40	23.968	3544	3550	3561	rVB2	2114001	4174494	43.77%	3.937%




Sum of corrected areas: 106021710

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036754.D
Acq On : 26 Sep 2022 20:35
Operator : CG/JU
Sample : PB147882BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK882

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

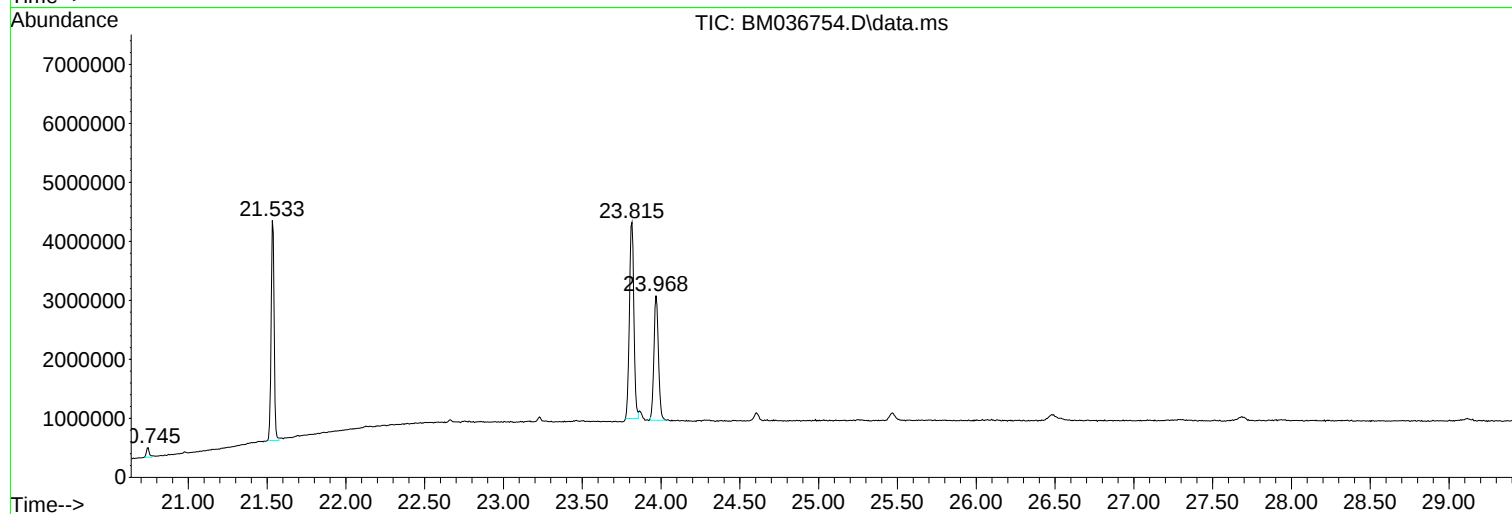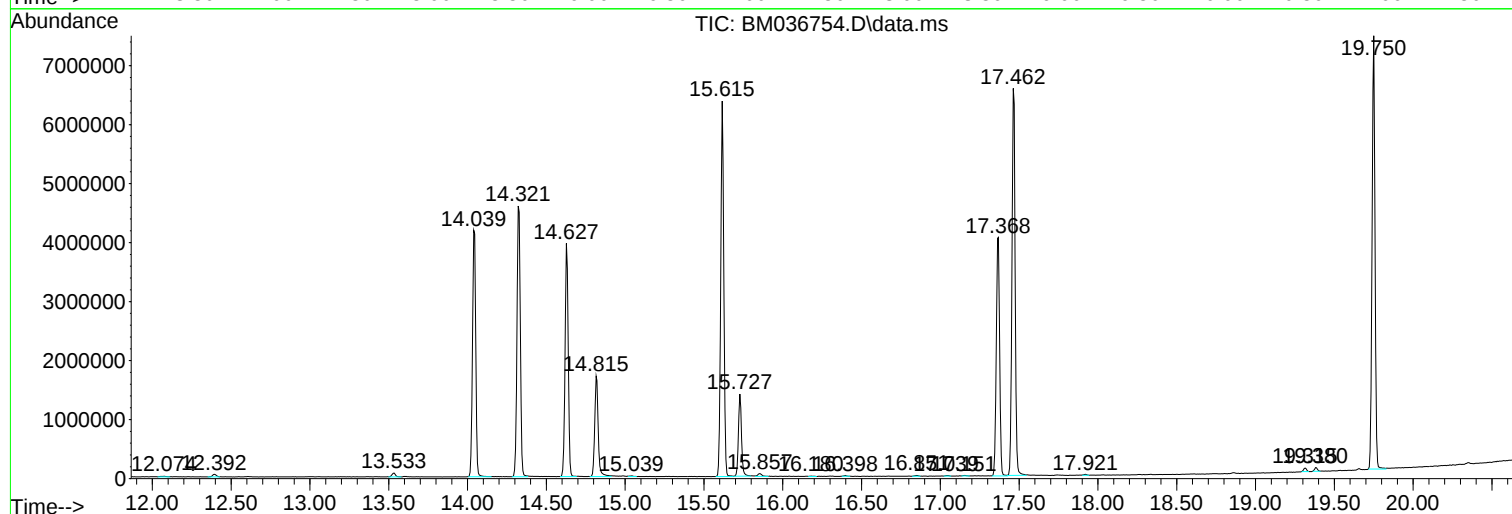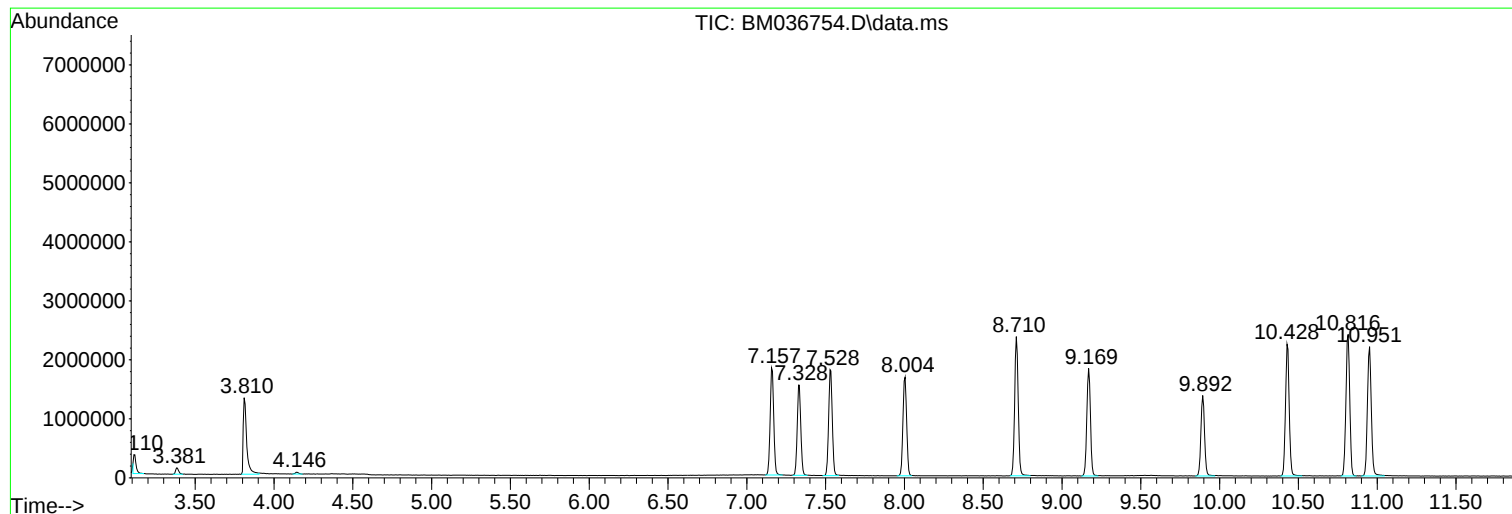

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036754.D
Acq On : 26 Sep 2022 20:35
Operator : CG/JU
Sample : PB147882BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK882










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.110	2.71 ng/ul	362501	1,4-Dichlorobenzene-d4	8.004

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	56
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
4			Scyllo-Inositol, 1-C-methyl-	194	C7H14O6	000564-92-1	36
5			2,5-Dimethyl-4-hydroxy-3-hexanone	144	C8H16O2	000815-77-0	25

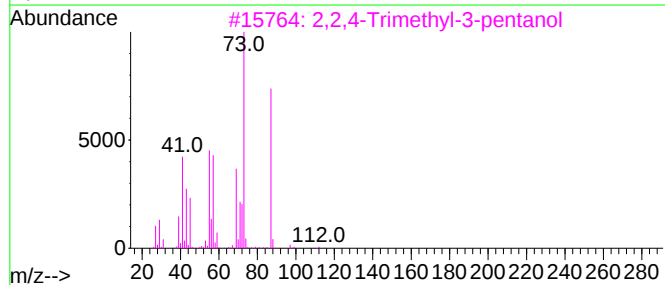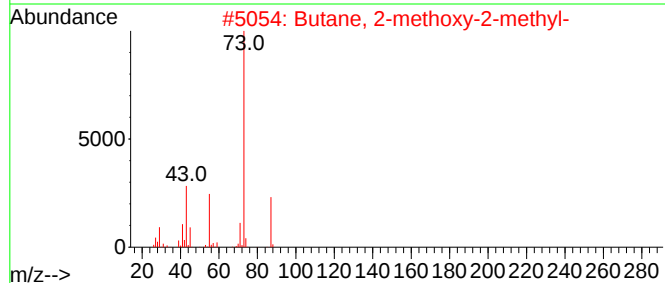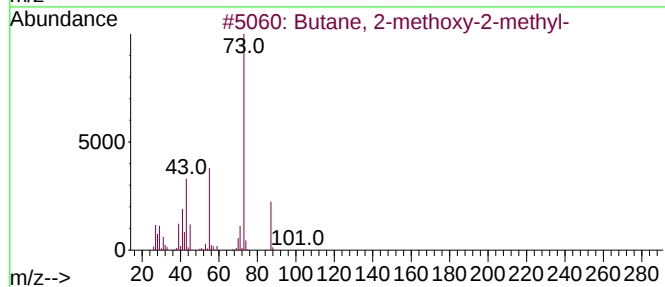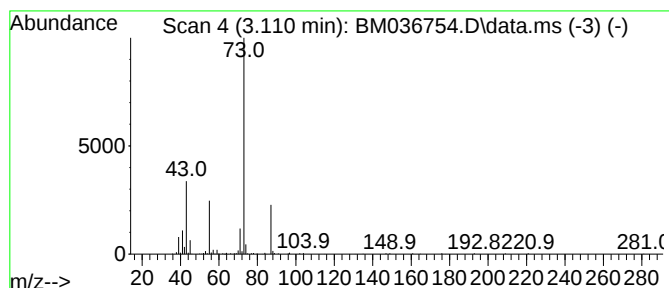

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036754.D
Acq On : 26 Sep 2022 20:35
Operator : CG/JU
Sample : PB147882BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK882

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.110	2.7	ng/u1	362501	1	8.004	2671960	20.0