

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
 Data File : BM036760.D
 Acq On : 27 Sep 2022 00:15
 Operator : CG/JU
 Sample : N4748-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ESQS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036760.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.110	3	4	23	rVB	8775159	9222771	79.03%	8.052%
2	3.381	46	50	58	rVB	91684	123352	1.06%	0.108%
3	3.816	122	124	144	rBV	329713	567656	4.86%	0.496%
4	4.046	159	163	168	rVB	50090	74084	0.63%	0.065%
5	4.146	176	180	186	rVB	29783	43503	0.37%	0.038%
6	5.081	336	339	344	rBV4	8706	13811	0.12%	0.012%
7	7.157	685	692	701	rVB	495718	777940	6.67%	0.679%
8	7.328	714	721	733	rBV	1827203	2821271	24.17%	2.463%
9	7.528	748	755	767	rBV	1748390	2716088	23.27%	2.371%
10	7.616	767	770	775	rVB7	9783	16197	0.14%	0.014%
11	7.998	827	835	844	rBV	1504341	2361613	20.24%	2.062%
12	8.063	844	846	853	rVB7	10851	17856	0.15%	0.016%
13	8.710	948	956	967	rBV	1401737	2271924	19.47%	1.983%
14	9.169	1026	1034	1047	rBV	2137794	3430879	29.40%	2.995%
15	9.334	1057	1062	1069	rVB10	7513	13774	0.12%	0.012%
16	9.587	1100	1105	1110	rVB5	13845	24521	0.21%	0.021%
17	9.892	1148	1157	1168	rBV	1538414	2516857	21.57%	2.197%
18	10.428	1239	1248	1263	rBV	2433603	3944265	33.80%	3.443%
19	10.598	1272	1277	1283	rBV9	10634	18826	0.16%	0.016%
20	10.810	1304	1313	1324	rBV	2091137	3512430	30.10%	3.066%
21	10.945	1329	1336	1355	rBV	1962375	3369511	28.87%	2.942%
22	11.598	1442	1447	1452	rBV8	18227	38850	0.33%	0.034%
23	12.392	1573	1582	1591	rBV2	47399	87198	0.75%	0.076%
24	12.575	1604	1613	1622	rBV3	36862	86002	0.74%	0.075%
25	13.151	1705	1711	1722	rBV5	30454	67759	0.58%	0.059%
26	13.251	1722	1728	1735	rVB4	14988	28973	0.25%	0.025%
27	13.474	1758	1766	1771	rBV2	44875	76043	0.65%	0.066%
28	13.527	1771	1775	1780	rVV3	34181	53786	0.46%	0.047%
29	13.604	1784	1788	1793	rVV4	7890	14928	0.13%	0.013%
30	13.669	1795	1799	1804	rVB5	7797	12951	0.11%	0.011%
31	14.039	1855	1862	1876	rBV	4845042	6399073	54.83%	5.586%
32	14.322	1898	1910	1926	rBV	5502593	7681180	65.82%	6.706%
33	14.627	1955	1962	1974	rBV	3152857	4644321	39.80%	4.055%
34	14.816	1987	1994	2007	rBV	371095	629619	5.39%	0.550%
35	15.033	2027	2031	2042	rVB10	24947	50204	0.43%	0.044%
36	15.421	2092	2097	2099	rBV4	8579	13273	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
 Data File : BM036760.D
 Acq On : 27 Sep 2022 00:15
 Operator : CG/JU
 Sample : N4748-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ESQS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

37	15.616	2123	2130	2142	rBV	7220568	10006906	85.75%	8.736%
38	15.727	2142	2149	2165	rVV	1716268	2387934	20.46%	2.085%
39	15.851	2165	2170	2177	rVB2	58056	95905	0.82%	0.084%
40	16.080	2206	2209	2218	rVB9	7836	14642	0.13%	0.013%
41	16.186	2221	2227	2230	rVB8	5975	12112	0.10%	0.011%
42	16.233	2230	2235	2241	rBV6	11052	17737	0.15%	0.015%
43	16.304	2241	2247	2248	rBV6	9305	12887	0.11%	0.011%
44	16.398	2257	2263	2268	rVB5	19399	26224	0.22%	0.023%
45	16.845	2334	2339	2347	rBV	11315	19034	0.16%	0.017%
46	17.045	2369	2373	2376	rVB6	10961	14370	0.12%	0.013%
47	17.362	2420	2427	2437	rBV	3812191	5048680	43.26%	4.408%
48	17.462	2437	2444	2456	rBV	7943934	10877299	93.20%	9.496%
49	17.915	2518	2521	2526	rVB2	11327	16088	0.14%	0.014%
50	18.027	2538	2540	2546	rVB6	12402	15251	0.13%	0.013%
51	18.251	2574	2578	2587	rBV3	54324	90378	0.77%	0.079%
52	18.857	2678	2681	2684	rBV4	14219	19268	0.17%	0.017%
53	19.309	2754	2758	2763	rBV2	86024	127007	1.09%	0.111%
54	19.380	2766	2770	2774	rVV	86094	112286	0.96%	0.098%
55	19.527	2792	2795	2799	rBV5	32513	47167	0.40%	0.041%
56	19.745	2826	2832	2848	rBV	9191484	11670504	100.00%	10.188%
57	20.739	2998	3001	3005	rVB	122962	136452	1.17%	0.119%
58	21.527	3130	3135	3143	rBV	3349300	4315987	36.98%	3.768%
59	23.803	3515	3522	3529	rBV2	4223113	8110251	69.49%	7.080%
60	23.962	3543	3549	3560	rVB2	1793808	3609304	30.93%	3.151%




Sum of corrected areas: 114546962

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036760.D
Acq On : 27 Sep 2022 00:15
Operator : CG/JU
Sample : N4748-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ESQS3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

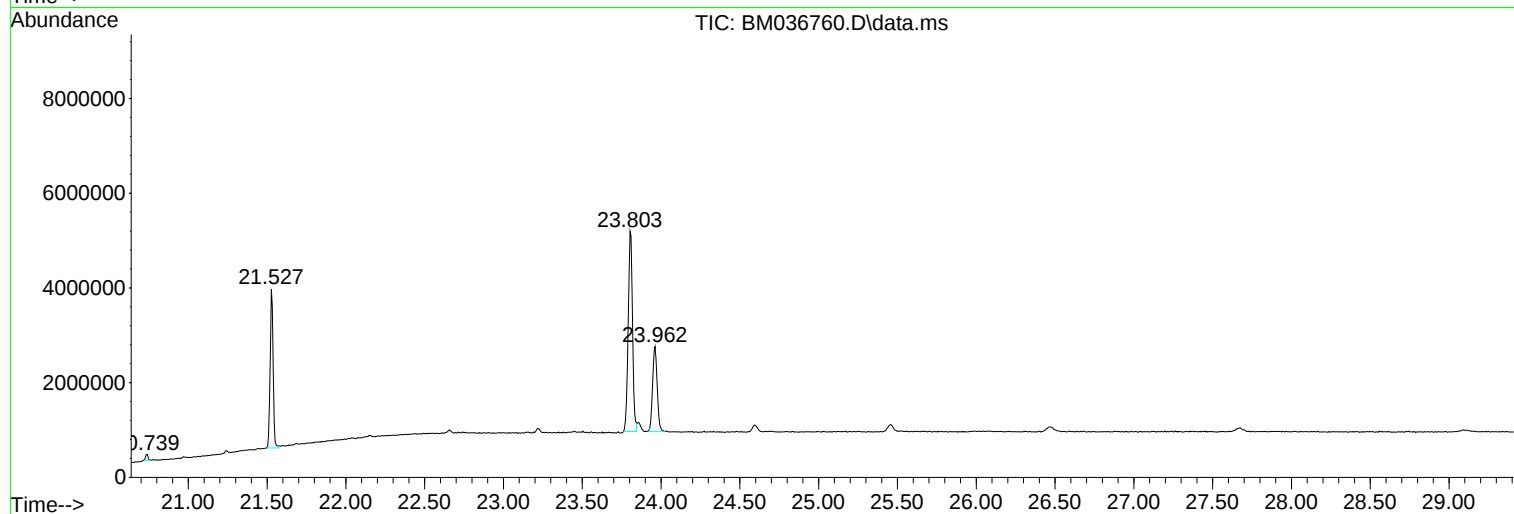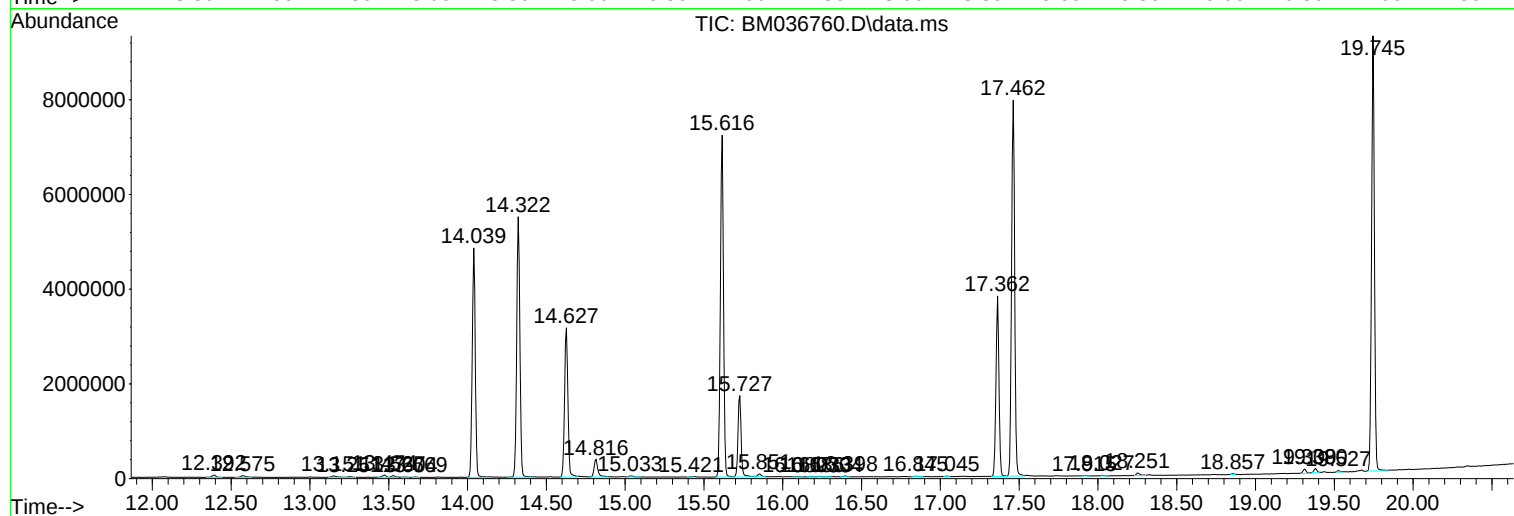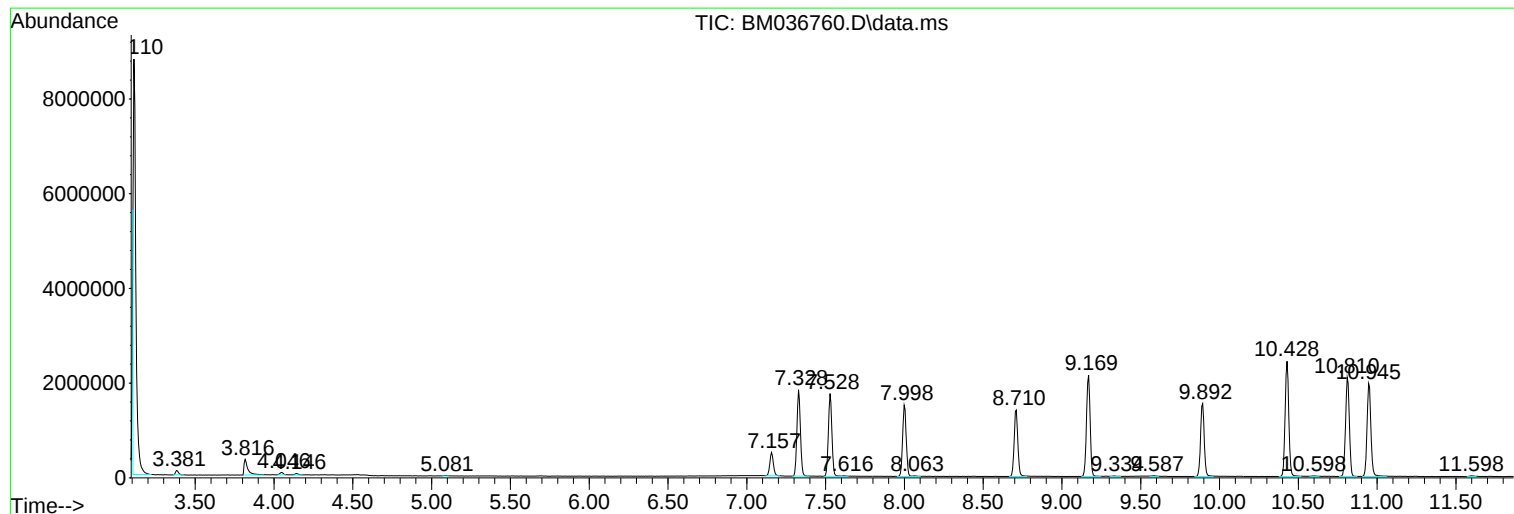

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036760.D
Acq On : 27 Sep 2022 00:15
Operator : CG/JU
Sample : N4748-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ESQS3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.110	78.11 ng/ul	9222770	1,4-Dichlorobenzene-d4	7.998

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40		
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17		
5	N-Ethylformamide	73	C3H7NO	000627-45-2	9		

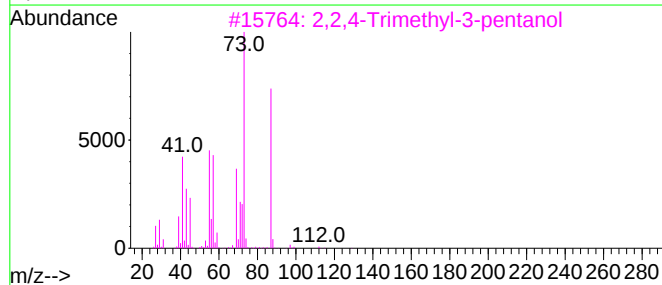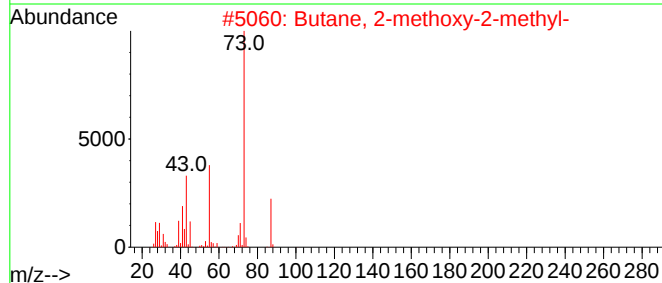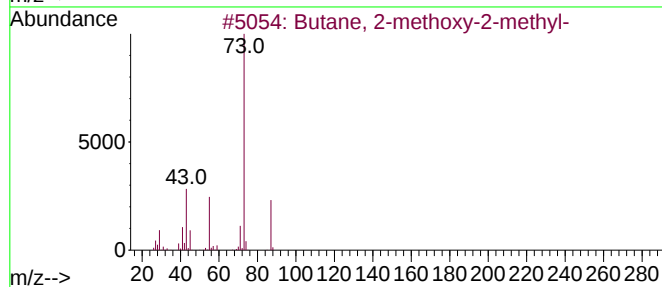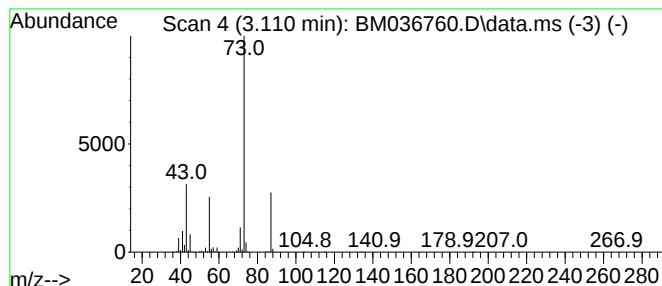

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036760.D
Acq On : 27 Sep 2022 00:15
Operator : CG/JU
Sample : N4748-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ESQS3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.110	78.1	ng/ul	9222770	1	7.998	2361610	20.0