

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
 Data File : BM036768.D
 Acq On : 27 Sep 2022 05:40
 Operator : CG/JU
 Sample : PB147898BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK898

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036768.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	46	50	57	rBV	125979	162522	1.71%	0.154%
2	3.810	120	123	142	rBV	1436122	2234077	23.50%	2.115%
3	4.140	175	179	188	rVB2	31711	52137	0.55%	0.049%
4	7.157	684	692	705	rBV	2003550	3122221	32.85%	2.956%
5	7.328	713	721	731	rVB	1723566	2624003	27.61%	2.484%
6	7.528	748	755	768	rBV	2058109	3175200	33.40%	3.006%
7	7.998	828	835	846	rBV	1584004	2452029	25.80%	2.322%
8	8.704	947	955	973	rBV	2522243	4040557	42.51%	3.826%
9	9.163	1025	1033	1047	rBV	1937754	3161034	33.26%	2.993%
10	9.275	1047	1052	1057	rVV9	8326	20607	0.22%	0.020%
11	9.886	1149	1156	1175	rBV	1491908	2425771	25.52%	2.297%
12	10.422	1239	1247	1260	rBV	2321744	3946185	41.52%	3.736%
13	10.810	1305	1313	1320	rBV	2173050	3685000	38.77%	3.489%
14	10.945	1328	1336	1349	rBV	2302115	3948890	41.54%	3.739%
15	12.063	1521	1526	1534	rVB9	9000	19767	0.21%	0.019%
16	12.386	1575	1581	1587	rBV	43700	75065	0.79%	0.071%
17	12.598	1613	1617	1625	rVB9	5347	11006	0.12%	0.010%
18	13.522	1769	1774	1780	rVB5	11908	18398	0.19%	0.017%
19	13.598	1782	1787	1790	rVB6	8026	12248	0.13%	0.012%
20	14.039	1855	1862	1874	rBV	4164500	5740954	60.40%	5.435%
21	14.322	1902	1910	1922	rBV	4794426	7037161	74.03%	6.663%
22	14.622	1954	1961	1971	rBV	3571940	4947520	52.05%	4.684%
23	14.816	1987	1994	2011	rBV	1692557	2603551	27.39%	2.465%
24	15.610	2122	2129	2142	rBV	6247664	8813063	92.72%	8.344%
25	15.721	2142	2148	2165	rVV	1370919	1913479	20.13%	1.812%
26	15.851	2165	2170	2176	rVB	51416	79701	0.84%	0.075%
27	16.174	2221	2225	2229	rBV6	5827	9853	0.10%	0.009%
28	16.392	2257	2262	2266	rBV3	16607	24711	0.26%	0.023%
29	16.845	2332	2339	2345	rBV6	9957	23325	0.25%	0.022%
30	17.039	2368	2372	2377	rVB8	10789	18352	0.19%	0.017%
31	17.145	2386	2390	2395	rBV6	9552	15835	0.17%	0.015%
32	17.363	2420	2427	2437	rBV	3942695	5429470	57.12%	5.141%
33	17.462	2437	2444	2459	rVV	6518257	9081693	95.54%	8.598%
34	17.915	2518	2521	2524	rVB3	15325	16663	0.18%	0.016%
35	19.309	2754	2758	2763	rBV3	68975	89776	0.94%	0.085%
36	19.380	2766	2770	2774	rBV	60774	87030	0.92%	0.082%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036768.D
Acq On : 27 Sep 2022 05:40
Operator : CG/JU
Sample : PB147898BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK898

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Title : SVOA CALIBRATION

37	19.745	2826	2832	2840	rBV	7207432	9505211	100.00%	8.999%
38	20.733	2997	3000	3004	rBV	112859	133061	1.40%	0.126%
39	21.527	3130	3135	3144	rBV	3647454	4613415	48.54%	4.368%
40	23.797	3515	3521	3529	rBV2	3268100	6363024	66.94%	6.024%
41	23.956	3542	3548	3558	rVB2	1987200	3887855	40.90%	3.681%




Sum of corrected areas: 105621420

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036768.D
Acq On : 27 Sep 2022 05:40
Operator : CG/JU
Sample : PB147898BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK898

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

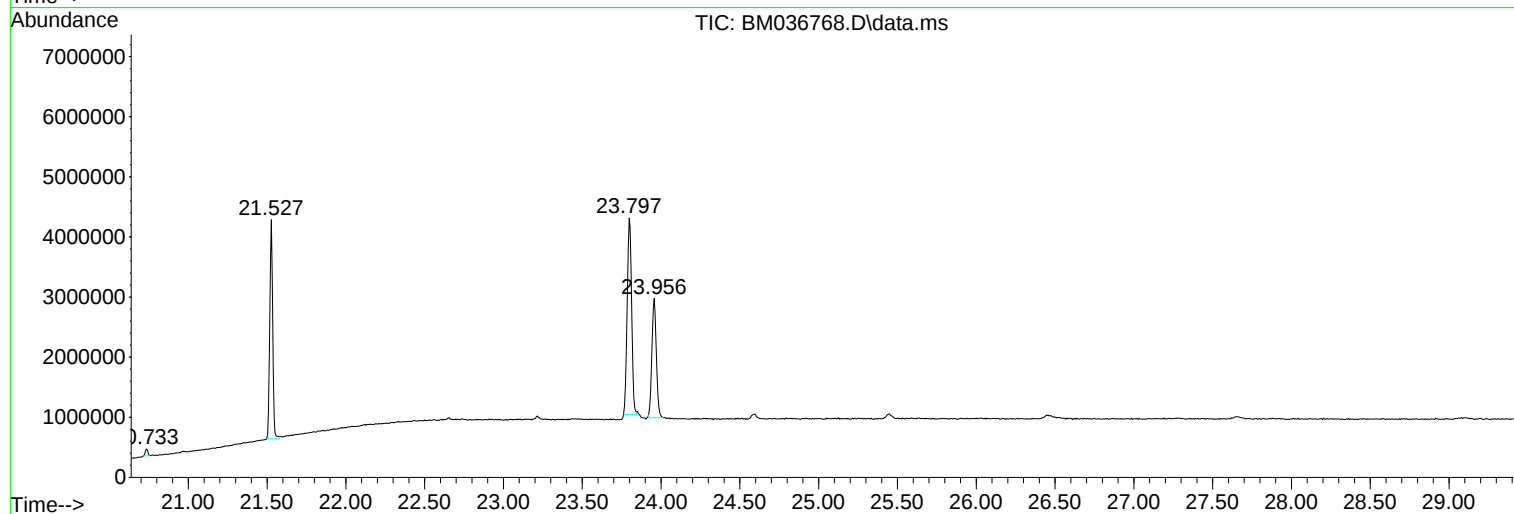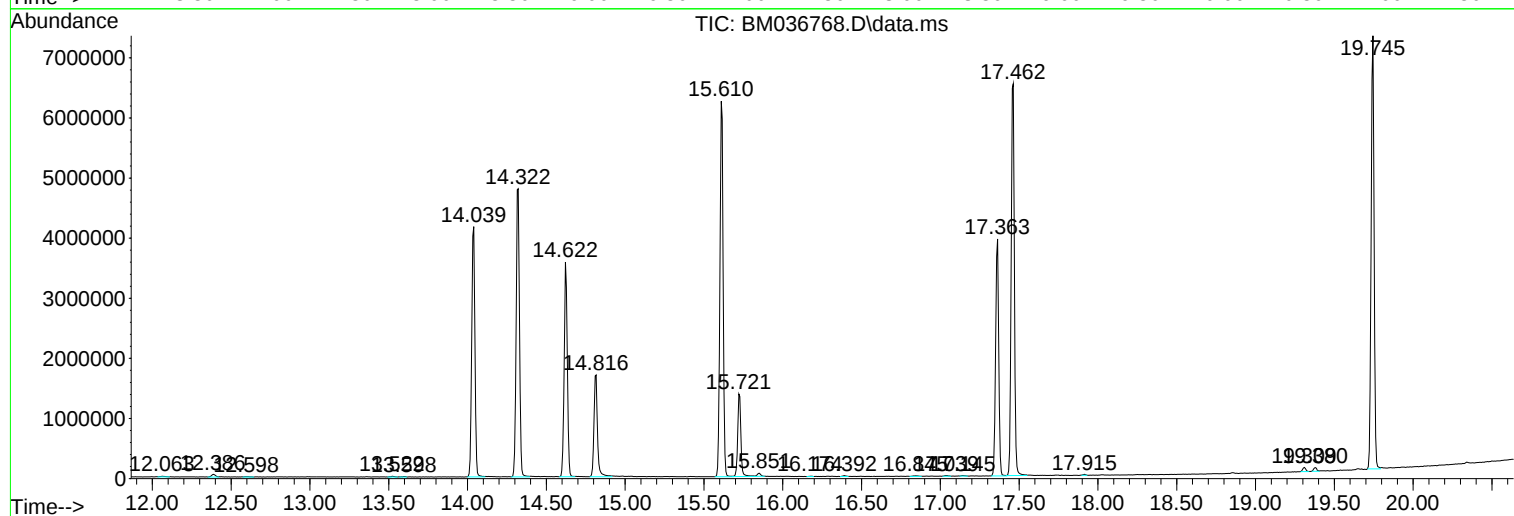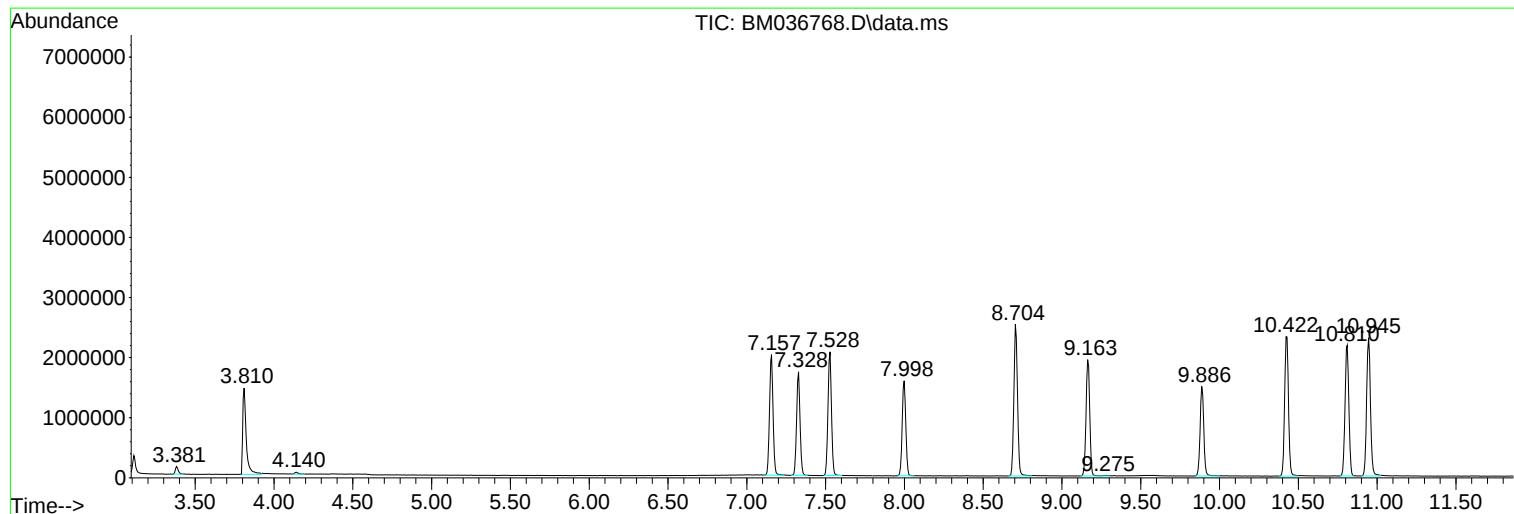

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036768.D
Acq On : 27 Sep 2022 05:40
Operator : CG/JU
Sample : PB147898BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK898

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036768.D
Acq On : 27 Sep 2022 05:40
Operator : CG/JU
Sample : PB147898BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK898

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc