

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
 Data File : BM036773.D
 Acq On : 27 Sep 2022 09:29
 Operator : CG/JU
 Sample : PB147764BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK764

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036773.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	46	50	59	rVB	111226	143429	2.06%	0.180%
2	3.811	120	123	139	rBV	1052869	1670785	24.01%	2.096%
3	4.140	176	179	185	rVB	24276	28953	0.42%	0.036%
4	6.828	630	636	637	rBV5	5265	8608	0.12%	0.011%
5	7.151	684	691	703	rVB	1699283	2612060	37.54%	3.277%
6	7.322	714	720	730	rBV	1436379	2194619	31.54%	2.753%
7	7.522	747	754	767	rVB	1715263	2659872	38.23%	3.337%
8	7.993	827	834	844	rVB	1261298	1986849	28.56%	2.493%
9	8.704	947	955	966	rBV	2078347	3358003	48.26%	4.213%
10	9.163	1023	1033	1045	rBV	1576648	2614781	37.58%	3.281%
11	9.887	1148	1156	1168	rBV	1204308	1962952	28.21%	2.463%
12	10.422	1236	1247	1257	rBV	2029255	3282772	47.18%	4.119%
13	10.804	1305	1312	1322	rBV	1793152	2942654	42.29%	3.692%
14	10.939	1329	1335	1352	rBV	695226	1243328	17.87%	1.560%
15	12.069	1521	1527	1532	rVB6	9055	20679	0.30%	0.026%
16	12.386	1574	1581	1586	rBV2	36581	60297	0.87%	0.076%
17	12.598	1613	1617	1621	rVB7	5357	9898	0.14%	0.012%
18	13.522	1771	1774	1779	rBV7	5988	9051	0.13%	0.011%
19	13.598	1782	1787	1790	rBV4	7163	11210	0.16%	0.014%
20	14.033	1852	1861	1873	rBV	3477353	4623963	66.46%	5.801%
21	14.316	1901	1909	1920	rBV	3961711	5569892	80.05%	6.988%
22	14.622	1954	1961	1973	rBV	2675481	3783543	54.38%	4.747%
23	14.810	1986	1993	2010	rBV	1246367	1889976	27.16%	2.371%
24	15.610	2121	2129	2141	rBV	4933029	6957676	100.00%	8.729%
25	15.722	2142	2148	2162	rVV	997490	1361029	19.56%	1.708%
26	15.845	2164	2169	2177	rVB3	43375	72419	1.04%	0.091%
27	16.392	2259	2262	2267	rVB6	10818	14833	0.21%	0.019%
28	16.839	2335	2338	2343	rBV4	12417	14735	0.21%	0.018%
29	17.033	2366	2371	2377	rBV9	7612	15362	0.22%	0.019%
30	17.139	2387	2389	2393	rBV5	7016	9411	0.14%	0.012%
31	17.357	2420	2426	2437	rBV	2855533	3948806	56.75%	4.954%
32	17.457	2437	2443	2460	rVV	4929229	6864048	98.65%	8.612%
33	17.910	2517	2520	2525	rBV3	12001	20362	0.29%	0.026%
34	18.851	2678	2680	2683	rVB4	15219	13084	0.19%	0.016%
35	19.310	2754	2758	2762	rBV2	47173	66007	0.95%	0.083%
36	19.374	2766	2769	2774	rVB	46927	64225	0.92%	0.081%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036773.D
Acq On : 27 Sep 2022 09:29
Operator : CG/JU
Sample : PB147764BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK764

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Title : SVOA CALIBRATION

37	19.739	2826	2831	2843	rBV	5008565	6836654	98.26%	8.577%
38	20.733	2997	3000	3004	rBV	128352	146009	2.10%	0.183%
39	21.527	3130	3135	3141	rBV	2496283	3130689	45.00%	3.928%
40	23.797	3515	3521	3529	rBV	2450823	4866495	69.94%	6.106%
41	23.956	3543	3548	3559	rVB	1368411	2616108	37.60%	3.282%




Sum of corrected areas: 79706126

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036773.D
Acq On : 27 Sep 2022 09:29
Operator : CG/JU
Sample : PB147764BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK764

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

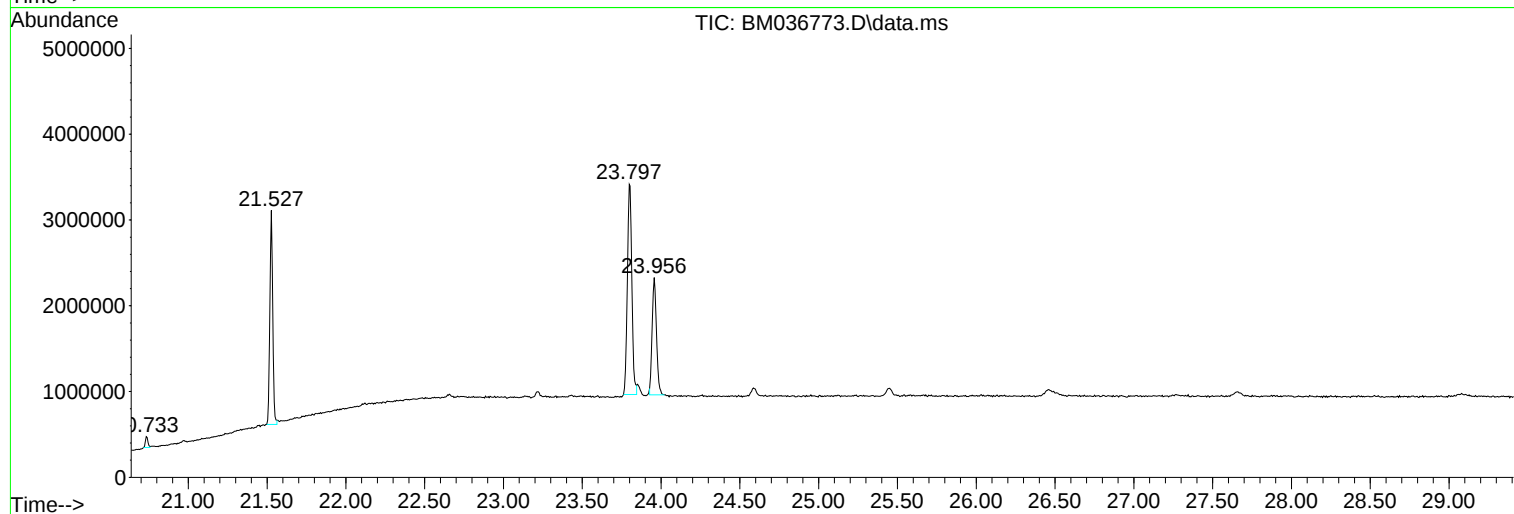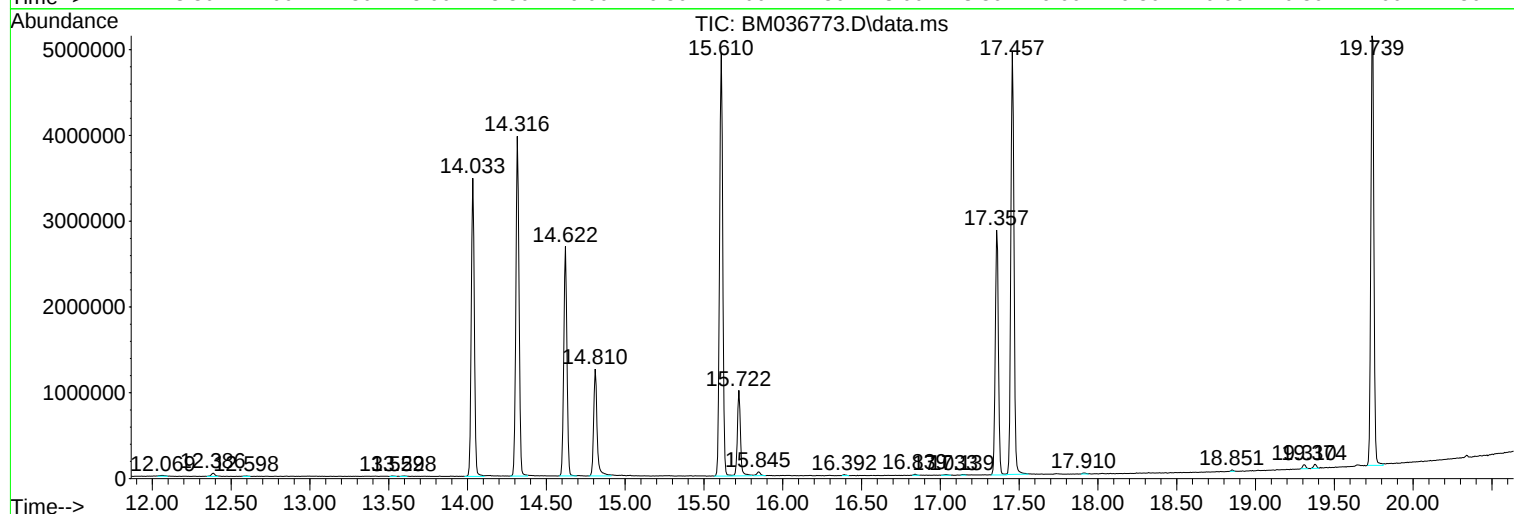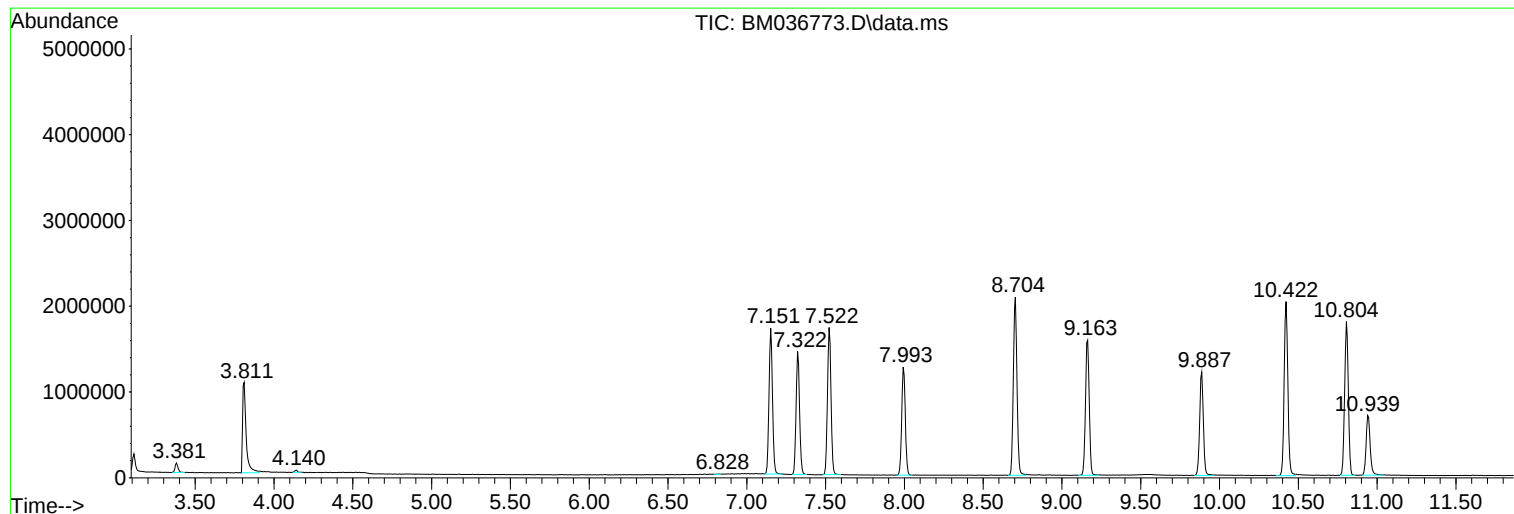

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036773.D
Acq On : 27 Sep 2022 09:29
Operator : CG/JU
Sample : PB147764BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK764

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036773.D
Acq On : 27 Sep 2022 09:29
Operator : CG/JU
Sample : PB147764BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK764

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc