

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
 Data File : BM036776.D
 Acq On : 27 Sep 2022 13:32
 Operator : CG/JU
 Sample : PB147827BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK827

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036776.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	17	19	22	rVB3	33871	32906	0.93%	0.180%
2	3.299	31	36	49	rVB	1709438	2084409	59.07%	11.408%
3	3.646	91	95	103	rVB	53591	77674	2.20%	0.425%
4	4.134	174	178	184	rVB	40259	58551	1.66%	0.320%
5	7.046	670	673	674	rBV3	4159	4205	0.12%	0.023%
6	7.369	725	728	731	rVB5	3942	6004	0.17%	0.033%
7	7.463	742	744	747	rBV4	3239	4340	0.12%	0.024%
8	7.498	749	750	755	rVB4	3201	3582	0.10%	0.020%
9	7.993	827	834	843	rBV	921685	1484361	42.07%	8.124%
10	8.069	845	847	851	rVB5	3453	4723	0.13%	0.026%
11	8.222	868	873	874	rBV5	3067	4745	0.13%	0.026%
12	8.245	874	877	880	rBV5	2409	3829	0.11%	0.021%
13	9.575	1101	1103	1108	rVB6	6512	7885	0.22%	0.043%
14	10.804	1303	1312	1323	rBV	1242846	2120878	60.11%	11.608%
15	10.892	1325	1327	1334	rVB8	3473	5386	0.15%	0.029%
16	12.033	1518	1521	1522	rVV3	4112	3960	0.11%	0.022%
17	12.063	1522	1526	1532	rVB4	7695	17700	0.50%	0.097%
18	12.192	1545	1548	1550	rBV4	2995	3967	0.11%	0.022%
19	13.104	1700	1703	1706	rVB5	3317	3630	0.10%	0.020%
20	13.263	1728	1730	1732	rBV3	3680	3908	0.11%	0.021%
21	13.886	1833	1836	1839	rBV5	2412	3717	0.11%	0.020%
22	14.045	1858	1863	1867	rBV2	10301	18639	0.53%	0.102%
23	14.622	1955	1961	1973	rBV	1928518	2786783	78.98%	15.252%
24	15.086	2037	2040	2043	rVB5	2978	3944	0.11%	0.022%
25	15.321	2077	2080	2083	rBV4	2668	4101	0.12%	0.022%
26	15.598	2123	2127	2129	rVV4	9606	13166	0.37%	0.072%
27	15.621	2129	2131	2134	rVB4	4156	4283	0.12%	0.023%
28	15.839	2164	2168	2172	rBV7	2504	5260	0.15%	0.029%
29	16.027	2196	2200	2201	rVB3	3036	3541	0.10%	0.019%
30	16.127	2215	2217	2222	rBV5	2886	4057	0.11%	0.022%
31	16.357	2253	2256	2259	rBV5	4579	4153	0.12%	0.023%
32	16.845	2334	2339	2345	rBV3	11069	17853	0.51%	0.098%
33	16.998	2361	2365	2366	rVB3	5168	4205	0.12%	0.023%
34	17.151	2385	2391	2394	rBV6	6994	11622	0.33%	0.064%
35	17.363	2420	2427	2442	rBV	2371216	3528468	100.00%	19.312%
36	17.915	2518	2521	2524	rVB3	10358	11872	0.34%	0.065%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036776.D
Acq On : 27 Sep 2022 13:32
Operator : CG/JU
Sample : PB147827BL
Misc : GCMS CONFIRMATION
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK827

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Title : SVOA CALIBRATION

37	20.733	2997	3000	3006	rBV2	109714	146922	4.16%	0.804%
38	21.527	3130	3135	3142	rBV	2575467	3268238	92.62%	17.887%
39	23.956	3543	3548	3557	rVB2	1276788	2493650	70.67%	13.648%




Sum of corrected areas: 18271117

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036776.D
Acq On : 27 Sep 2022 13:32
Operator : CG/JU
Sample : PB147827BL
Misc : GCMS CONFIRMATION
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK827

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

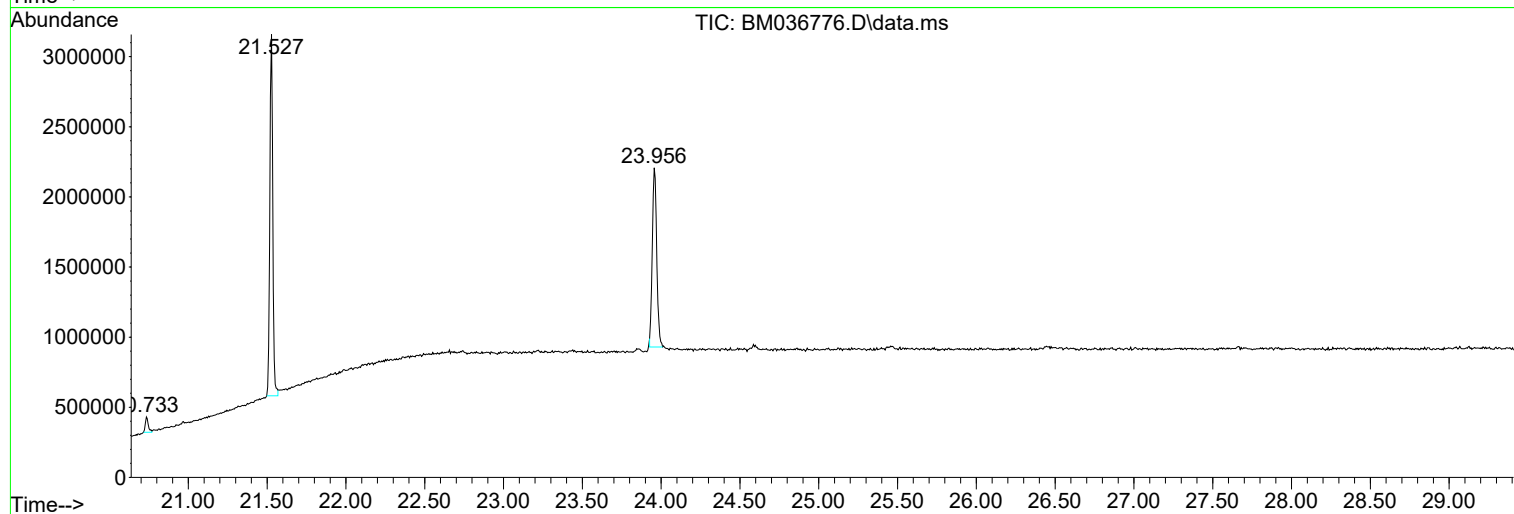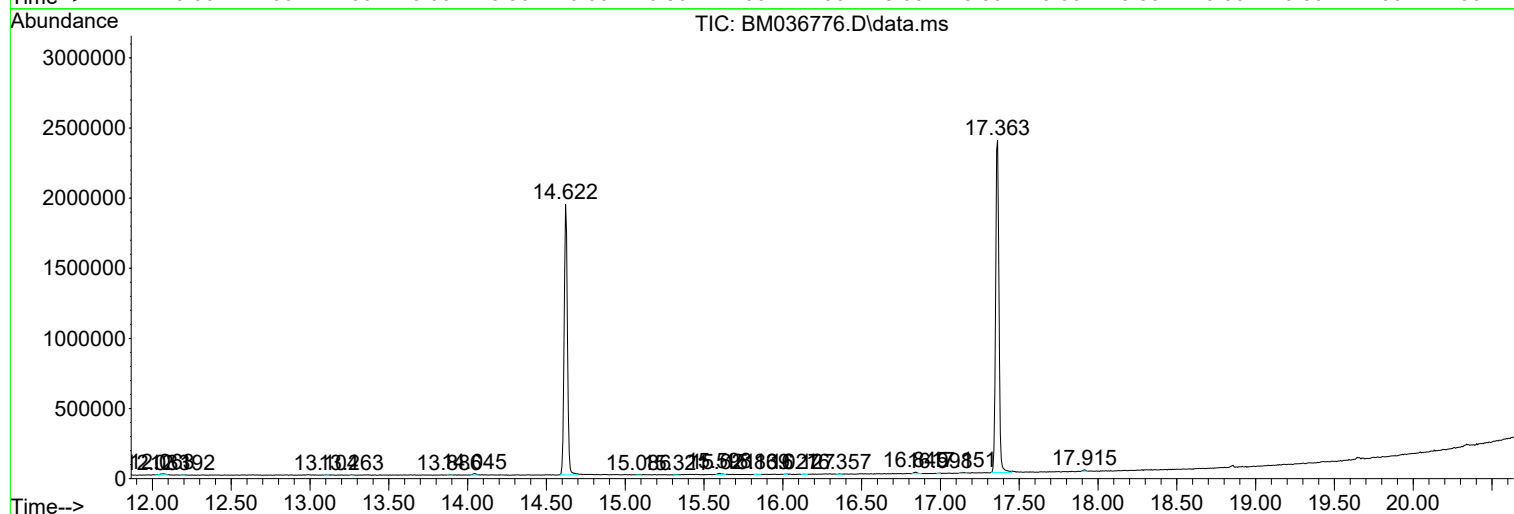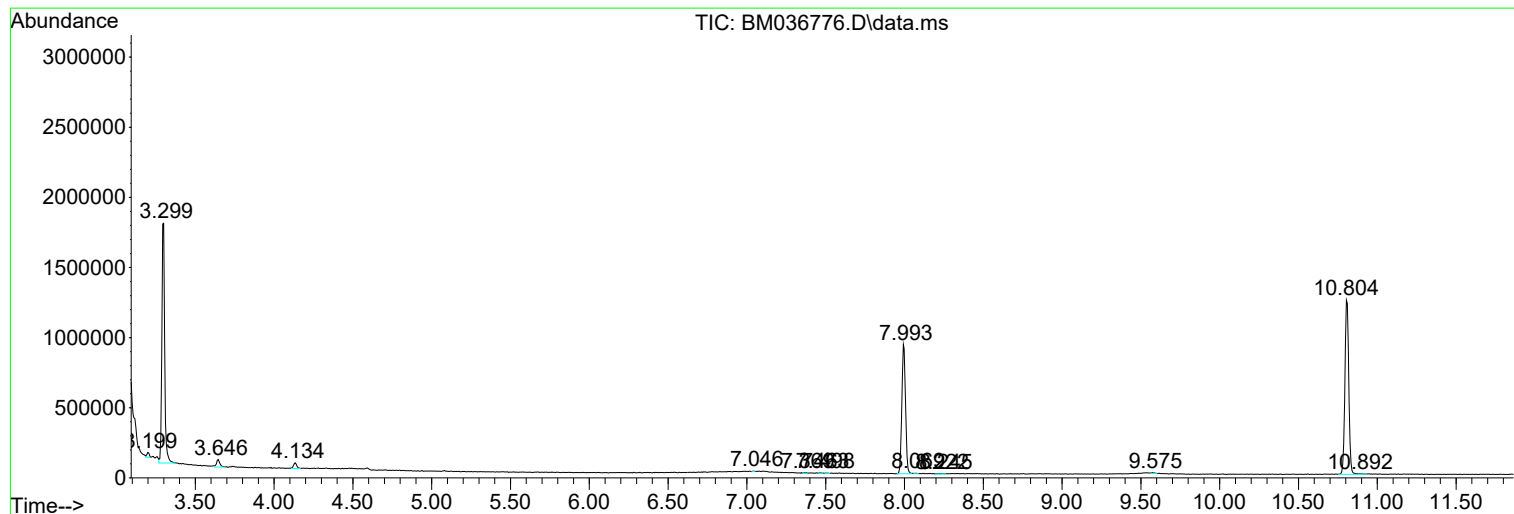

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036776.D
Acq On : 27 Sep 2022 13:32
Operator : CG/JU
Sample : PB147827BL
Misc : GCMS CONFIRMATION
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK827










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.299	28.08 ng/ul	2084410	1,4-Dichlorobenzene-d4	7.993

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Heptane			100	C7H16	000142-82-5	91
2	Heptane			100	C7H16	000142-82-5	90
3	Heptane			100	C7H16	000142-82-5	87
4	Heptane			100	C7H16	000142-82-5	86
5	Pentane, 2-methyl-			86	C6H14	000107-83-5	50

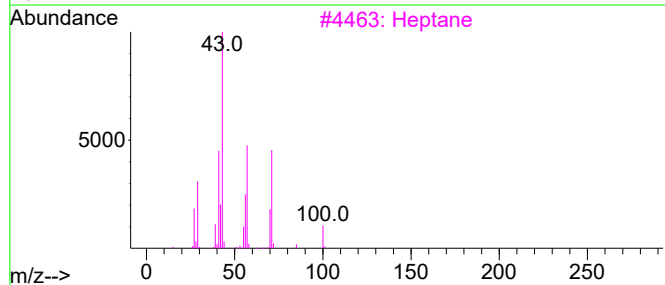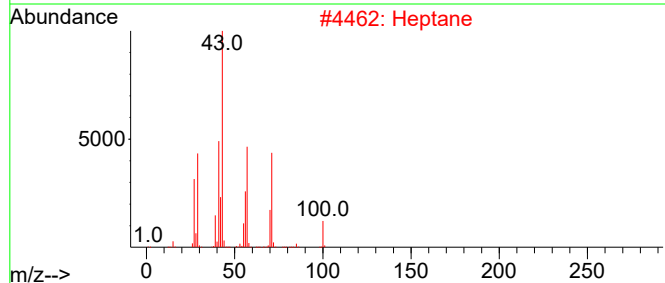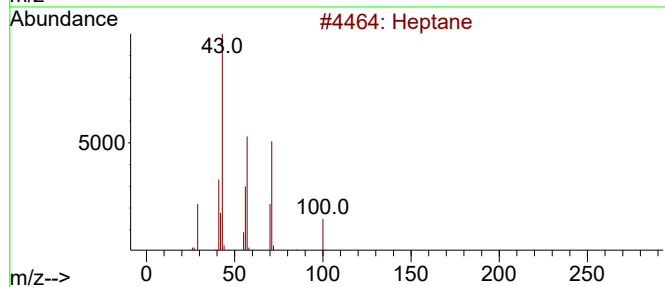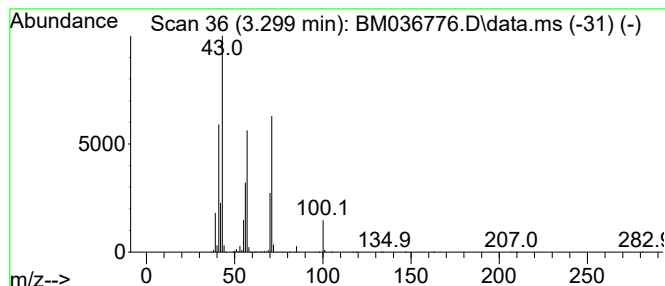

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036776.D
Acq On : 27 Sep 2022 13:32
Operator : CG/JU
Sample : PB147827BL
Misc : GCMS CONFIRMATION
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK827

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.299	28.1	ng/ul	2084410	1	7.993	1484360	20.0