

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
 Data File : BM036778.D
 Acq On : 27 Sep 2022 14:47
 Operator : CG/JU
 Sample : N4793-10
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036778.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.140	176	179	183	rVB	21386	24984	0.61%	0.130%
2	5.428	396	398	401	rBV4	4197	5929	0.14%	0.031%
3	7.622	766	771	775	rVB7	2876	4381	0.11%	0.023%
4	7.998	828	835	845	rBV	1325193	2057060	49.86%	10.700%
5	8.328	887	891	893	rBV5	3031	4748	0.12%	0.025%
6	9.386	1065	1071	1072	rBV6	3646	4334	0.11%	0.023%
7	9.498	1084	1090	1092	rBV7	4949	9153	0.22%	0.048%
8	10.675	1284	1290	1293	rBV7	3508	7189	0.17%	0.037%
9	10.810	1304	1313	1323	rBV	1823185	3014256	73.06%	15.679%
10	10.951	1332	1337	1339	rVB5	3928	4484	0.11%	0.023%
11	12.074	1518	1528	1530	rBV5	8011	17931	0.43%	0.093%
12	12.592	1614	1616	1621	rVB6	3149	4762	0.12%	0.025%
13	13.363	1743	1747	1750	rBV5	4365	4361	0.11%	0.023%
14	13.898	1831	1838	1840	rBV5	2775	6104	0.15%	0.032%
15	14.045	1858	1863	1868	rBV5	9170	14909	0.36%	0.078%
16	14.521	1938	1944	1949	rBV9	3307	5887	0.14%	0.031%
17	14.621	1954	1961	1978	rVV	2592488	3843779	93.17%	19.993%
18	14.727	1978	1979	1982	rVV3	9042	8585	0.21%	0.045%
19	14.751	1982	1983	1986	rVV3	6895	6503	0.16%	0.034%
20	14.933	2012	2014	2017	rVB4	3775	4242	0.10%	0.022%
21	15.598	2121	2127	2136	rBV6	10622	21283	0.52%	0.111%
22	15.909	2175	2180	2184	rVB7	2494	5268	0.13%	0.027%
23	16.086	2206	2210	2212	rVB5	2973	4343	0.11%	0.023%
24	16.839	2336	2338	2343	rVV3	9570	15931	0.39%	0.083%
25	17.151	2388	2391	2396	rVB6	5501	7286	0.18%	0.038%
26	17.362	2420	2427	2442	rBV	2830390	4125488	100.00%	21.459%
27	17.915	2518	2521	2524	rVB	11436	11902	0.29%	0.062%
28	20.733	2997	3000	3005	rBV	126561	163909	3.97%	0.853%
29	21.527	3130	3135	3142	rBV	2507034	3195184	77.45%	16.620%
30	23.956	3543	3548	3560	rVB2	1320931	2621191	63.54%	13.634%




Sum of corrected areas: 19225366

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036778.D
Acq On : 27 Sep 2022 14:47
Operator : CG/JU
Sample : N4793-10
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

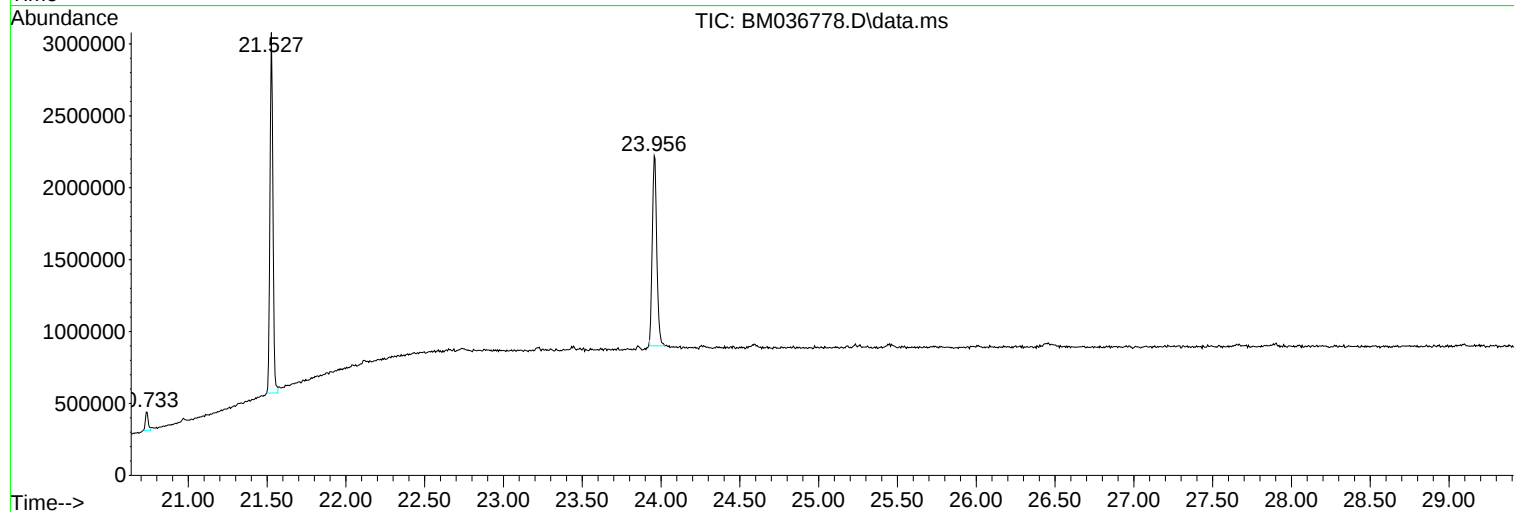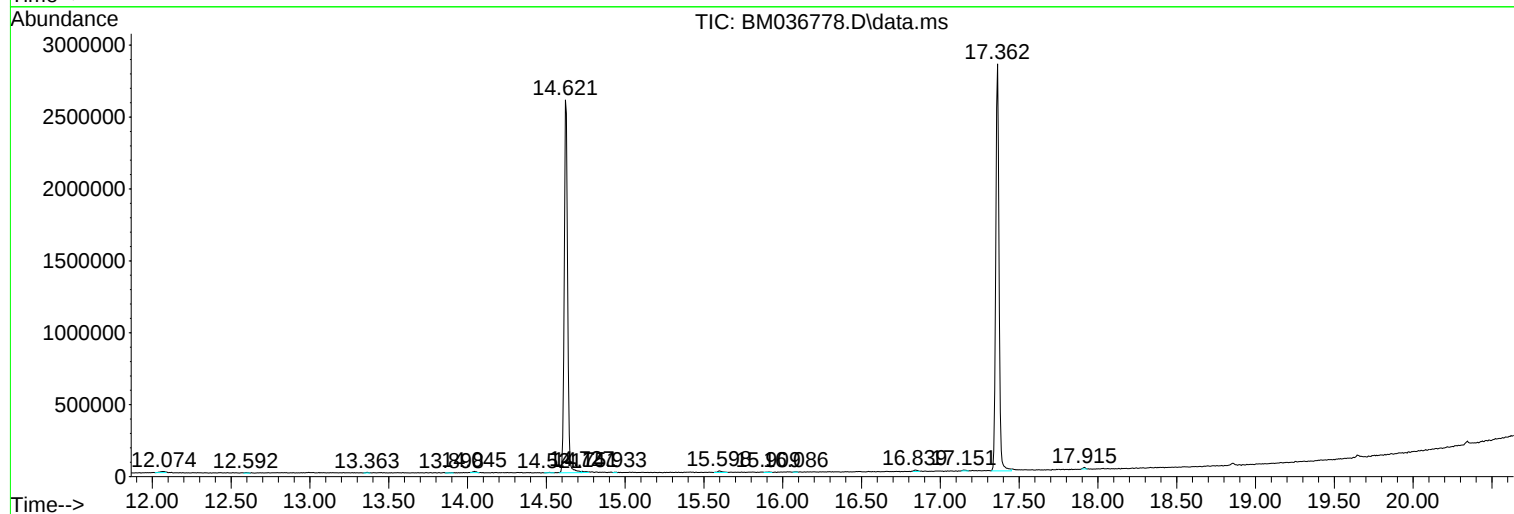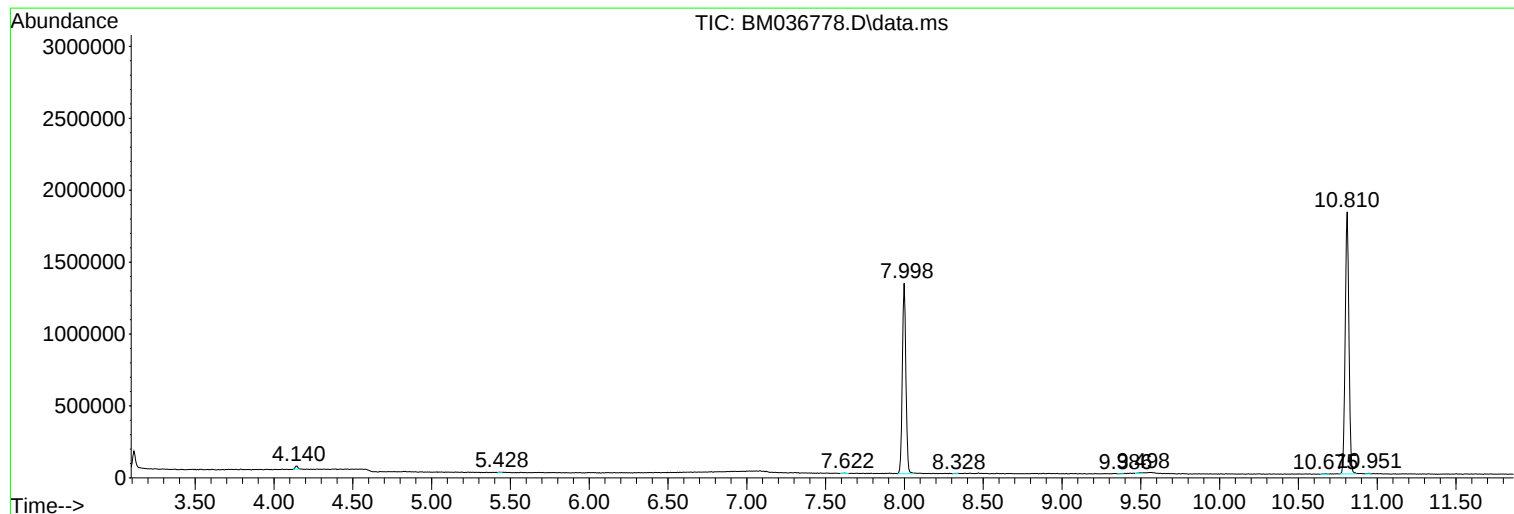

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036778.D
Acq On : 27 Sep 2022 14:47
Operator : CG/JU
Sample : N4793-10
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092622\
Data File : BM036778.D
Acq On : 27 Sep 2022 14:47
Operator : CG/JU
Sample : N4793-10
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc