

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092717\
 Data File : BM011734.D
 Acq On : 27 Sep 2017 21:44
 Operator : SJ/JU
 Sample : I5405-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB3F3

Manual Integrations
 APPROVED

Sohil
 9/29/2017 2:22:46 PM

Quant Time: Sep 28 04:29:30 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM092717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 04:06:20 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.94	152	174166	20.00	ng/ul	0.00
18) Naphthalene-d8	10.74	136	773176	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.57	164	440643	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.32	188	1005466	20.00	ng/ul	0.00
75) Chrysene-d12	21.48	240	1304213	20.00	ng/ul	0.00
83) Perylene-d12	23.84	264	1263193	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.36	96	1821	0.47	ng/uL	0.00
5) Phenol-d5	7.09	99	30581	1.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.26	67	96009m	7.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.47	132	31606	2.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.64	113	28392	2.12	ng/ul	0.00
19) Nitrobenzene-d5	9.10	128	43610	7.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.83	143	4663	0.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.36	165	18553m	1.51	ng/ul	0.00
29) 4-Chloroaniline-d4	10.92	131	235	0.02	ng/ul	0.05
43) Dimethylphthalate-d6	13.97	166	99347	2.63	ng/ul	0.00
46) Acenaphthylene-d8	14.26	160	345050	7.55	ng/ul	0.00
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.56	176	288173	8.85	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.69	200	266	0.04	ng/ul	0.00
70) Anthracene-d10	17.41	188	482988	9.44	ng/ul	0.00
76) Pyrene-d10	19.70	212	622019	9.99	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.69	264	561268	9.28	ng/ul	0.00
Target Compounds				Ovalue		
69) Phenanthrene	17.36	178	468057	8.317	ng/ul	98
71) Anthracene	17.44	178	79414	1.370	ng/ul	99
74) Fluoranthene	19.36	202	1018211	14.819	ng/ul#	88
77) Pyrene	19.73	202	973009	12.519	ng/ul#	87
80) Benzo(a)anthracene	21.46	228	558093	7.649	ng/ul	97
82) Chrysene	21.52	228	555403	8.071	ng/ul	98
85) Benzo(b)fluoranthene	23.13	252	678625	9.105	ng/ul#	96
86) Benzo(k)fluoranthene	23.17	252	260494m	3.426	ng/ul	
88) Benzo(a)pyrene	23.74	252	426615	5.926	ng/ul#	97
89) Indeno(1,2,3-cd)pyrene	26.26	276	249428	3.328	ng/ul#	91
91) Benzo(g,h,i)perylene	27.00	276	206615	3.321	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM092717\
Data File : BM011734.D
Acq On : 27 Sep 2017 21:44
Operator : SJ/JU
Sample : I5405-01
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
CB3F3

Manual Integrations
APPROVED

Sohil
9/29/2017 2:22:46 PM

Quant Time: Sep 28 04:29:30 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM092717.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 28 04:06:20 2017
Response via : Initial Calibration

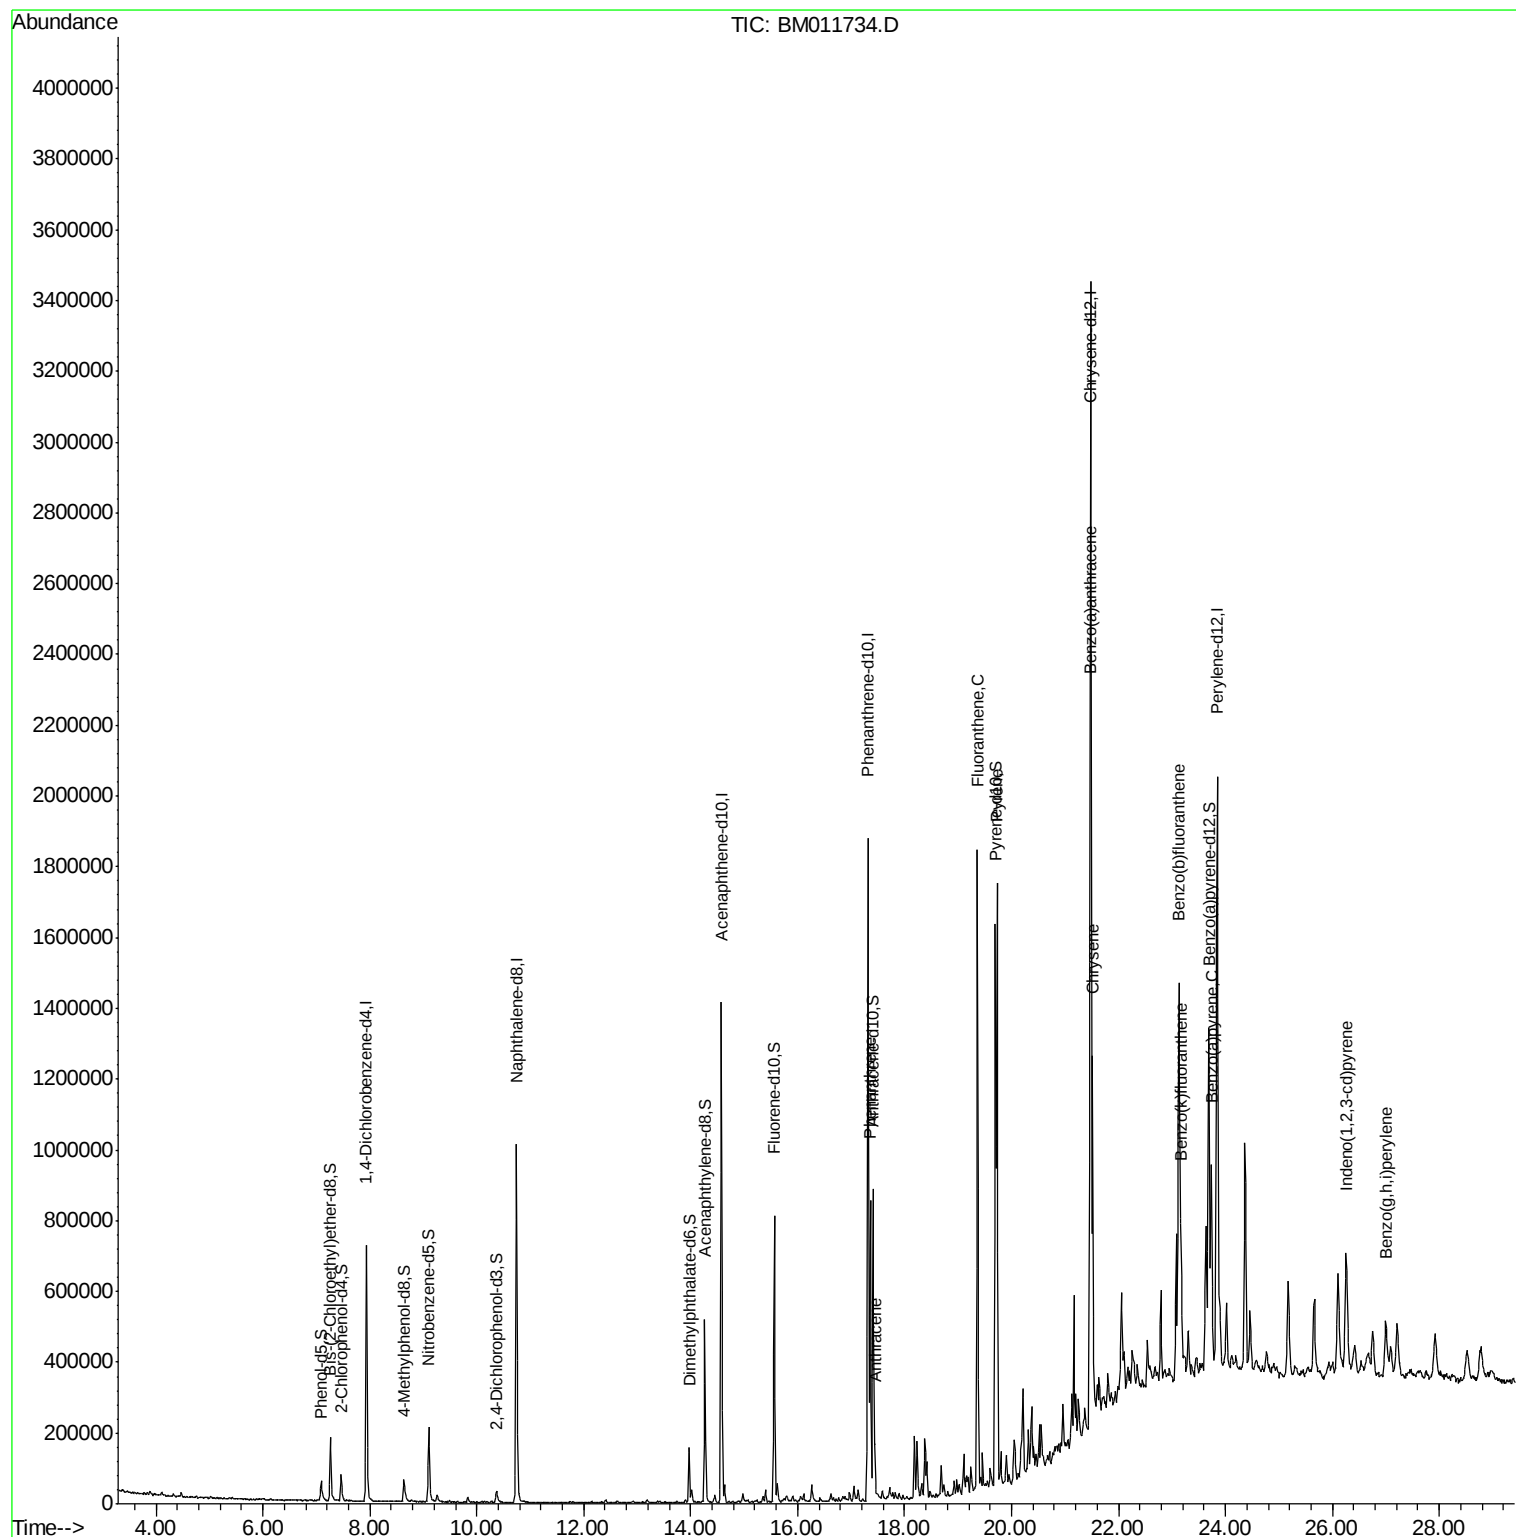

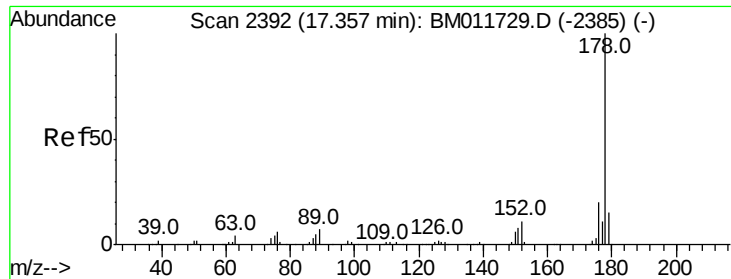

#69

Phenanthrene

Concen: 8.317 ng/ul

RT: 17.36 min Scan# 2392

Delta R.T. -0.00 min

Lab File: BM011734.D

Acq: 27 Sep 2017 21:44

Instrument :

BNA_M





ClientSampleId :

CB3F3

Tot Ion:	178	Resp:	468057
Ion Ratio	Lower	Upper	
178	100		
179	15.0	12.6	19.0
176	19.5	14.9	22.3

Manual Integrations
APPROVED

Sohil
9/29/2017 2:22:46 PM

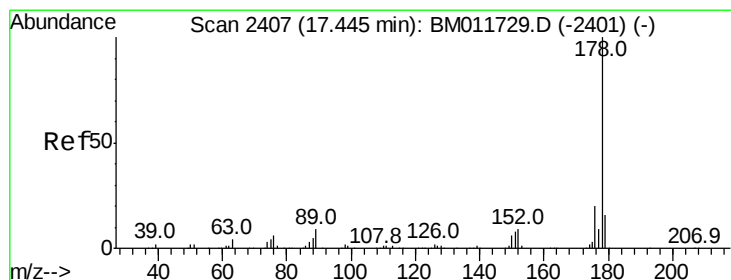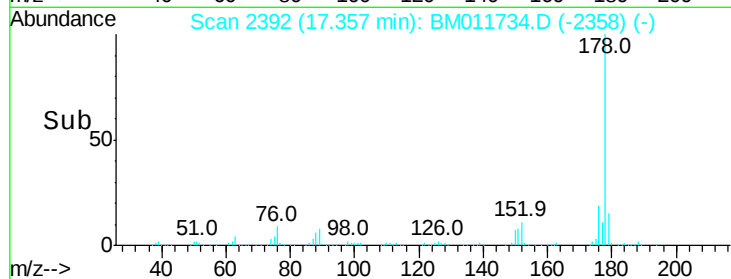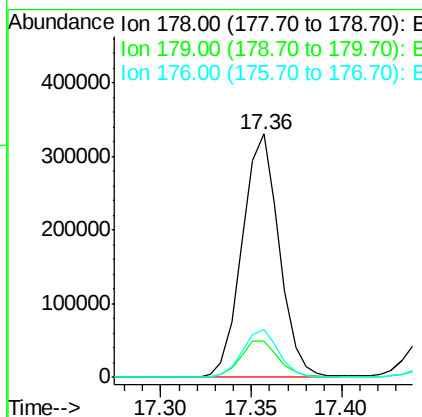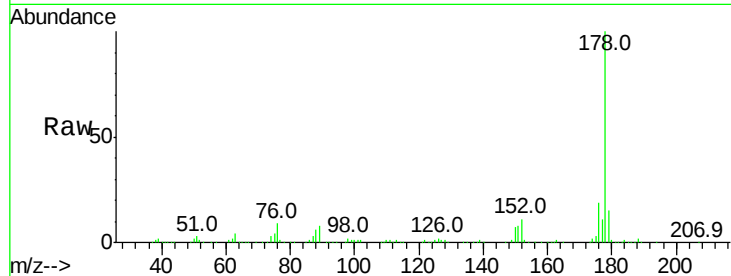

#71

Anthracene

Concen: 1.370 ng/ul




RT: 17.44 min Scan# 2407


Delta R.T. -0.00 min

Lab File: BM011734.D

Acq: 27 Sep 2017 21:44

Tgt Ion:	178	Resp:	79414
Ion Ratio	Lower	Upper	
178	100		
179	14.4	11.7	17.5
176	17.7	14.6	21.8

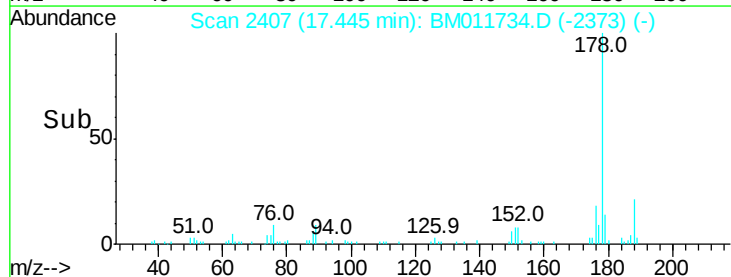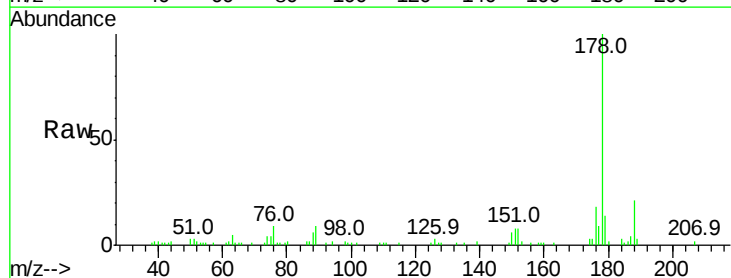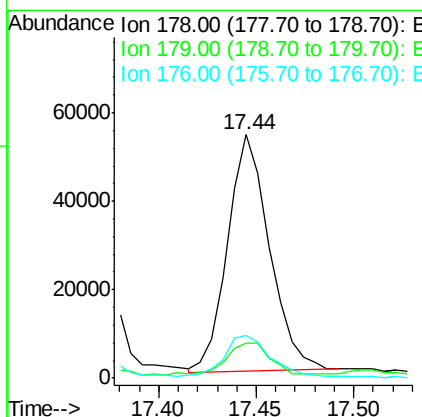

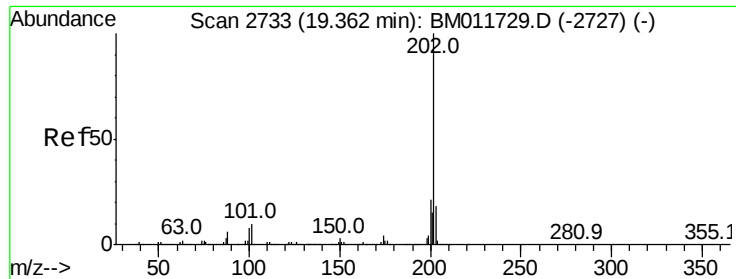





#74
 Fluoranthene
 Concen: 14.819 ng/ul
 RT: 19.36 min Scan# 2733
 Delta R.T. -0.00 min
 Lab File: BM011734.D
 Acq: 27 Sep 2017 21:44

Instrument :
 BNA_M
 ClientSampled :
 CB3F3

Tot Ion	Ratio	Resp	Lower	Upper
202	100	1018211		
101	9.9	4.6	7.0#	
100	8.1	3.4	5.2#	




Manual Integrations
 APPROVED


Sohil
 9/29/2017 2:22:46 PM

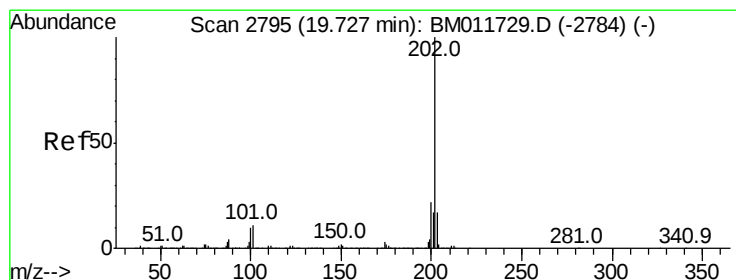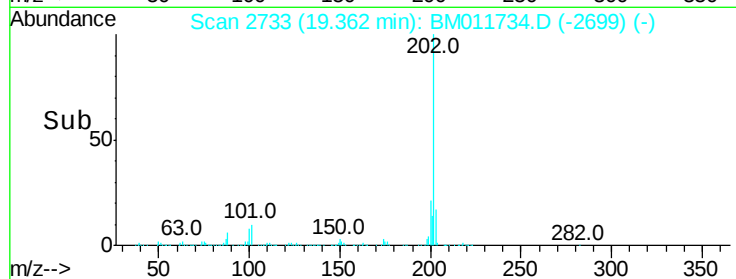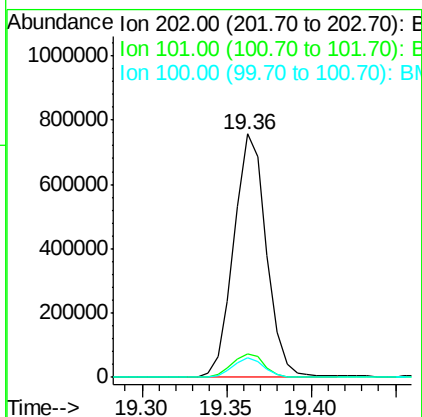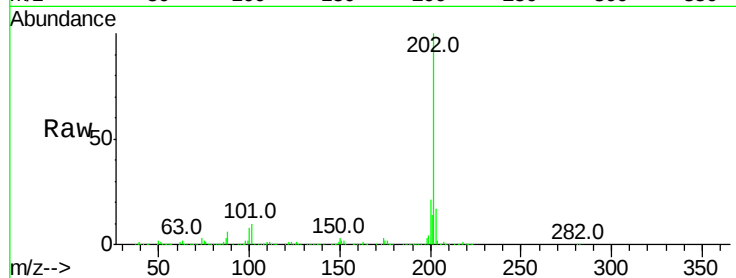

#77
 Pyrene
 Concen: 12.519 ng/ul
 RT: 19.73 min Scan# 2795
 Delta R.T. -0.00 min
 Lab File: BM011734.D
 Acq: 27 Sep 2017 21:44

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	973009		
101	11.4	5.1	7.7#	
100	9.6	4.9	7.3#	

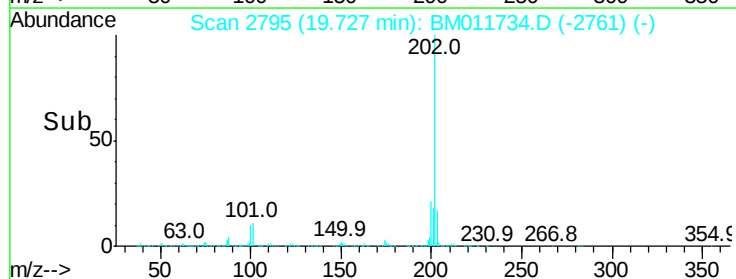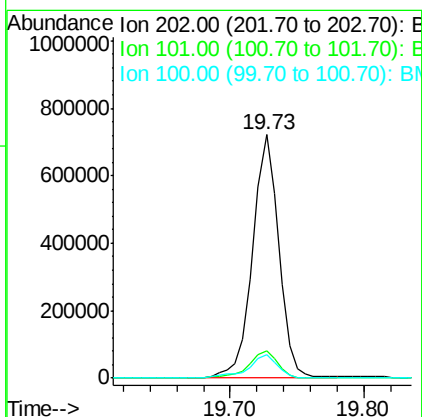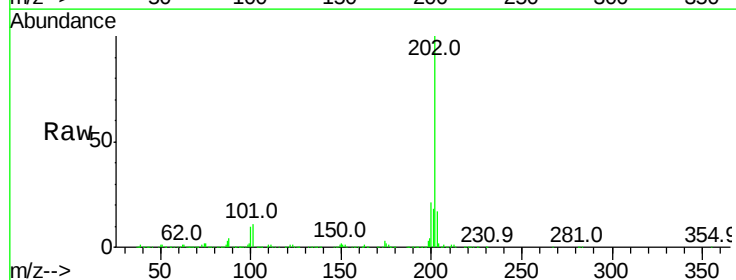

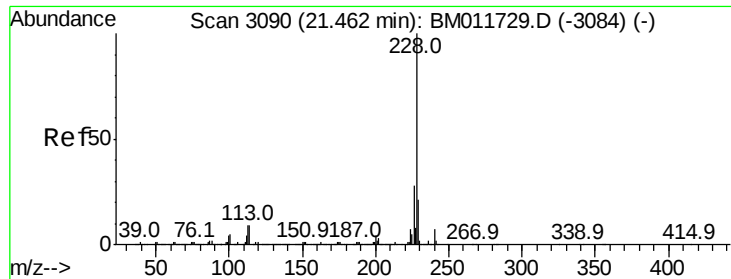





#80
Benzo(a)anthracene
Concen: 7.649 ng/ul
RT: 21.46 min Scan# 3090
Delta R.T. -0.00 min
Lab File: BM011734.D
Acq: 27 Sep 2017 21:44

Instrument :
BNA_M
ClientSampled :
CB3F3

Tot Ion	Ratio	Lower	Upper
228	100		
229	20.6	15.4	23.0
226	27.9	21.4	32.0




Manual Integrations
APPROVED


Sohil
9/29/2017 2:22:46 PM

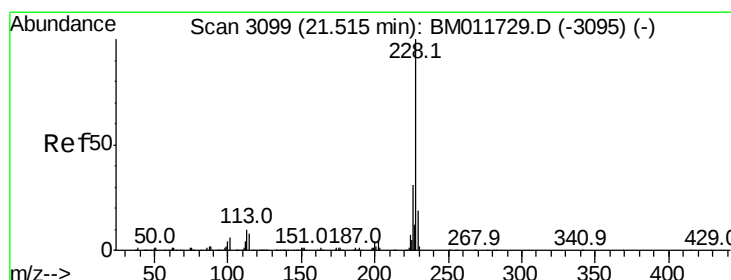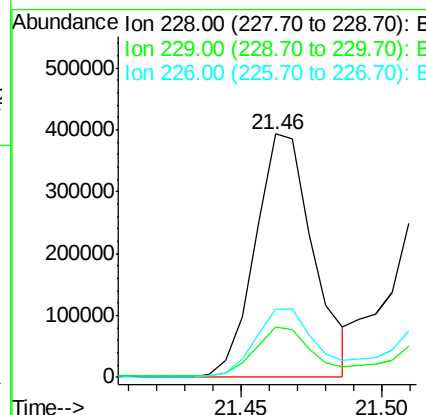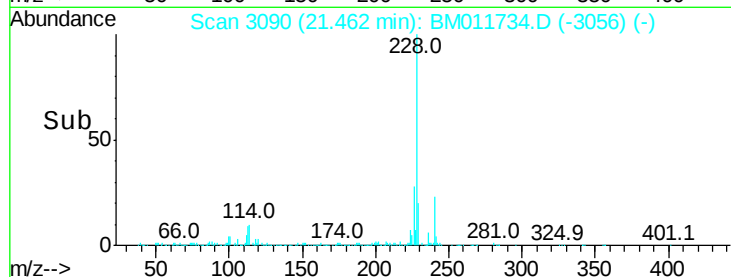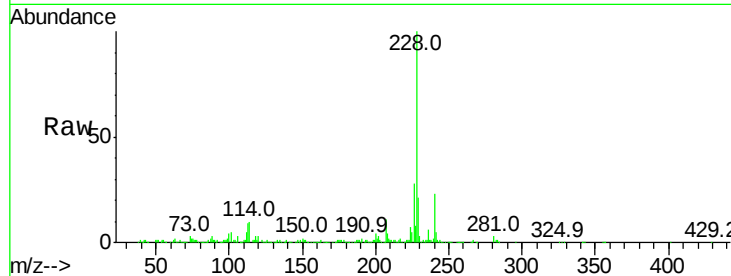

#82
Chrysene
Concen: 8.071 ng/ul
RT: 21.52 min Scan# 3099
Delta R.T. -0.00 min
Lab File: BM011734.D
Acq: 27 Sep 2017 21:44

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.8	23.4	35.2
229	19.5	15.5	23.3

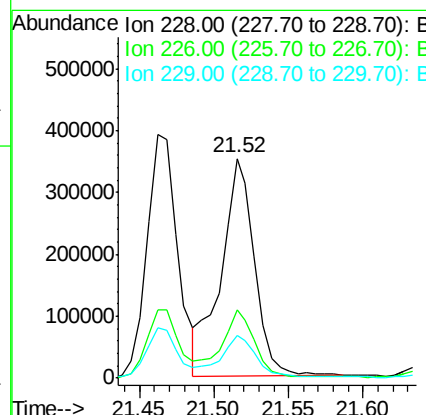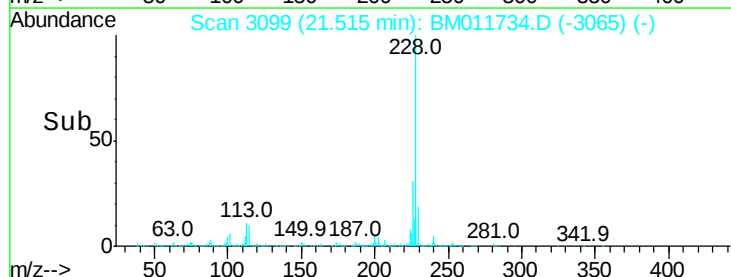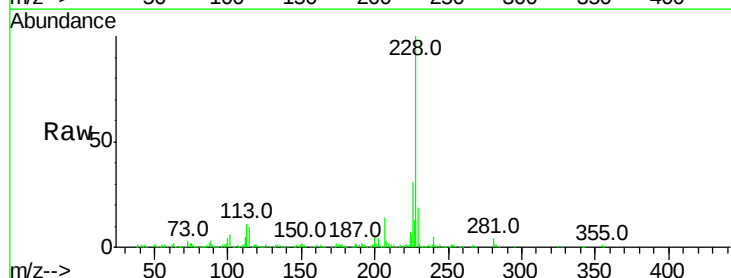

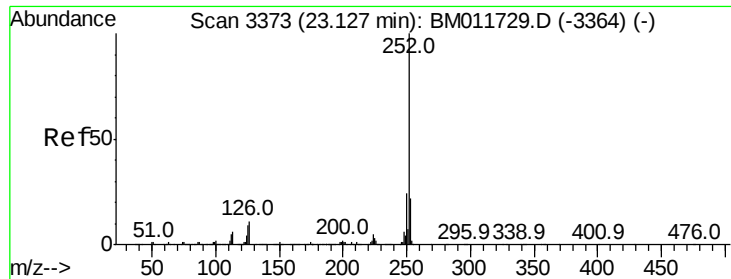

#85

Benzo(b)fluoranthene

Concen: 9.105 ng/ul

RT: 23.13 min Scan# 3373

Delta R.T. -0.00 min

Lab File: BM011734.D

Acq: 27 Sep 2017 21:44

Instrument :

BNA_M





ClientSampleId :

CB3F3

Tot Ion:	252	Resp:	678625
Ion Ratio	Lower	Upper	
252	100		
253	22.5	17.9	26.9
125	11.6	3.6	5.4#

Manual Integrations
APPROVED

Sohil
9/29/2017 2:22:46 PM

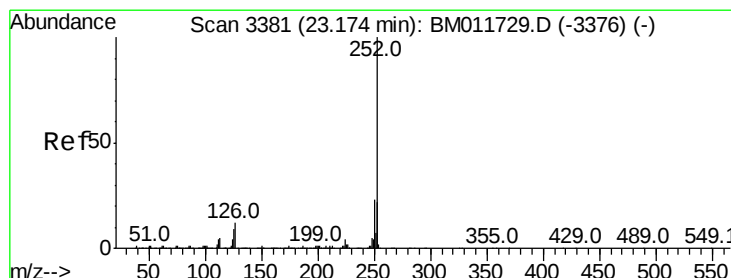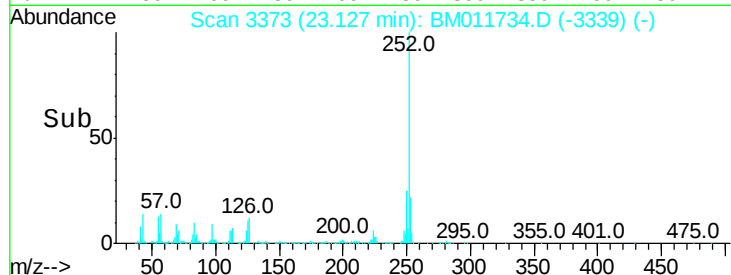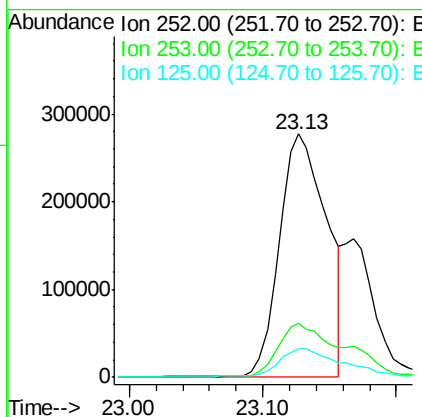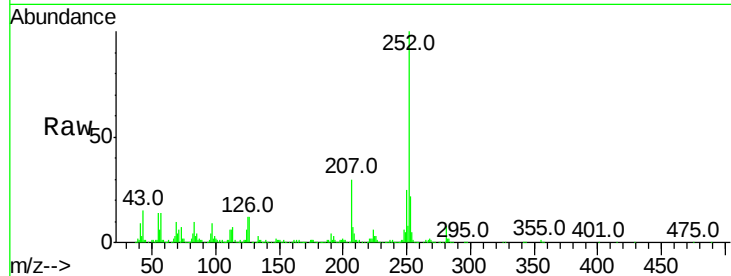

#86

Benzo(k)fluoranthene

Concen: 3.426 ng/ul m




RT: 23.17 min Scan# 3380


Delta R.T. -0.01 min

Lab File: BM011734.D

Acq: 27 Sep 2017 21:44

Tgt Ion:	252	Resp:	260494
Ion Ratio	Lower	Upper	
252	100		
253	22.1	17.1	25.7
125	8.9	3.4	5.2#

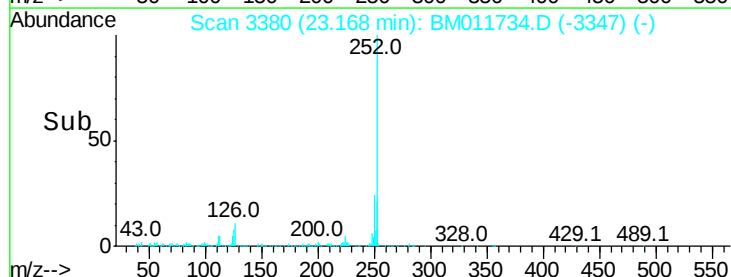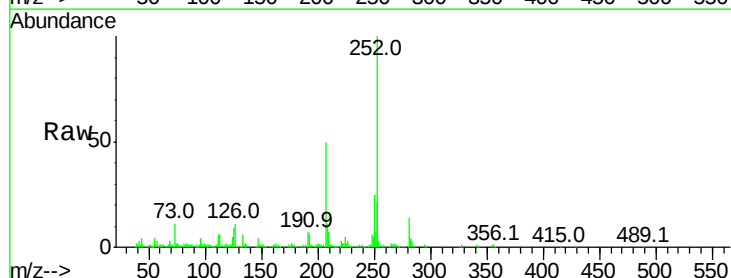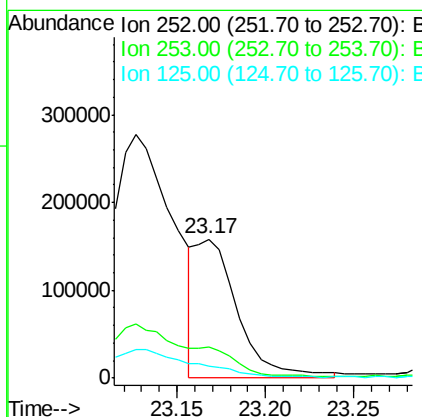

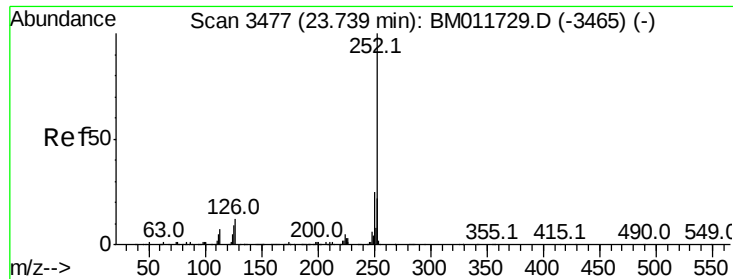

#88

Benzo(a)pyrene

Concen: 5.926 ng/ul

RT: 23.74 min Scan# 3477

Delta R.T. -0.00 min

Lab File: BM011734.D

Acq: 27 Sep 2017 21:44

Instrument :

BNA_M





ClientSampled :

CB3F3

Tot Ion:	252	Resp:	426615
Ion Ratio	Lower	Upper	
252	100		
253	22.6	18.2	27.2
125	10.0	4.0	6.0#

Manual Integrations
APPROVED

Sohil
9/29/2017 2:22:46 PM

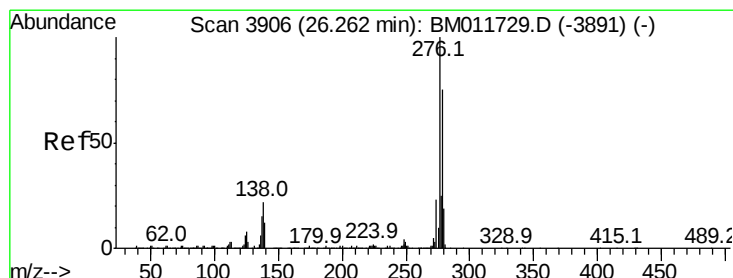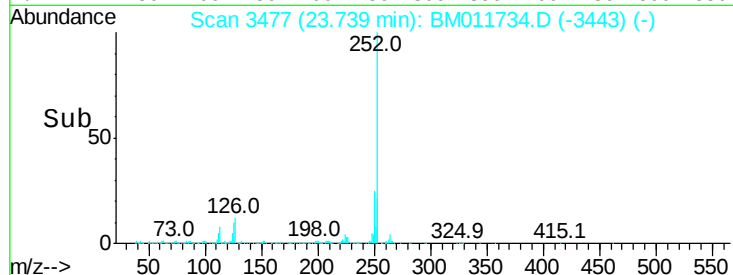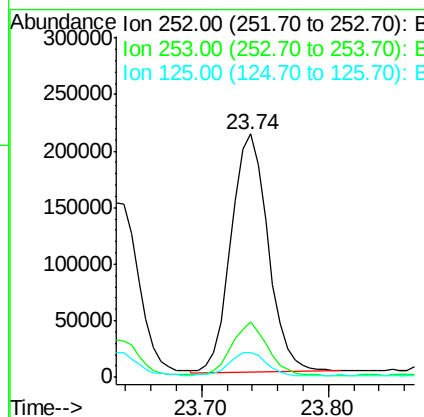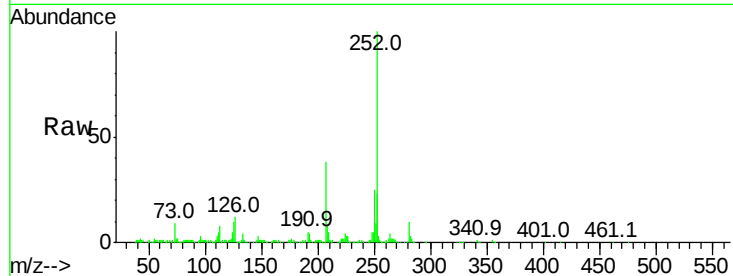

#89

Indeno(1,2,3-cd)pyrene

Concen: 3.328 ng/ul




RT: 26.26 min Scan# 3905




Delta R.T. -0.01 min

Lab File: BM011734.D

Acq: 27 Sep 2017 21:44

Tgt Ion:	276	Resp:	249428
Ion Ratio	Lower	Upper	
276	100		
138	20.1	9.3	13.9#
277	23.5	19.9	29.9

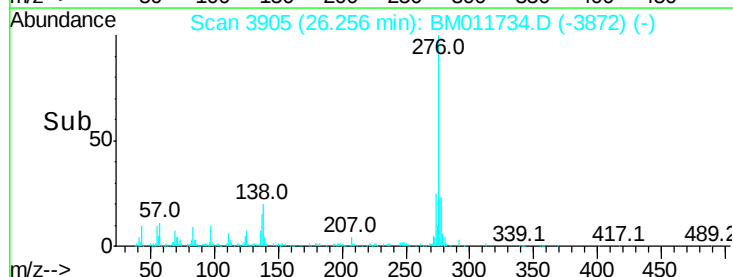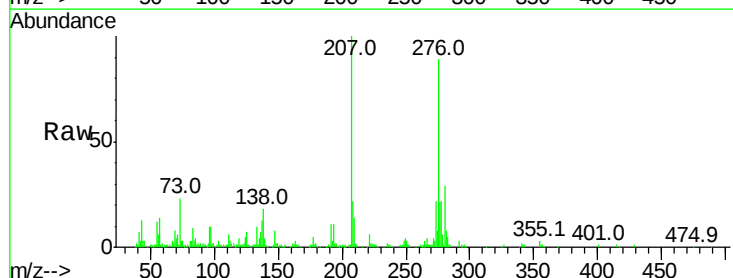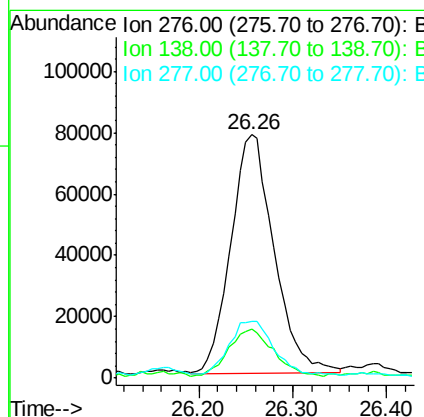

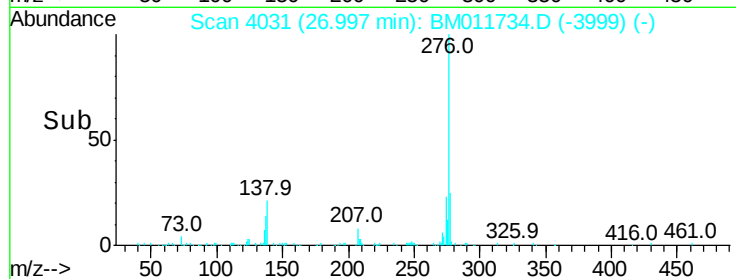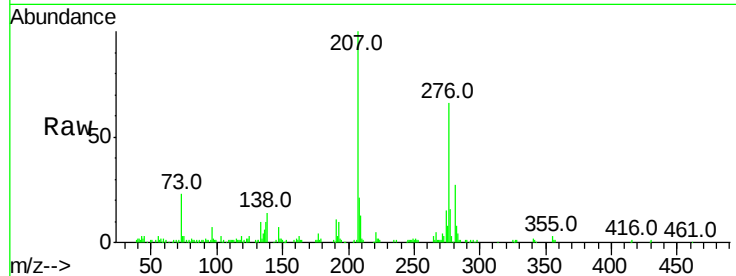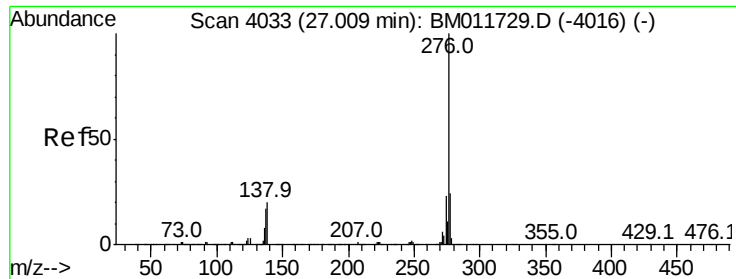

#91

Benzo(a,h,i)perylene

Concen: 3.321 ng/ul

RT: 27.00 min Scan# 4031

Delta R.T. -0.01 min

Lab File: BM011734.D

Acq: 27 Sep 2017 21:44

Tot Ion:	276	Resp:	206615
Ion Ratio	Lower	Upper	
276	100		
138	21.7	8.5	12.7#
277	24.6	18.6	28.0

Instrument :

BNA_M

ClientSampleId :

CB3F3

Manual Integrations
APPROVED

Sohil

9/29/2017 2:22:46 PM

