

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092722\
 Data File : BM036789.D
 Acq On : 27 Sep 2022 23:42
 Operator : CG/JU
 Sample : PB147850BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB147850BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036789.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.087	334	340	350	rVB	115815	169633	1.22%	0.206%
2	5.545	411	418	432	rBV	7545365	10444900	75.38%	12.696%
3	7.151	683	691	707	rBV	7054088	10804507	77.97%	13.133%
4	7.987	826	833	842	rBV	1436489	2233323	16.12%	2.715%
5	9.157	1024	1032	1044	rBV	3988755	6346831	45.80%	7.715%
6	10.798	1303	1311	1320	rBV	1834302	3030869	21.87%	3.684%
7	13.245	1720	1727	1737	rBV	10200835	13856526	100.00%	16.843%
8	14.615	1953	1960	1971	rBV	2589922	3729762	26.92%	4.534%
9	16.098	2204	2212	2230	rBV	6036864	8456828	61.03%	10.280%
10	17.351	2418	2425	2433	rBV	2916179	3963273	28.60%	4.818%
11	19.962	2864	2869	2874	rBV	11649796	13693128	98.82%	16.645%
12	20.727	2995	2999	3003	rBV	280872	328259	2.37%	0.399%
13	21.515	3128	3133	3139	rBV	2307458	2985131	21.54%	3.629%
14	23.938	3540	3545	3553	rVB2	1169010	2224776	16.06%	2.704%




Sum of corrected areas: 82267746

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092722\
Data File : BM036789.D
Acq On : 27 Sep 2022 23:42
Operator : CG/JU
Sample : PB147850BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB147850BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

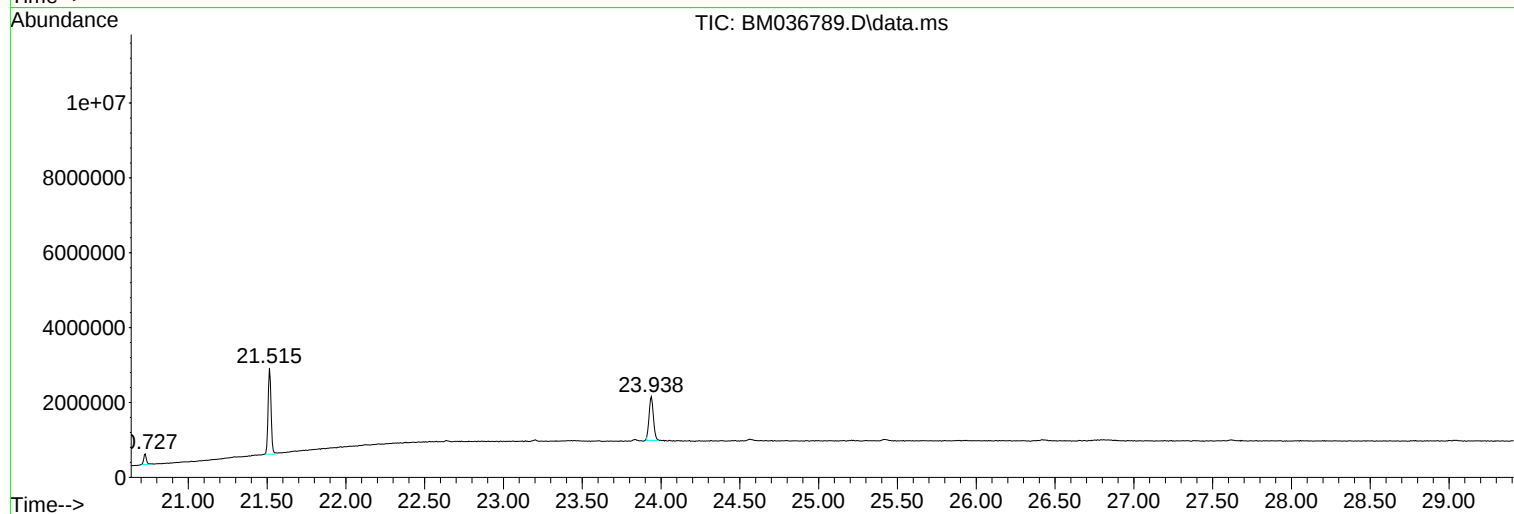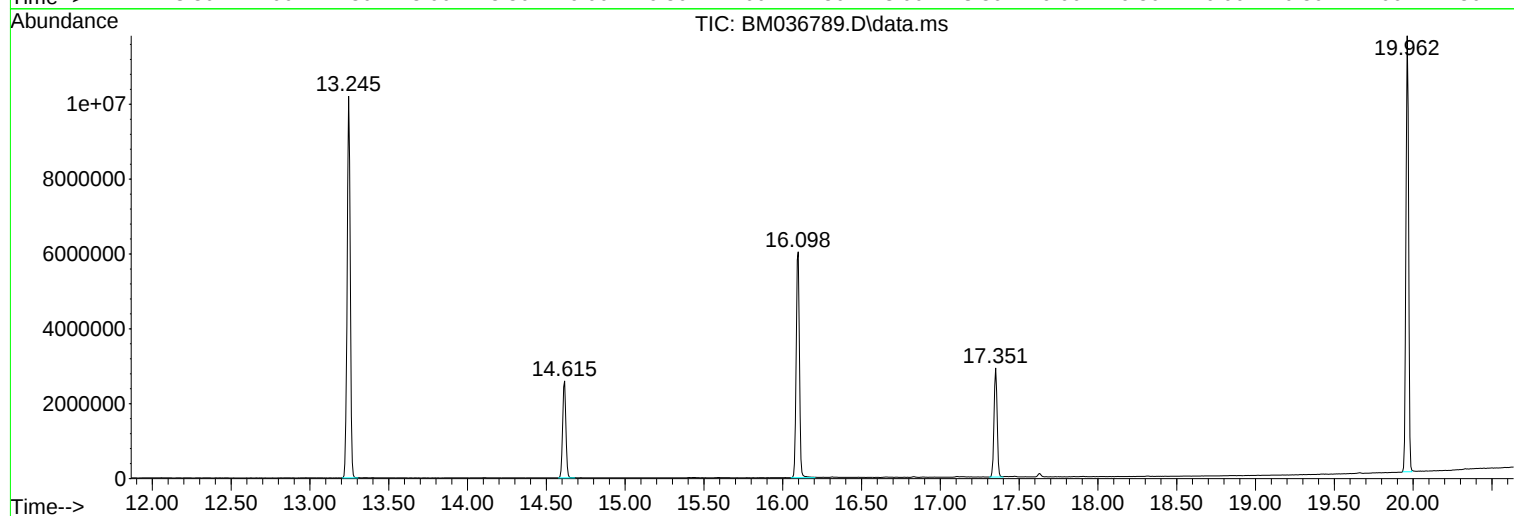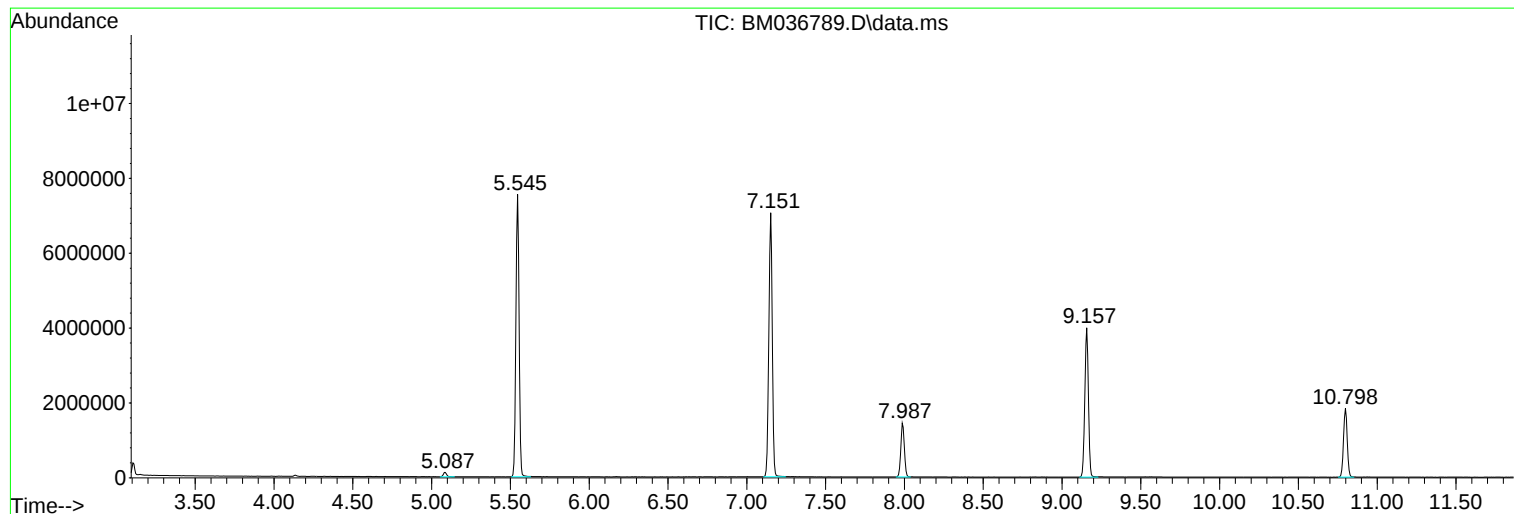

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092722\
Data File : BM036789.D
Acq On : 27 Sep 2022 23:42
Operator : CG/JU
Sample : PB147850BL
Misc :
ALS Vial : 10 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
PB147850BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, bis(2-eth... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
20.727	2.20 ng	328259	Chrysene-d12	21.515	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	91
2	Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	91
3	Diisooctyl adipate	370	C22H42O4	001330-86-5	91
4	Hexanedioic acid, mono(2-ethylhe...	258	C14H26O4	004337-65-9	64
5	Adipic acid, 2-ethylhexyl isohex...	342	C20H38O4	1000324-48-3	50

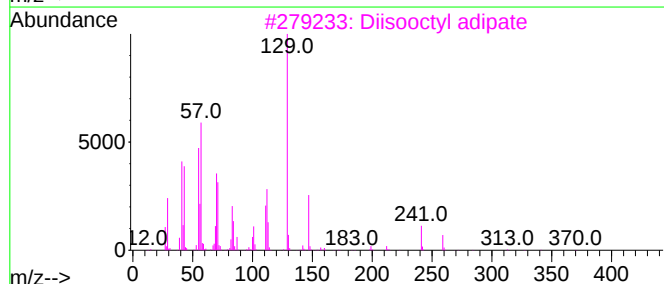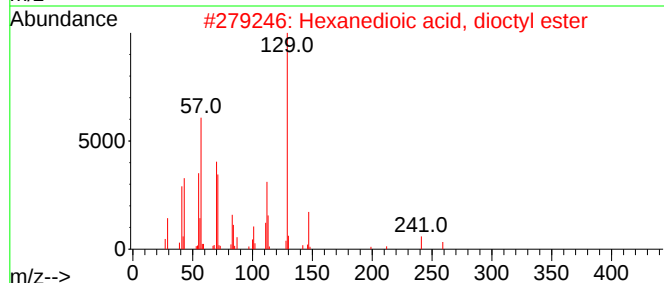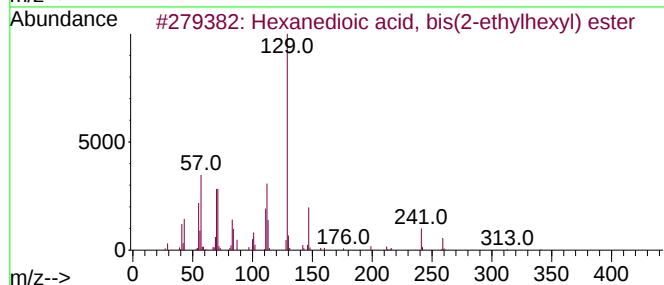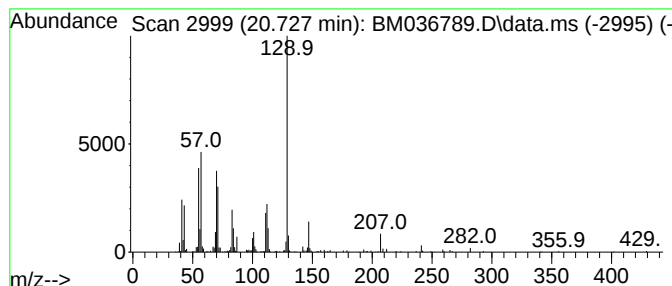

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092722\
Data File : BM036789.D
Acq On : 27 Sep 2022 23:42
Operator : CG/JU
Sample : PB147850BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB147850BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	20.727	2.2	ng	328259	5	21.515	2985130	20.0