
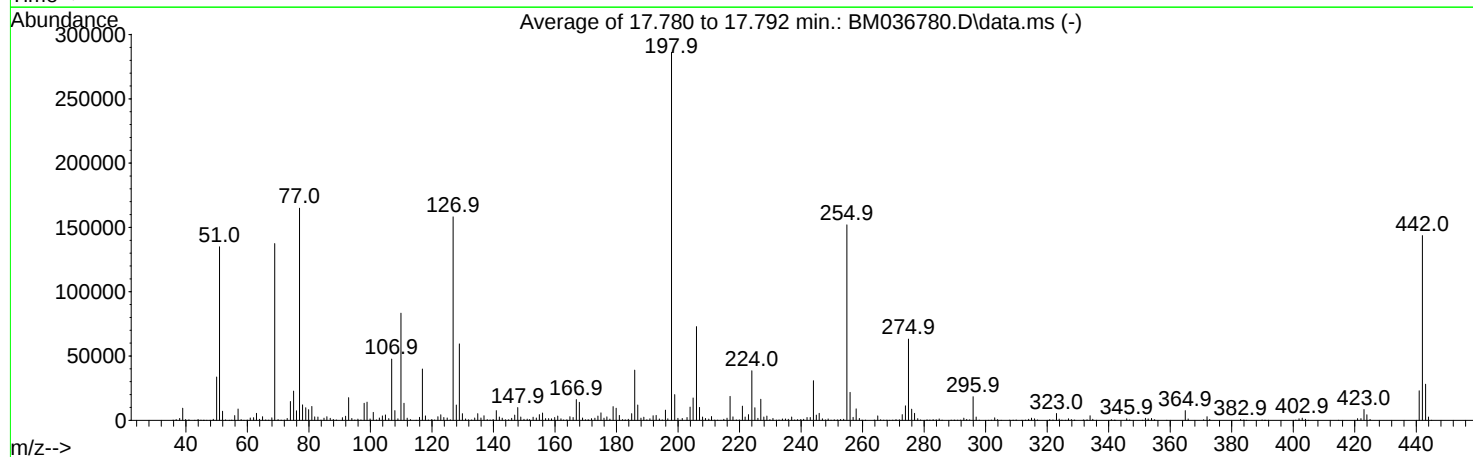


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092722\
 Data File : BM036780.D
 Acq On : 27 Sep 2022 16:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 28 01:39:14 2022

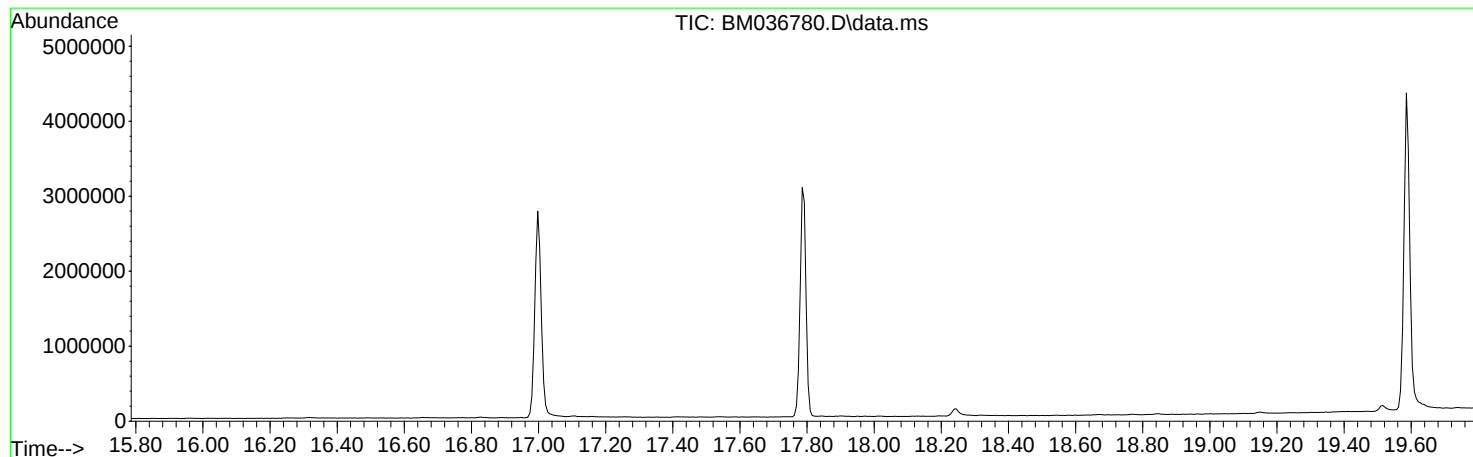




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	134921	PASS
68	69	0.00	2	1.4	1963	PASS
69	198	0.00	100	48.1	137498	PASS
70	69	0.00	2	0.5	625	PASS
127	198	10	80	55.3	158221	PASS
197	198	0.00	2	0.4	1225	PASS
198	198	100	100	100.0	286123	PASS
199	198	5	9	7.0	19931	PASS
275	198	10	60	22.1	63200	PASS
365	198	1	100	2.6	7558	PASS
441	198	0.01	100	8.0	22949	PASS
442	442	50	100	100.0	143651	PASS
443	442	15	24	19.6	28126	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092722\
Data File : BM036780.D
Acq On : 27 Sep 2022 16:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 28 07:09:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 01:39:14 2022
Response via : Initial Calibration

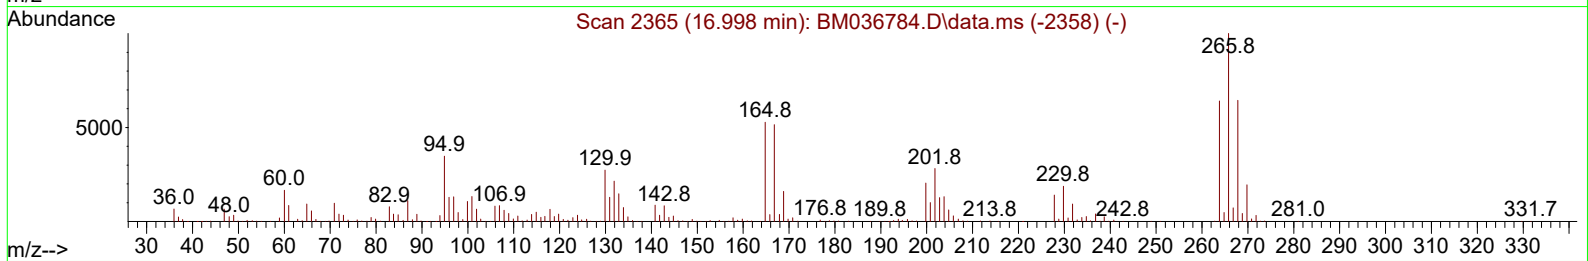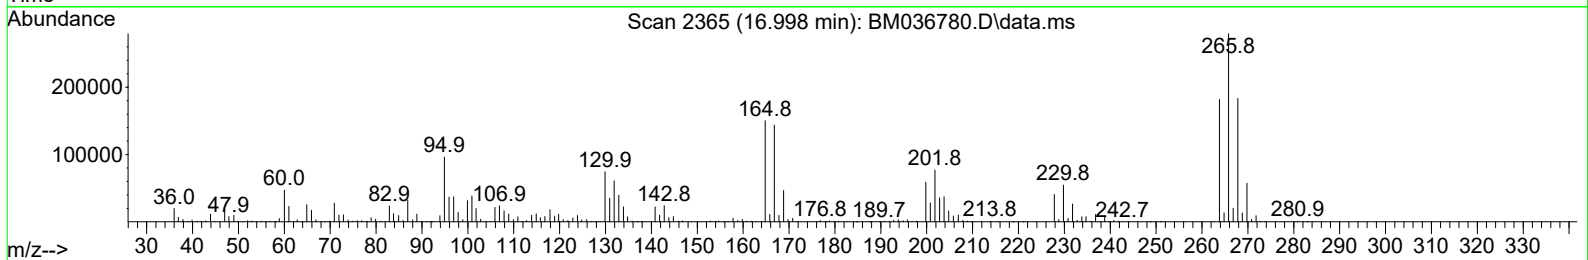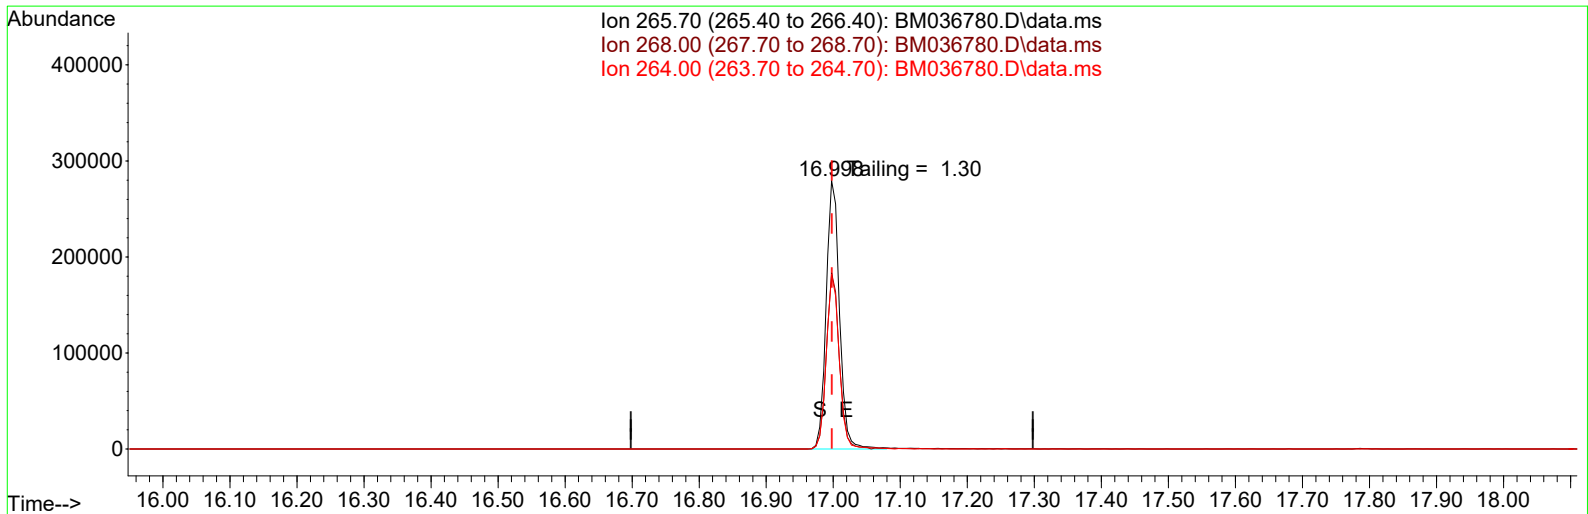

TIC: BM036780.D\data.ms

(70) Pentachlorophenol (C)

16.998min (-0.000) 752232.86 ng




response 386968

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	65.61
264.00	64.10	65.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092722\
 Data File : BM036780.D
 Acq On : 27 Sep 2022 16:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Sep 28 07:09:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 01:39:14 2022
 Response via : Initial Calibration

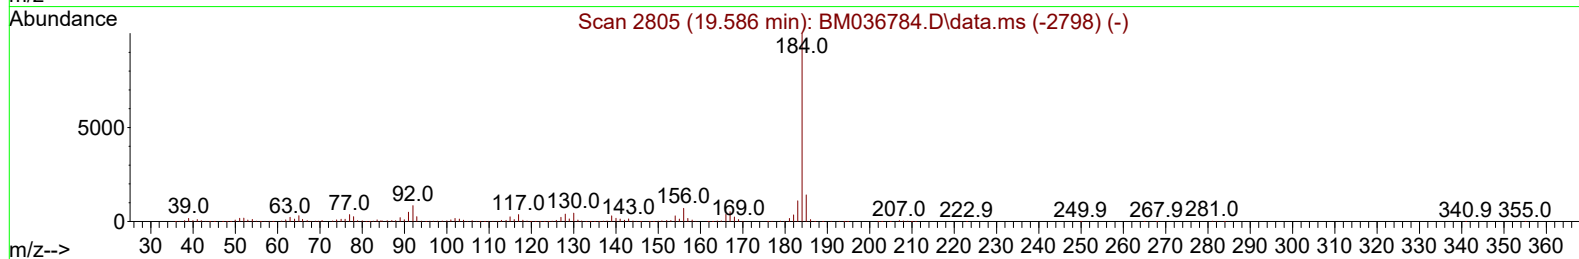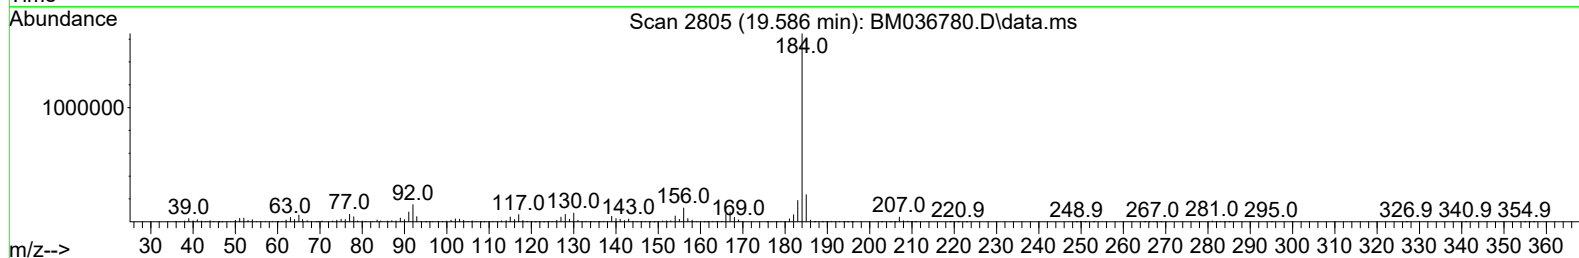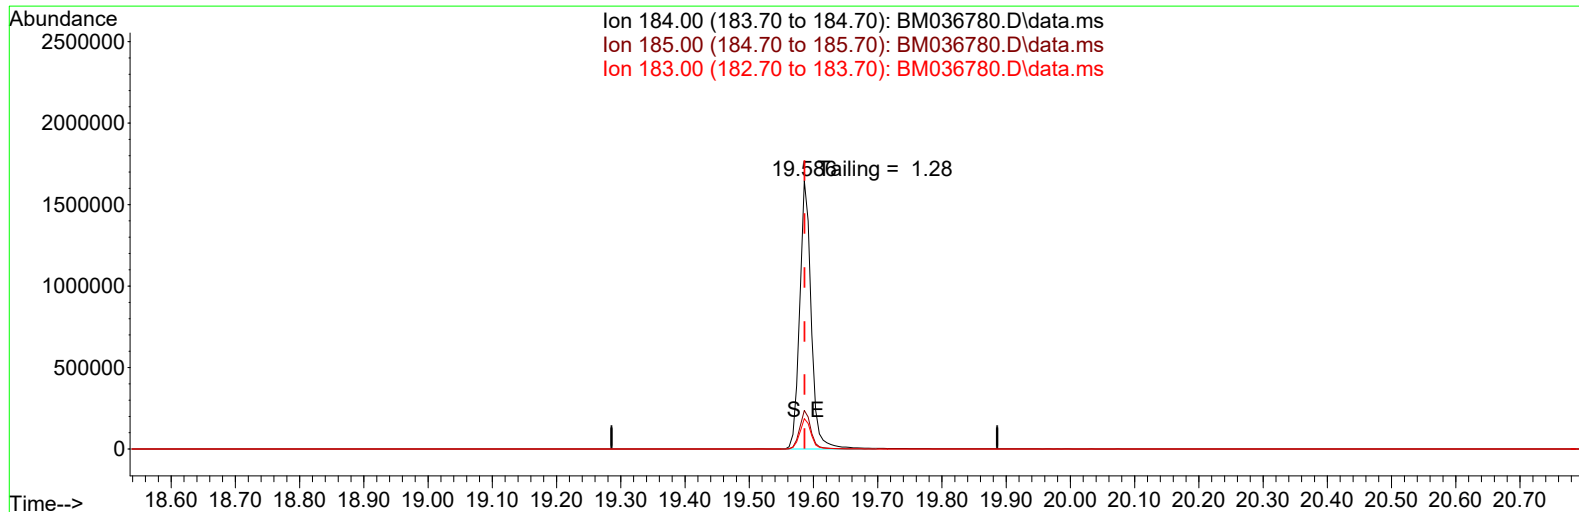

TIC: BM036780.D\data.ms

(77) Benzidine

19.586min (-0.000) 126995.02 ng

response 2072598

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.41
183.00	11.00	11.35
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/27/2022	BNA_M	<u>BM036780.D</u>
Compound Name	Response	Retention Time
DDT	877621	20.815
DDD	5506	20.433
DDE	0	19.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5506	883127	0.62

Instrument :
BNA_M
ClientSampleId :
DFTPP