

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092816\
 Data File : BM007595.D
 Acq On : 28 Sep 2016 09:56
 Operator : UM/SJ
 Sample : PB93637BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK37

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.945	735	741	756	rBV	697867	1193043	14.77%	1.719%
2	7.110	763	769	782	rBV	552243	915808	11.33%	1.320%
3	7.310	796	803	816	rBV	737317	1223084	15.14%	1.763%
4	7.775	875	882	897	rBV	657198	1097317	13.58%	1.581%
5	8.481	995	1002	1022	rBV	948457	1663620	20.59%	2.398%
6	8.934	1071	1079	1090	rBV	786423	1343340	16.63%	1.936%
7	9.651	1194	1201	1216	rBV	661620	1158312	14.34%	1.669%
8	10.186	1285	1292	1307	rBV	911438	1748503	21.64%	2.520%
9	10.557	1346	1355	1368	rBV	1057185	1785871	22.10%	2.574%
10	10.698	1372	1379	1402	rBV	926555	1871163	23.16%	2.697%
11	13.822	1903	1910	1924	rBV	2280582	3423211	42.37%	4.934%
12	14.098	1950	1957	1975	rBV	2435531	3680392	45.55%	5.304%
13	14.404	2003	2009	2022	rBV	1890722	2873434	35.56%	4.141%
14	14.621	2039	2046	2070	rBV	722728	1651998	20.45%	2.381%
15	15.404	2172	2179	2191	rBV	3380353	5080432	62.88%	7.322%
16	15.533	2194	2201	2215	rBV	1001355	1608568	19.91%	2.318%
17	17.151	2469	2476	2486	rBV2	2689164	4014252	49.68%	5.785%
18	17.251	2486	2493	2511	rVB2	4161757	6190886	76.62%	8.922%
19	19.186	2817	2822	2827	rBV	54203	81816	1.01%	0.118%
20	19.545	2877	2883	2893	rBV	5829578	8079589	100.00%	11.644%
21	21.333	3182	3187	3197	rBV	4359735	5765222	71.36%	8.309%
22	23.450	3540	3547	3560	rBV2	3902152	7719064	95.54%	11.125%
23	23.597	3565	3572	3588	rVB	2509701	5218046	64.58%	7.520%


Sum of corrected areas: 69386971

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092816\
Data File : BM007595.D
Acq On : 28 Sep 2016 09:56
Operator : UM/SJ
Sample : PB93637BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK37

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

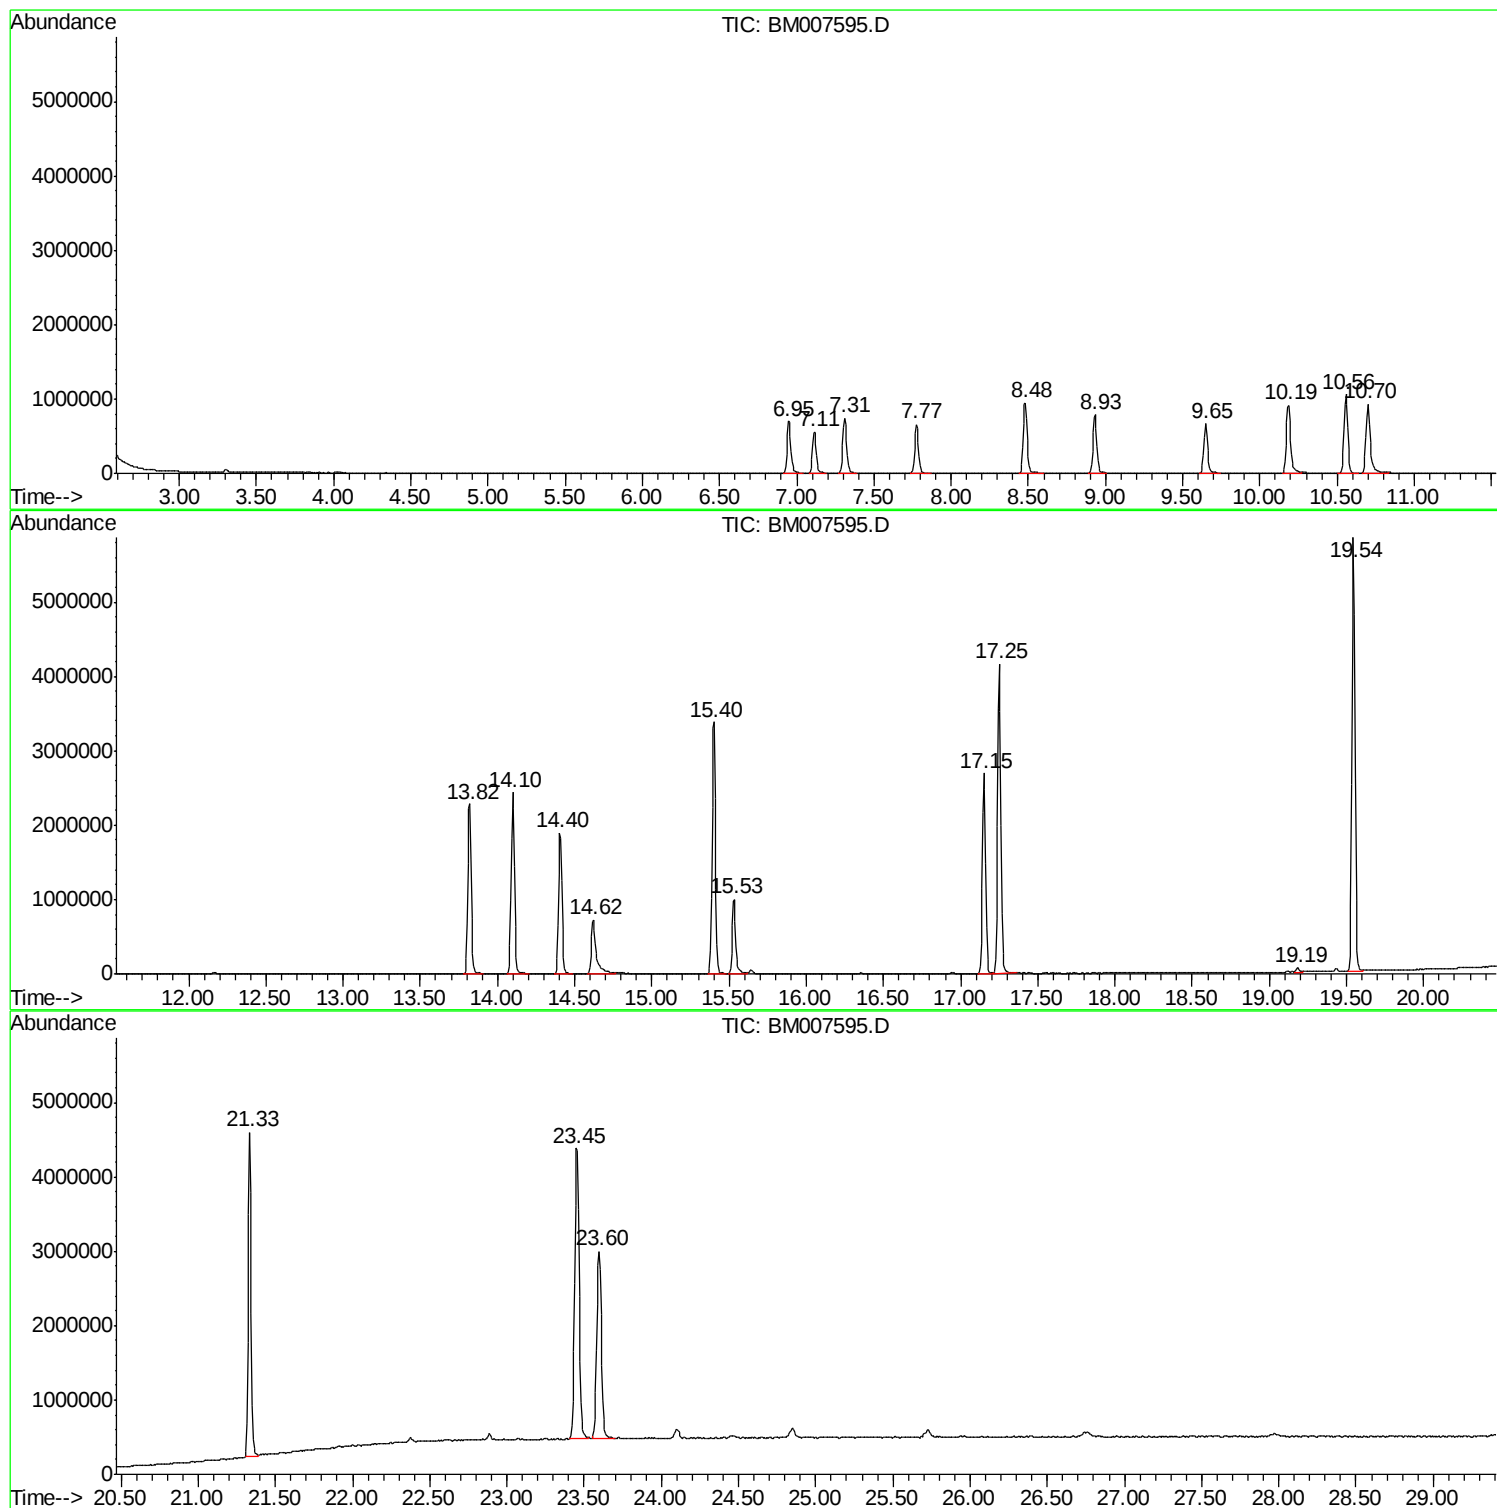

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092816\
Data File : BM007595.D
Acq On : 28 Sep 2016 09:56
Operator : UM/SJ
Sample : PB93637BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK37

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092816\
Data File : BM007595.D
Acq On : 28 Sep 2016 09:56
Operator : UM/SJ
Sample : PB93637BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK37

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc