

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092816\
 Data File : BM007618.D
 Acq On : 29 Sep 2016 00:54
 Operator : UM/SJ
 Sample : H4955-26
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4VN7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.945	735	741	752	rBV	247782	431279	4.28%	0.537%
2	7.110	762	769	781	rBV	728532	1167654	11.58%	1.453%
3	7.310	796	803	815	rBV	822569	1371396	13.59%	1.707%
4	7.775	875	882	891	rBV	773257	1282290	12.71%	1.596%
5	8.475	995	1001	1019	rBV	777788	1346906	13.35%	1.676%
6	8.928	1071	1078	1090	rBV	1031011	1781374	17.66%	2.217%
7	9.645	1193	1200	1215	rBV	898305	1549589	15.36%	1.928%
8	10.181	1282	1291	1317	rBV	1220632	2409151	23.88%	2.998%
9	10.557	1346	1355	1364	rBV	1211321	2078973	20.61%	2.587%
10	10.710	1375	1381	1392	rBV2	71324	160547	1.59%	0.200%
11	13.816	1902	1909	1925	rBV	3111972	4409765	43.72%	5.488%
12	14.098	1950	1957	1972	rBV	3270359	4950618	49.08%	6.161%
13	14.404	2002	2009	2024	rBV	2201014	3298741	32.70%	4.105%
14	14.627	2039	2047	2060	rBV2	182070	471579	4.67%	0.587%
15	15.398	2171	2178	2194	rBV	4403908	6669022	66.11%	8.299%
16	15.527	2194	2200	2214	rVV	1508587	2300468	22.81%	2.863%
17	15.639	2214	2219	2224	rVB2	61232	101068	1.00%	0.126%
18	17.151	2469	2476	2486	rBV	3116442	4499395	44.60%	5.599%
19	17.251	2486	2493	2510	rVB2	5204733	7834775	77.67%	9.750%
20	19.180	2816	2821	2825	rBV	101842	141663	1.40%	0.176%
21	19.545	2876	2883	2897	rBV	7276082	10087524	100.00%	12.554%
22	21.333	3181	3187	3198	rBV	4725844	6448998	63.93%	8.026%
23	23.450	3540	3547	3562	rVB2	4951576	9713957	96.30%	12.089%
24	23.597	3565	3572	3586	rVB	2951469	5848081	57.97%	7.278%


Sum of corrected areas: 80354813

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092816\
Data File : BM007618.D
Acq On : 29 Sep 2016 00:54
Operator : UM/SJ
Sample : H4955-26
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4VN7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

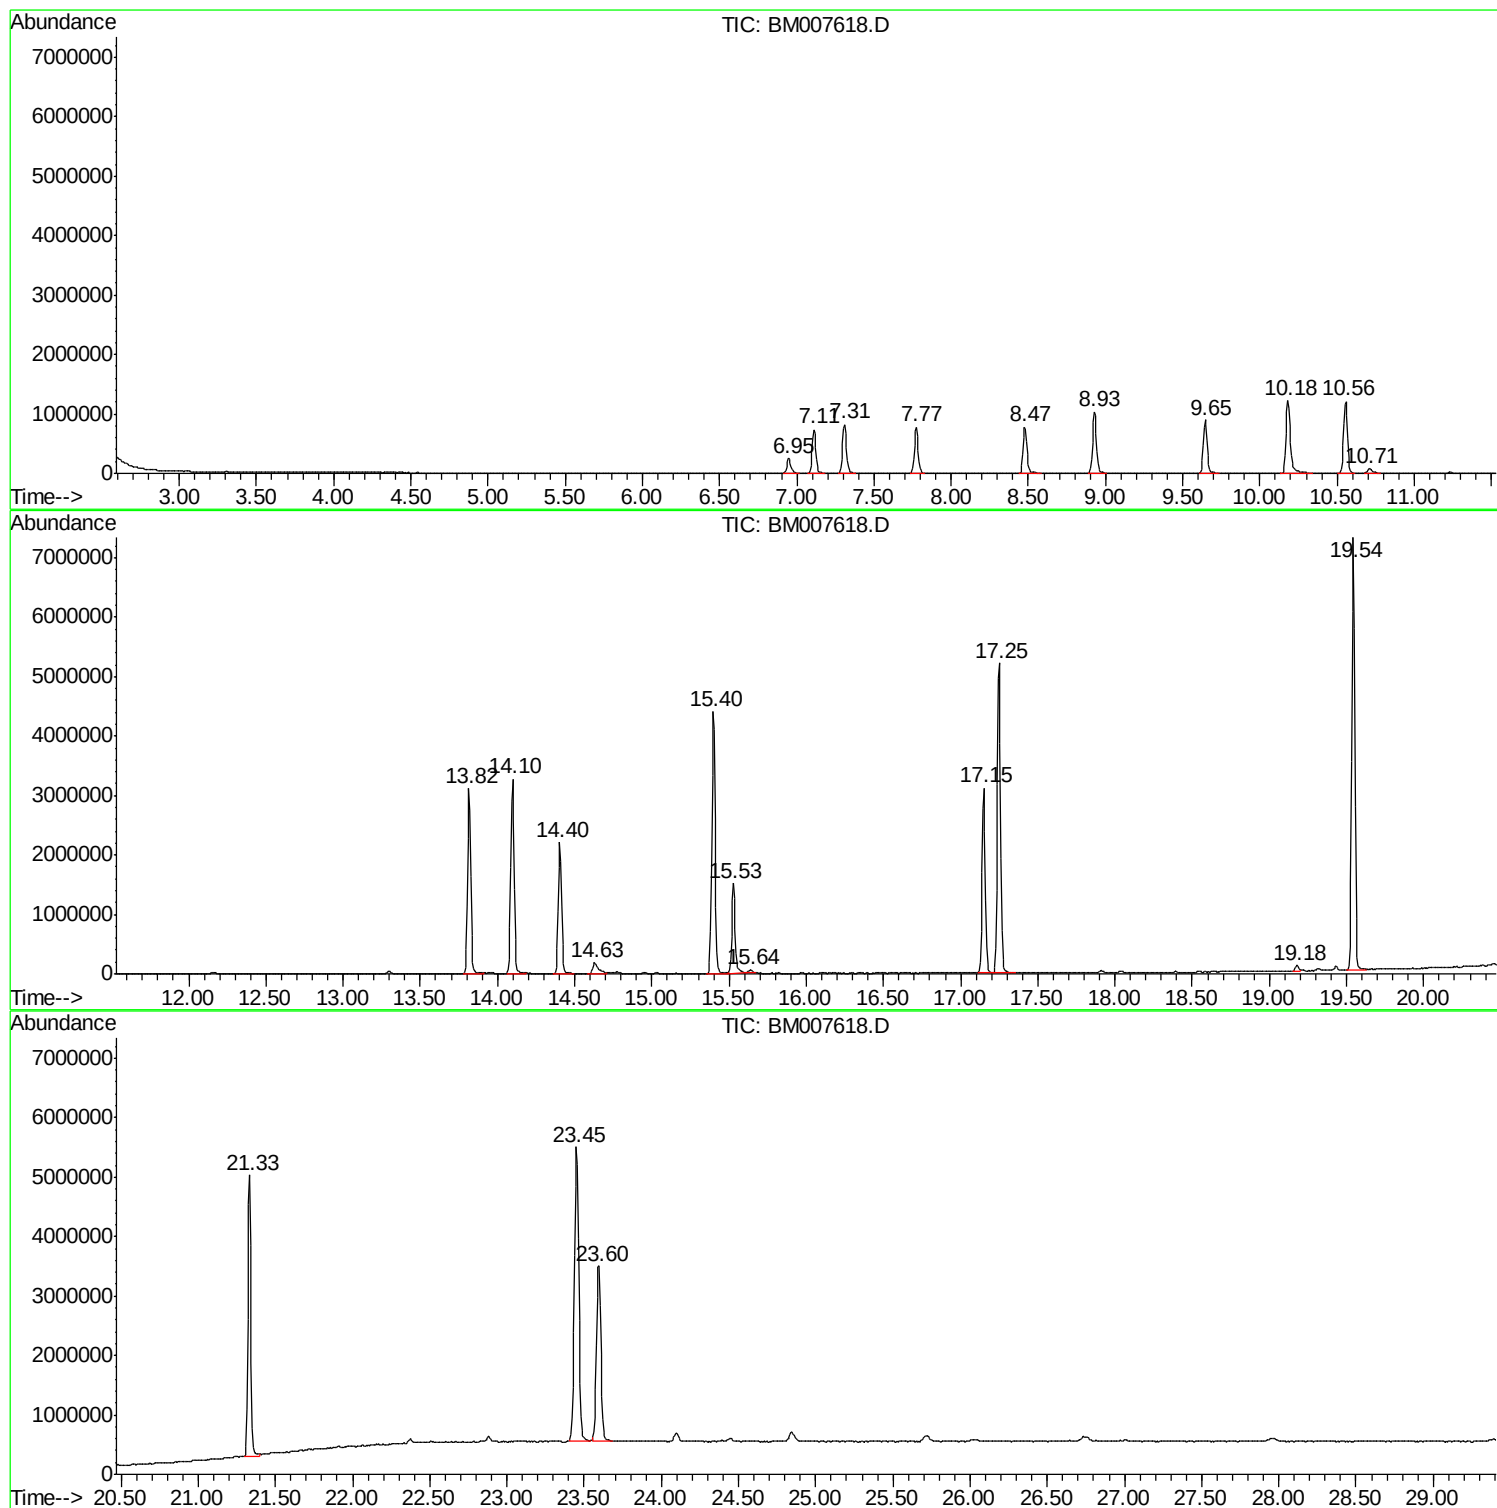

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092816\
Data File : BM007618.D
Acq On : 29 Sep 2016 00:54
Operator : UM/SJ
Sample : H4955-26
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4VN7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092816\
Data File : BM007618.D
Acq On : 29 Sep 2016 00:54
Operator : UM/SJ
Sample : H4955-26
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4VN7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc