

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092822\
 Data File : BM036792.D
 Acq On : 28 Sep 2022 10:38
 Operator : CG/JU
 Sample : PB147926BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB147926BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.081	333	339	349	rBV	559921	764715	4.43%	0.798%
2	5.546	410	418	432	rBV	8536695	12314647	71.42%	12.846%
3	7.151	683	691	708	rBV	8235625	12648816	73.35%	13.195%
4	7.987	825	833	846	rBV	1482280	2275413	13.20%	2.374%
5	9.157	1021	1032	1044	rBV	4543857	7421906	43.04%	7.742%
6	10.798	1303	1311	1324	rBV	1806254	3095276	17.95%	3.229%
7	13.245	1720	1727	1738	rBV	11387707	15985074	92.70%	16.675%
8	14.610	1953	1959	1972	rBV	2622620	3729230	21.63%	3.890%
9	16.092	2204	2211	2226	rBV	7428914	10278546	59.61%	10.722%
10	17.351	2418	2425	2433	rBV	2915283	4038707	23.42%	4.213%
11	19.962	2863	2869	2880	rBV	14868614	17243482	100.00%	17.988%
12	20.727	2995	2999	3003	rVB	279184	323200	1.87%	0.337%
13	21.515	3128	3133	3140	rBV	2560678	3248071	18.84%	3.388%
14	23.938	3539	3545	3557	rVB2	1259708	2495325	14.47%	2.603%




Sum of corrected areas: 95862408

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092822\
Data File : BM036792.D
Acq On : 28 Sep 2022 10:38
Operator : CG/JU
Sample : PB147926BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB147926BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

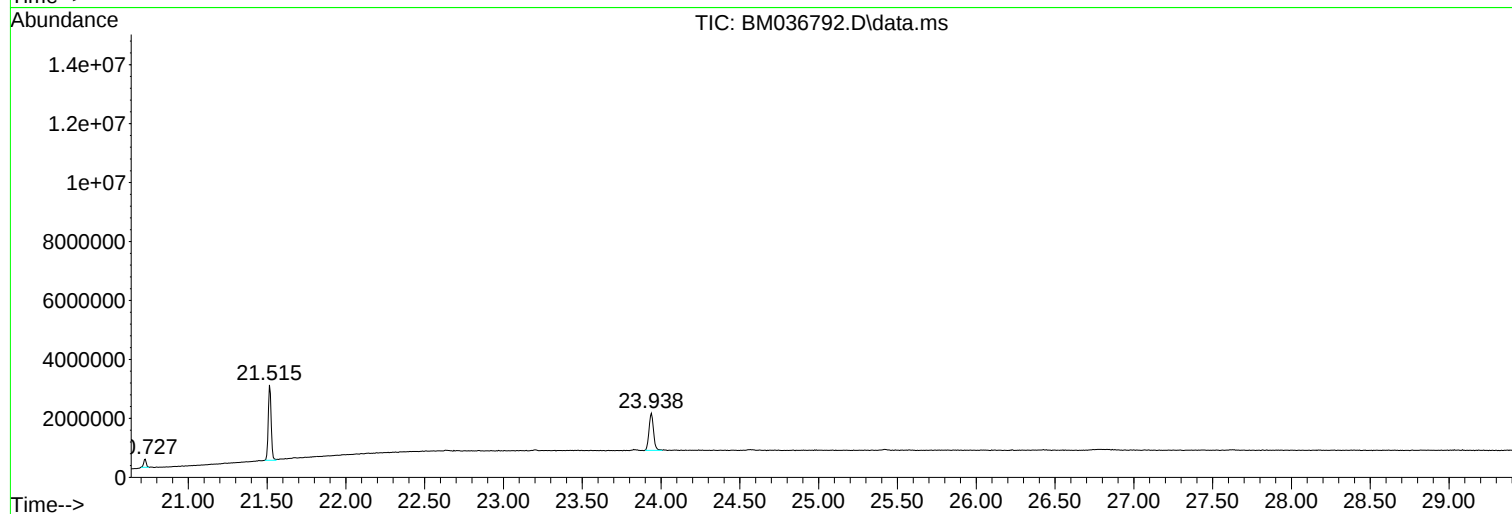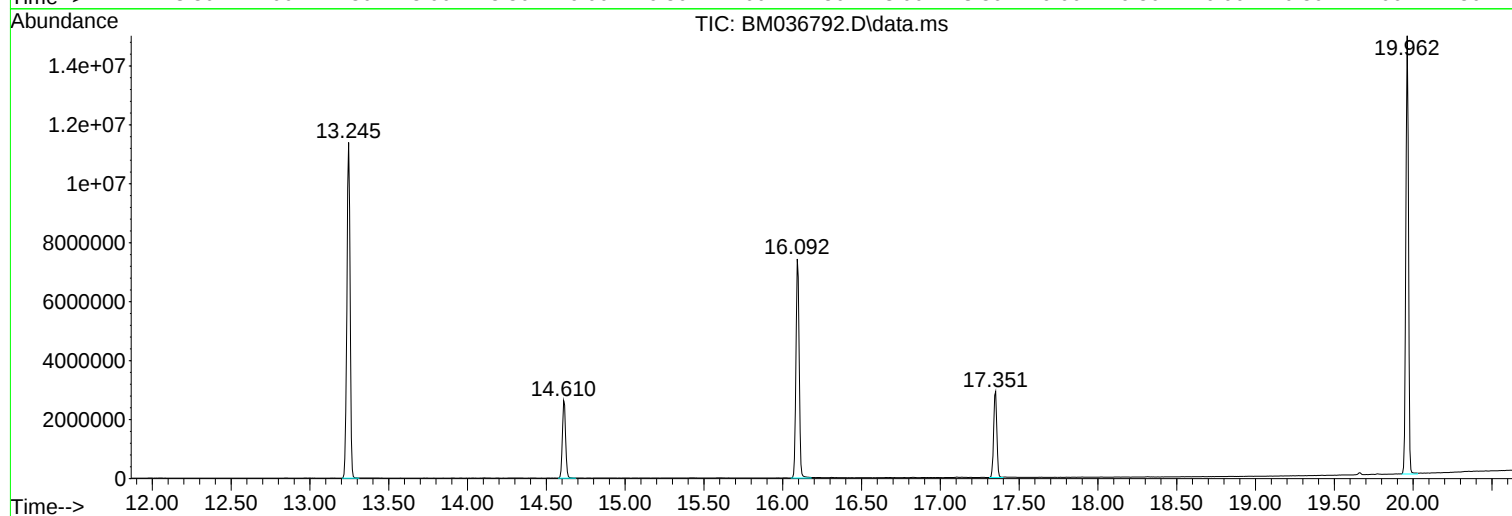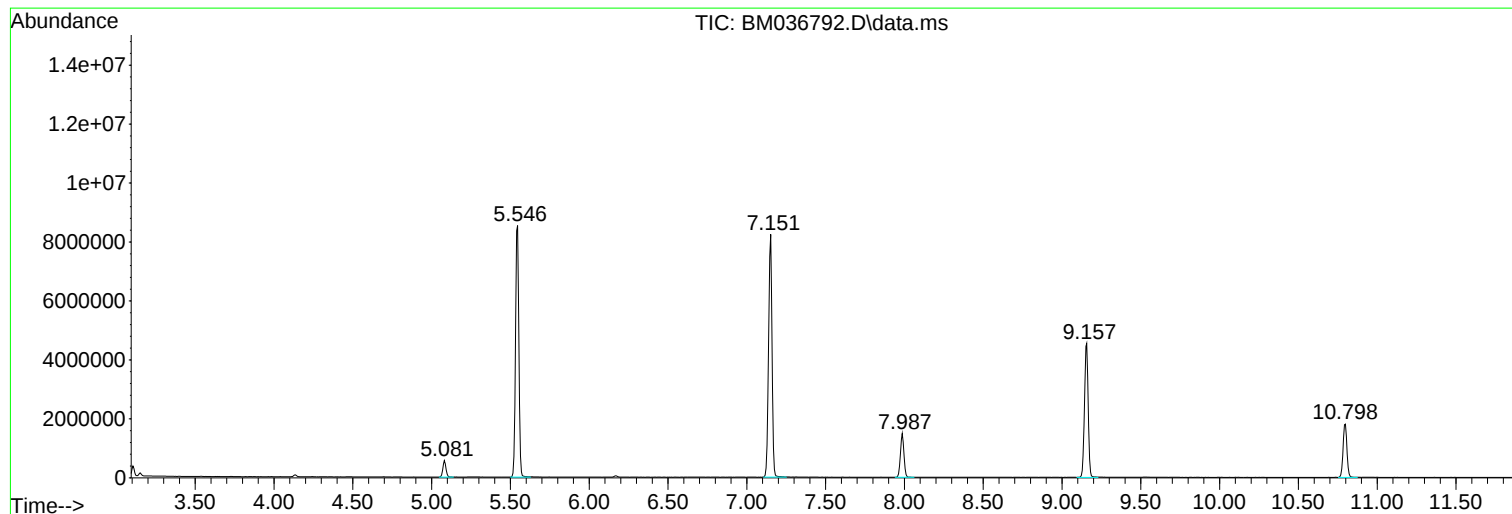

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092822\
Data File : BM036792.D
Acq On : 28 Sep 2022 10:38
Operator : CG/JU
Sample : PB147926BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB147926BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.081	6.72 ng	764715	1,4-Dichlorobenzene-d4	7.987

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	32		
3	Acetone	58	C3H6O	000067-64-1	10		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	5-Hexen-2-one	98	C6H10O	000109-49-9	9		

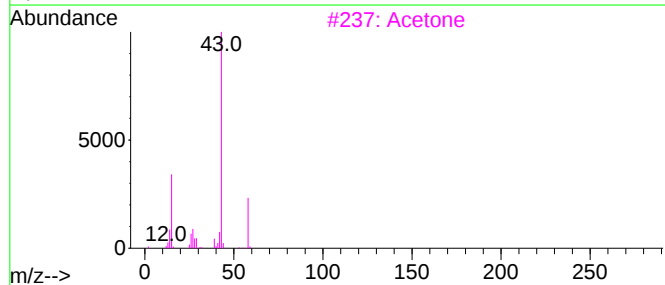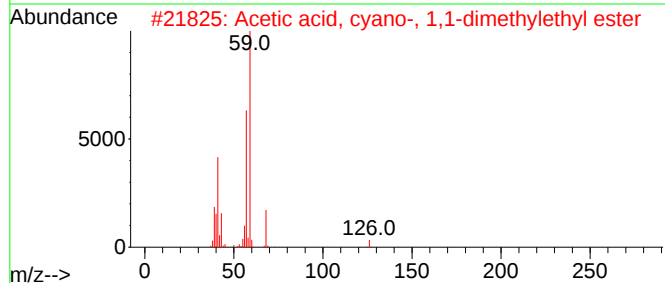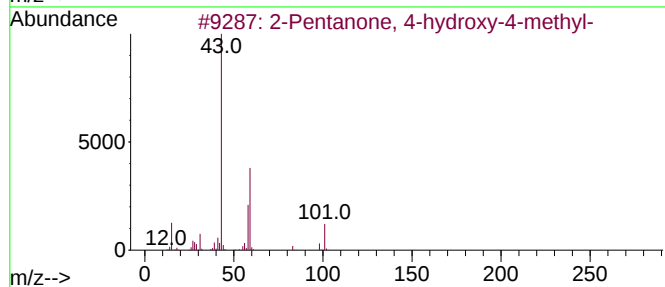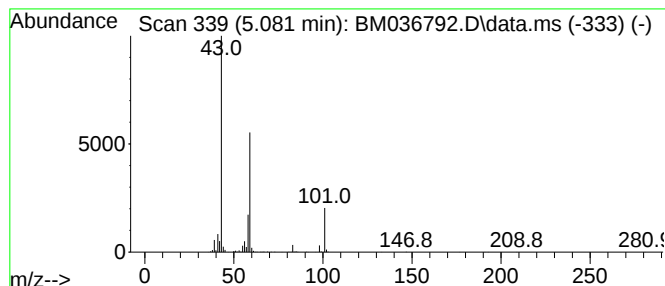

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092822\
Data File : BM036792.D
Acq On : 28 Sep 2022 10:38
Operator : CG/JU
Sample : PB147926BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB147926BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.081	6.7	ng	764715	1	7.987	2275410	20.0