


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092822\
 Data File : BM036790.D
 Acq On : 28 Sep 2022 09:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 28 01:39:14 2022

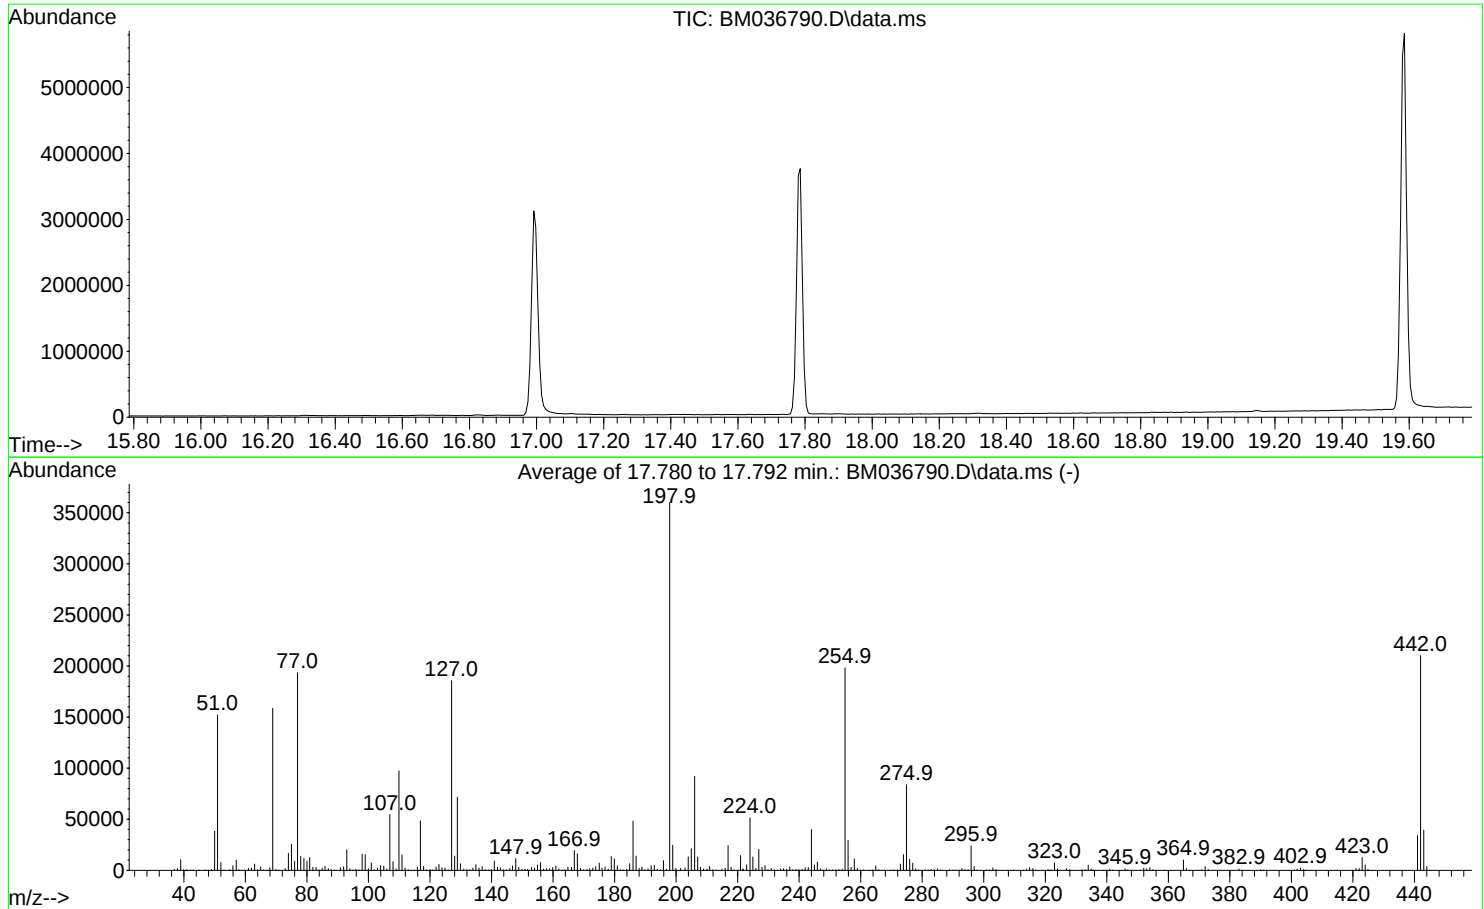




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	152054	PASS
68	69	0.00	2	1.6	2503	PASS
69	198	0.00	100	44.0	158603	PASS
70	69	0.00	2	0.5	765	PASS
127	198	10	80	51.5	185653	PASS
197	198	0.00	2	0.3	999	PASS
198	198	100	100	100.0	360149	PASS
199	198	5	9	6.8	24477	PASS
275	198	10	60	23.3	83821	PASS
365	198	1	100	2.8	10141	PASS
441	198	0.01	100	9.5	34096	PASS
442	442	50	100	100.0	210176	PASS
443	442	15	24	18.6	39181	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092822\
Data File : BM036790.D
Acq On : 28 Sep 2022 09:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 29 05:41:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 01:39:14 2022
Response via : Initial Calibration

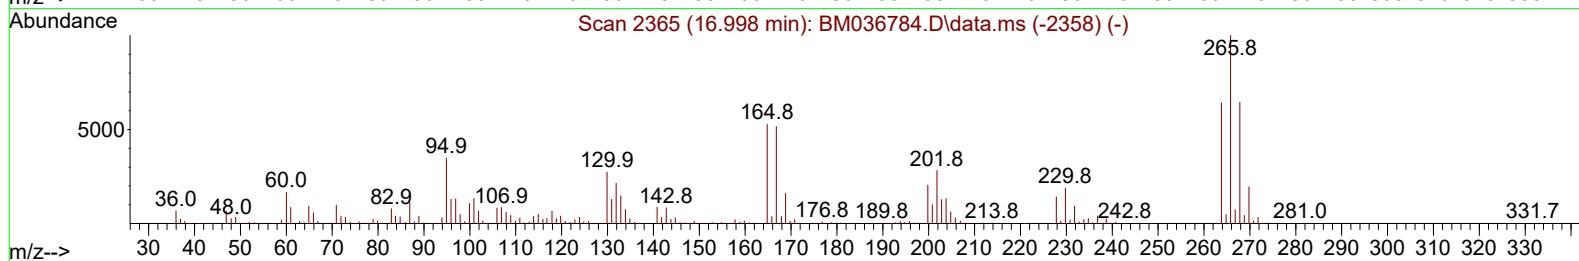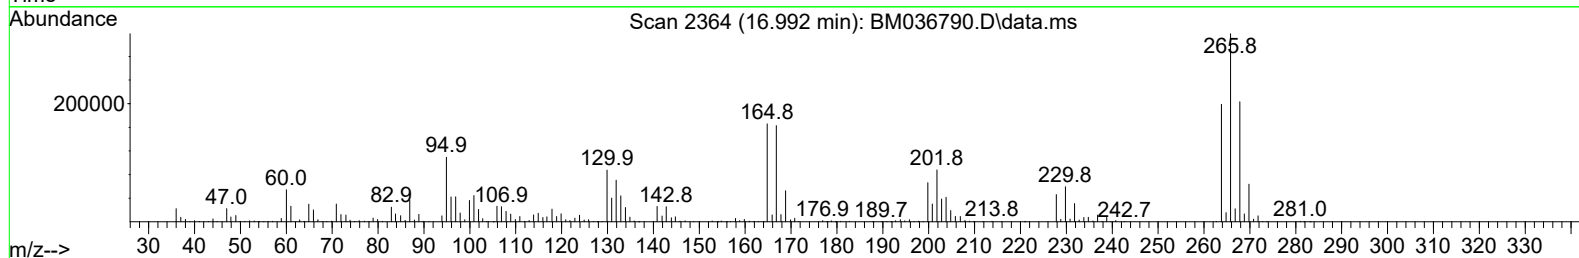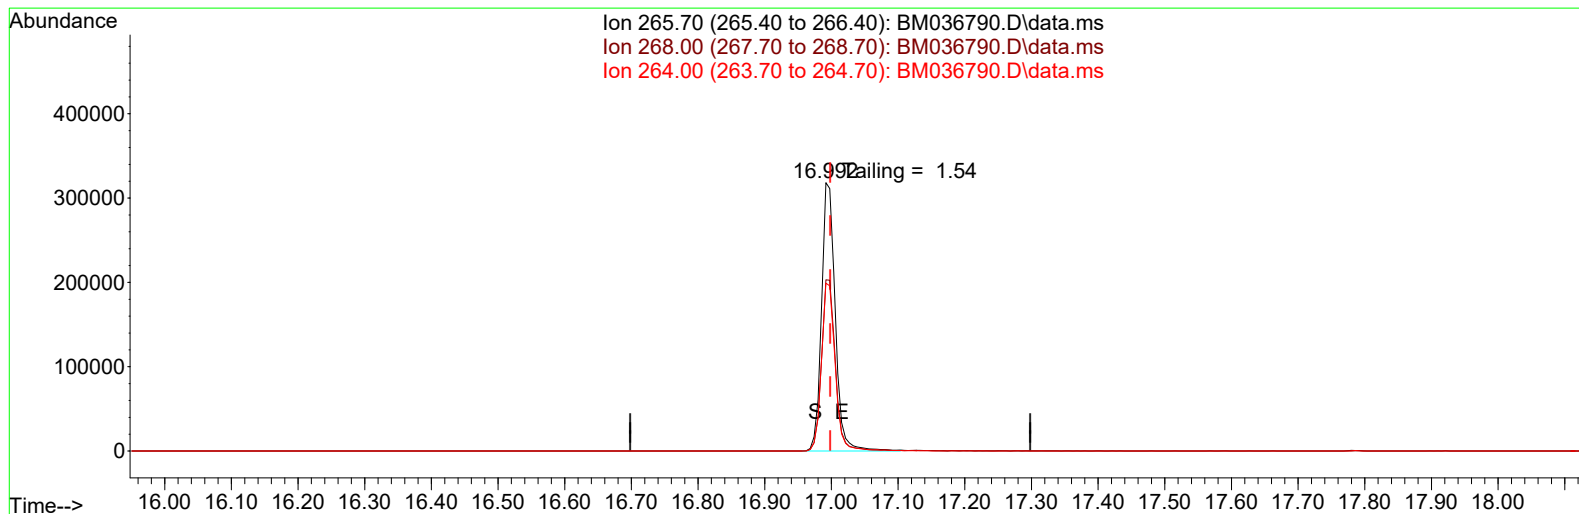

TIC: BM036790.D\data.ms

(70) Pentachlorophenol (C)

16.992min (-0.006) 0.00 ng




response 457798

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	63.83
264.00	64.10	62.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092822\
 Data File : BM036790.D
 Acq On : 28 Sep 2022 09:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Sep 29 05:41:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 01:39:14 2022
 Response via : Initial Calibration

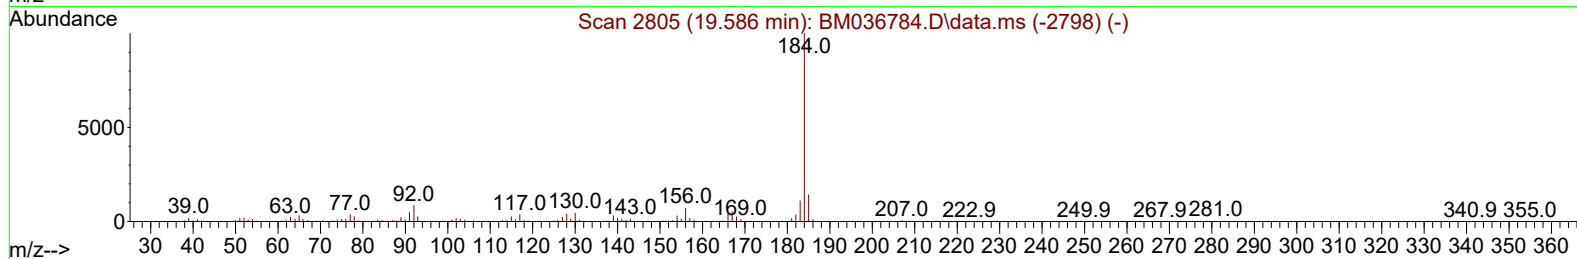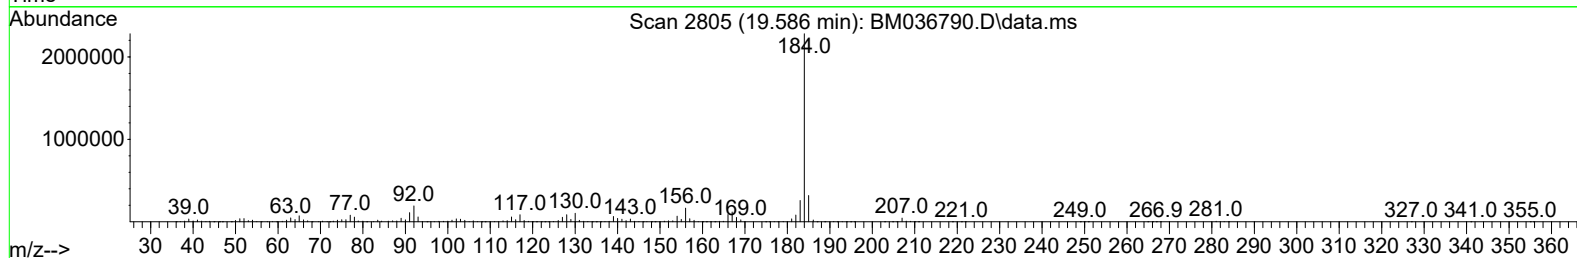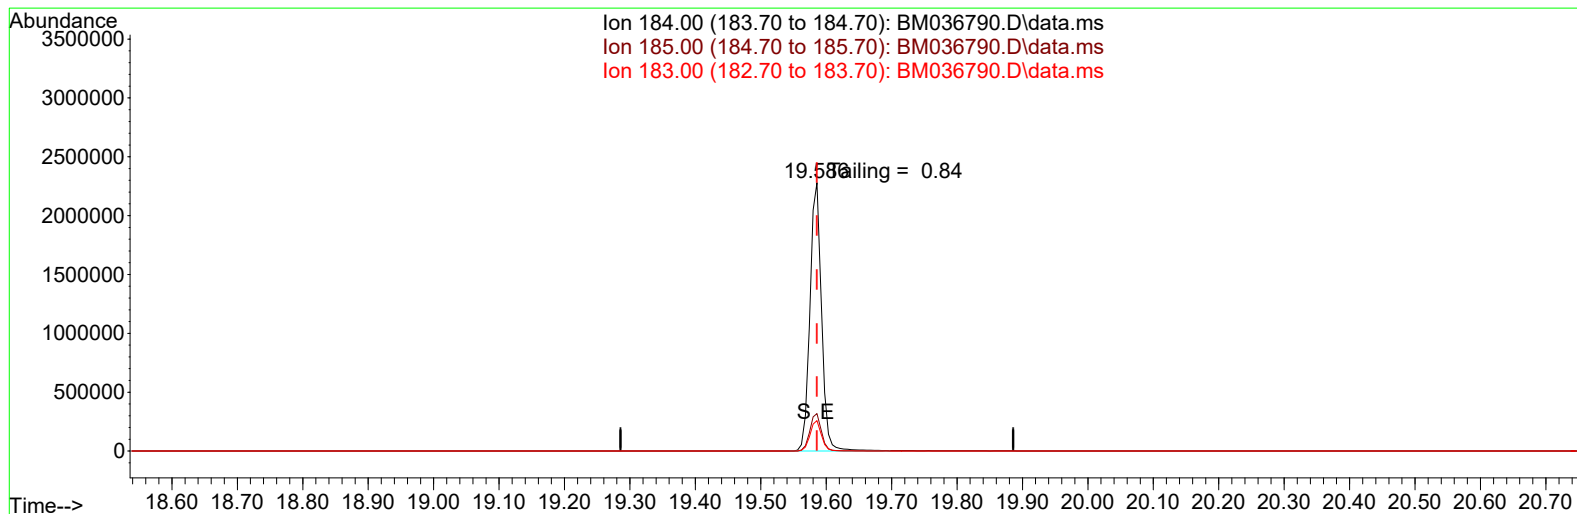

TIC: BM036790.D\data.ms

(77) Benzidine

19.586min (-0.000) 593665.90 ng

response 2820117

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.95
183.00	11.00	11.35
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/28/2022	BNA_M	<u>BM036790.D</u>
Compound Name	Response	Retention Time
DDT	1099587	20.815
DDD	9300	20.374
DDE	174	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9474	1109061	0.85

Instrument :
BNA_M
ClientSampleId :
DFTPP