

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092915\
 Data File : BM002787.D
 Acq On : 30 Sep 2015 18:21
 Operator : UM/IZ
 Sample : G3838-19
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E5MX5

Quant Time: Oct 01 07:07:32 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 01 07:01:42 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.70	152	119308	20.00	ng/ul	0.00
18) Naphthalene-d8	11.56	136	539582	20.00	ng/ul	0.00
36) Acenaphthene-d10	15.30	164	281876	20.00	ng/ul	0.00
62) Phenanthrene-d10	18.01	188	546303	20.00	ng/ul	0.00
78) Chrysene-d12	22.10	240	391252	20.00	ng/ul	0.00
86) Perylene-d12	24.70	264	376981	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.76	96	6751	2.63	ng/uL	0.00
5) Phenol-d5	7.82	99	164564	18.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.99	67	94433	18.57	ng/ul	0.00
9) 2-Chlorophenol-d4	8.22	132	155683	18.50	ng/ul	0.00
13) 4-Methylphenol-d8	9.40	113	128003	17.17	ng/ul	0.00
19) Nitrobenzene-d5	9.89	128	76218	18.52	ng/ul	0.00
22) 2-Nitrophenol-d4	10.63	143	81287	18.90	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	11.17	165	141099	18.59	ng/ul	0.00
29) 4-Chloroaniline-d4	11.69	131	91859	10.05	ng/ul	0.00
44) Dimethylphthalate-d6	14.67	166	419229	19.77	ng/ul	0.00
47) Acenaphthylene-d8	15.00	160	549825	19.43	ng/ul	0.00
52) 4-Nitrophenol-d4	15.47	143	48118	12.78	ng/ul	0.00
58) Fluorene-d10	16.27	176	370338	19.39	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	16.39	200	29814	11.19	ng/ul	0.00
71) Anthracene-d10	18.11	188	515592	19.78	ng/ul	0.00
79) Pyrene-d10	20.34	212	434031	23.77	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.53	264	381616	19.79	ng/ul	0.00

Target Compounds


						Qvalue
2) 1,4-Dioxane	3.45	88	17531	6.17	ng/uL#	1
4) Benzaldehyde	7.81	77	7766	1.53	ng/ul#	67
28) Naphthalene	11.61	128	90300	3.28	ng/ul	99
32) Caprolactam	12.48	113	3033	1.25	ng/ul#	64
34) 2-Methylnaphthalene	13.17	142	130881	6.83	ng/ul	98
35) 1-Methylnaphthalene	13.39	142	83618	4.49	ng/ul	99
45) Dimethylphthalate	14.72	163	222865	10.34	ng/ul	100
54) Dibenzofuran	15.69	168	46081	1.72	ng/ul	96
70) Phenanthrene	18.05	178	348079	11.01	ng/ul	99
72) Anthracene	18.14	178	79241	2.46	ng/ul	97
76) Di-n-butylphthalate	18.89	149	36374	1.01	ng/ul#	91
77) Fluoranthene	20.01	202	591481	18.13	ng/ul	99
80) Pyrene	20.37	202	591759	23.81	ng/ul	99
83) Benzo(a)anthracene	22.08	228	317397	13.65	ng/ul	99
85) Chrysene	22.08	228	315996	14.40	ng/ul	97
88) Benzo(b)fluoranthene	23.90	252	395481	17.46	ng/ul#	96
91) Benzo(a)pyrene	24.58	252	279647	12.86	ng/ul	96
92) Indeno(1,2,3-cd)pyrene	27.43	276	181316	7.14	ng/ul	94
93) Dibenzo(a,h)anthracene	27.41	278	59586	2.78	ng/ul#	79
94) Benzo(g,h,i)perylene	28.29	276	183506	8.59	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092915\
Data File : BM002787.D
Acq On : 30 Sep 2015 18:21
Operator : UM/IZ
Sample : G3838-19
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5MX5

Quant Time: Oct 01 07:07:32 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092915.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 01 07:01:42 2015
Response via : Initial Calibration

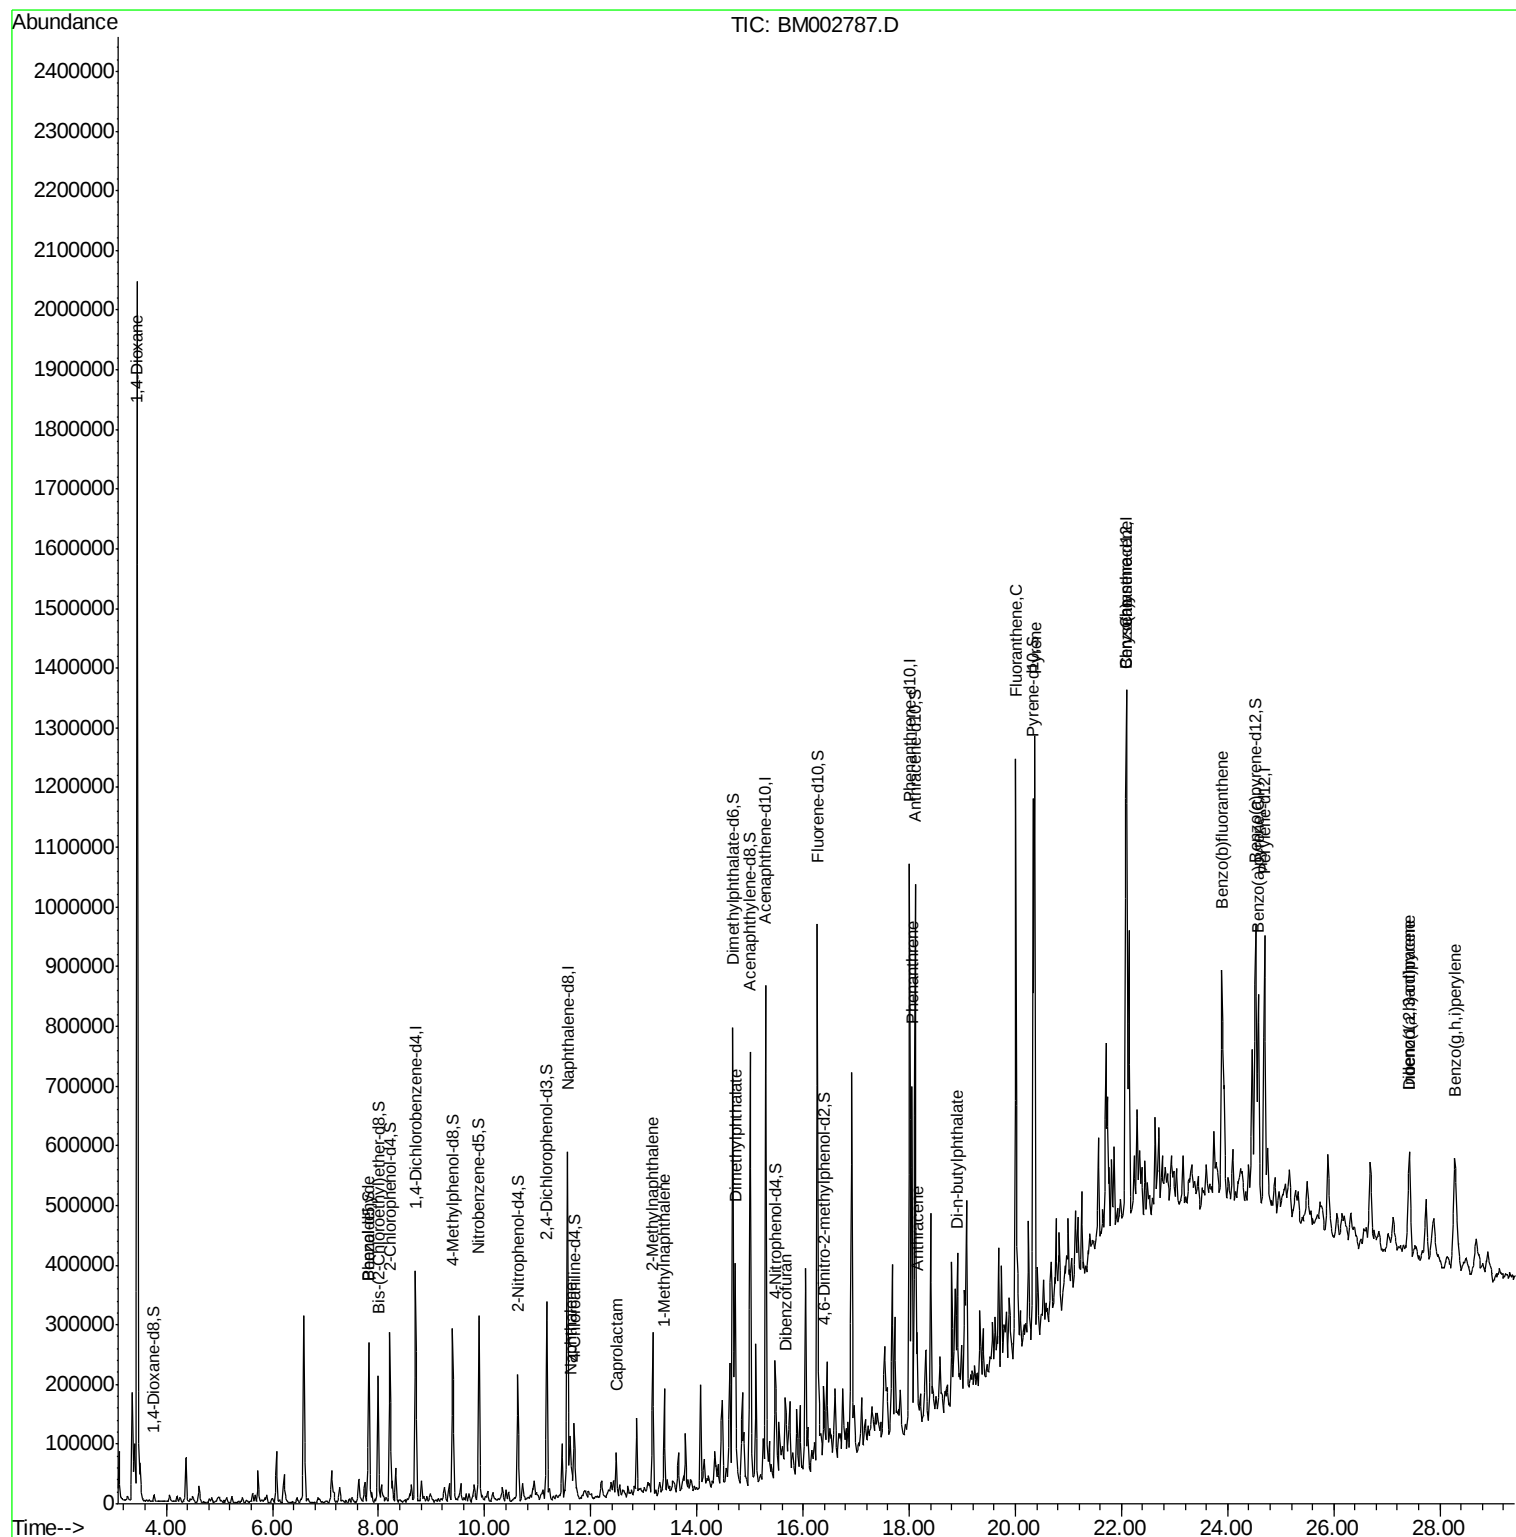



#2

1,4-Dioxane

Concen: 6.17 ng/uL

RT: 3.45 min Scan# 62

Delta R.T. -0.35 min

Lab File: BM002787.D

Acq: 30 Sep 2015 18:21

Instrument :

BNA_M

ClientSampleId :

E5MX5


Tgt Ion: 88 Resp: 17531

Ion Ratio Lower Upper

88 100

43 2451.4 26.2 39.4#




58 23.4 58.5 87.7#

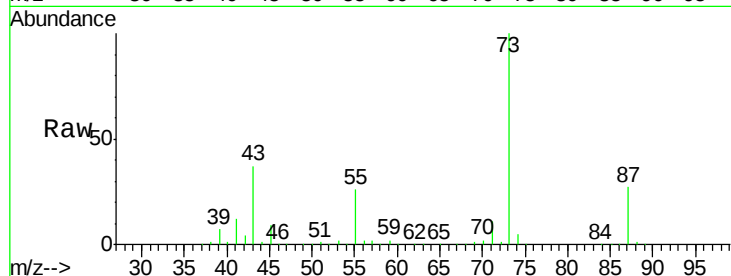

Abundance Ion 88.00 (87.70 to 88.70): BM002787.D (-37) (-)

Ion 43.00 (42.70 to 43.70): BM002787.D (-37) (-)

Ion 58.00 (57.70 to 58.70): BM002787.D (-37) (-)

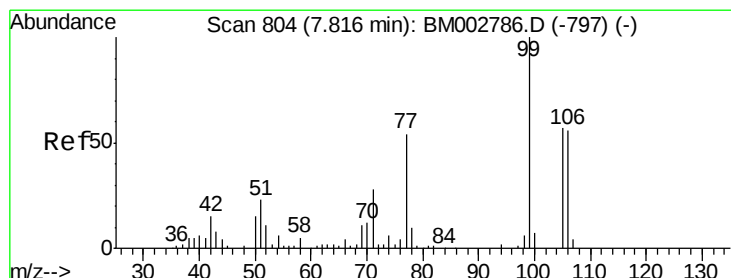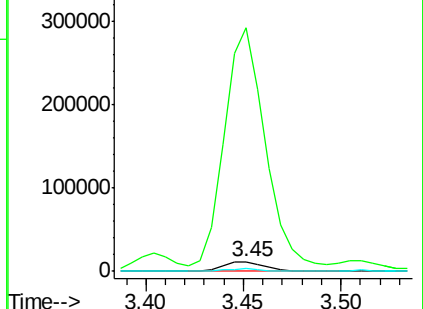

#4

Benzaldehyde

Concen: 1.53 ng/uL

RT: 7.81 min Scan# 803

Delta R.T. -0.01 min

Lab File: BM002787.D

Acq: 30 Sep 2015 18:21


Tgt Ion: 77 Resp: 7766

Ion Ratio Lower Upper

77 100

105 164.5 86.2 129.2#



106 93.2 82.5 123.7

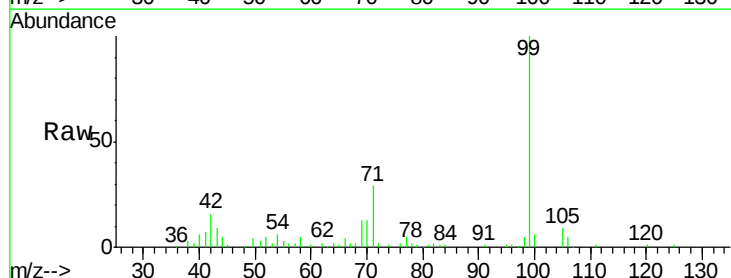


Abundance Ion 77.00 (76.70 to 77.70): BM002787.D (-770) (-)

Ion 105.00 (104.70 to 105.70): BM002787.D (-770) (-)

Ion 106.00 (105.70 to 106.70): BM002787.D (-770) (-)

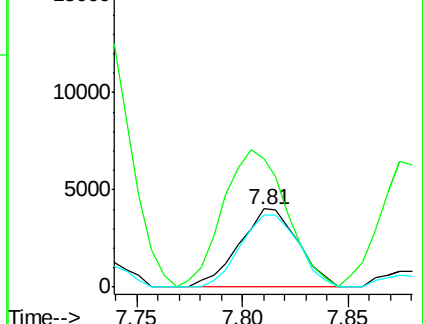

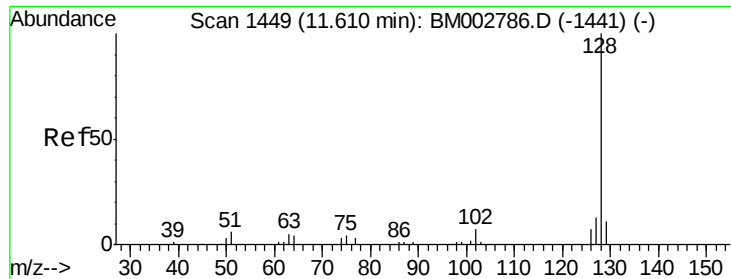

#28

Naphthalene

Concen: 3.28 ng/ul

RT: 11.61 min Scan# 1449

Delta R.T. -0.00 min

Lab File: BM002787.D

Acq: 30 Sep 2015 18:21

Instrument :

BNA_M

ClientSampleId :

E5MX5


Tgt Ion:128 Resp: 90300

Ion Ratio Lower Upper

128 100

129 10.8 8.7 13.1




127 12.9 9.9 14.9

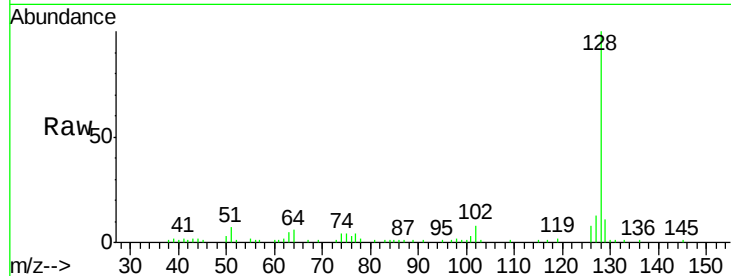

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

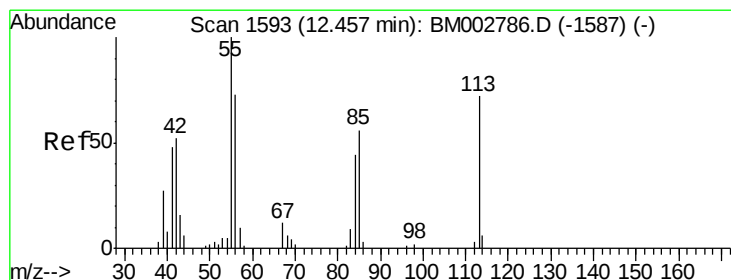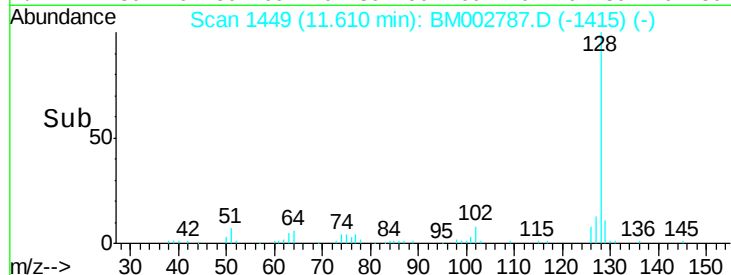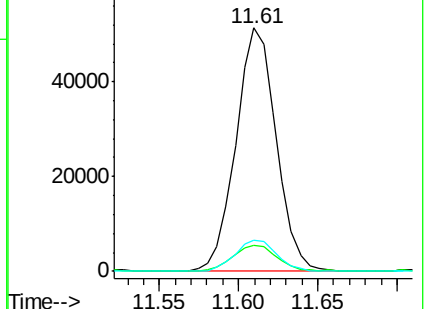

#32

Caprolactam

Concen: 1.25 ng/ul

RT: 12.48 min Scan# 1597

Delta R.T. 0.02 min

Lab File: BM002787.D

Acq: 30 Sep 2015 18:21


Tgt Ion:113 Resp: 3033

Ion Ratio Lower Upper

113 100

55 166.1 118.3 177.5



56 178.6 87.4 131.0#

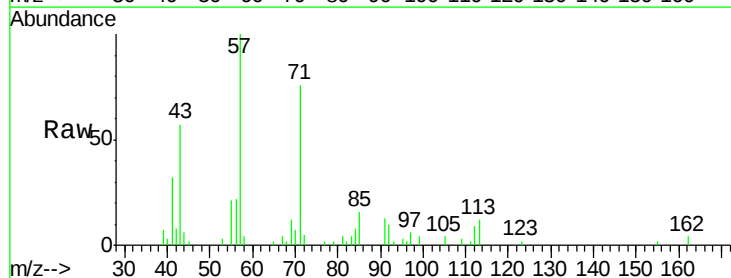


Abundance Ion 113.00 (112.70 to 113.70): E

Ion 55.00 (54.70 to 55.70): BM0

Ion 56.00 (55.70 to 56.70): BM0




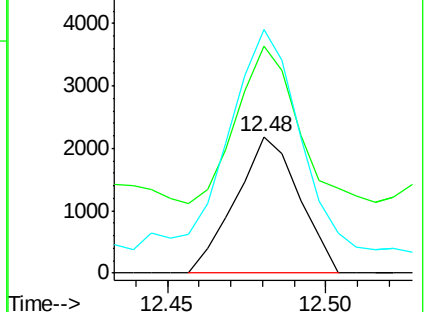


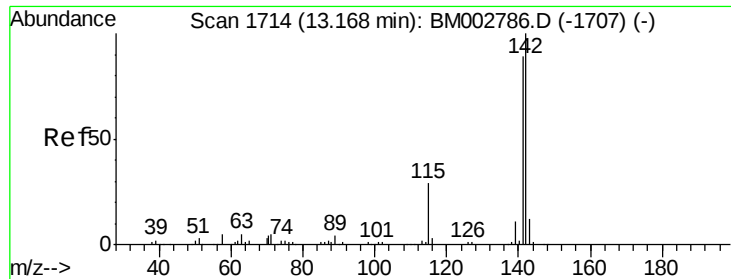

#34
 2-Methylnaphthalene
 Concen: 6.83 ng/ul
 RT: 13.17 min Scan# 1714
 Delta R.T. -0.00 min
 Lab File: BM002787.D
 Acq: 30 Sep 2015 18:21




Instrument :
 BNA_M
 ClientSampleId :
 E5MX5


Tgt Ion:142 Resp: 130881
 Ion Ratio Lower Upper
 142 100
 141 87.5 71.2 106.8

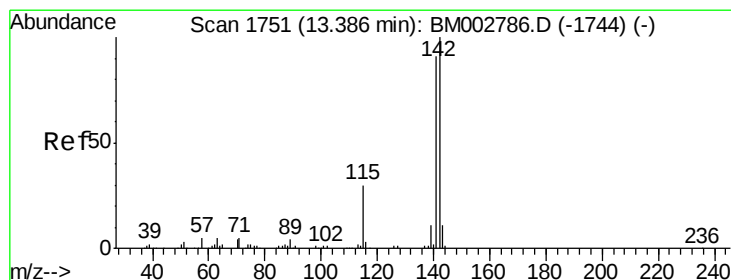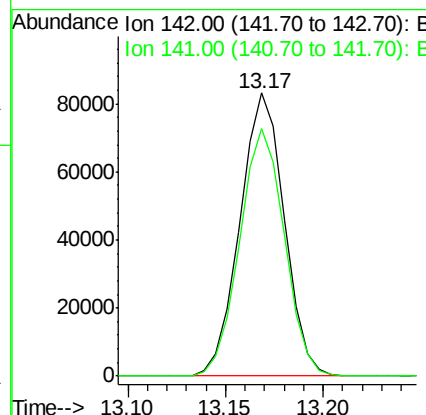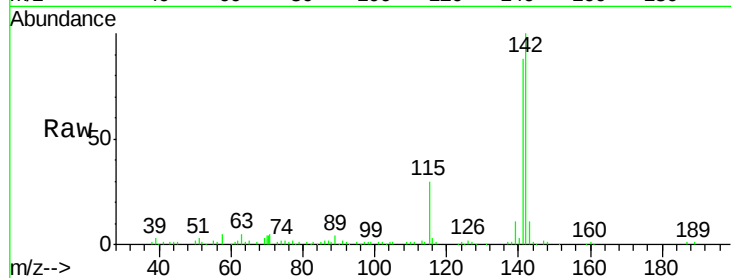

#35
 1-Methylnaphthalene
 Concen: 4.49 ng/ul
 RT: 13.39 min Scan# 1751
 Delta R.T. -0.00 min
 Lab File: BM002787.D
 Acq: 30 Sep 2015 18:21

Tgt Ion:142 Resp: 83618
 Ion Ratio Lower Upper
 142 100
 141 92.2 74.4 111.6
 116 3.6 2.6 4.0

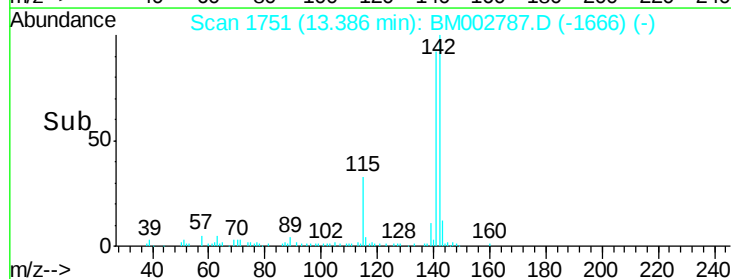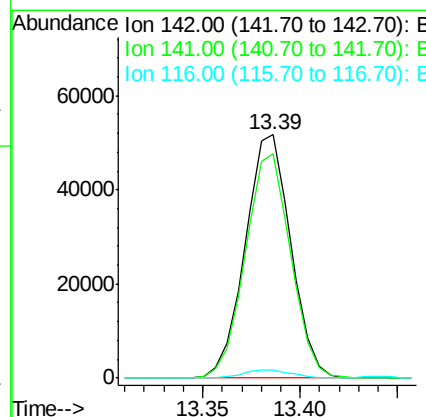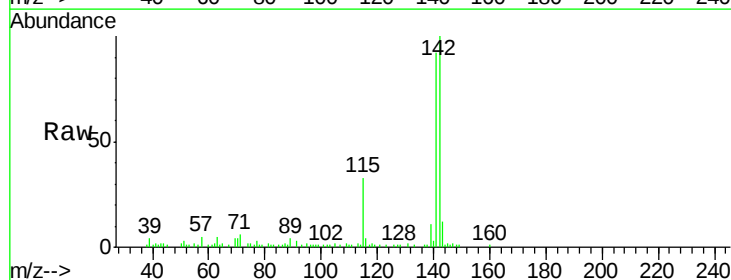

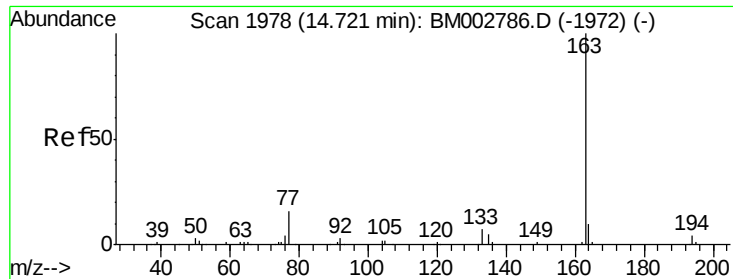

#45

Dimethylphthalate

Concen: 10.34 ng/ul

RT: 14.72 min Scan# 1978

Delta R.T. 0.00 min

Lab File: BM002787.D

Acq: 30 Sep 2015 18:21


Instrument :

BNA_M

ClientSampleId :

E5MX5




Tgt Ion:	163	Resp:	222865
Ion Ratio	Lower	Upper	
163	100		
194	4.0	3.2	4.8
164	10.3	8.1	12.1

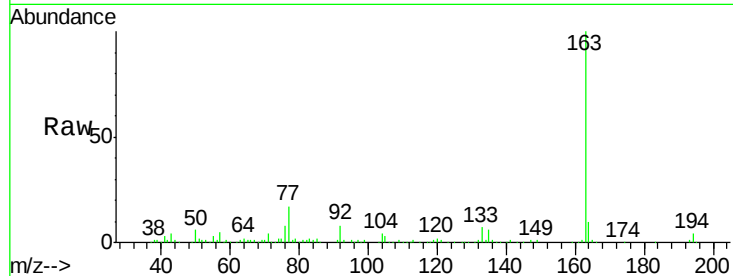

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

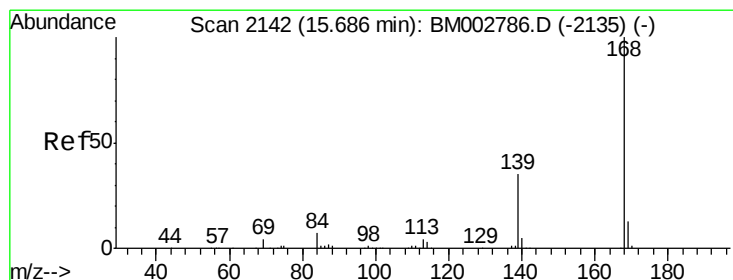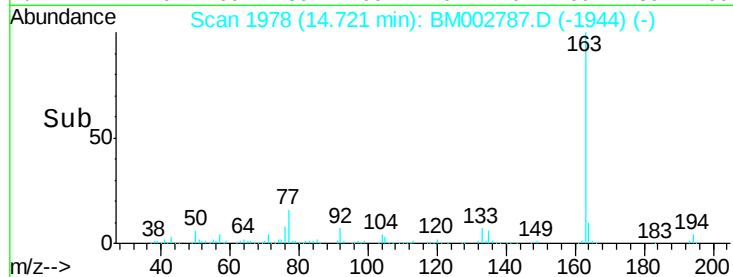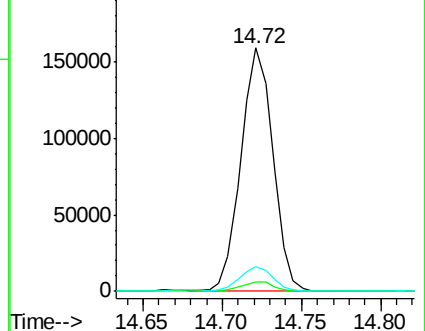

#54

Dibenzofuran

Concen: 1.72 ng/ul


RT: 15.69 min Scan# 2142

Delta R.T. -0.00 min

Lab File: BM002787.D



Acq: 30 Sep 2015 18:21


Tgt Ion:	168	Resp:	46081
Ion Ratio	Lower	Upper	
168	100		
139	38.5	28.7	43.1

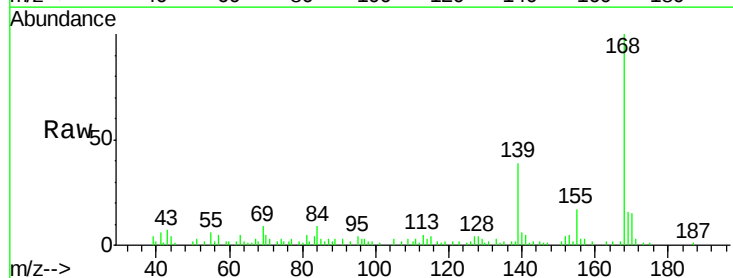

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

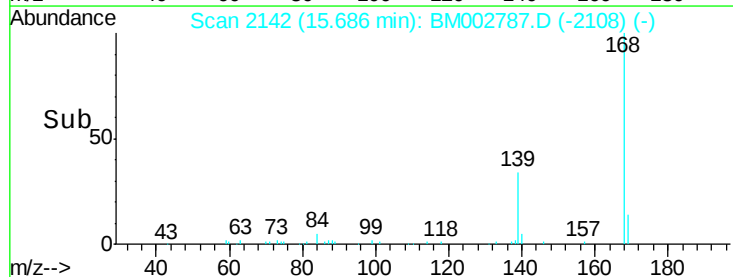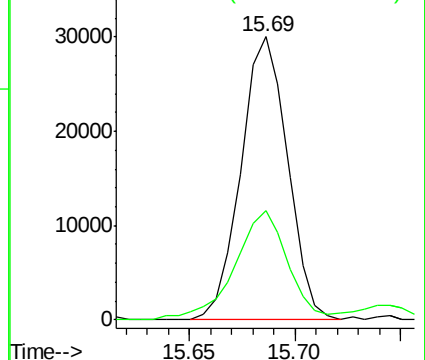

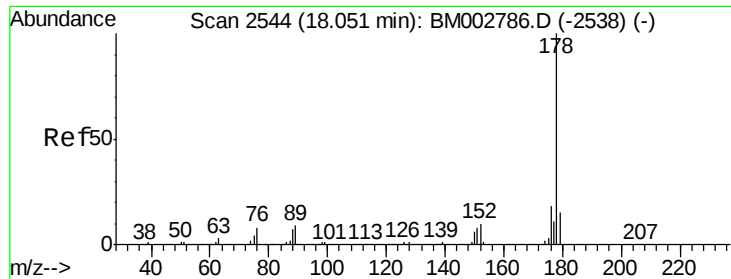

#70

Phenanthrene

Concen: 11.01 ng/ul

RT: 18.05 min Scan# 2544

Delta R.T. 0.00 min

Lab File: BM002787.D

Acq: 30 Sep 2015 18:21

Instrument :

BNA_M

ClientSampleId :

E5MX5


Tgt Ion:178 Resp: 348079

Ion Ratio Lower Upper

178 100

179 15.6 12.0 18.0




176 18.7 14.6 22.0

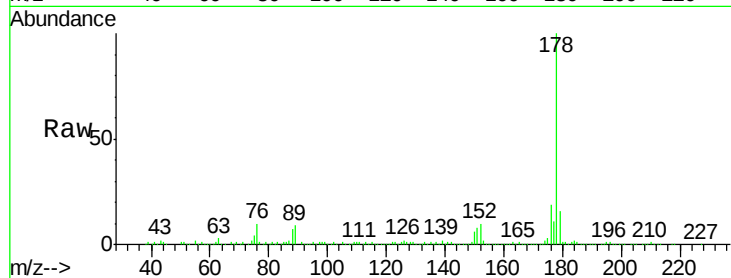

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

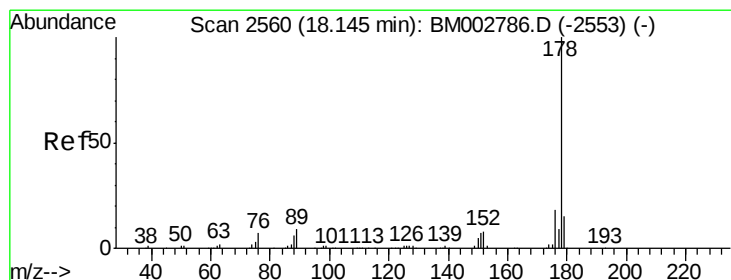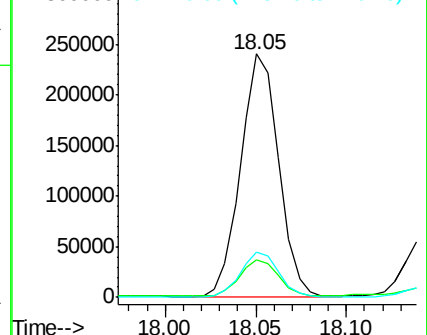

#72

Anthracene

Concen: 2.46 ng/ul

RT: 18.14 min Scan# 2560

Delta R.T. -0.00 min

Lab File: BM002787.D

Acq: 30 Sep 2015 18:21


Tgt Ion:178 Resp: 79241

Ion Ratio Lower Upper

178 100

179 17.2 11.9 17.9



176 17.9 14.4 21.6

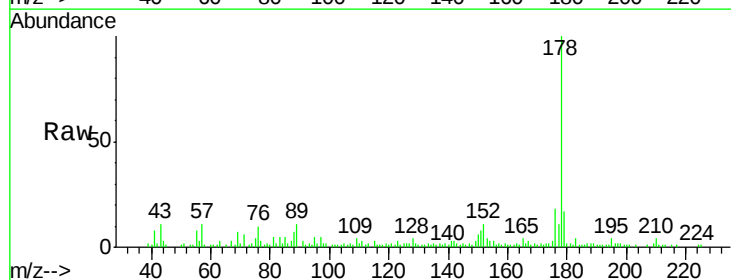


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E




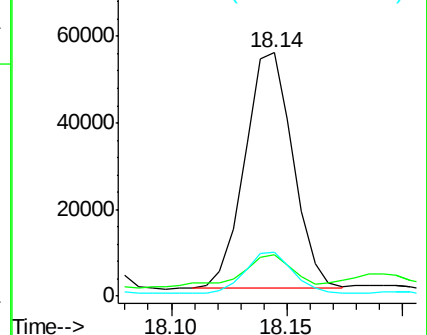


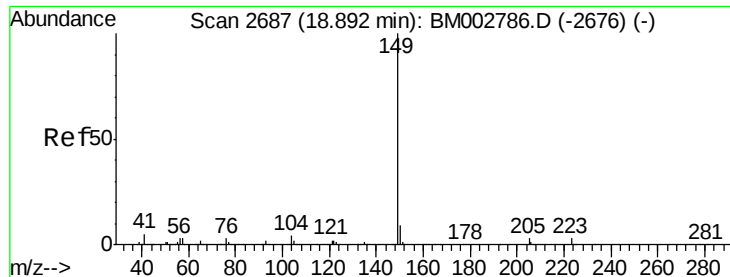

#76
Di-n-butylphthalate
Concen: 1.01 ng/ul
RT: 18.89 min Scan# 2687
Delta R.T. 0.00 min
Lab File: BM002787.D
Acq: 30 Sep 2015 18:21




Instrument :
BNA_M
ClientSampleId :
E5MX5


Tgt Ion:149 Resp: 36374
Ion Ratio Lower Upper
149 100
150 12.6 7.1 10.7#
104 6.7 3.3 4.9#

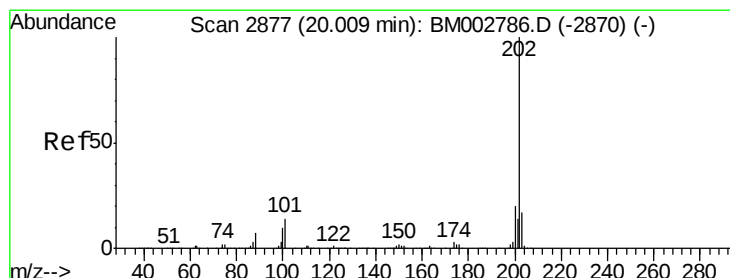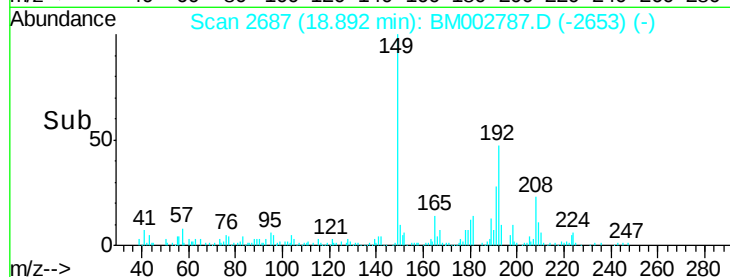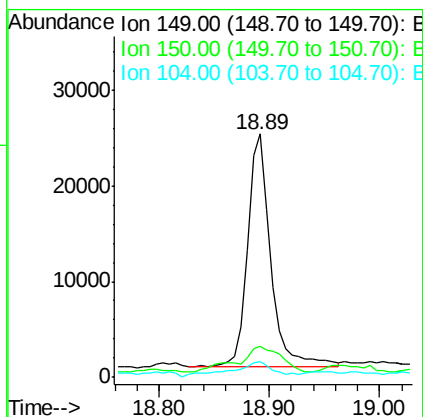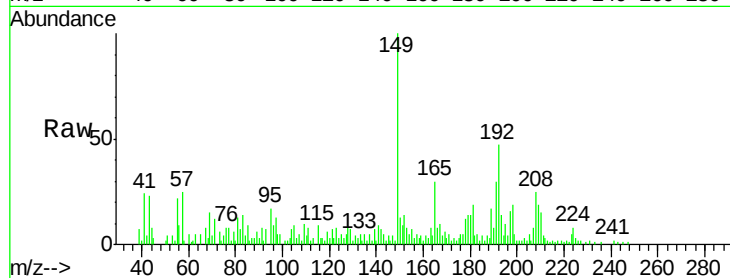

#77
Fluoranthene
Concen: 18.13 ng/ul
RT: 20.01 min Scan# 2877
Delta R.T. -0.00 min
Lab File: BM002787.D
Acq: 30 Sep 2015 18:21

Tgt Ion:202 Resp: 591481
Ion Ratio Lower Upper
202 100
101 13.6 11.0 16.4
100 10.0 8.3 12.5

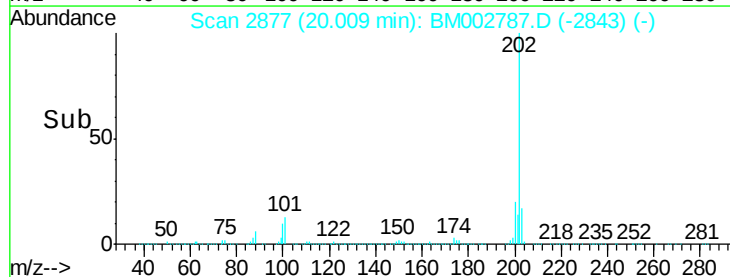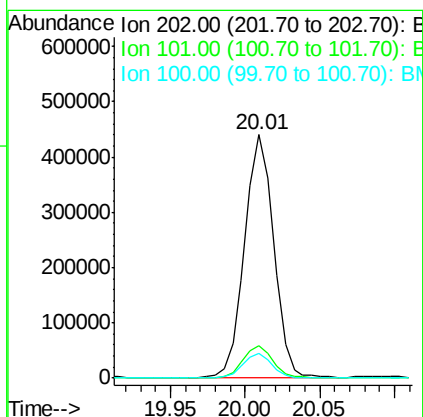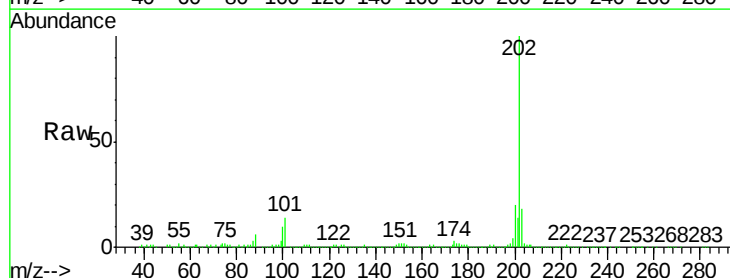

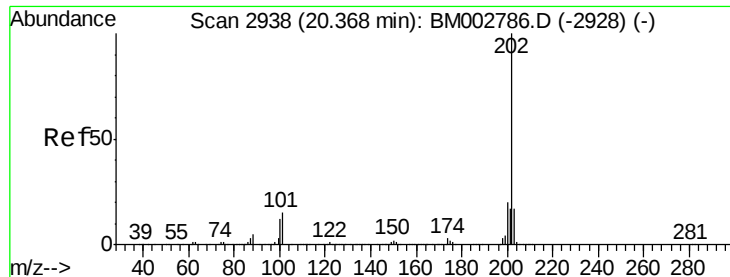

#80

Pyrene

Concen: 23.81 ng/ul

RT: 20.37 min Scan# 2938

Delta R.T. -0.00 min

Lab File: BM002787.D

Acq: 30 Sep 2015 18:21





Instrument :

BNA_M

ClientSampleId :

E5MX5

Tgt Ion:	202	Resp:	591759
Ion	Ratio	Lower	Upper
202	100		
101	15.3	12.1	18.1
100	12.5	10.2	15.4

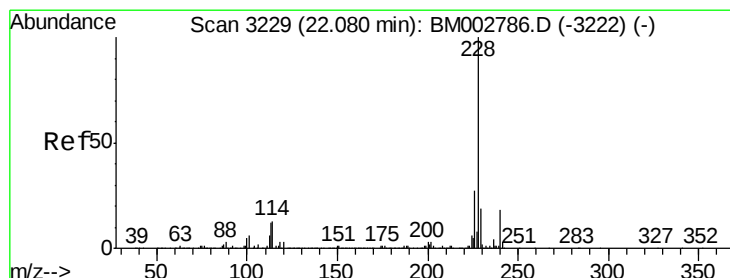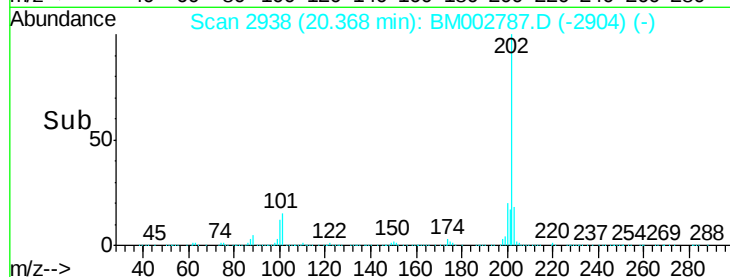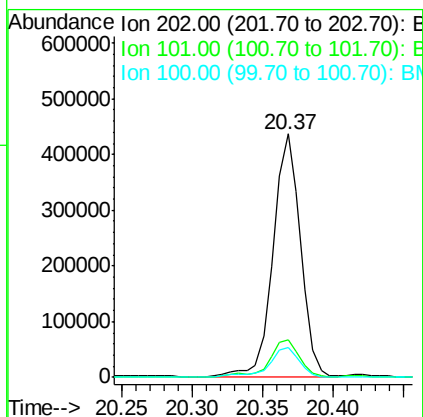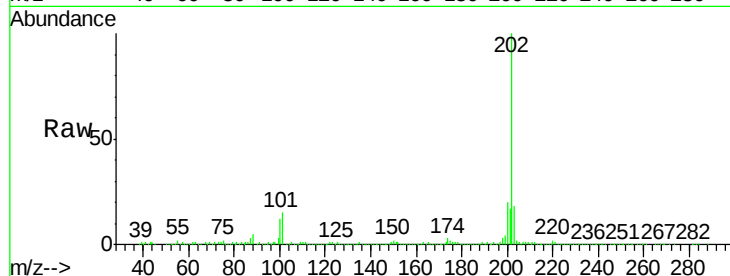

#83

Benzo(a)anthracene

Concen: 13.65 ng/ul




RT: 22.08 min Scan# 3229


Delta R.T. 0.00 min

Lab File: BM002787.D

Acq: 30 Sep 2015 18:21

Tgt Ion:	228	Resp:	317397
Ion	Ratio	Lower	Upper
228	100		
229	20.9	16.1	24.1
226	26.2	20.9	31.3

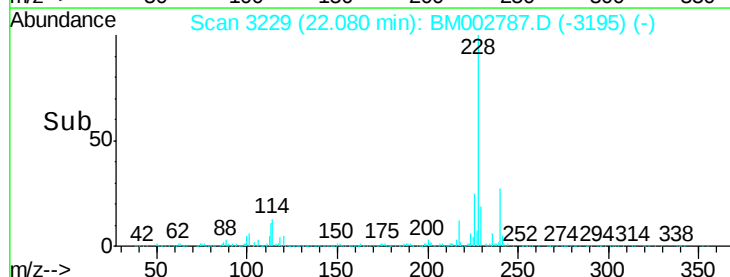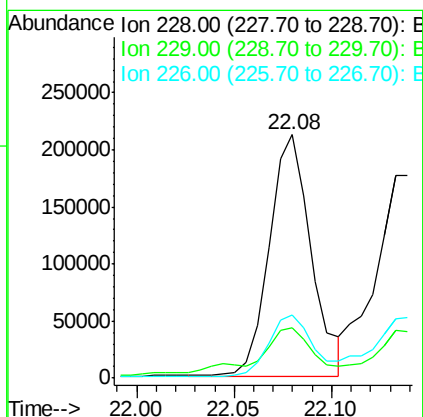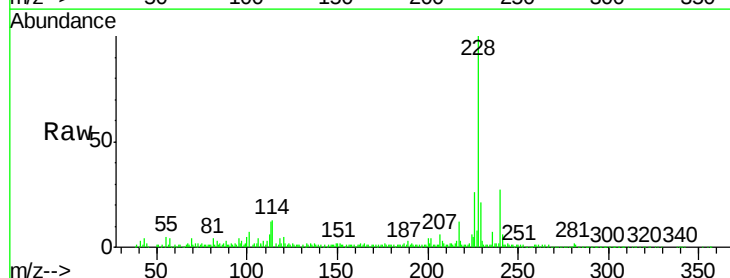



#85

Chrysene

Concen: 14.40 ng/ul

RT: 22.08 min Scan# 3229

Delta R.T. -0.05 min

Lab File: BM002787.D

Acq: 30 Sep 2015 18:21

Instrument :

BNA_M

ClientSampled :

E5MX5


Tgt Ion:228 Resp: 315996

Ion Ratio Lower Upper

228 100

226 26.2 22.4 33.6




229 20.9 15.4 23.2

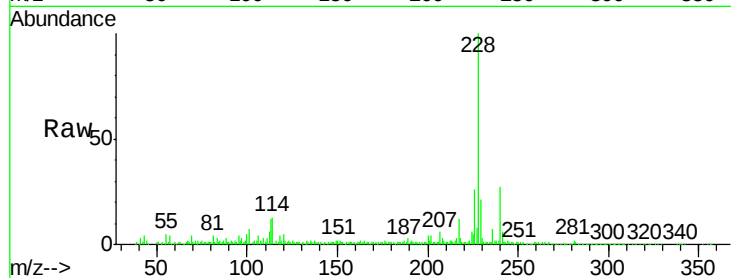

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

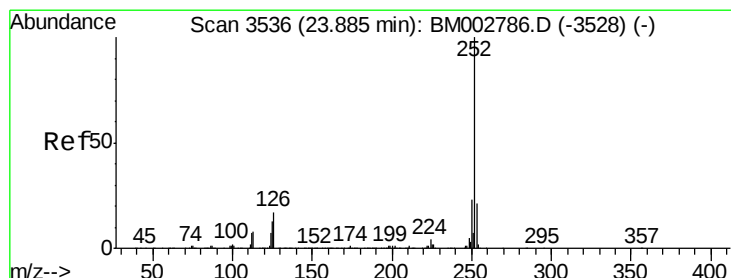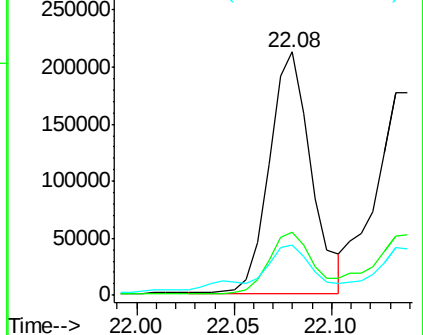

#88

Benzo(b)fluoranthene

Concen: 17.46 ng/ul

RT: 23.90 min Scan# 3538

Delta R.T. 0.01 min

Lab File: BM002787.D

Acq: 30 Sep 2015 18:21


Tgt Ion:252 Resp: 395481

Ion Ratio Lower Upper

252 100

253 23.4 17.6 26.4



125 16.0 10.6 15.8#

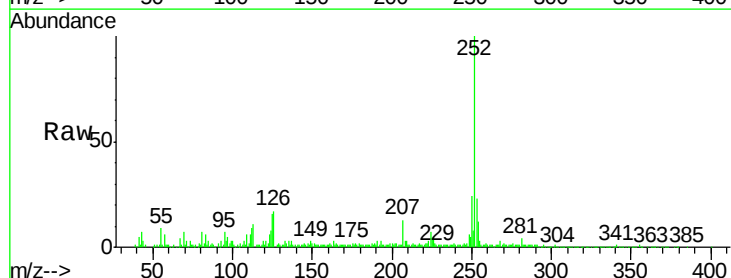


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

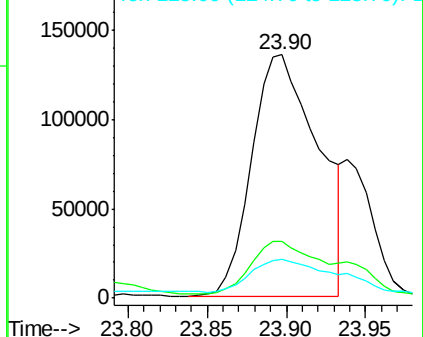

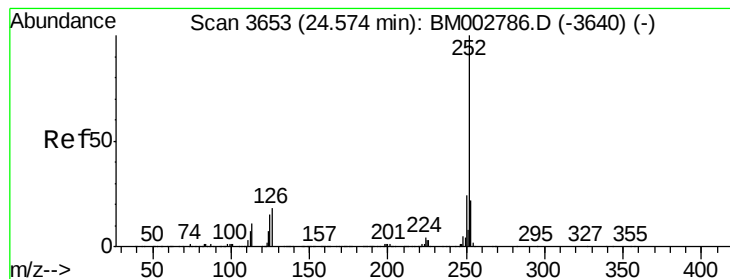

#91

Benzo(a)pyrene

Concen: 12.86 ng/ul

RT: 24.58 min Scan# 3654

Delta R.T. 0.01 min

Lab File: BM002787.D

Acq: 30 Sep 2015 18:21


Instrument :

BNA_M

ClientSampleId :

E5MX5




Tgt Ion:	252	Resp:	279647
Ion	Ratio	Lower	Upper
252	100		
253	23.4	17.4	26.0
125	16.4	11.4	17.2

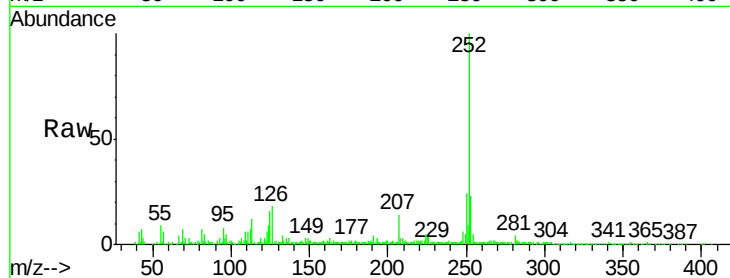

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

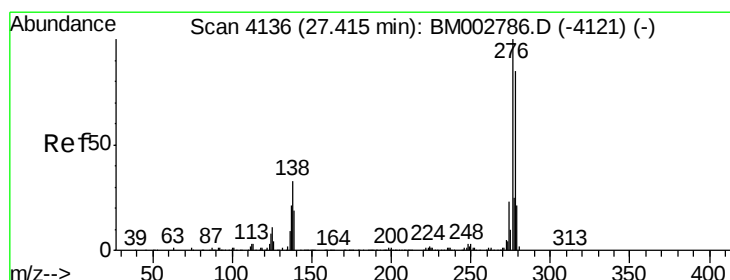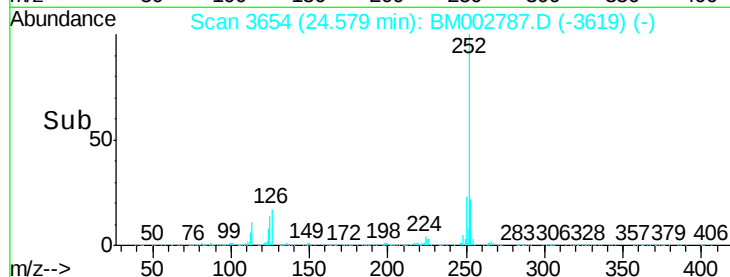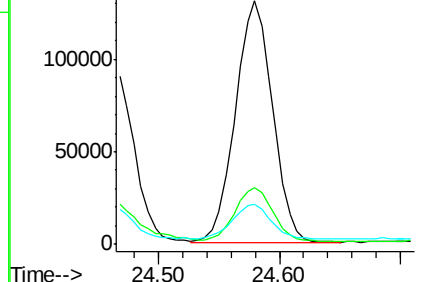

#92

Indeno(1,2,3-cd)pyrene

Concen: 7.14 ng/ul


RT: 27.43 min Scan# 4138

Delta R.T. 0.01 min

Lab File: BM002787.D

Acq: 30 Sep 2015 18:21



Tgt Ion:	276	Resp:	181316
Ion	Ratio	Lower	Upper
276	100		
138	28.5	27.7	41.5
277	25.7	20.2	30.4

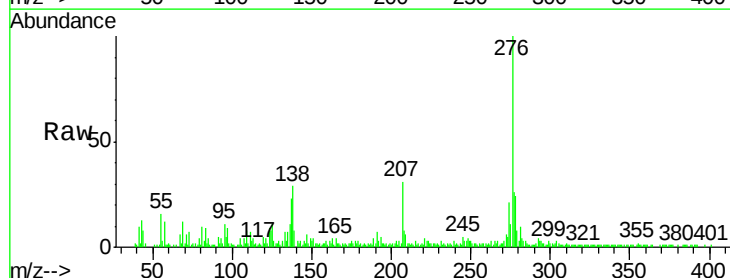


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

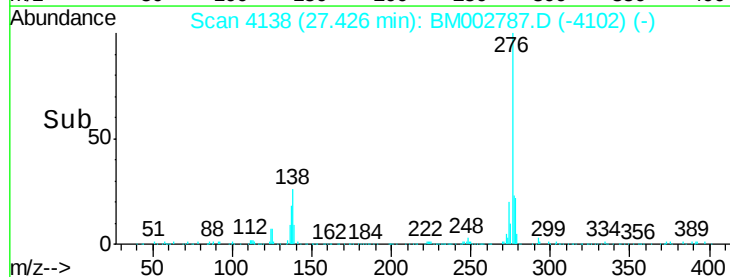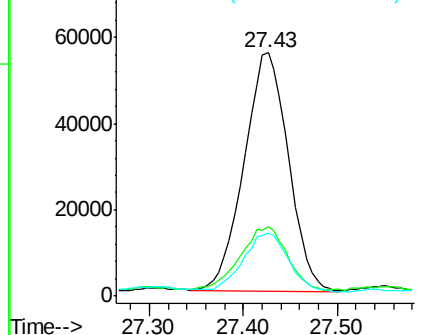

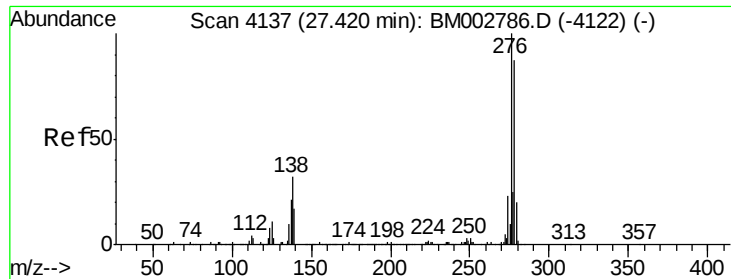

#93

Dibenzo(a,h)anthracene

Concen: 2.78 ng/ul

RT: 27.41 min Scan# 4136

Delta R.T. -0.01 min

Lab File: BM002787.D

Acq: 30 Sep 2015 18:21

Instrument :

BNA_M

ClientSampleId :

E5MX5





Tgt Ion:278 Resp: 59586

Ion Ratio Lower Upper

278 100

139 32.9 17.0 25.6#

279 32.7 19.0 28.6#

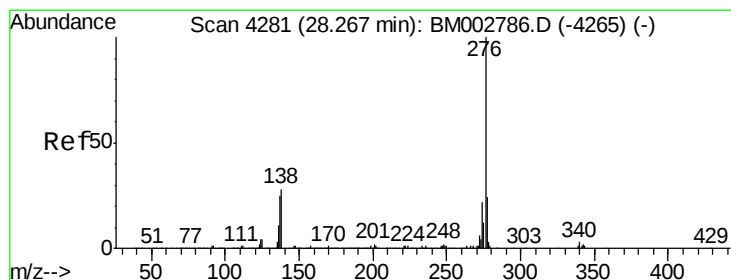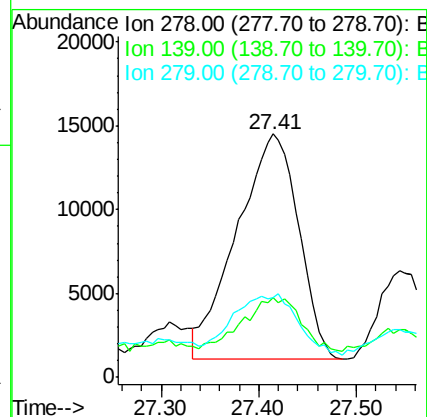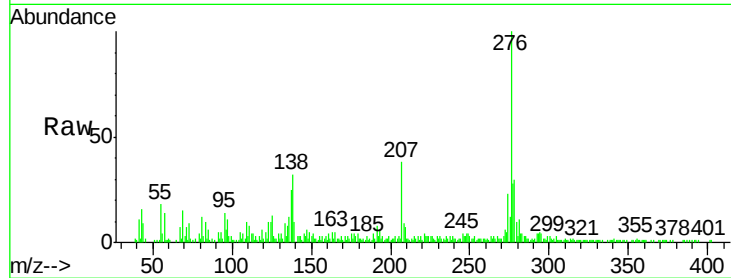

#94

Benzo(g,h,i)perylene

Concen: 8.59 ng/ul

RT: 28.29 min Scan# 4284

Delta R.T. 0.02 min

Lab File: BM002787.D

Acq: 30 Sep 2015 18:21

Tgt Ion:276 Resp: 183506

Ion Ratio Lower Upper

276 100

138 29.1 21.8 32.8

277 24.4 18.9 28.3

