


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092915\
Data File : BM002797.D
Acq On : 01 Oct 2015 00:25
Operator : UM/IZ
Sample : G3798-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9G71

Quant Time: Oct 01 08:42:23 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092915.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 01 07:01:42 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
10/1/2015 4:44:16 PM

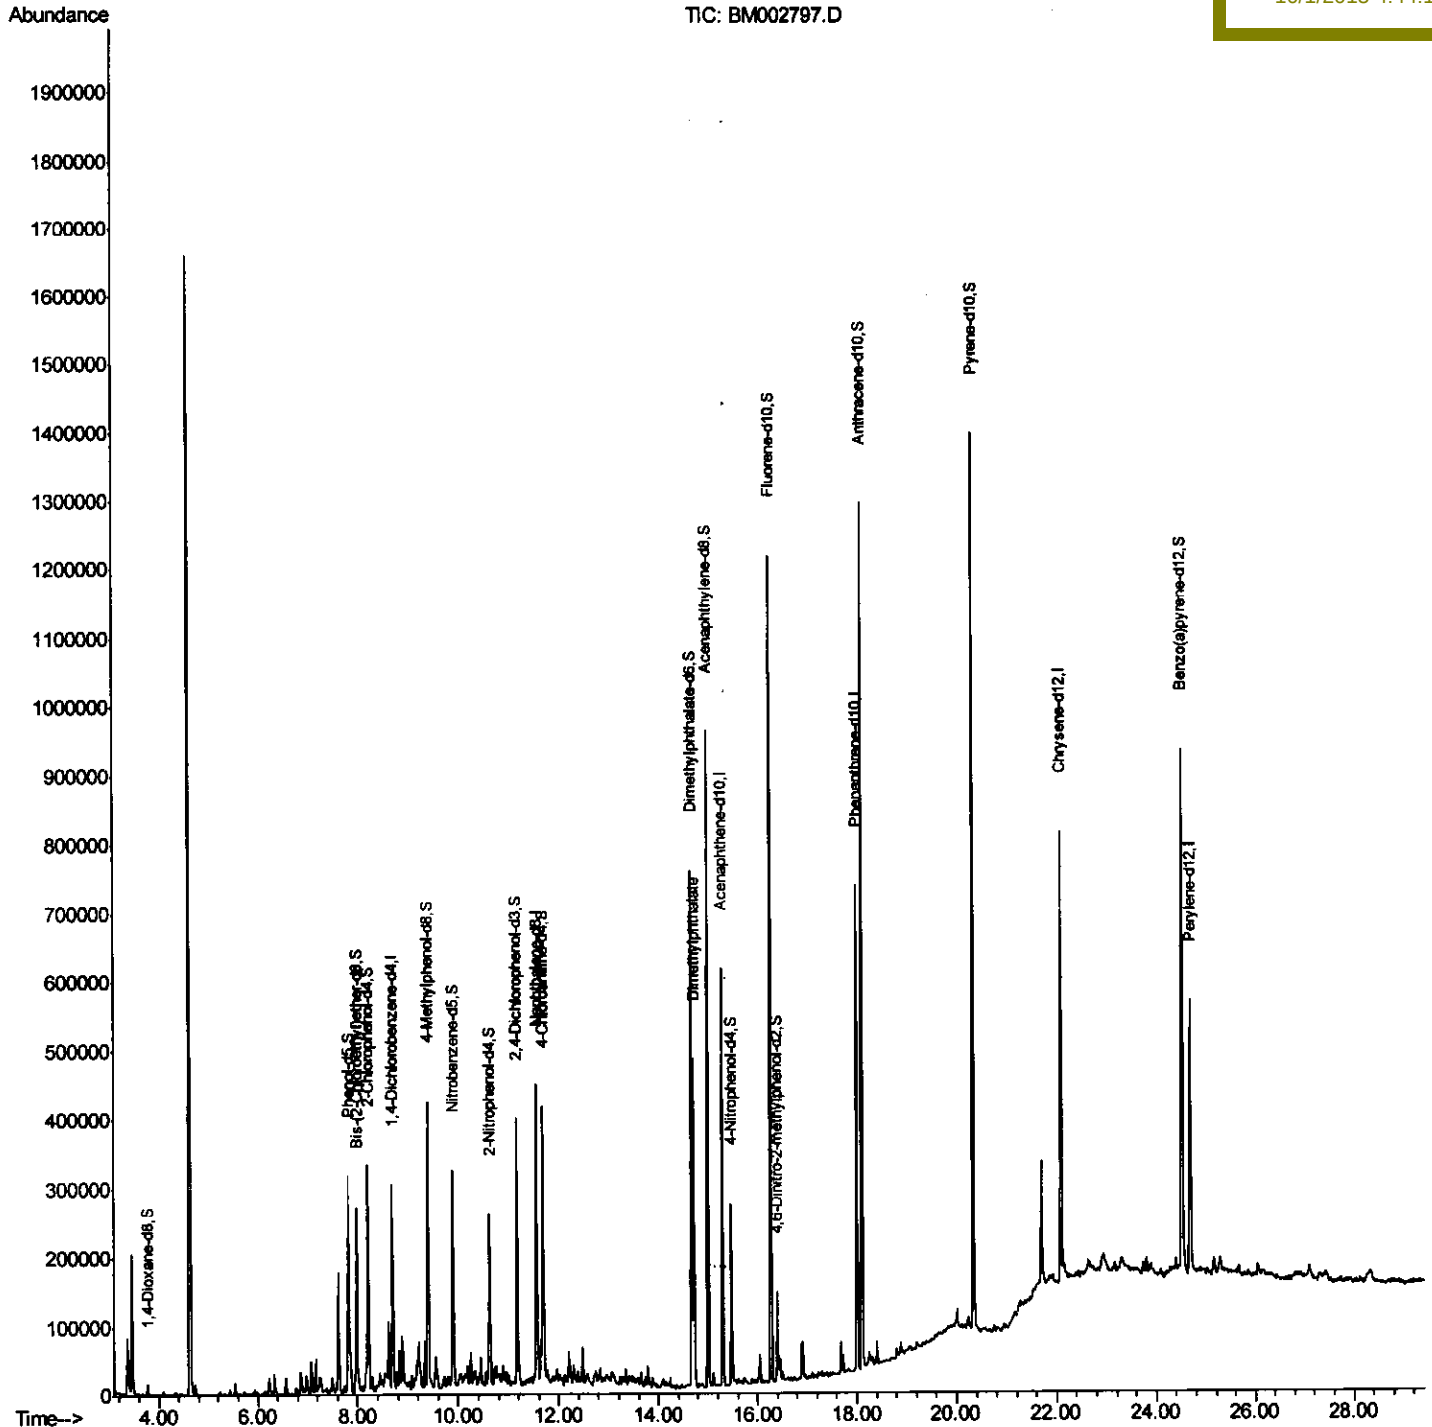

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092915\
 Data File : BM002797.D
 Acq On : 01 Oct 2015 00:25
 Operator : UM/IZ
 Sample : G3798-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9G71

Quant Time: Oct 01 07:10:26 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 01 07:01:42 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/1/2015 4:44:16 PM

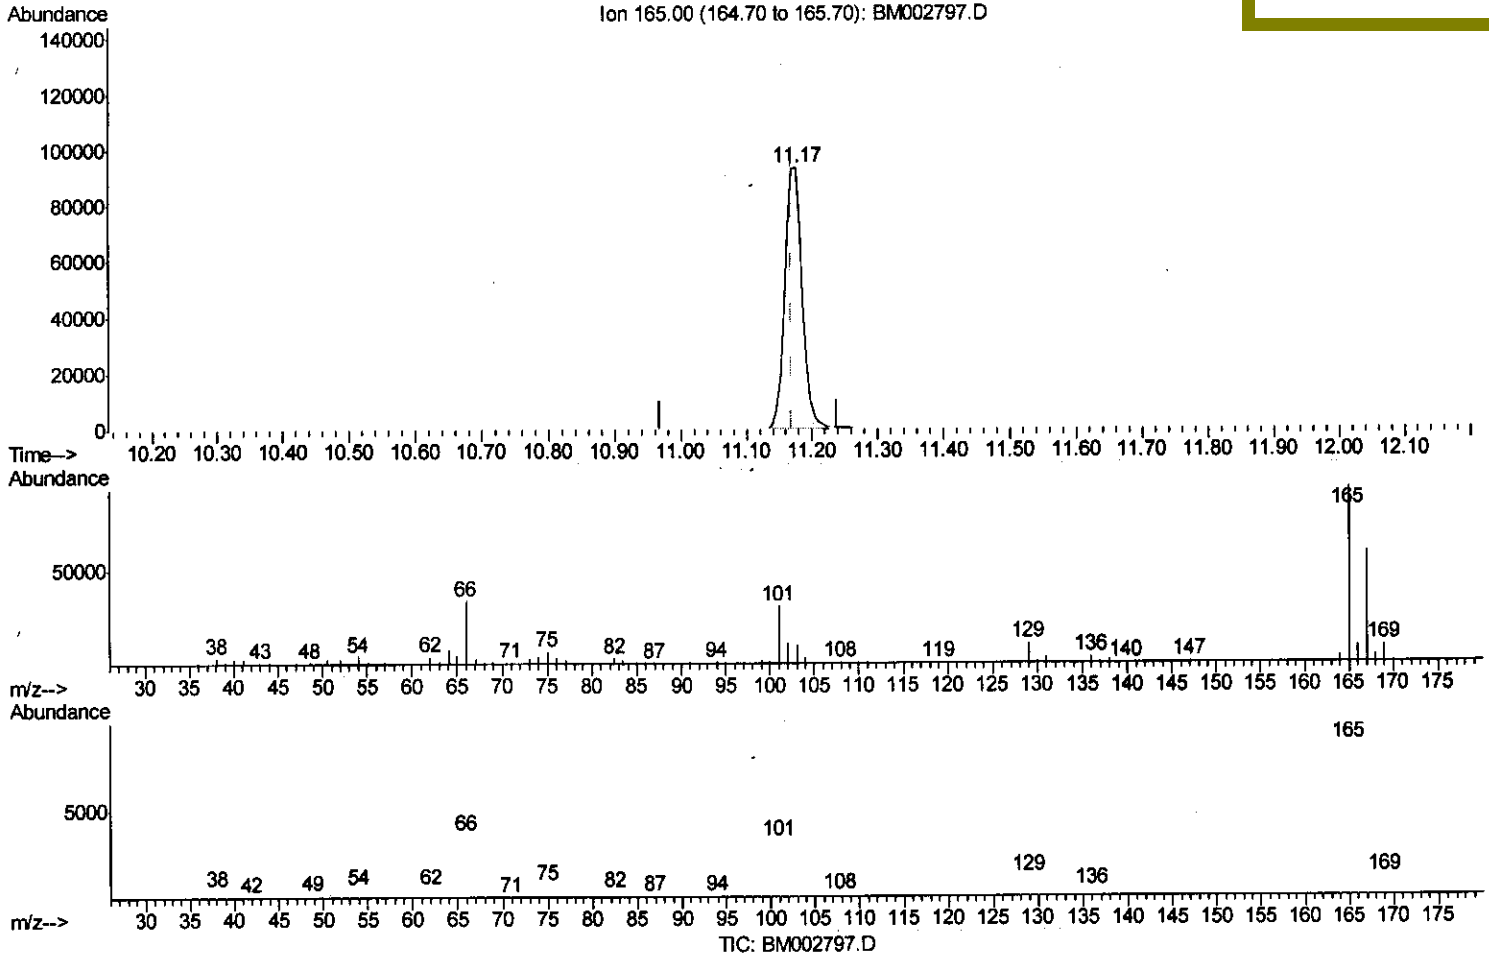

(26) 2,4-Dichlorophenol-d3 (S)

11.175min (+0.006) 30.47ng/ul

response 170750

Ion	Exp%	Act%
165.00	100	100
167.00	61.90	63.26
101.00	32.10	32.85
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092915\
 Data File : BM002797.D
 Acq On : 01 Oct 2015 00:25
 Operator : UM/IZ
 Sample : G3798-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9G71

Quant Time: Oct 01 07:10:26 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 01 07:01:42 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/1/2015 4:44:16 PM

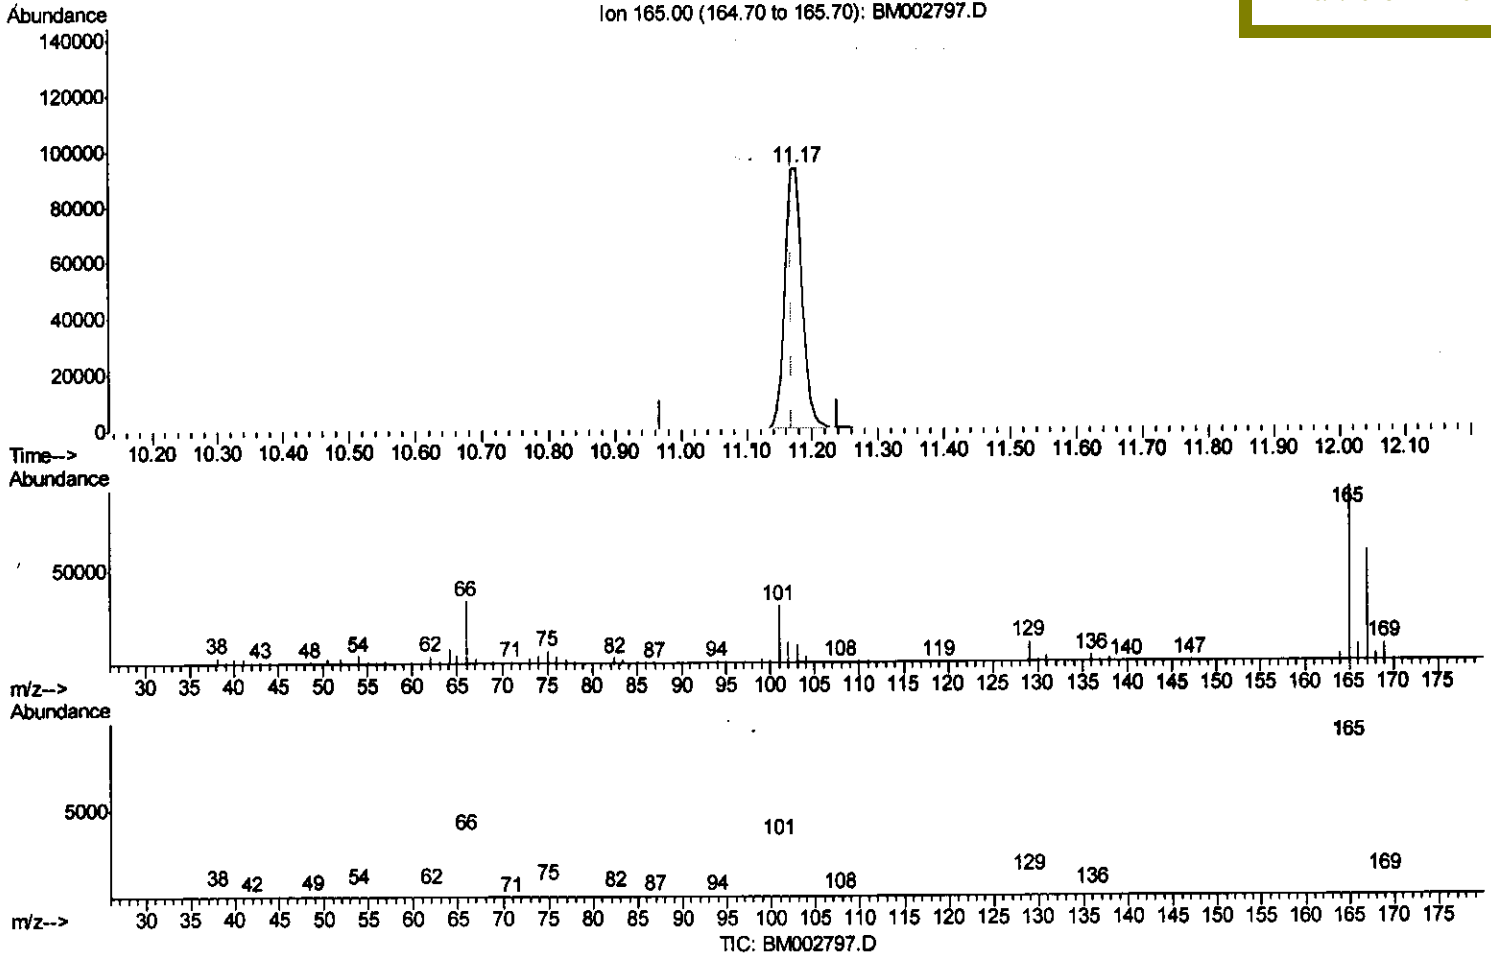

(26) 2,4-Dichlorophenol-d3 (S)

11.175min (+0.006) 30.70ng/ul m U.M
 response 172033 10/8/15

Ion	Exp%	Act%
165.00	100	100
167.00	61.90	63.26
101.00	32.10	32.85
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092915\
 Data File : BM002797.D
 Acq On : 01 Oct 2015 00:25
 Operator : UM/IZ
 Sample : G3798-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9G71

Quant Time: Oct 01 08:42:23 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 01 07:01:42 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/1/2015 4:44:16 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.70	152	89392	20.00	ng/ul	0.00
18) Naphthalene-d8	11.56	136	398465	20.00	ng/ul	0.00
36) Acenaphthene-d10	15.30	164	209347	20.00	ng/ul	0.00
62) Phenanthrene-d10	18.01	188	423354	20.00	ng/ul	0.00
78) Chrysene-d12	22.10	240	320397	20.00	ng/ul	0.00
86) Perylene-d12	24.70	264	309255	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.77	96	8976	4.66	ng/uL	0.00
5) Phenol-d5	7.82	99	207445	30.63	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.99	67	115591	30.34	ng/ul	0.00
9) 2-Chlorophenol-d4	8.22	132	187987	29.82	ng/ul	0.00
13) 4-Methylphenol-d8	9.40	113	181994	32.59	ng/ul	0.00
19) Nitrobenzene-d5	9.90	128	94596	31.13	ng/ul	0.00
22) 2-Nitrophenol-d4	10.63	143	99606	31.36	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	11.17	165	172033m	30.70	ng/ul	0.00
29) 4-Chloroaniline-d4	11.69	131	262048	38.84	ng/ul	0.00
44) Dimethylphthalate-d6	14.68	166	554996	35.24	ng/ul	0.00
47) Acenaphthylene-d8	15.00	160	720253	34.27	ng/ul	0.00
52) 4-Nitrophenol-d4	15.47	143	92687	33.14	ng/ul	0.00
58) Fluorene-d10	16.27	176	495819	34.95	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	16.40	200	30117	14.59	ng/ul	0.00
71) Anthracene-d10	18.11	188	742003	36.72	ng/ul	0.00
79) Pyrene-d10	20.34	212	661818	44.26	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.53	264	609024	38.50	ng/ul	0.00

6 U.M
 10/8/15

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.72	163	327795	20.47	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed