

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092915\
 Data File : BM002762.D
 Acq On : 30 Sep 2015 01:03
 Operator : UM/IZ
 Sample : G3838-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E5MW2

Quant Time: Sep 30 03:41:14 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 30 02:06:21 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.70	152	95096	20.00	ng/ul	0.00
18) Naphthalene-d8	11.56	136	406340	20.00	ng/ul	0.00
36) Acenaphthene-d10	15.29	164	204122	20.00	ng/ul	0.00
62) Phenanthrene-d10	18.00	188	411669	20.00	ng/ul	0.00
78) Chrysene-d12	22.09	240	428582	20.00	ng/ul	0.00
86) Perylene-d12	24.68	264	430305	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.77	96	8693	4.24	ng/uL	0.00
5) Phenol-d5	7.81	99	172172	23.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.99	67	99433	24.53	ng/ul	0.00
9) 2-Chlorophenol-d4	8.21	132	158387	23.62	ng/ul	0.00
13) 4-Methylphenol-d8	9.39	113	140828	23.70	ng/ul	0.00
19) Nitrobenzene-d5	9.89	128	75521	24.37	ng/ul	0.00
22) 2-Nitrophenol-d4	10.62	143	79034	24.40	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	11.16	165	128502	22.48	ng/ul	0.00
29) 4-Chloroaniline-d4	11.69	131	198154	28.80	ng/ul	0.00
44) Dimethylphthalate-d6	14.67	166	382584	24.91	ng/ul	0.00
47) Acenaphthylene-d8	15.00	160	504102	24.60	ng/ul	0.00
52) 4-Nitrophenol-d4	15.46	143	61344	22.50	ng/ul	0.00
58) Fluorene-d10	16.27	176	331997	24.00	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	16.39	200	36066	17.96	ng/ul	0.00
71) Anthracene-d10	18.10	188	479623	24.41	ng/ul	0.00
79) Pyrene-d10	20.33	212	500160	25.00	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.51	264	553545	25.15	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.72	163	185245	11.87	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092915\
Data File : BM002762.D
Acq On : 30 Sep 2015 01:03
Operator : UM/IZ
Sample : G3838-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5MW2

Quant Time: Sep 30 03:41:14 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM092915.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 30 02:06:21 2015
Response via : Initial Calibration

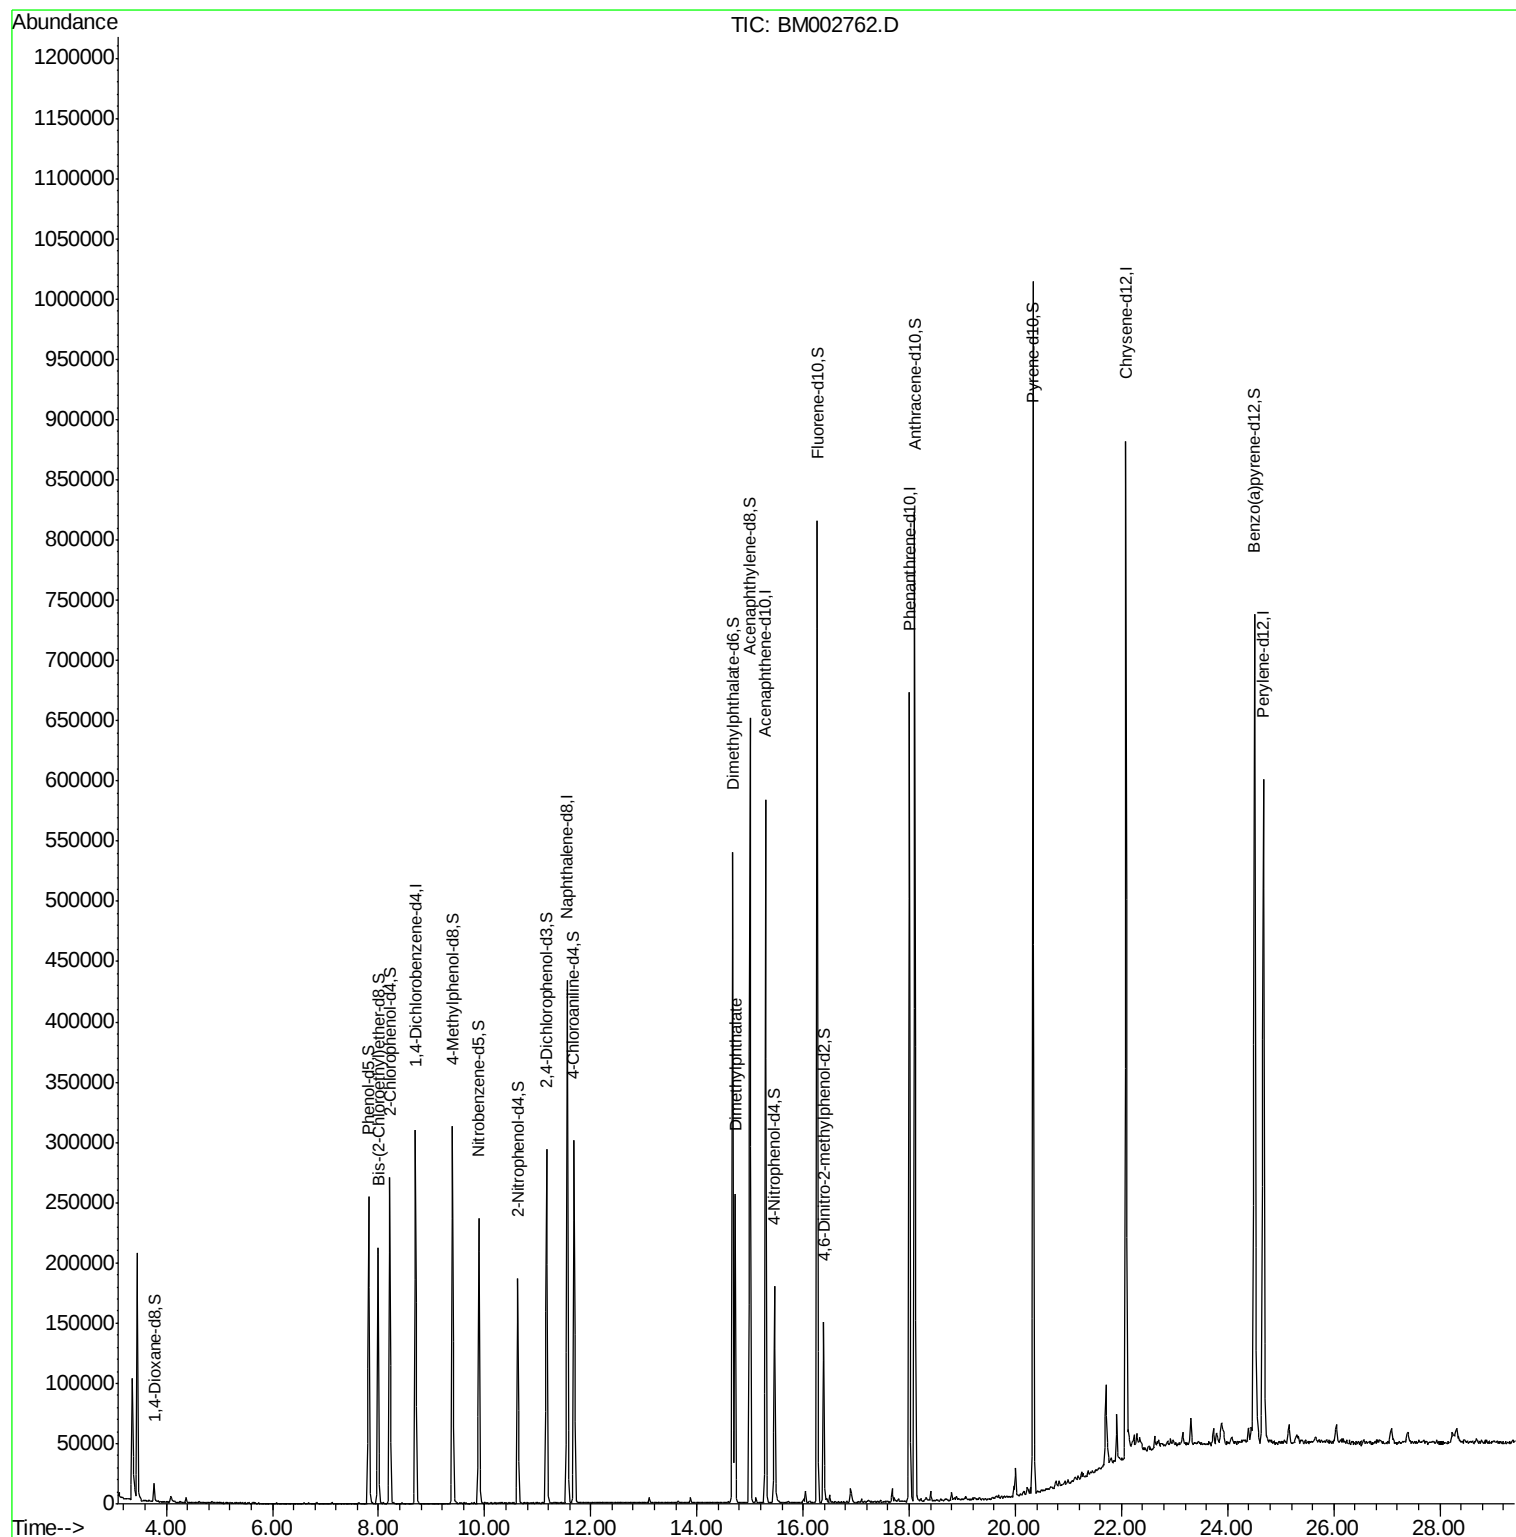

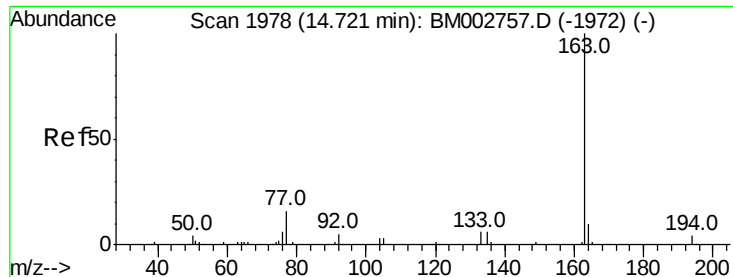

#45

Dimethylphthalate

Concen: 11.87 ng/ul

RT: 14.72 min Scan# 1978

Delta R.T. 0.00 min

Lab File: BM002762.D

Acq: 30 Sep 2015 01:03

Instrument :

BNA_M

ClientSampleId :

E5MW2


Tot Ion:163 Resp: 185245

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 9.9 8.1 12.1

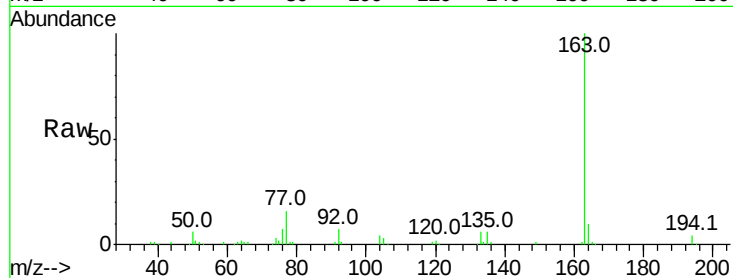

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

