

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092915\
 Data File : BM002764.D
 Acq On : 30 Sep 2015 02:17
 Operator : UM/IZ
 Sample : G3838-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E5MW8

Quant Time: Sep 30 03:41:27 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 30 02:06:21 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.70	152	96756	20.00	ng/ul	0.00
18) Naphthalene-d8	11.56	136	419386	20.00	ng/ul	0.00
36) Acenaphthene-d10	15.29	164	207934	20.00	ng/ul	0.00
62) Phenanthrene-d10	18.00	188	410294	20.00	ng/ul	0.00
78) Chrysene-d12	22.09	240	408745	20.00	ng/ul	0.00
86) Perylene-d12	24.68	264	404380	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.77	96	10359	4.97	ng/uL	0.00
5) Phenol-d5	7.81	99	216600	29.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.99	67	125723	30.49	ng/ul	0.00
9) 2-Chlorophenol-d4	8.21	132	200000	29.31	ng/ul	0.00
13) 4-Methylphenol-d8	9.40	113	183704	30.39	ng/ul	0.00
19) Nitrobenzene-d5	9.89	128	95620	29.90	ng/ul	0.00
22) 2-Nitrophenol-d4	10.62	143	101367	30.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	11.16	165	164873	27.95	ng/ul	0.00
29) 4-Chloroaniline-d4	11.69	131	244622	34.45	ng/ul	0.00
44) Dimethylphthalate-d6	14.67	166	484234	30.95	ng/ul	0.00
47) Acenaphthylene-d8	15.00	160	636476	30.49	ng/ul	0.00
52) 4-Nitrophenol-d4	15.46	143	79855	28.75	ng/ul	0.00
58) Fluorene-d10	16.27	176	418607	29.71	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	16.39	200	49248	24.61	ng/ul	0.00
71) Anthracene-d10	18.10	188	601927	30.74	ng/ul	0.00
79) Pyrene-d10	20.33	212	611876	32.07	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.51	264	664461	32.12	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.72	163	168353	10.59	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092915\
Data File : BM002764.D
Acq On : 30 Sep 2015 02:17
Operator : UM/IZ
Sample : G3838-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5MW8

Quant Time: Sep 30 03:41:27 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM092915.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 30 02:06:21 2015
Response via : Initial Calibration

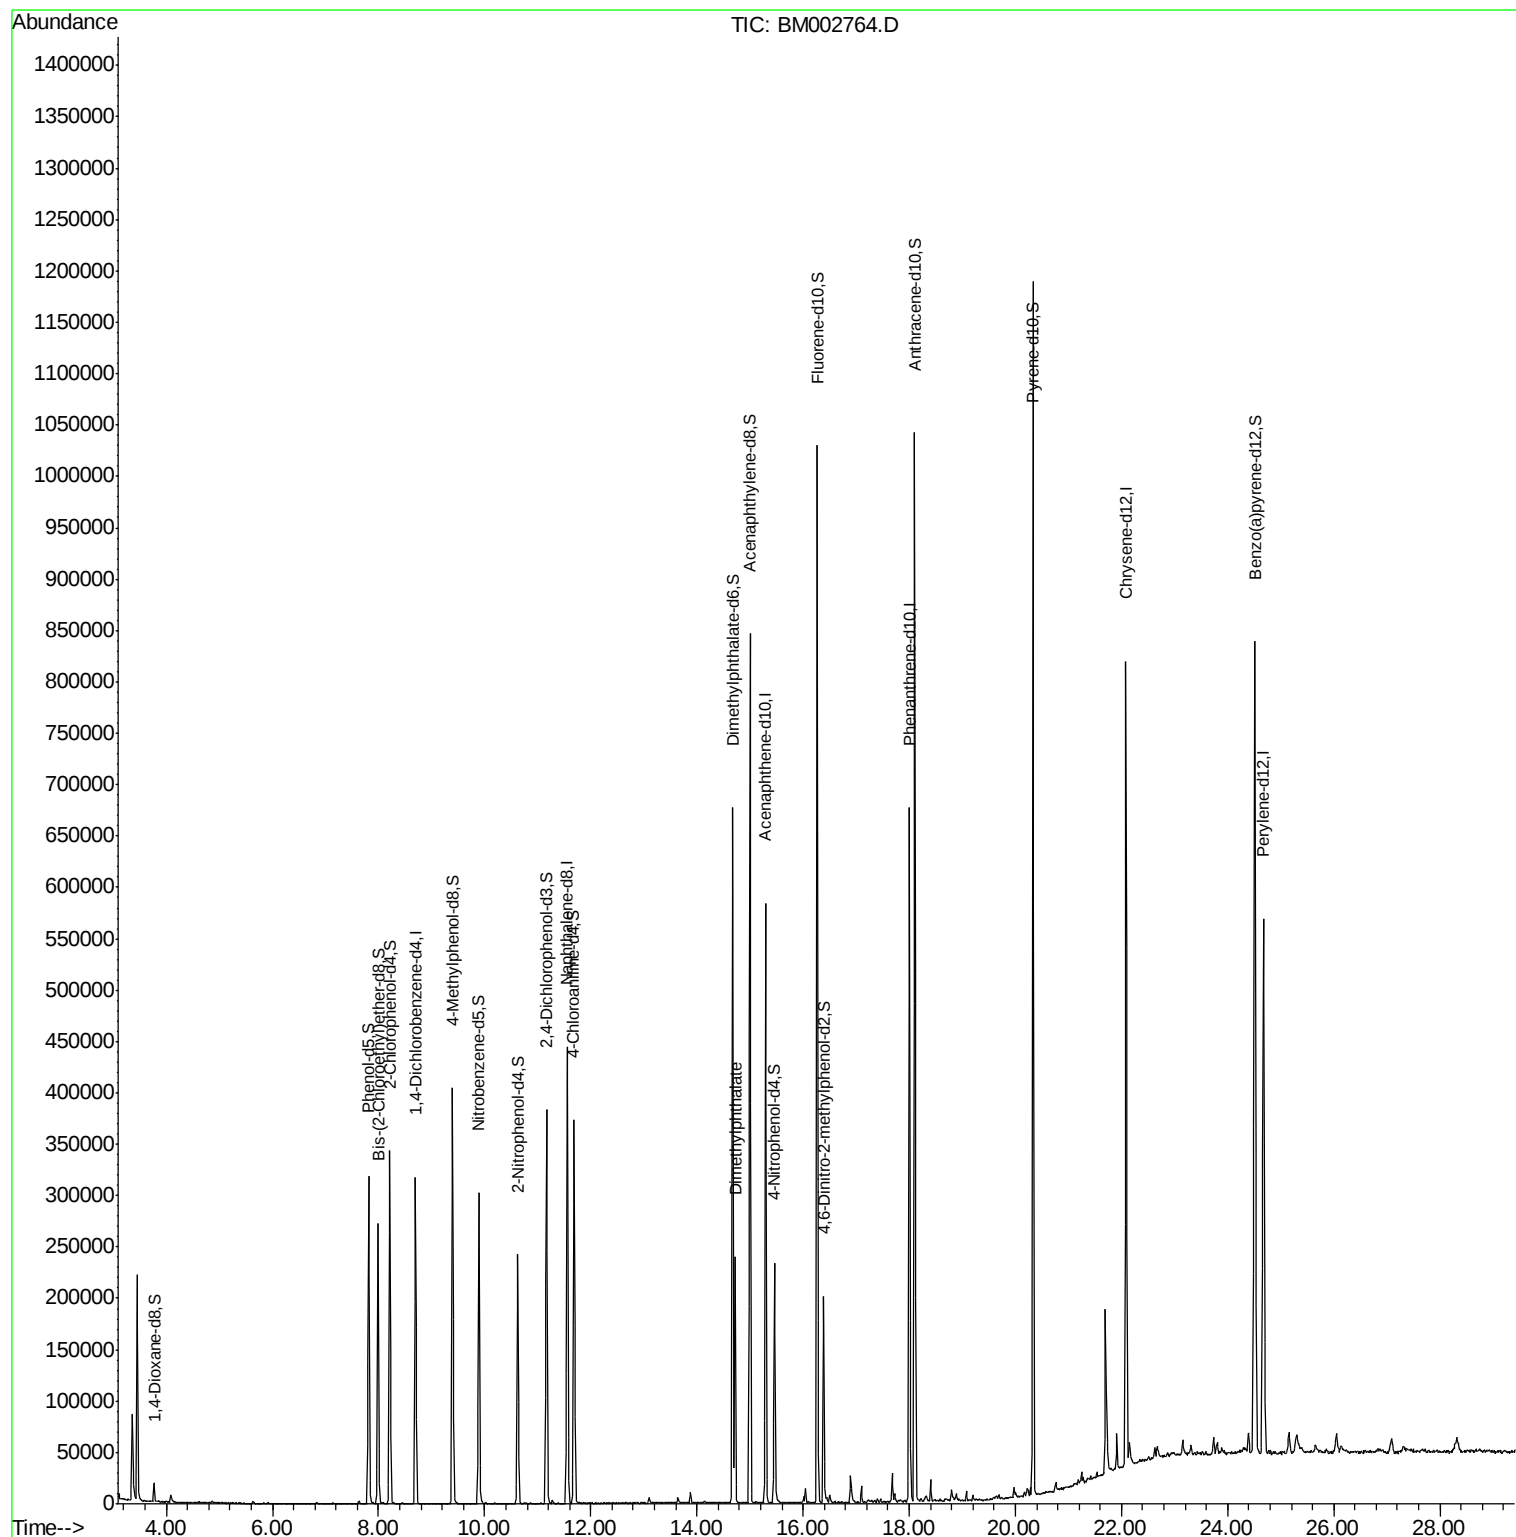

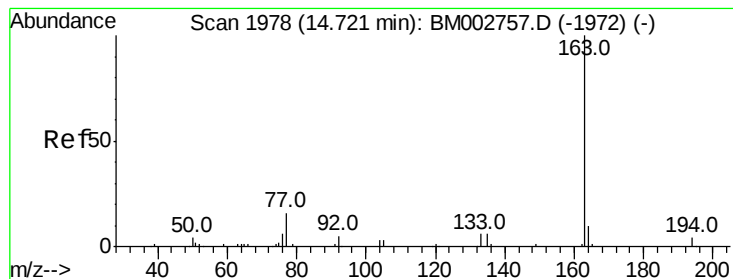

#45

Dimethylphthalate

Concen: 10.59 ng/ul

RT: 14.72 min Scan# 1978

Delta R.T. 0.00 min

Lab File: BM002764.D

Acq: 30 Sep 2015 02:17

Instrument :

BNA_M

ClientSampleId :

E5MW8



Tot Ion:163 Resp: 168353

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 9.8 8.1 12.1

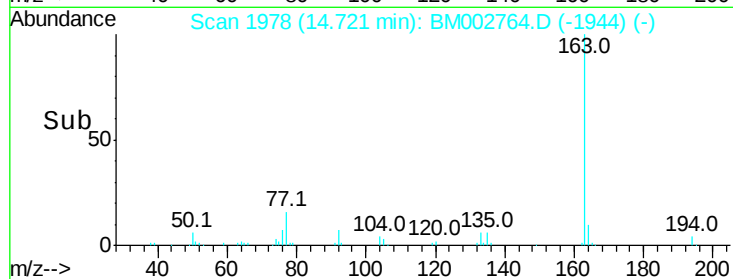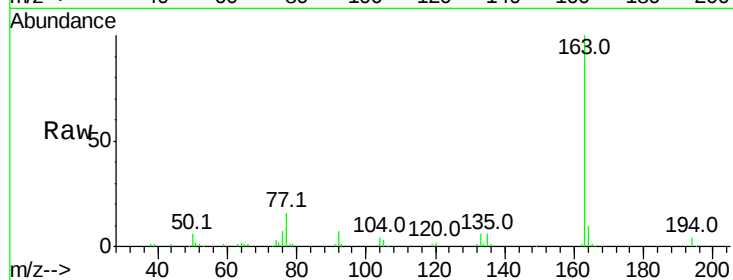

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

